
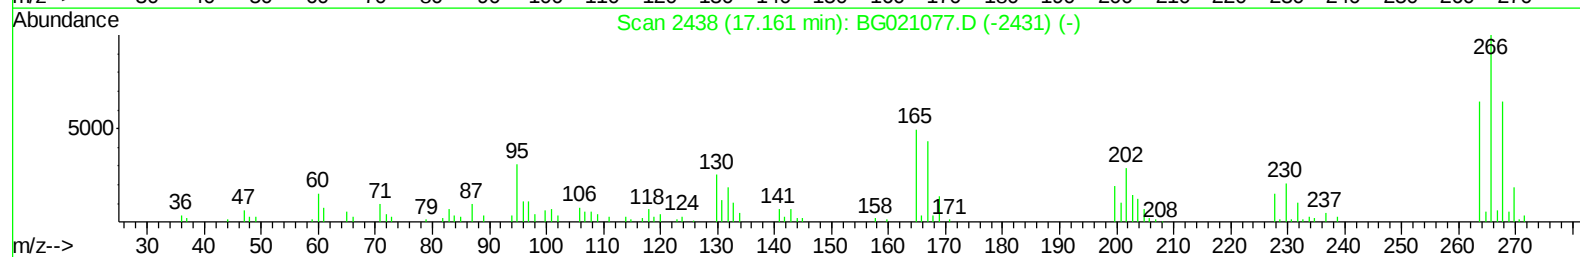
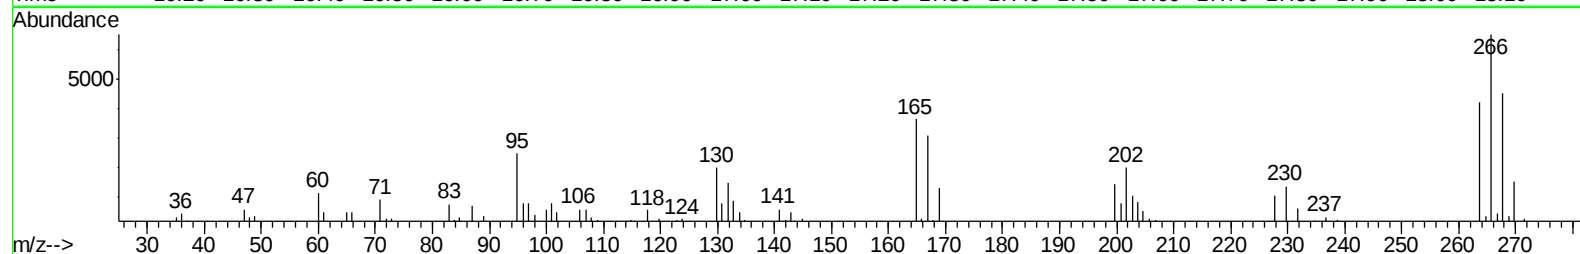


Data Path : Z:\HPCHEM1\BNA G\Data\BG022716\
Data File : BG021133.D
Acq On : 28 Feb 2016 2:53
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 29 05:45:34 2016
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG022616.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Feb 26 16:39:44 2016
Response via : Initial Calibration

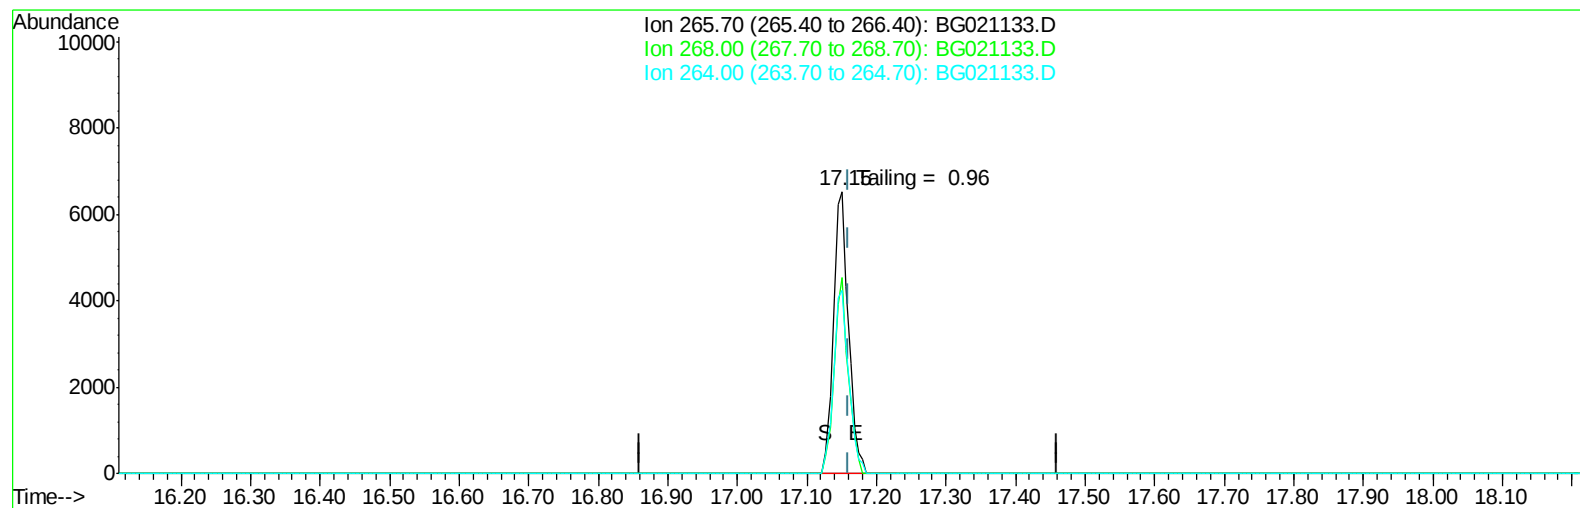

TIC: BG021133.D

(69) Pentachlorophenol (C)




17.151min (-0.011) 0.00ng

response 9787

Ion	Exp%	Act%
265.70	100	100
268.00	63.80	74.36
264.00	59.80	70.19
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA G\Data\BG022716\
Data File : BG021133.D
Acq On : 28 Feb 2016 2:53
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 29 05:45:34 2016
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG022616.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Feb 26 16:39:44 2016
Response via : Initial Calibration

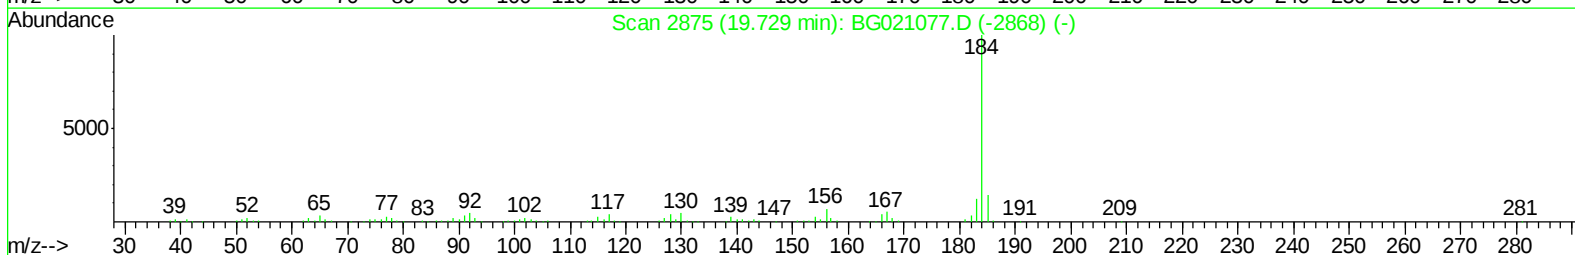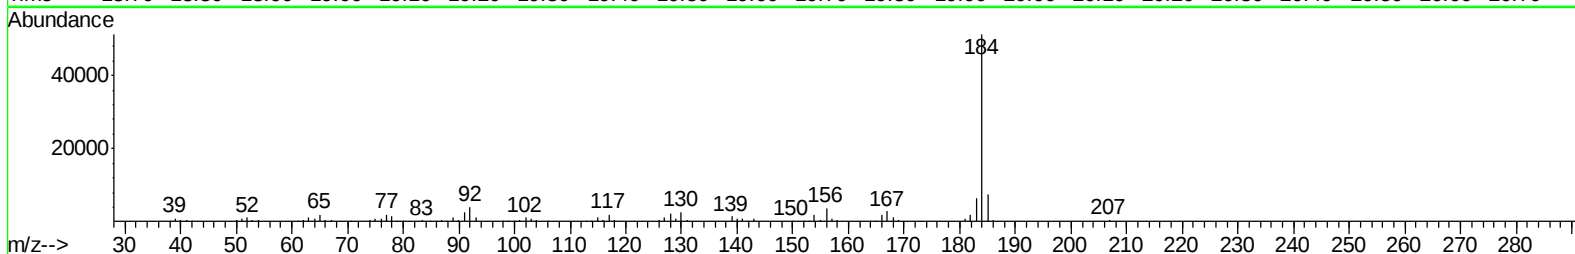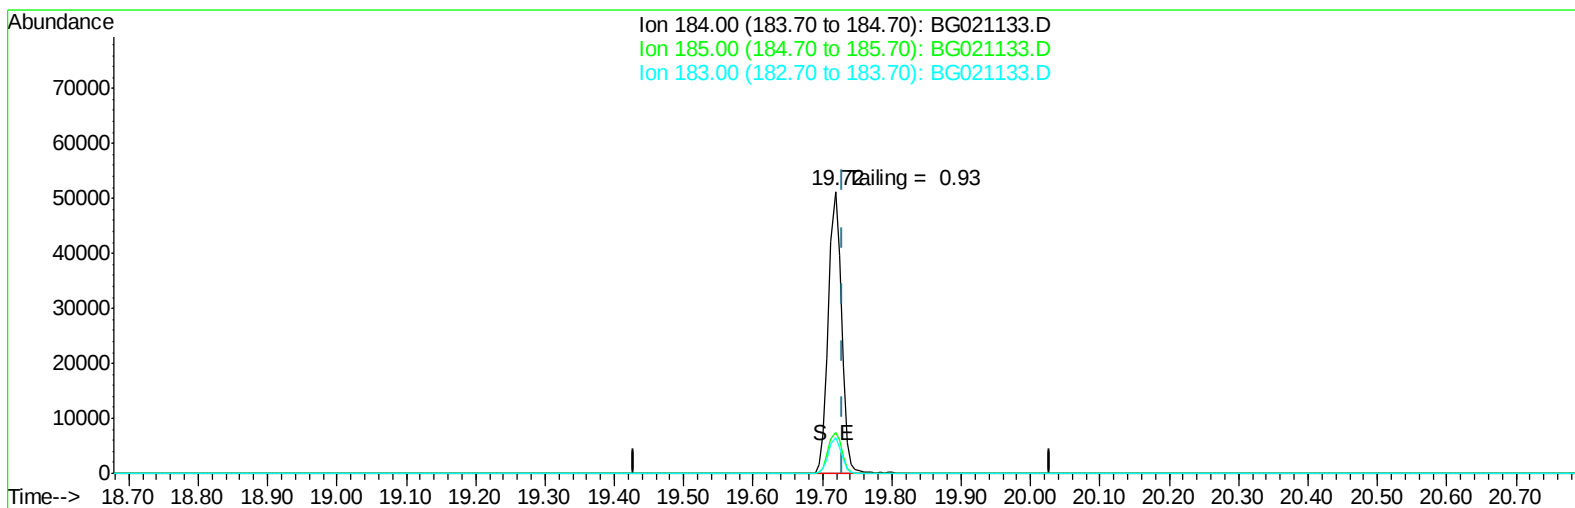

TIC: BG021133.D

(76) Benzidine

19.718min (-0.011) 0.00ng

response 67537

Ion	Exp%	Act%
184.00	100	100
185.00	14.40	14.56
183.00	12.60	12.60
0.00	0.00	0.00