


Data Path : Z:\HPCHEM1\BNA G\Data\BG022716\
 Data File : BG021099.D
 Acq On : 27 Feb 2016 4:40
 Operator : UM/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG022616.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Feb 26 16:39:44 2016

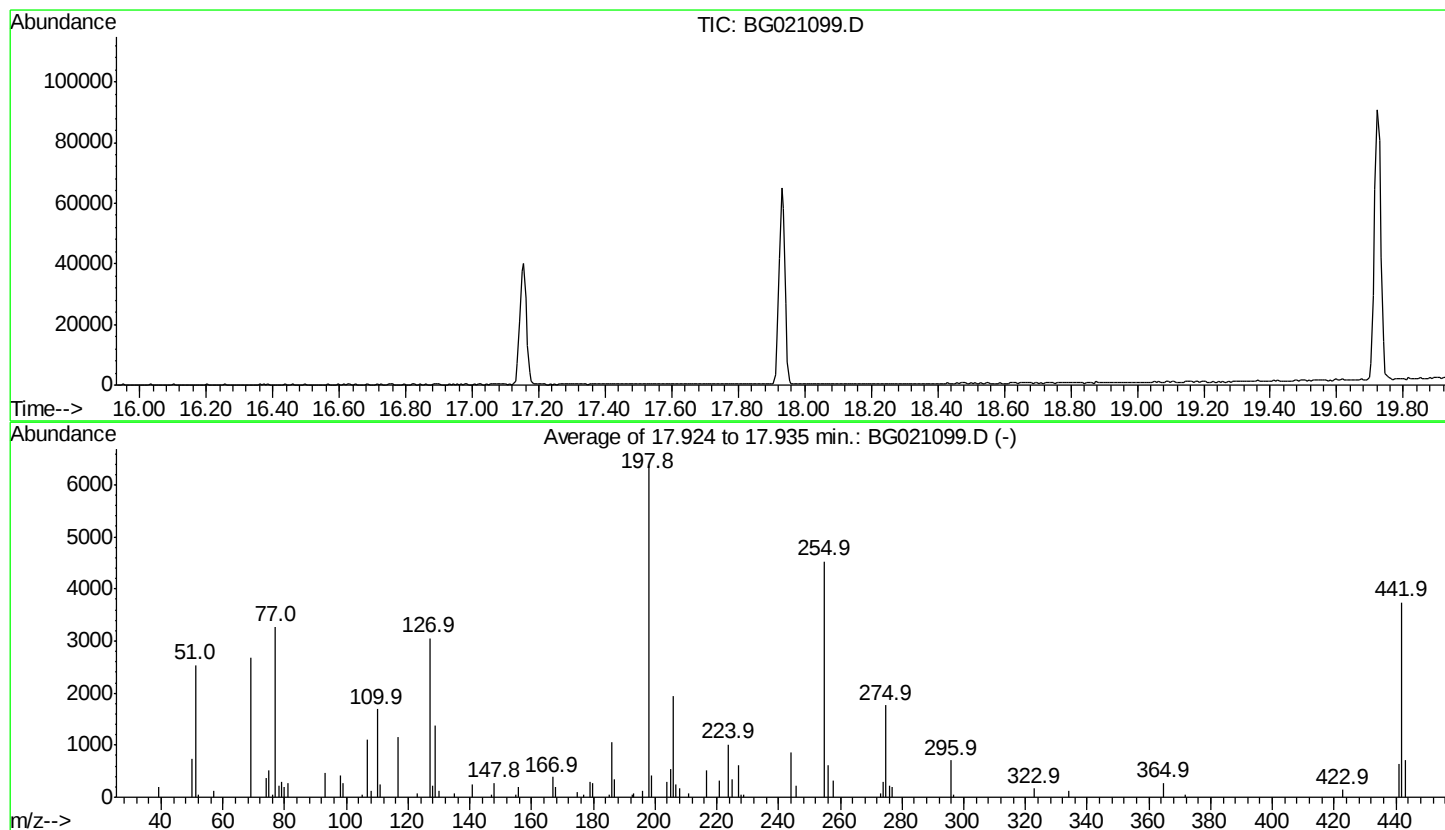

AutoFind: Scans 2567, 2568, 2569; Background Corrected with Scan 2562

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	39.9	2539	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	42.1	2684	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	47.9	3050	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	6368	PASS
199	198	5	9	6.6	422	PASS
275	198	10	60	27.6	1759	PASS
365	198	1	100	4.3	274	PASS
441	442	0.01	24	17.2	643	PASS
442	198	50	100	58.8	3746	PASS
443	442	15	24	19.0	710	PASS