


Data Path : Z:\HPCHEM1\BNA G\DATA\BG022716\
 Data File : BG021115.D
 Acq On : 27 Feb 2016 15:07
 Operator : UM/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG022616.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Feb 26 16:39:44 2016

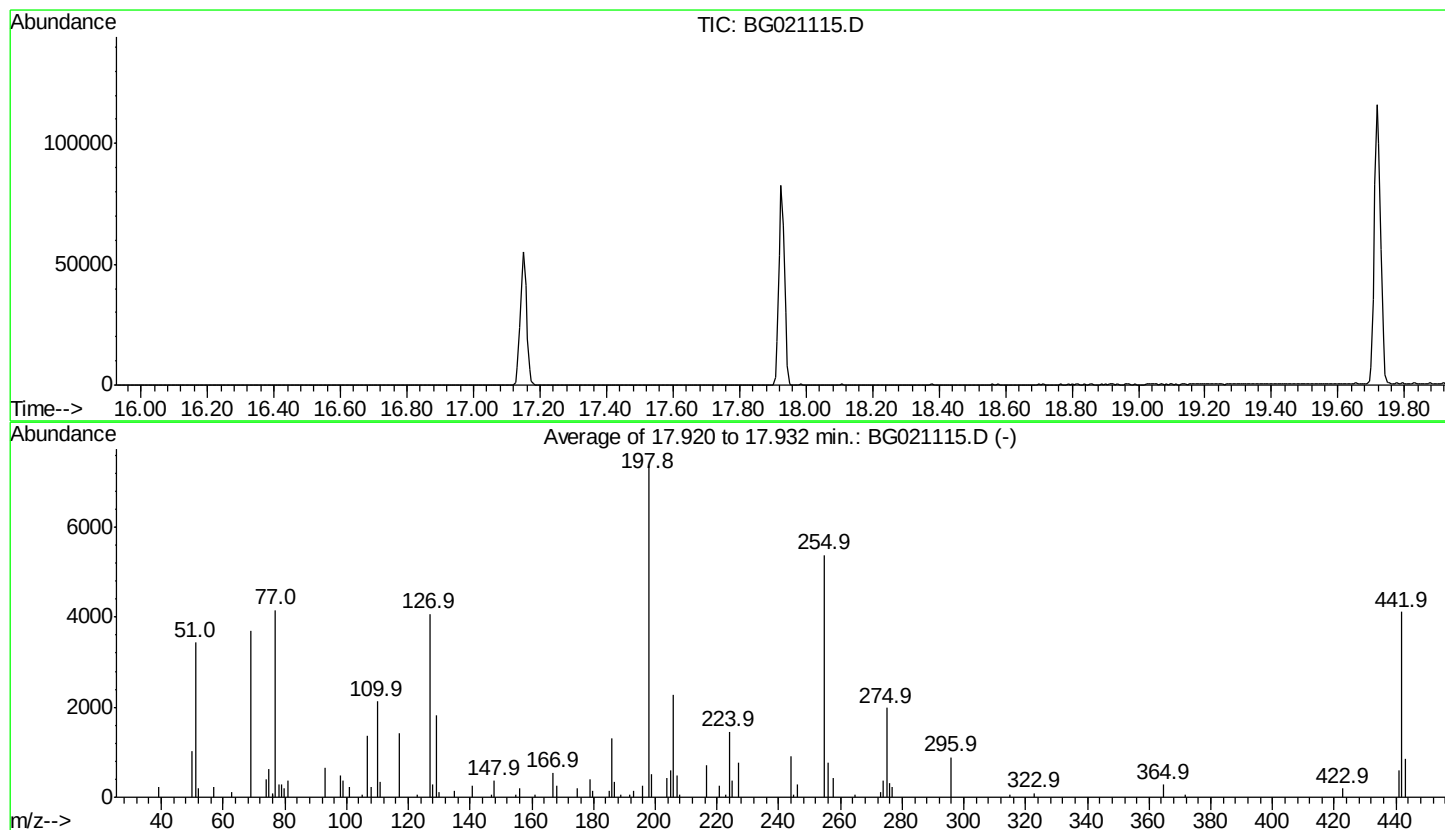

AutoFind: Scans 2567, 2568, 2569; Background Corrected with Scan 2562

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	46.7	3439	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	50.3	3704	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	55.4	4079	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	7363	PASS
199	198	5	9	6.9	511	PASS
275	198	10	60	26.9	1981	PASS
365	198	1	100	3.8	279	PASS
441	442	0.01	24	14.3	588	PASS
442	198	50	100	55.8	4108	PASS
443	442	15	24	20.5	842	PASS