


Data Path : Z:\HPCHEM1\BNA_G\Data\BG022716\
 Data File : BG021133.D
 Acq On : 28 Feb 2016 2:53
 Operator : UM/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG022616.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Feb 26 16:39:44 2016

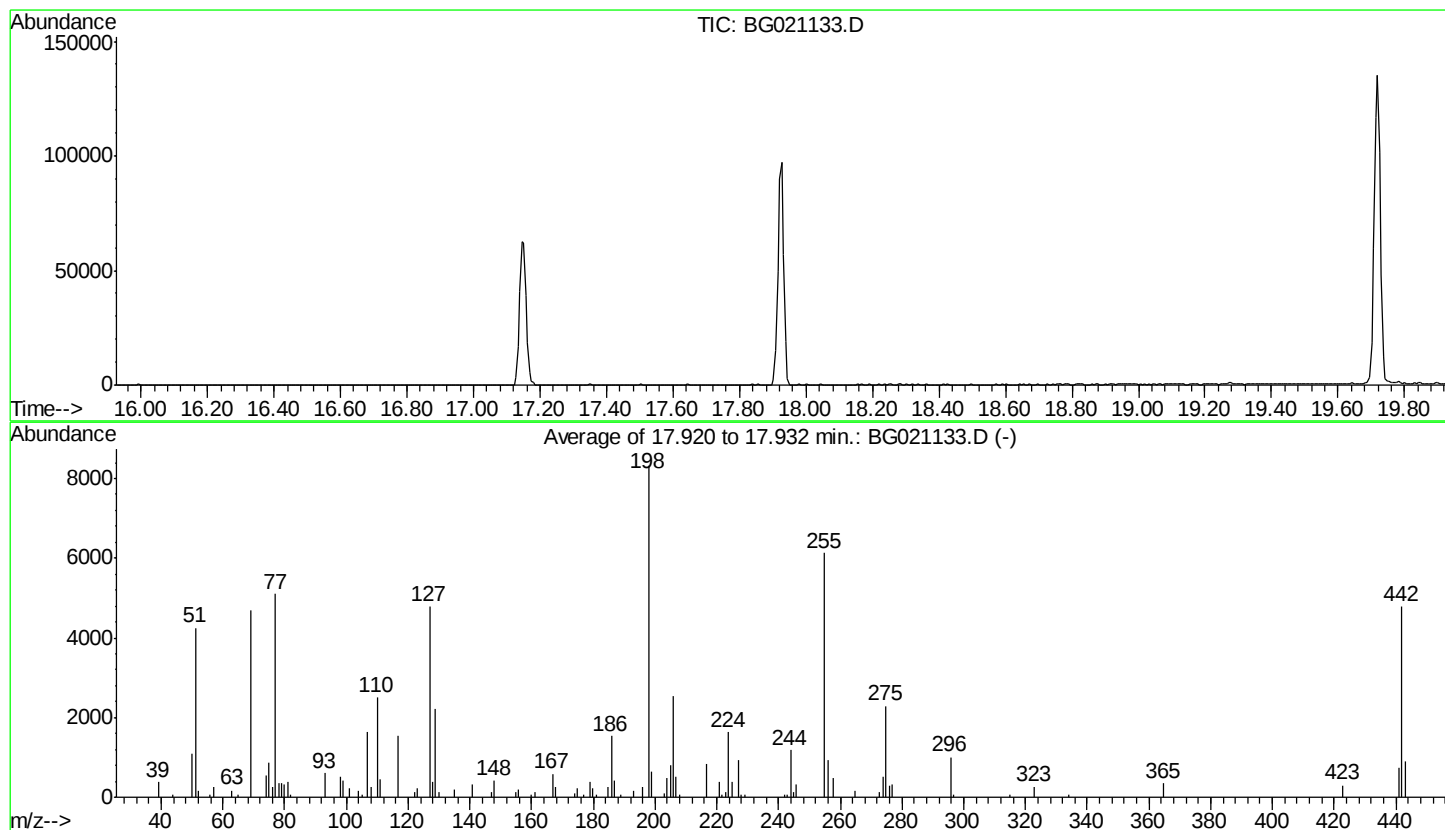

AutoFind: Scans 2567, 2568, 2569; Background Corrected with Scan 2561

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	51.2	4258	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	56.5	4699	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	57.4	4781	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	8323	PASS
199	198	5	9	7.8	651	PASS
275	198	10	60	27.5	2287	PASS
365	198	1	100	4.2	349	PASS
441	442	0.01	24	15.7	752	PASS
442	198	50	100	57.5	4783	PASS
443	442	15	24	18.6	892	PASS