
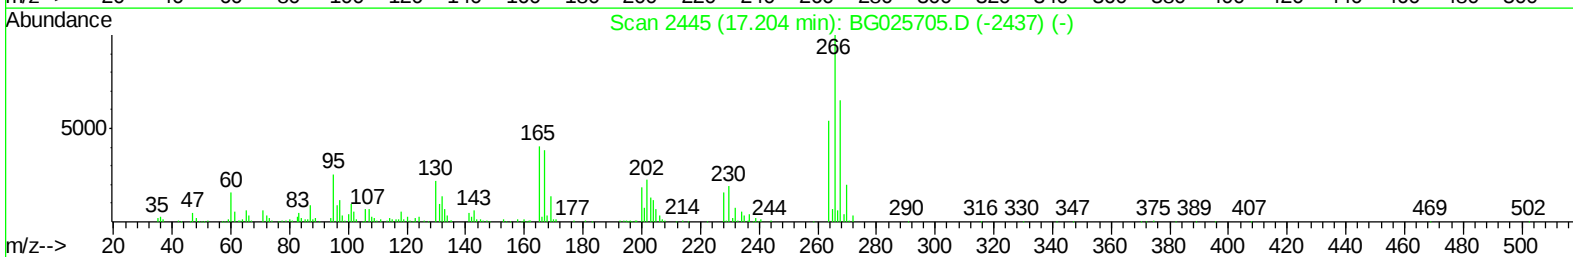
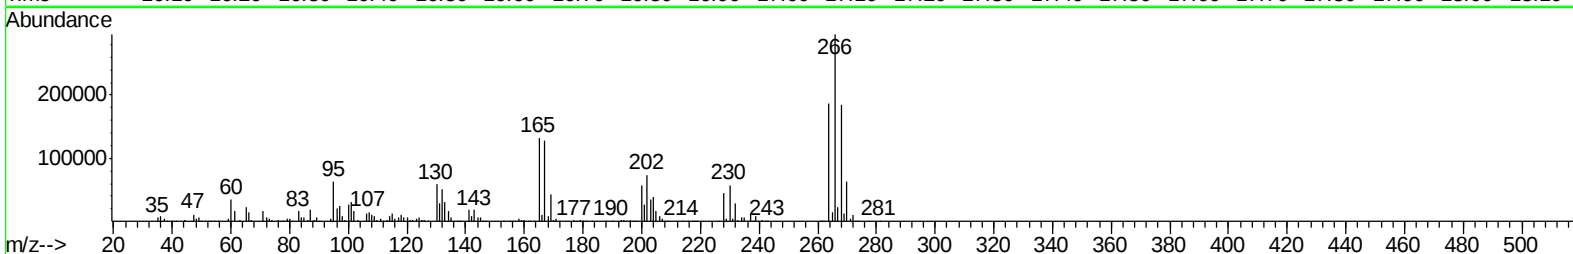


Data File : BG025962.D
Acq On : 27 Feb 2017 13:55
Operator : SJ/MA
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 28 06:07:04 2017
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG021717.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Feb 17 15:48:21 2017
Response via : Initial Calibration

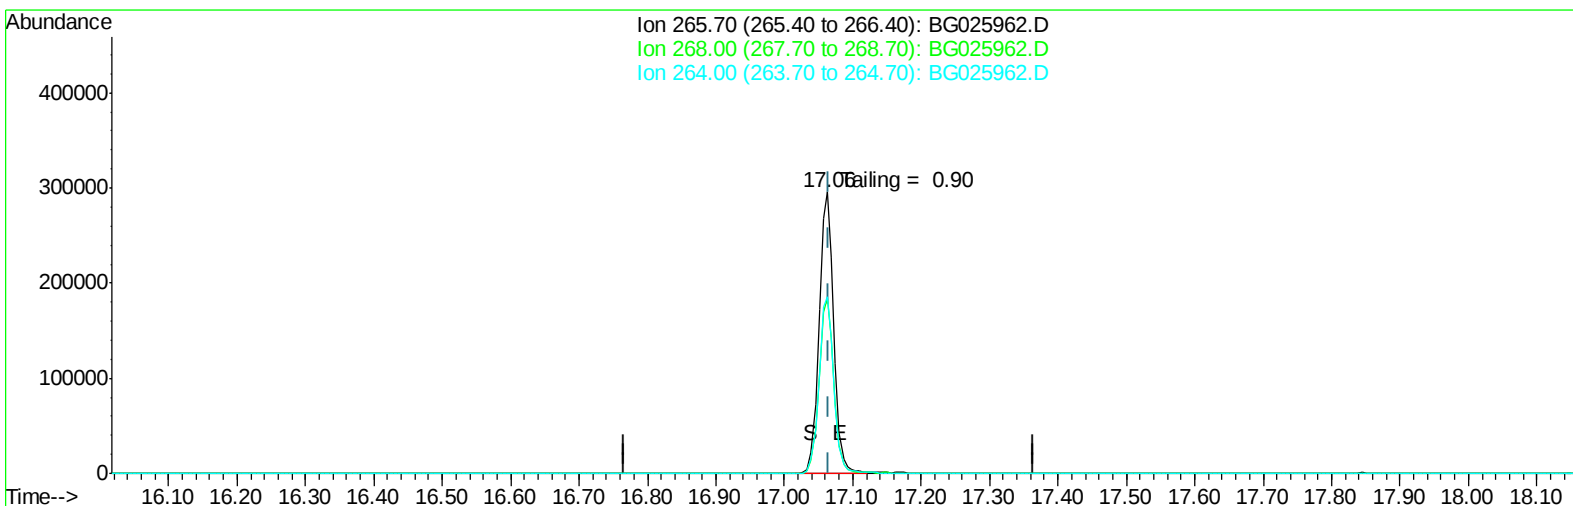

TIC: BG025962.D

(69) Pentachlorophenol (C)




17.063min (-0.003) 1094016.29ng

response 444685

Ion	Exp%	Act%
265.70	100	100
268.00	60.70	62.25
264.00	62.60	62.72
0.00	0.00	0.00

Data File : BG025962.D
Acq On : 27 Feb 2017 13:55
Operator : SJ/MA
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 28 06:07:04 2017
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG021717.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Feb 17 15:48:21 2017
Response via : Initial Calibration

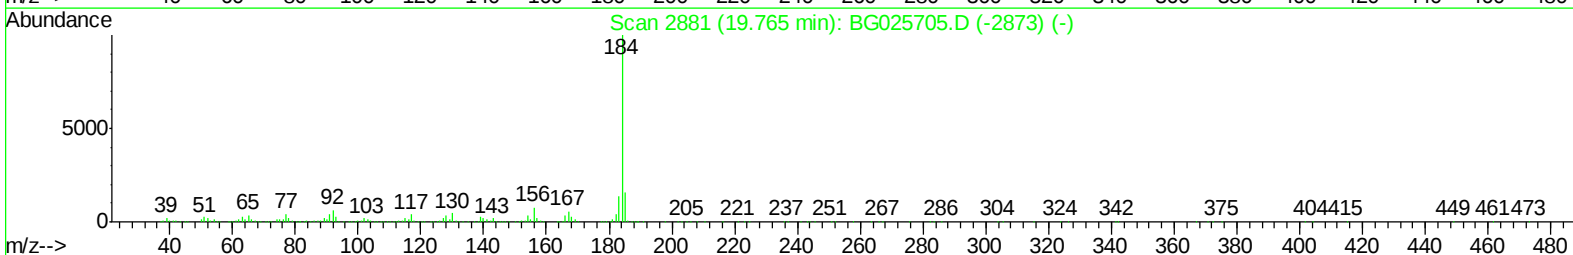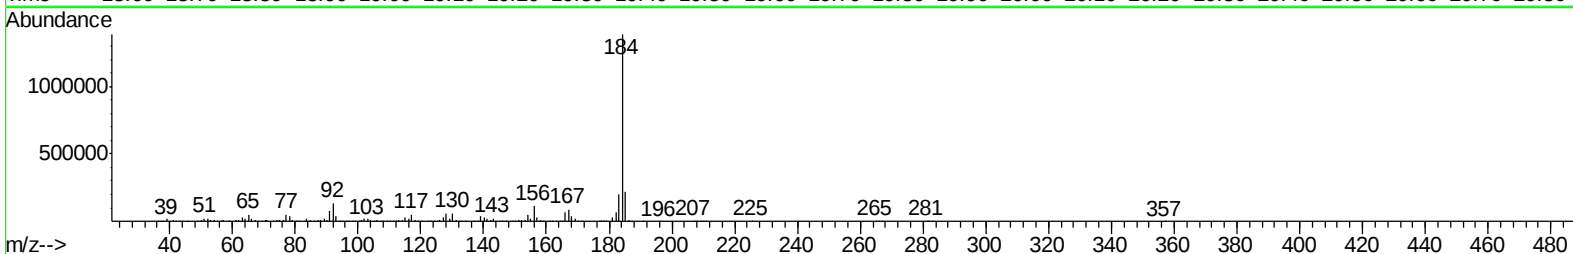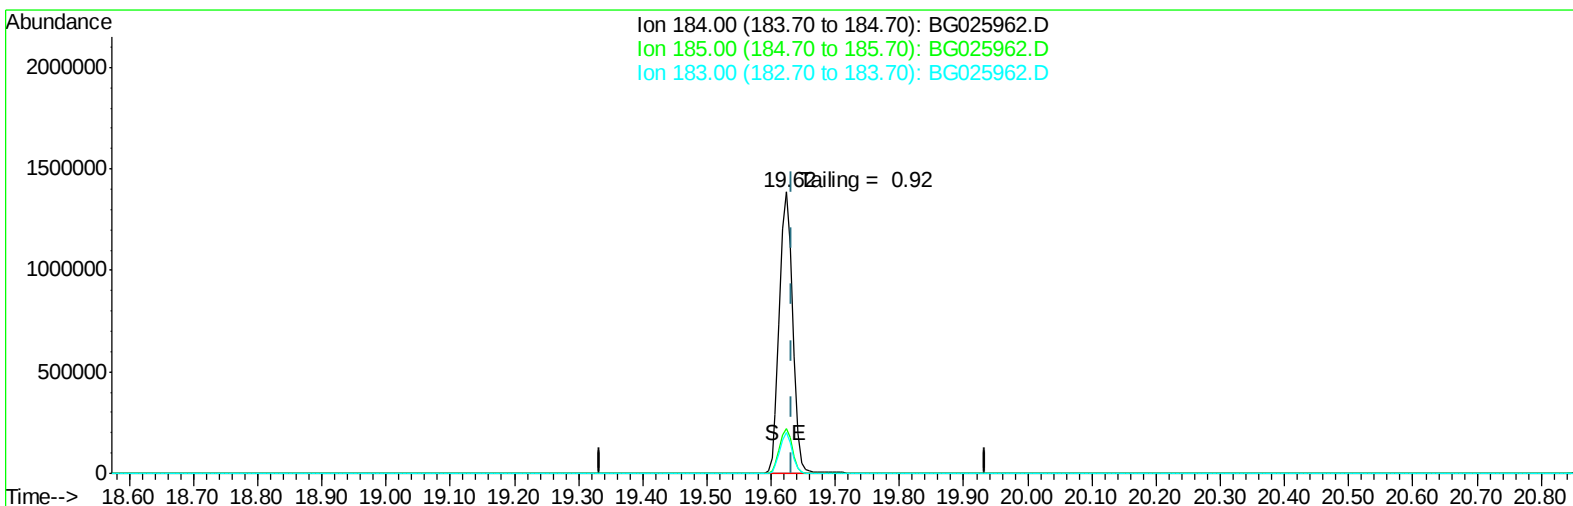

TIC: BG025962.D

(76) Benzidine

19.624min (-0.009) 58131.51ng

response 2033244

Ion	Exp%	Act%
184.00	100	100
185.00	16.30	16.07
183.00	13.80	14.42
0.00	0.00	0.00