
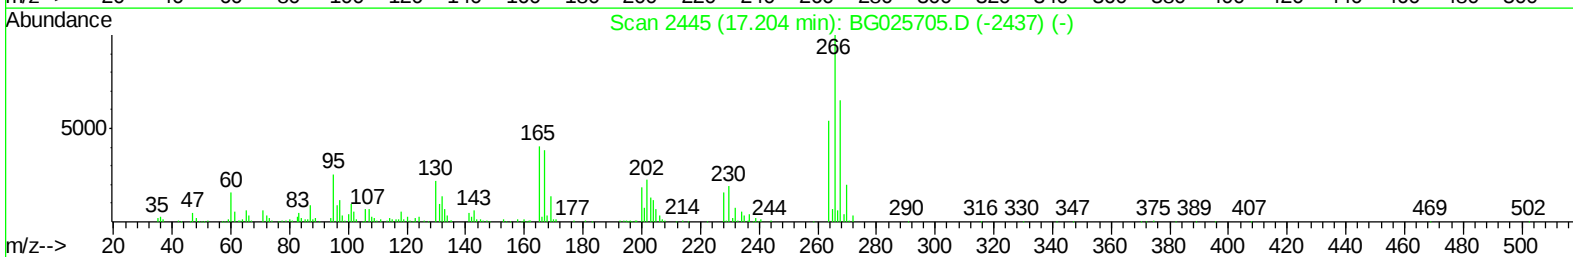
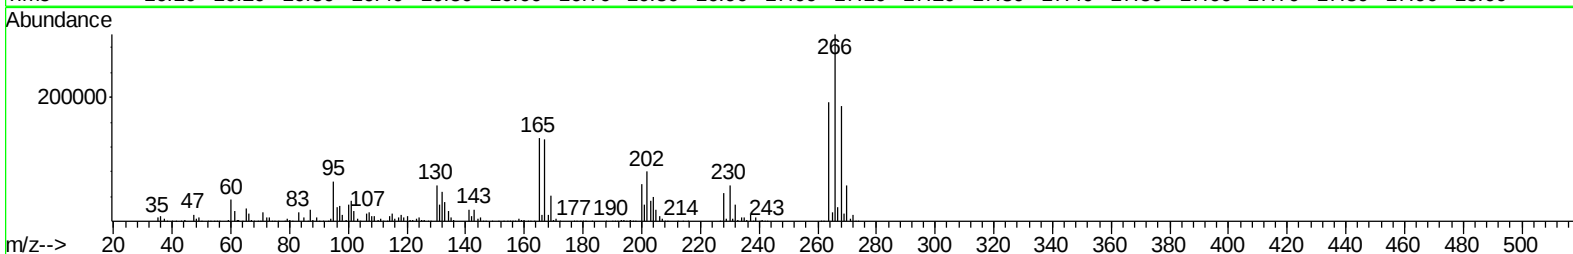


Data File : BG025977.D
Acq On : 27 Feb 2017 23:47
Operator : SJ/MA
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 28 06:09:21 2017
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG021717.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Feb 17 15:48:21 2017
Response via : Initial Calibration

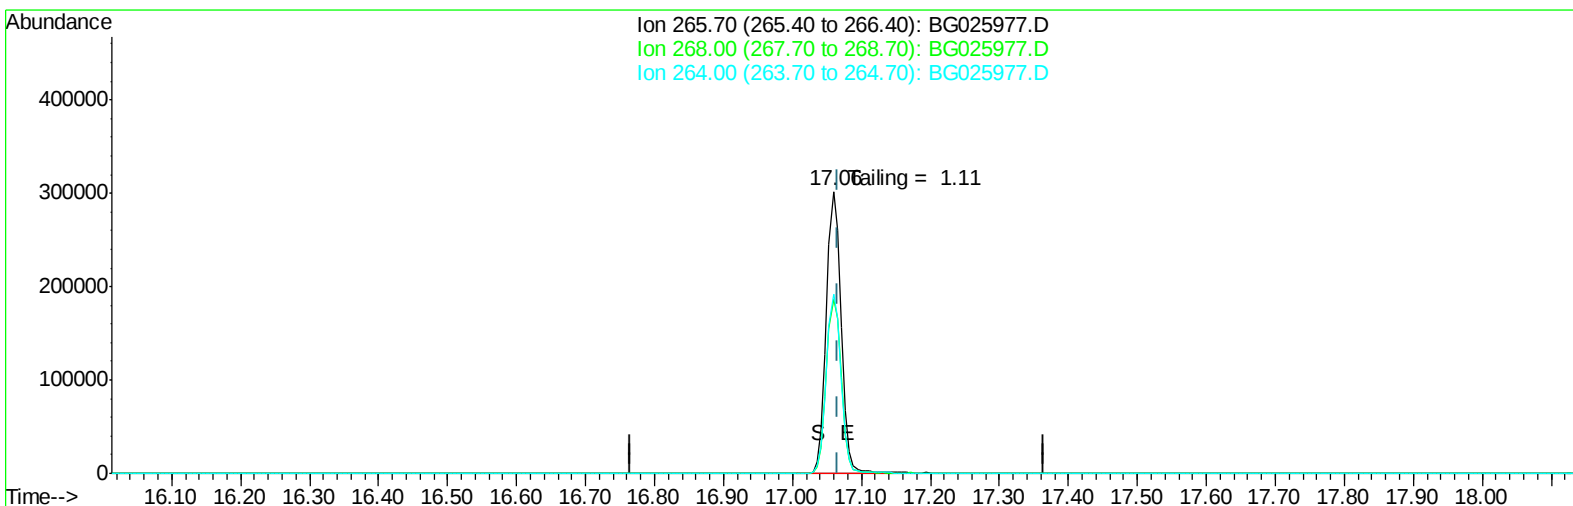

TIC: BG025977.D

(69) Pentachlorophenol (C)




17.059min (-0.007) 537012.26ng

response 447294

Ion	Exp%	Act%
265.70	100	100
268.00	60.70	61.88
264.00	62.60	63.51
0.00	0.00	0.00

Data File : BG025977.D
Acq On : 27 Feb 2017 23:47
Operator : SJ/MA
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 28 06:09:21 2017
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG021717.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Feb 17 15:48:21 2017
Response via : Initial Calibration

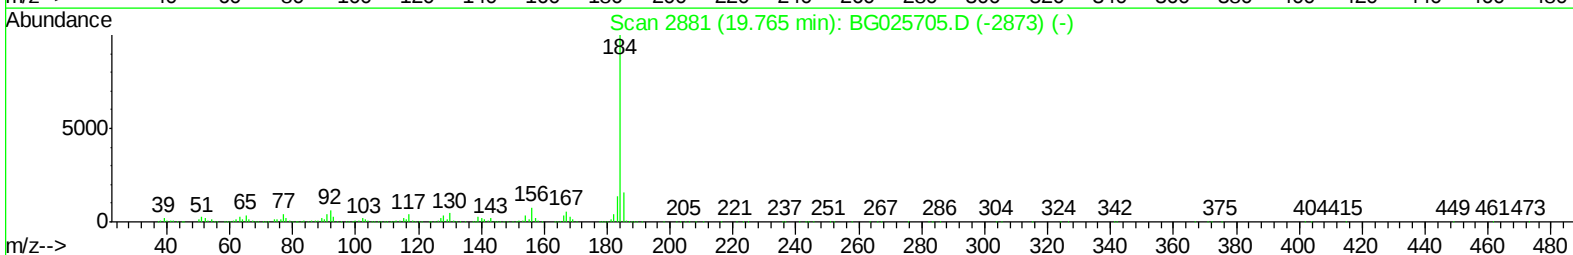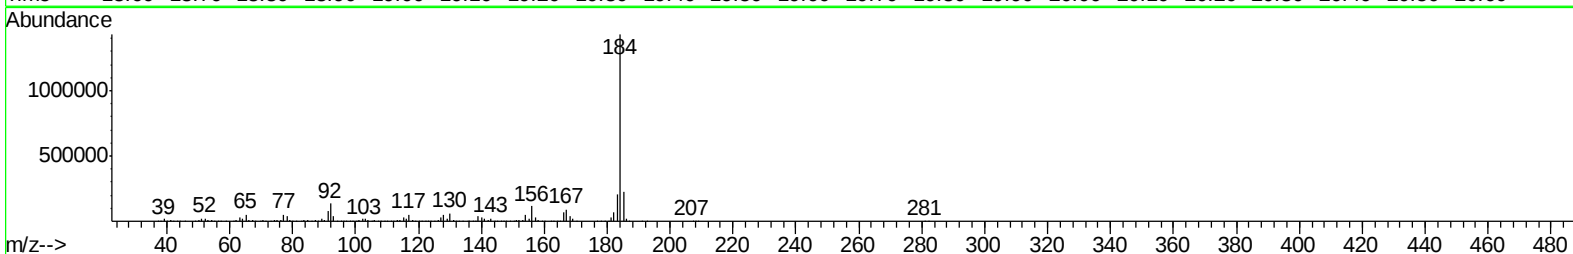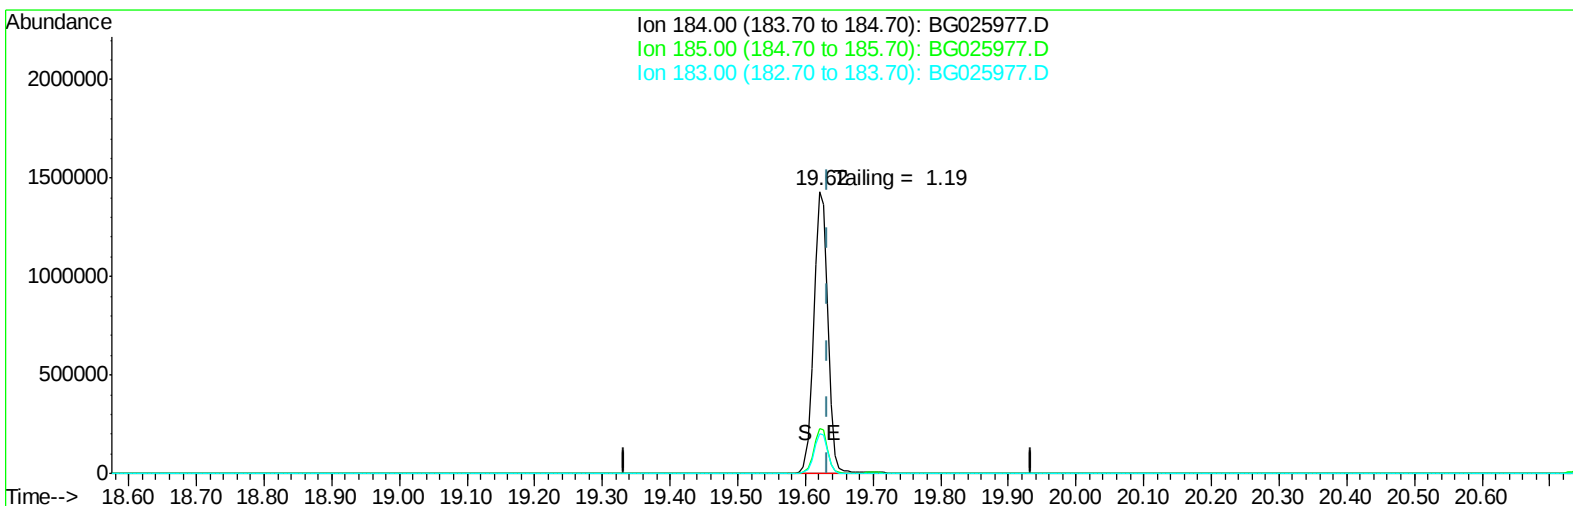

TIC: BG025977.D

(76) Benzidine

19.621min (-0.013) 457373.69ng

response 2122397

Ion	Exp%	Act%
184.00	100	100
185.00	16.30	15.99
183.00	13.80	14.25
0.00	0.00	0.00