

Data Path : Z:\HPCHEM1\BNA G\DATA\BG022717\
 Data File : BG025964.D
 Acq On : 27 Feb 2017 15:14
 Operator : SJ/MA
 Sample : PB97193BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 PB97193BL

Quant Time: Feb 27 23:57:07 2017
 Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG021717.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Feb 17 15:48:21 2017
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.08	152	79552	20.00	ng	0.00
21) Naphthalene-d8	10.88	136	358381	20.00	ng	-0.01
38) Acenaphthene-d10	14.68	164	241234	20.00	ng	-0.01
63) Phenanthrene-d10	17.41	188	698023	20.00	ng	0.00
75) Chrysene-d12	21.65	240	773600	20.00	ng	-0.03
86) Perylene-d12	24.85	264	749657	20.00	ng	-0.03
System Monitoring Compounds						
5) 2-Fluorophenol	5.65	112	711154	155.64	ng	0.00
7) Phenol-d6	7.23	99	981590	145.17	ng	0.00
23) Nitrobenzene-d5	9.23	82	527770	92.94	ng	-0.01
41) 2,4,6-Tribromophenol	16.16	330	444068	199.25	ng	0.00
44) 2-Fluorobiphenyl	13.31	172	1400048	101.41	ng	-0.01
78) Terphenyl-d14	20.01	244	2441524	76.76	ng	-0.01


Target Compounds Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA G\DATA\BG022717\
Data File : BG025964.D
Acq On : 27 Feb 2017 15:14
Operator : SJ/MA
Sample : PB97193BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
PB97193BL

Quant Time: Feb 27 23:57:07 2017
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG021717.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Feb 17 15:48:21 2017
Response via : Initial Calibration

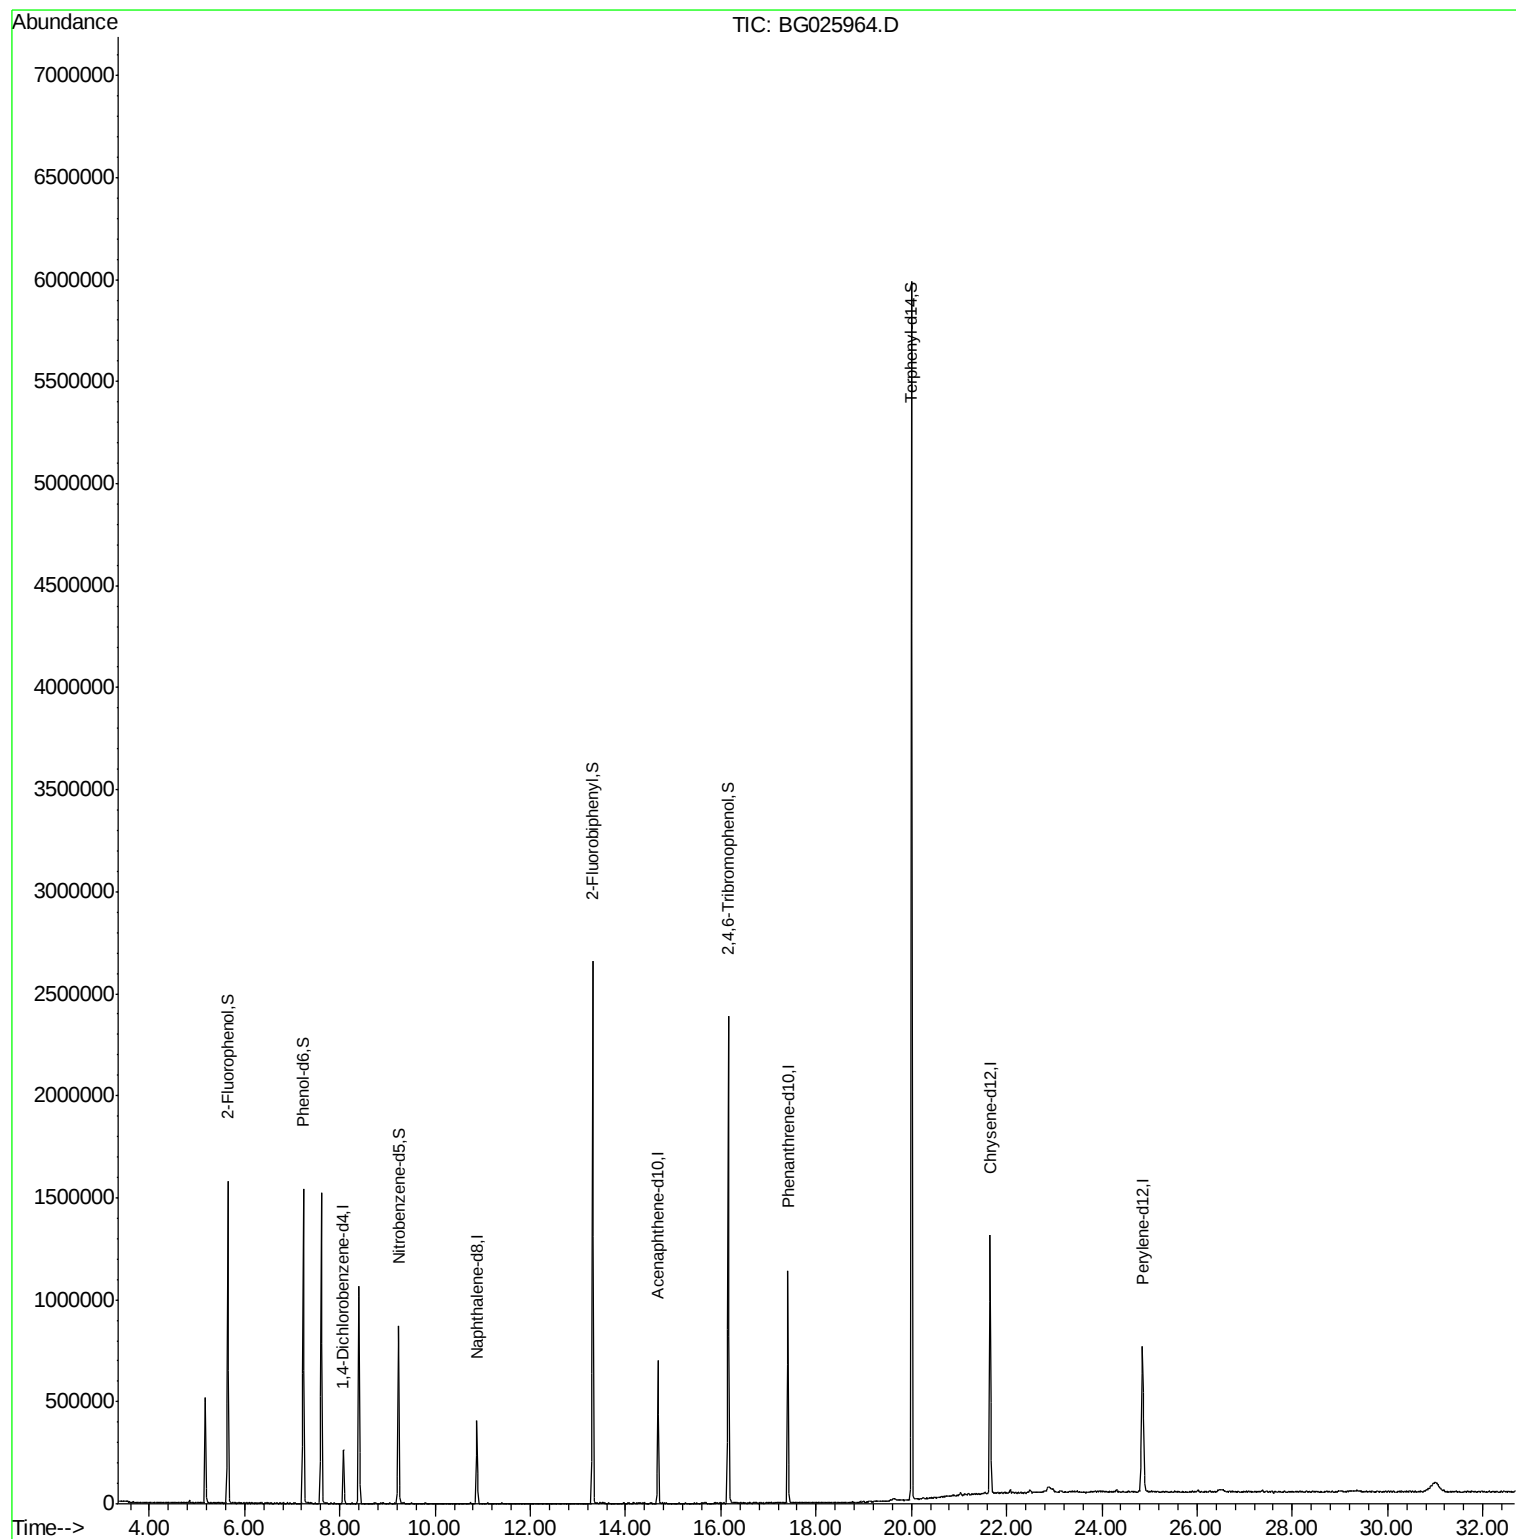




#1




1,4-Dichlorobenzene-d4
Concen: 20.00 ng
RT: 8.08 min Scan# 807
Delta R.T. -0.01 min
Lab File: BG025964.D
Acq: 27 Feb 2017 15:14

Instrument :
BNA_G
ClientSampleID :
PB97193BL

Tot Ion	Ratio	Lower	Upper
152	100		
150	151.1	114.0	171.0
115	54.1	48.1	72.1

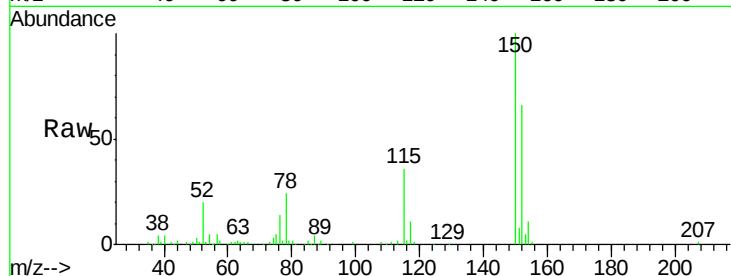


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

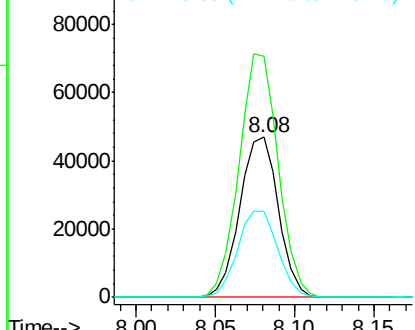



#5


2-Fluorophenol
Concen: 155.64 ng
RT: 5.65 min Scan# 393
Delta R.T. -0.01 min
Lab File: BG025964.D
Acq: 27 Feb 2017 15:14

Tgt Ion	Ratio	Lower	Upper
112	100		
64	65.5	61.8	92.6
63	32.6	37.2	55.8



Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BGC
Ion 63.00 (62.70 to 63.70): BGC

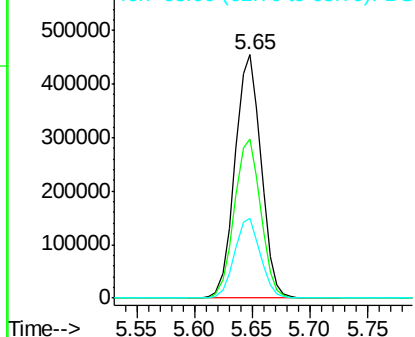

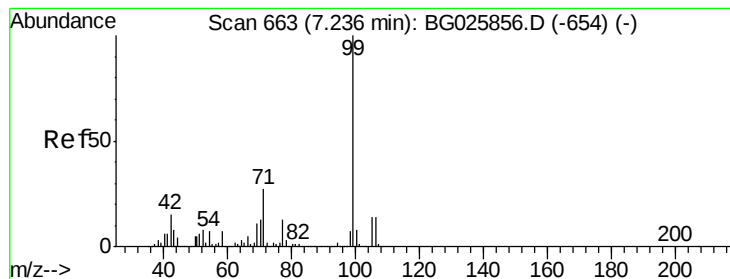

#7

Phenol-d6

Concen: 145.17 ng

RT: 7.23 min Scan# 663

Delta R.T. -0.00 min

Lab File: BG025964.D

Acq: 27 Feb 2017 15:14

Instrument :

BNA_G

ClientSampleId :

PB97193BL


Tot Ion: 99 Resp: 981590

Ion Ratio Lower Upper




99 100

42 15.0 20.5 30.7#

71 28.8 37.6 56.4#

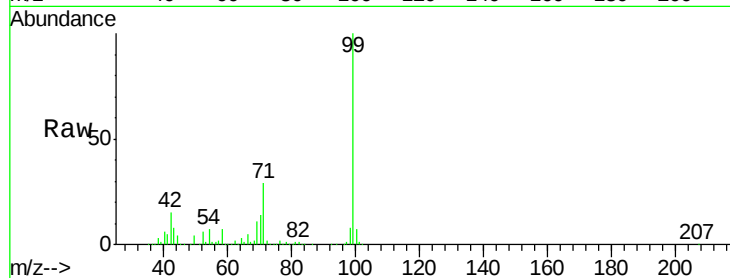

Abundance Ion 99.00 (98.70 to 99.70): BGC
Ion 42.00 (41.70 to 42.70): BGC
Ion 71.00 (70.70 to 71.70): BGC

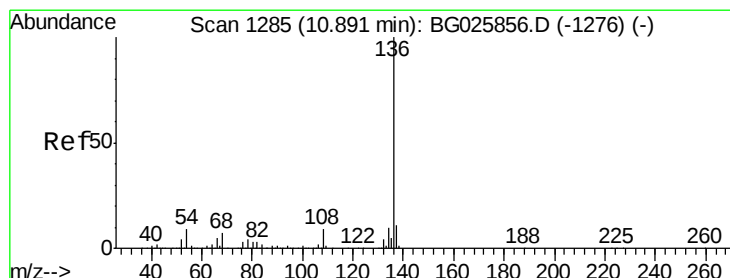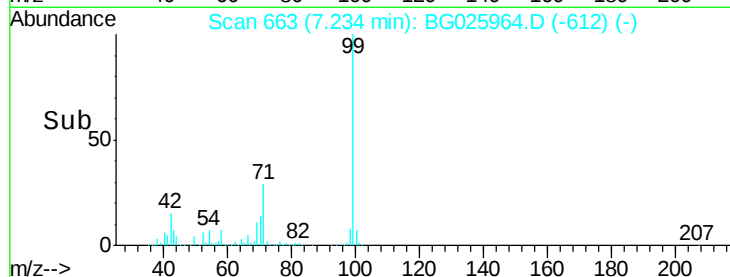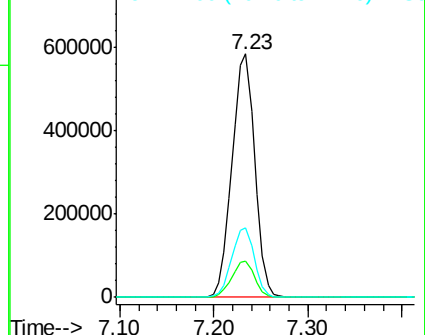

#21

Naphthalene-d8

Concen: 20.00 ng

RT: 10.88 min Scan# 1283

Delta R.T. -0.01 min

Lab File: BG025964.D

Acq: 27 Feb 2017 15:14

Tgt Ion: 136 Resp: 358381


Ion Ratio Lower Upper

136 100



137 11.6 8.9 13.3

54 9.2 9.3 13.9#

68 7.4 5.1 7.7

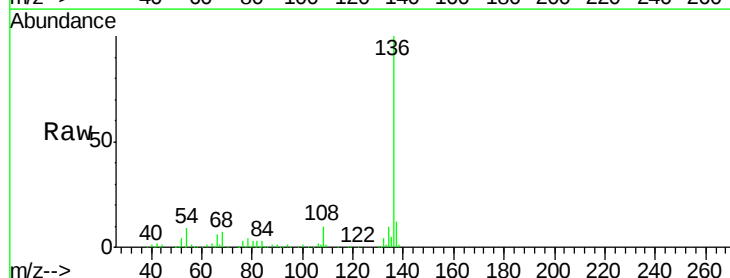

Abundance Ion 136.00 (135.70 to 136.70): BGC
Ion 137.00 (136.70 to 137.70): BGC
Ion 54.00 (53.70 to 54.70): BGC
Ion 68.00 (67.70 to 68.70): BGC



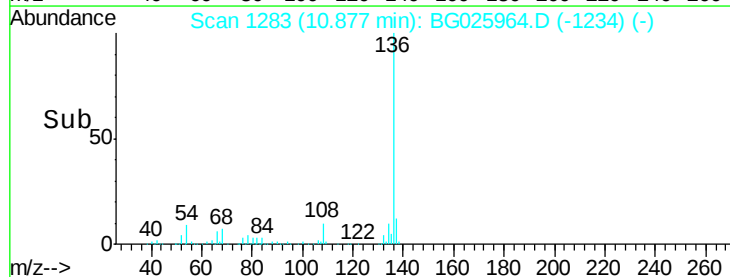
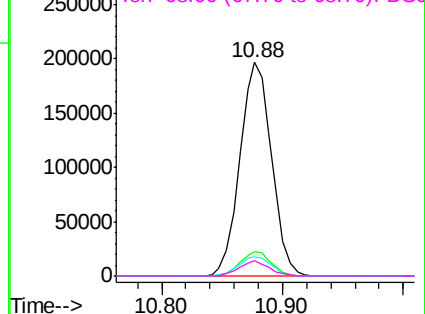




#23
 Nitrobenzene-d5
 Concen: 92.94 ng
 RT: 9.23 min Scan# 1003
 Delta R.T. -0.01 min
 Lab File: BG025964.D
 Acq: 27 Feb 2017 15:14




Instrument :
 BNA_G
 ClientSampleID :
 PB97193BL


Tot Ion: 82 Resp: 527770
 Ion Ratio Lower Upper
 82 100
 128 48.2 26.4 39.6#
 54 52.5 49.4 74.2

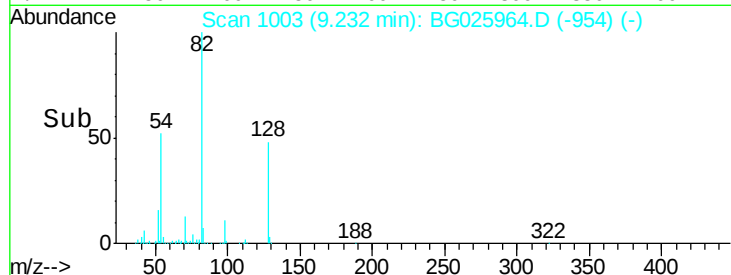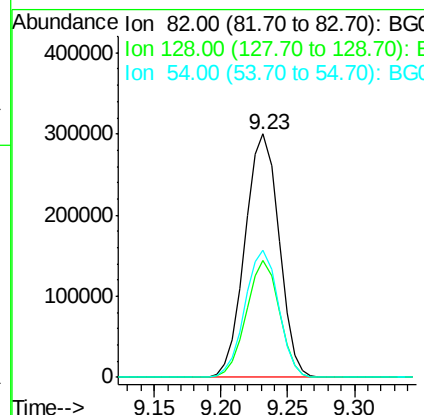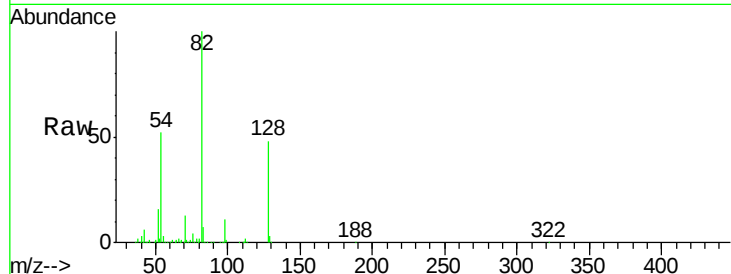

#38
 Acenaphthene-d10
 Concen: 20.00 ng
 RT: 14.68 min Scan# 1930
 Delta R.T. -0.01 min
 Lab File: BG025964.D
 Acq: 27 Feb 2017 15:14

Tgt Ion: 164 Resp: 241234
 Ion Ratio Lower Upper
 164 100
 162 102.2 85.1 127.7
 160 45.9 34.7 52.1

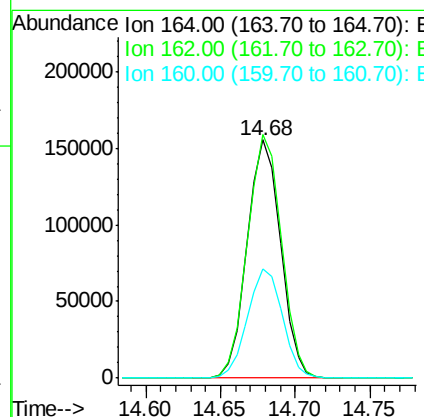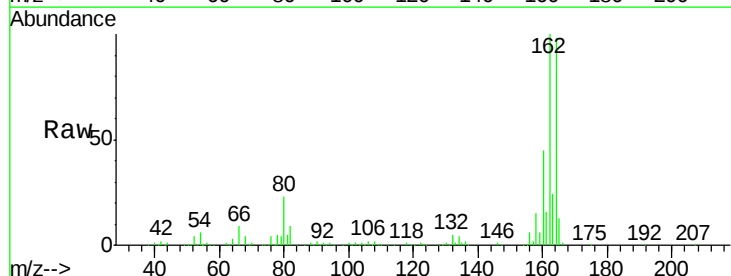







#41
2,4,6-Tribromophenol
Concen: 199.25 ng
RT: 16.16 min Scan# 2182
Delta R.T. -0.01 min
Lab File: BG025964.D
Acq: 27 Feb 2017 15:14

Instrument :
BNA_G
ClientSampleId :
PB97193BL

Tot Ion:330 Resp: 444068
Ion Ratio Lower Upper
330 100
332 96.6 77.3 115.9
141 39.4 32.1 48.1

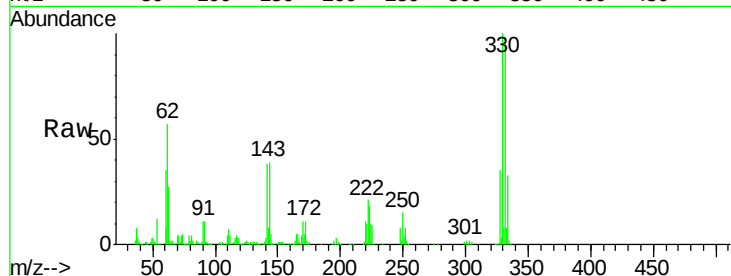


Abundance Ion 329.80 (329.50 to 330.50): E
Ion 331.80 (331.50 to 332.50): E
Ion 141.00 (140.70 to 141.70): E


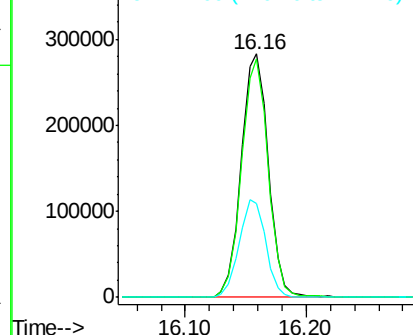



#44
2-Fluorobiphenyl
Concen: 101.41 ng
RT: 13.31 min Scan# 1697
Delta R.T. -0.01 min
Lab File: BG025964.D
Acq: 27 Feb 2017 15:14

Tgt Ion:172 Resp: 1400048
Ion Ratio Lower Upper
172 100
171 37.6 32.2 48.2
170 24.7 21.8 32.6



Abundance Ion 172.00 (171.70 to 172.70): E
Ion 171.00 (170.70 to 171.70): E
Ion 170.00 (169.70 to 170.70): E



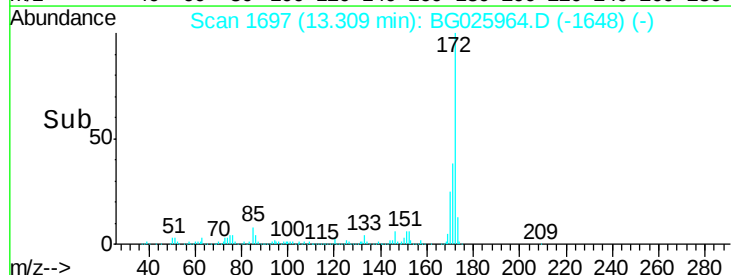
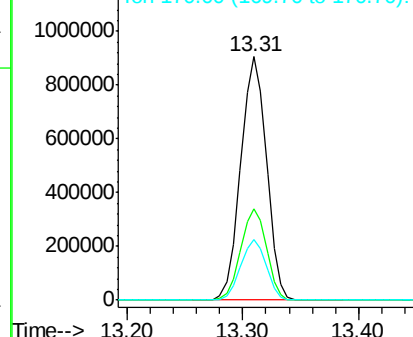


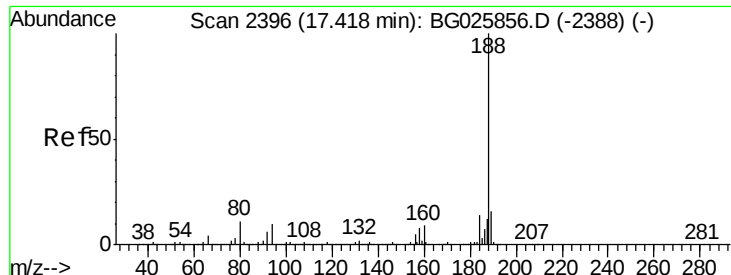

#63
Phenanthrene-d10
Concen: 20.00 ng
RT: 17.41 min Scan# 2395
Delta R.T. -0.01 min
Lab File: BG025964.D
Acq: 27 Feb 2017 15:14




Instrument :
BNA_G
ClientSampleId :
PB97193BL


Tot Ion:188 Resp: 698023
Ion Ratio Lower Upper
188 100
94 9.3 5.8 8.8#
80 10.4 7.5 11.3

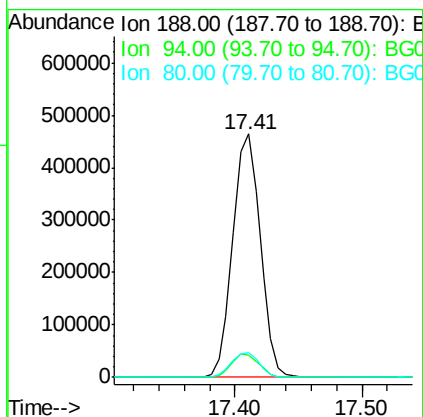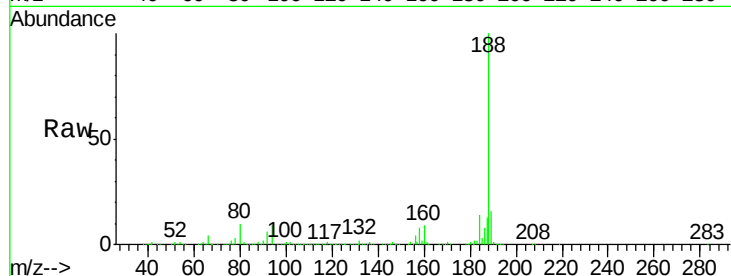

#75
Chrysene-d12
Concen: 20.00 ng
RT: 21.65 min Scan# 3117
Delta R.T. -0.03 min
Lab File: BG025964.D
Acq: 27 Feb 2017 15:14

Tgt Ion:240 Resp: 773600
Ion Ratio Lower Upper
240 100
120 12.6 5.7 8.5#
236 25.1 22.2 33.4

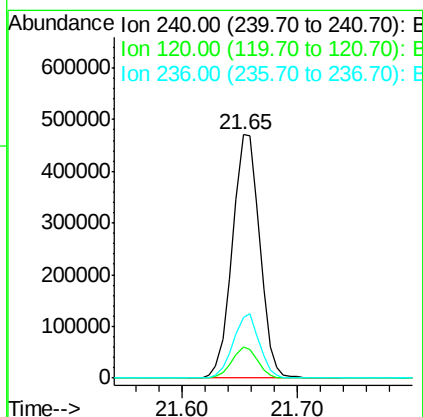



#78

Terphenyl-d14

Concen: 76.76 ng

RT: 20.01 min Scan# 2837

Delta R.T. -0.01 min

Lab File: BG025964.D

Acq: 27 Feb 2017 15:14

Instrument :

BNA_G

ClientSampleId :

PB97193BL


Tot Ion:244 Resp: 2441524

Ion Ratio Lower Upper

244 100

212 9.2 10.0 15.0#




122 14.0 8.6 12.8#



Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

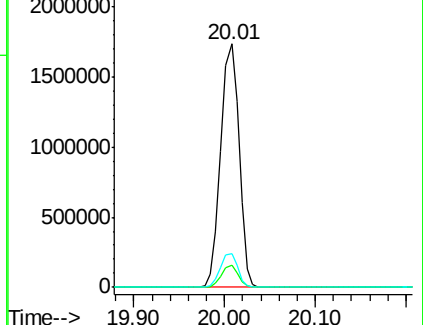

#86

Perylene-d12

Concen: 20.00 ng

RT: 24.85 min Scan# 3662

Delta R.T. -0.03 min

Lab File: BG025964.D

Acq: 27 Feb 2017 15:14


Tgt Ion:264 Resp: 749657

Ion Ratio Lower Upper

264 100

260 24.2 21.8 32.8

265 21.2 18.2 27.4



Abundance Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

