

Data Path : Z:\HPCHEM1\BNA G\DATA\BG022717\
 Data File : BG025984.D
 Acq On : 28 Feb 2017 4:23
 Operator : SJ/MA
 Sample : I1998-12
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 ROLL-OFF-1615-COMP

Quant Time: Feb 28 05:28:53 2017
 Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG021717.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Feb 17 15:48:21 2017
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.08	152	86946	20.00	ng	0.00
21) Naphthalene-d8	10.88	136	406966	20.00	ng	-0.01
38) Acenaphthene-d10	14.68	164	280126	20.00	ng	-0.01
63) Phenanthrene-d10	17.41	188	802259	20.00	ng	0.00
75) Chrysene-d12	21.65	240	832079	20.00	ng	-0.03
86) Perylene-d12	24.85	264	804624	20.00	ng	-0.04
System Monitoring Compounds						
5) 2-Fluorophenol	5.65	112	761484	152.48	ng	0.00
7) Phenol-d6	7.23	99	1016854	137.60	ng	0.00
23) Nitrobenzene-d5	9.23	82	601668	93.30	ng	-0.01
41) 2,4,6-Tribromophenol	16.16	330	544512	210.39	ng	0.00
44) 2-Fluorobiphenyl	13.31	172	1661966	103.67	ng	-0.01
78) Terphenyl-d14	20.01	244	2702969	79.01	ng	-0.01


Target Compounds Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA G\DATA\BG022717\
Data File : BG025984.D
Acq On : 28 Feb 2017 4:23
Operator : SJ/MA
Sample : I1998-12
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
ROLL-OFF-1615-COMP

Quant Time: Feb 28 05:28:53 2017
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG021717.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Feb 17 15:48:21 2017
Response via : Initial Calibration

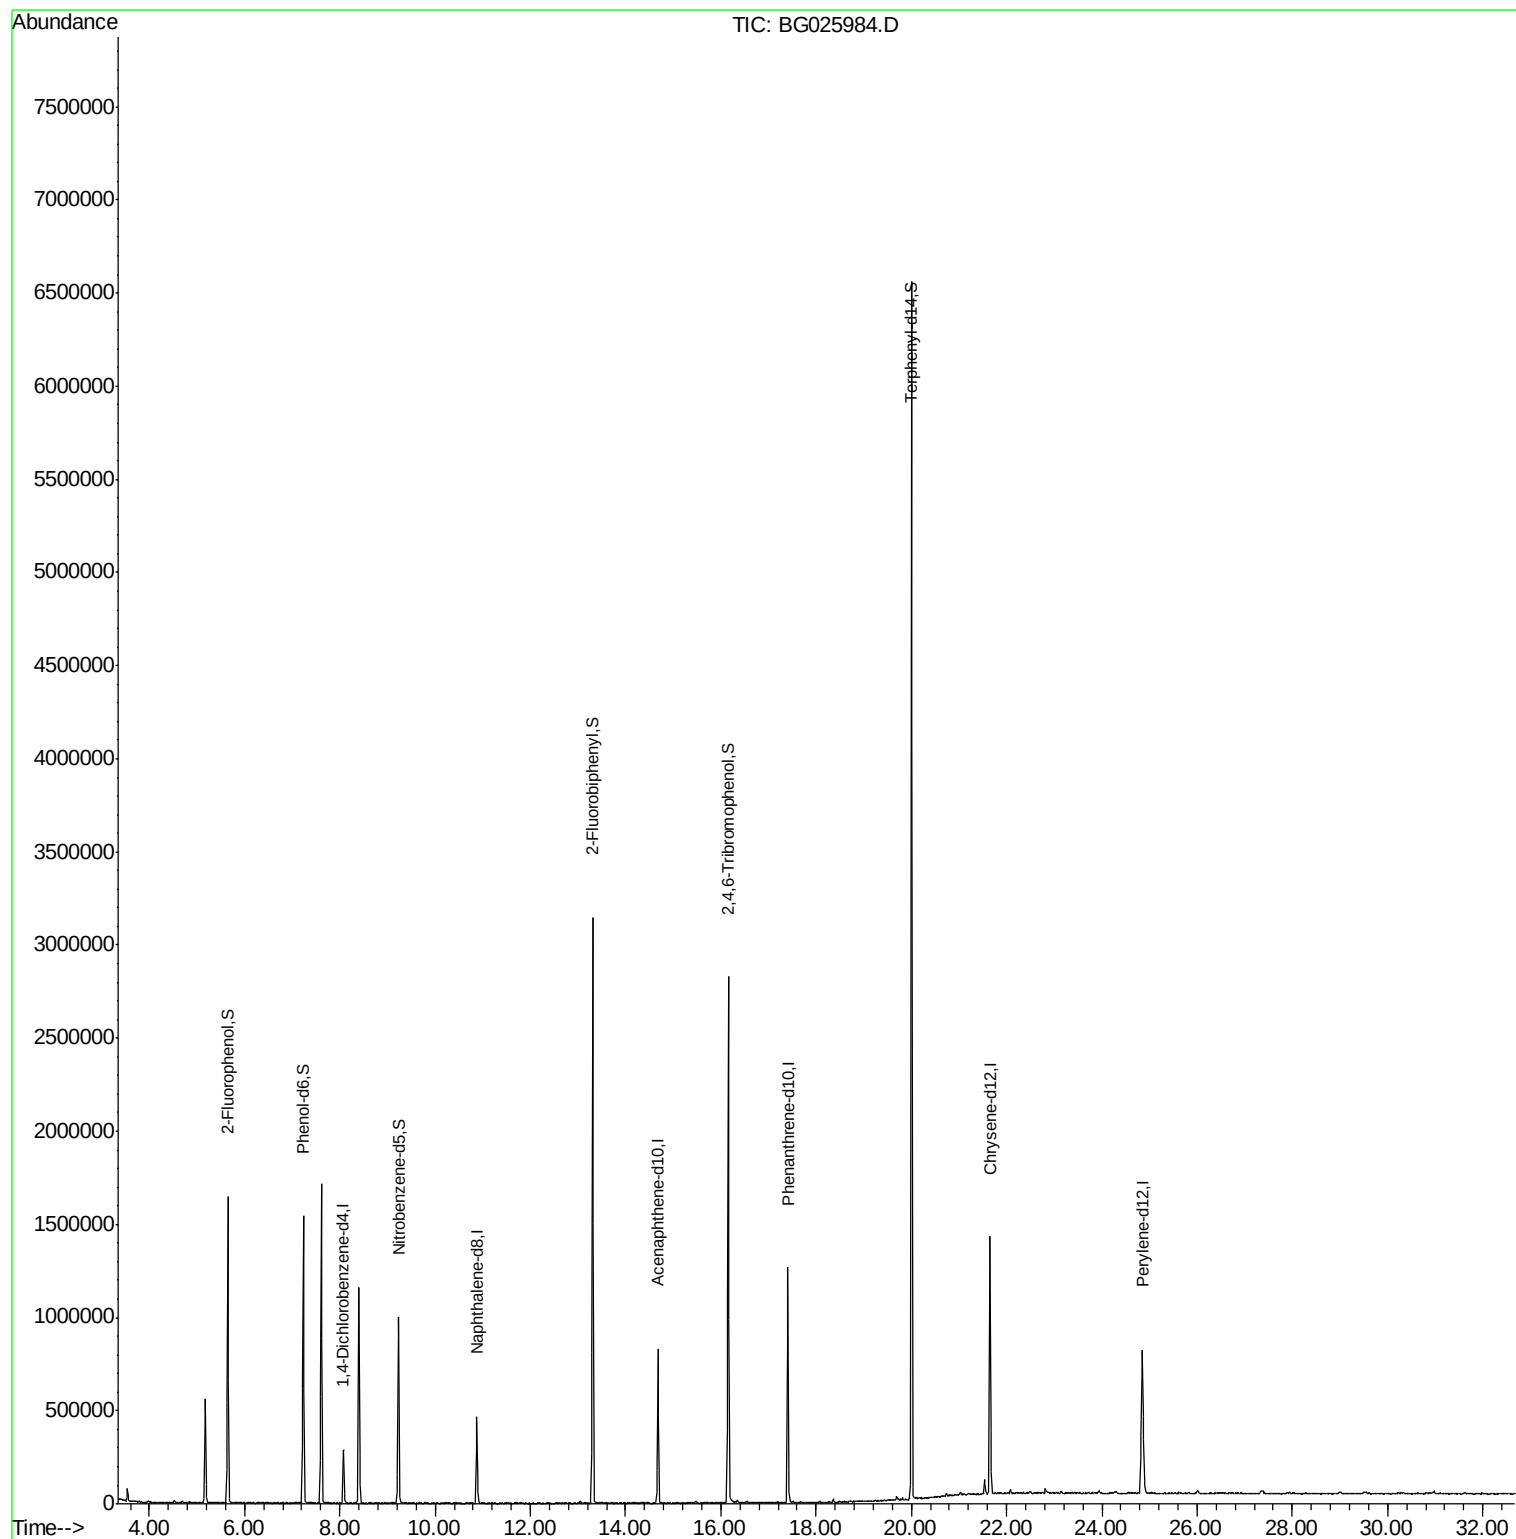



#1

1,4-Dichlorobenzene-d4

Concen: 20.00 ng

RT: 8.08 min Scan# 807

Delta R.T. -0.01 min

Lab File: BG025984.D

Acq: 28 Feb 2017 4:23

Instrument :

BNA_G

ClientSampleId :

ROLL-OFF-1615-COMP


Tot Ion:152 Resp: 86946

Ion Ratio Lower Upper

152 100

150 148.2 114.0 171.0




115 55.3 48.1 72.1

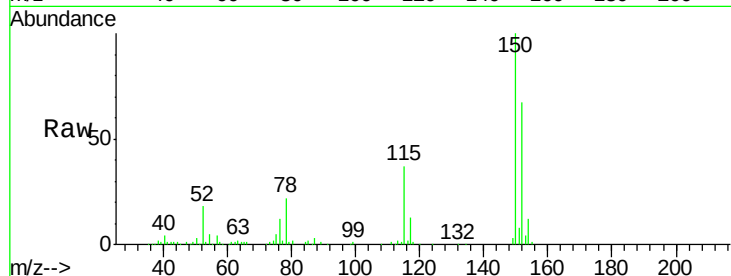

Abundance Ion 152.00 (151.70 to 152.70): E

Ion 150.00 (149.70 to 150.70): E

Ion 115.00 (114.70 to 115.70): E

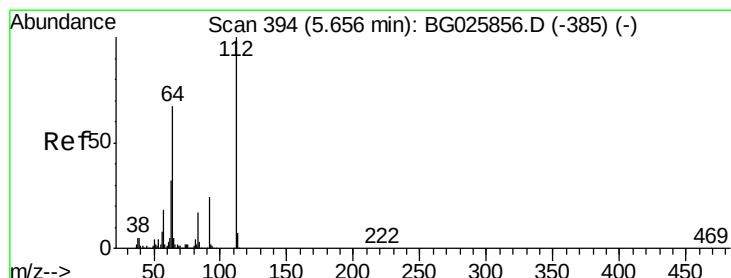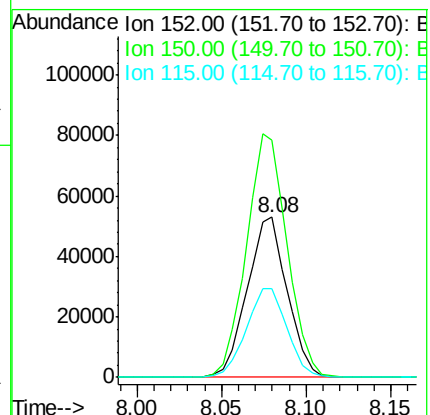

#5

2-Fluorophenol

Concen: 152.48 ng

RT: 5.65 min Scan# 393

Delta R.T. -0.01 min

Lab File: BG025984.D

Acq: 28 Feb 2017 4:23


Tgt Ion:112 Resp: 761484

Ion Ratio Lower Upper

112 100

64 63.4 61.8 92.6



63 31.4 37.2 55.8#

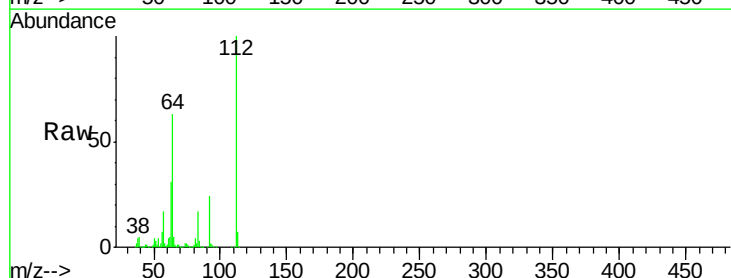


Abundance Ion 112.00 (111.70 to 112.70): E

Ion 64.00 (63.70 to 64.70): BGC

Ion 63.00 (62.70 to 63.70): BGC

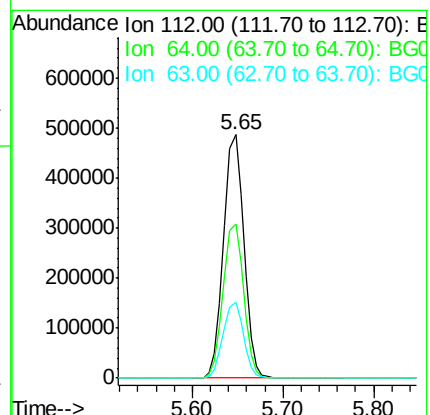

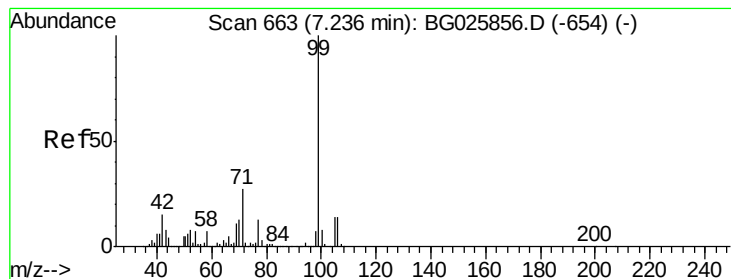

#7

Phenol-d6

Concen: 137.60 ng

RT: 7.23 min Scan# 663

Delta R.T. -0.00 min

Lab File: BG025984.D

Acq: 28 Feb 2017 4:23

Instrument :

BNA_G

ClientSampleId :

ROLL-OFF-1615-COMP


Tot Ion: 99 Resp: 1016854

Ion Ratio Lower Upper




99 100

42 13.5 20.5 30.7#

71 27.6 37.6 56.4#

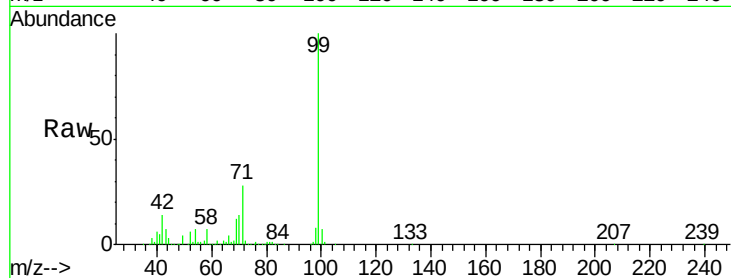

Abundance Ion 99.00 (98.70 to 99.70): BGC
Ion 42.00 (41.70 to 42.70): BGC
Ion 71.00 (70.70 to 71.70): BGC

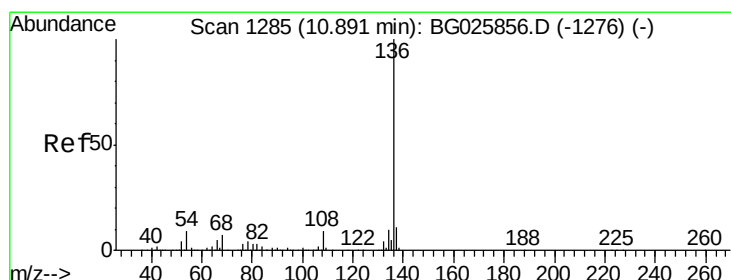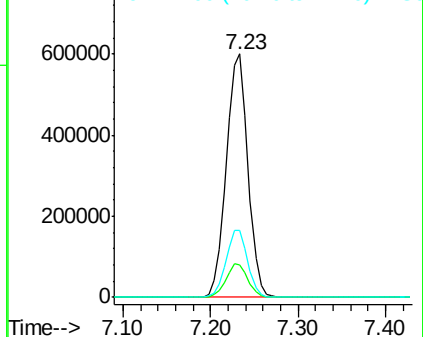

#21

Naphthalene-d8

Concen: 20.00 ng

RT: 10.88 min Scan# 1283

Delta R.T. -0.01 min

Lab File: BG025984.D

Acq: 28 Feb 2017 4:23

Tgt Ion: 136 Resp: 406966


Ion Ratio Lower Upper

136 100



137 11.0 8.9 13.3


54 8.3 9.3 13.9#

68 6.4 5.1 7.7

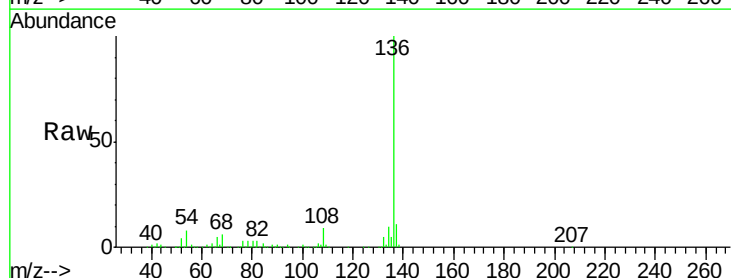

Abundance Ion 136.00 (135.70 to 136.70): BGC
Ion 137.00 (136.70 to 137.70): BGC
Ion 54.00 (53.70 to 54.70): BGC
Ion 68.00 (67.70 to 68.70): BGC




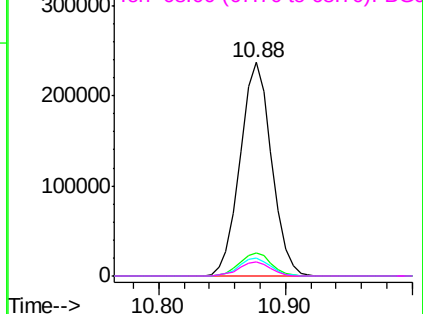




#23
 Nitrobenzene-d5
 Concen: 93.30 ng
 RT: 9.23 min Scan# 1003
 Delta R.T. -0.01 min
 Lab File: BG025984.D
 Acq: 28 Feb 2017 4:23




Instrument :
 BNA_G
 ClientSampleId :
 ROLL-OFF-1615-COMP


Tot Ion	82	Resp	601668
Ion	Ratio	Lower	Upper
82	100		
128	48.8	26.4	39.6#
54	50.5	49.4	74.2

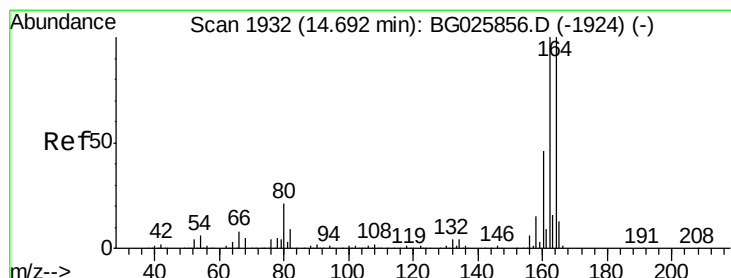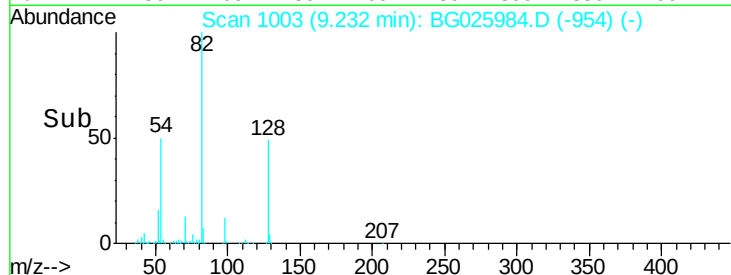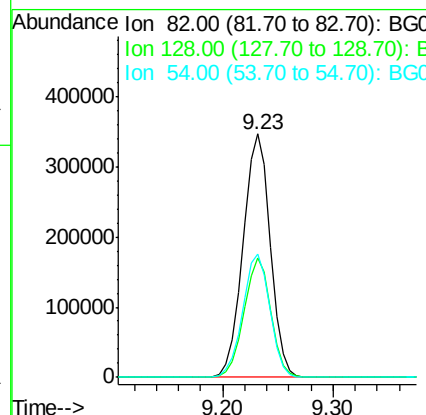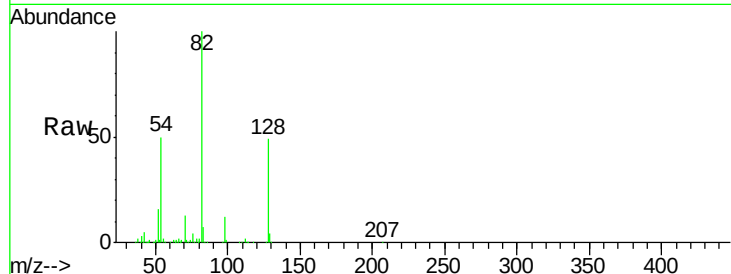

#38
 Acenaphthene-d10
 Concen: 20.00 ng
 RT: 14.68 min Scan# 1930
 Delta R.T. -0.01 min
 Lab File: BG025984.D
 Acq: 28 Feb 2017 4:23

Tgt Ion	164	Resp	280126
Ion	Ratio	Lower	Upper
164	100		
162	101.3	85.1	127.7
160	46.8	34.7	52.1



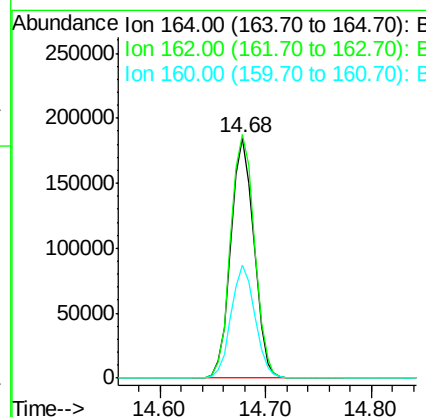
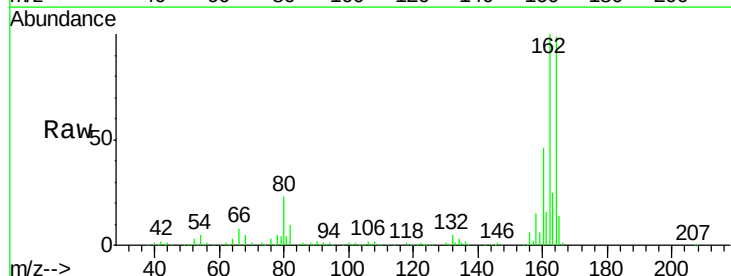




#41
2,4,6-Tribromophenol
Concen: 210.39 ng
RT: 16.16 min Scan# 2182
Delta R.T. -0.01 min
Lab File: BG025984.D
Acq: 28 Feb 2017 4:23




Instrument :
BNA_G
ClientSampleId :
ROLL-OFF-1615-COMP


Tot Ion:330 Resp: 544512
Ion Ratio Lower Upper
330 100
332 97.1 77.3 115.9
141 36.9 32.1 48.1

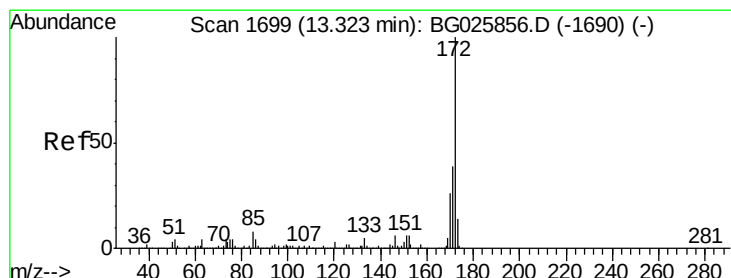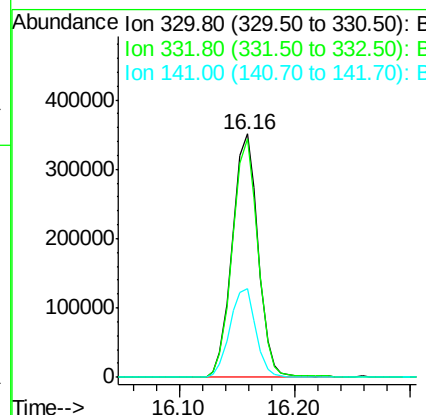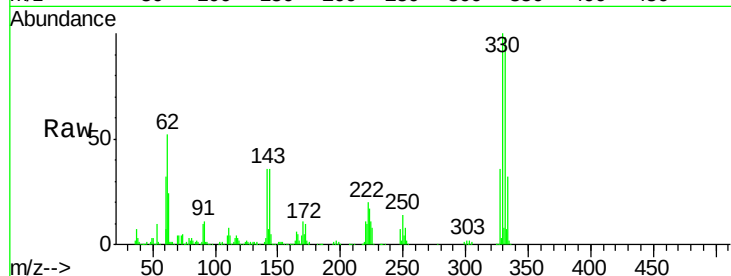

#44
2-Fluorobiphenyl
Concen: 103.67 ng
RT: 13.31 min Scan# 1697
Delta R.T. -0.01 min
Lab File: BG025984.D
Acq: 28 Feb 2017 4:23

Tgt Ion:172 Resp: 1661966
Ion Ratio Lower Upper
172 100
171 38.8 32.2 48.2
170 26.4 21.8 32.6

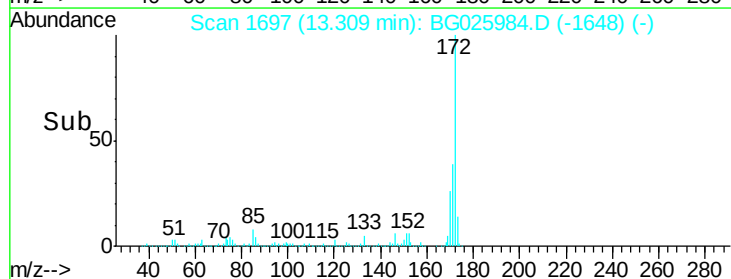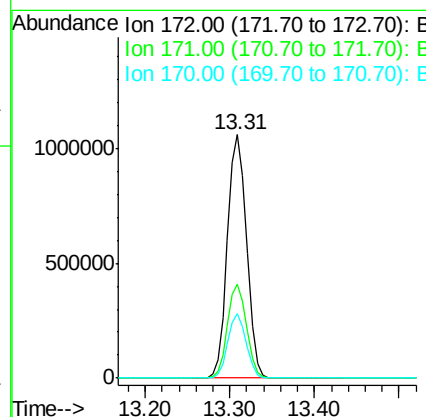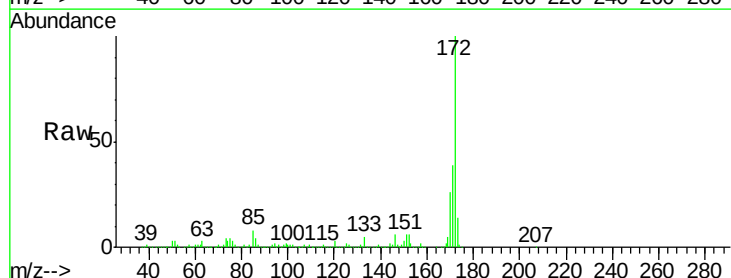

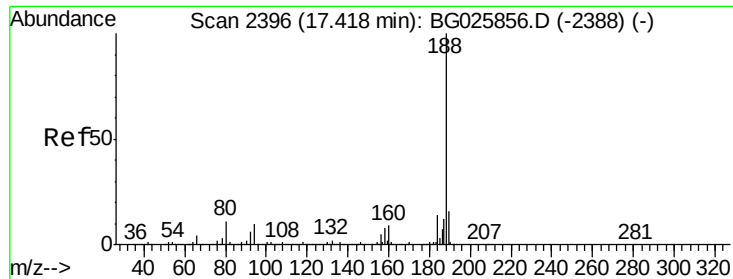

#63

Phenanthrene-d10

Concen: 20.00 ng

RT: 17.41 min Scan# 2395

Delta R.T. -0.01 min

Lab File: BG025984.D

Acq: 28 Feb 2017 4:23

Instrument :

BNA_G

ClientSampleId :

ROLL-OFF-1615-COMP


Tot Ion:188 Resp: 802259

Ion Ratio Lower Upper

188 100

94 9.3 5.8 8.8#




80 9.8 7.5 11.3

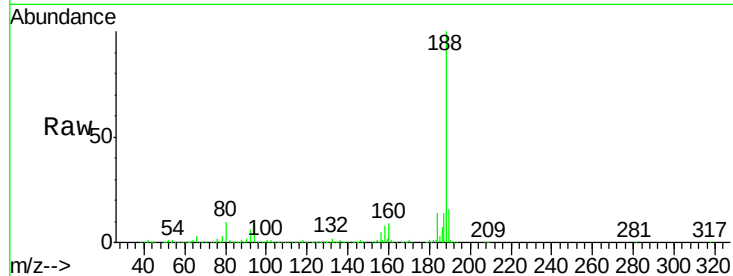

Abundance Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BGC

Ion 80.00 (79.70 to 80.70): BGC

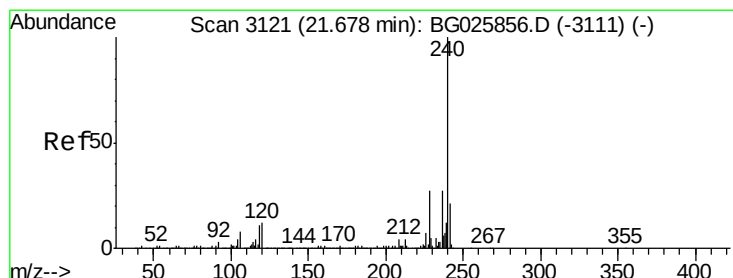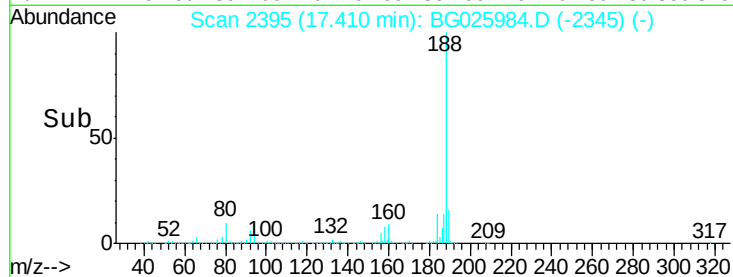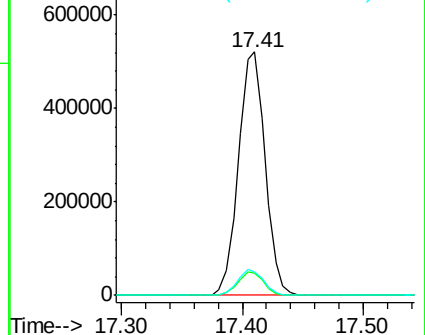

#75

Chrysene-d12

Concen: 20.00 ng

RT: 21.65 min Scan# 3117

Delta R.T. -0.03 min

Lab File: BG025984.D

Acq: 28 Feb 2017 4:23


Tgt Ion:240 Resp: 832079

Ion Ratio Lower Upper

240 100

120 12.1 5.7 8.5#



236 25.9 22.2 33.4

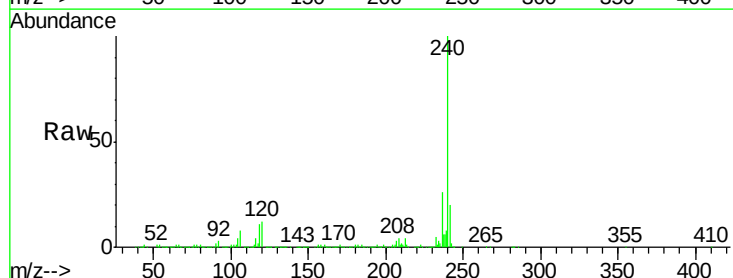


Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

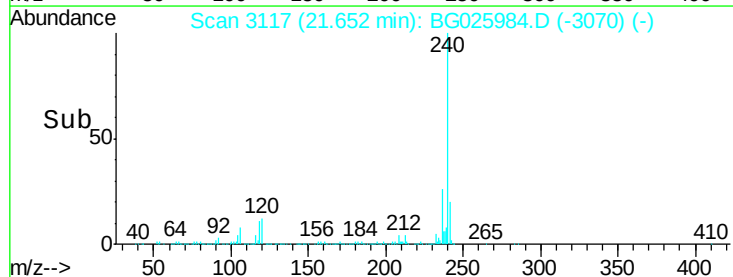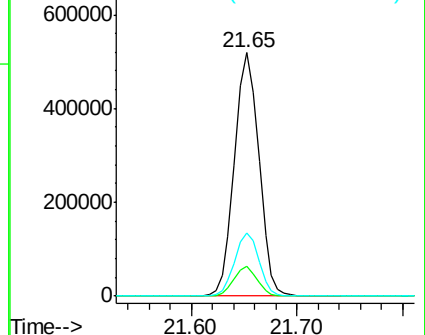

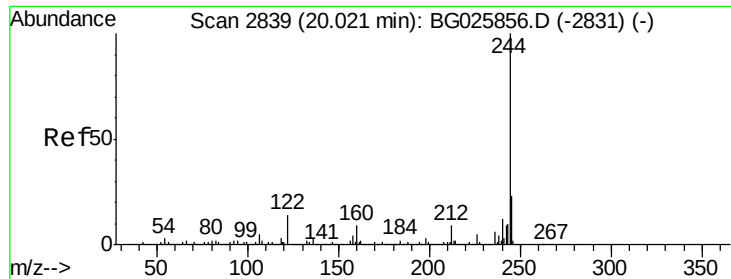

#78

Terphenyl-d14

Concen: 79.01 ng

RT: 20.01 min Scan# 2837

Delta R.T. -0.01 min

Lab File: BG025984.D

Acq: 28 Feb 2017 4:23

Instrument :

BNA_G

ClientSampleId :

ROLL-OFF-1615-COMP


Tot Ion:244 Resp: 2702969

Ion Ratio Lower Upper

244 100

212 9.3 10.0 15.0#




122 13.8 8.6 12.8#

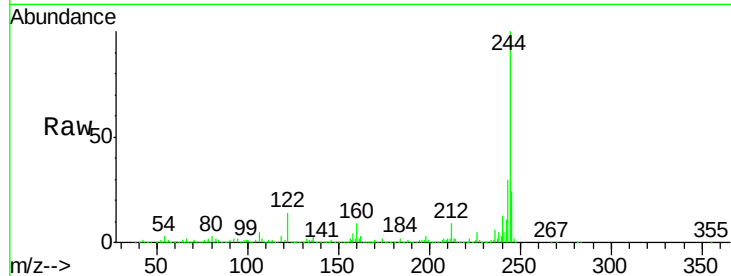

Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

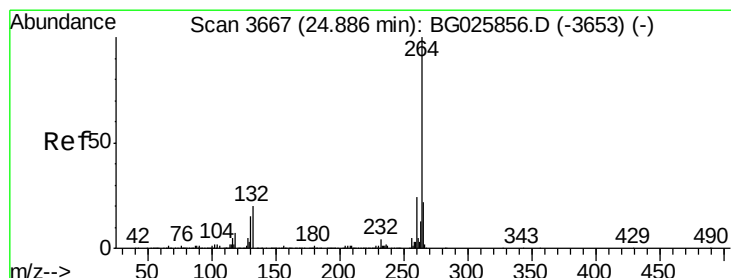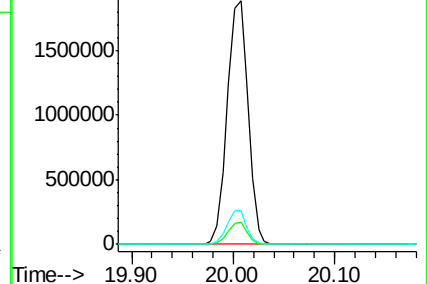

#86

Perylene-d12

Concen: 20.00 ng

RT: 24.85 min Scan# 3661

Delta R.T. -0.04 min

Lab File: BG025984.D

Acq: 28 Feb 2017 4:23


Tgt Ion:264 Resp: 804624

Ion Ratio Lower Upper

264 100

260 24.1 21.8 32.8

265 22.0 18.2 27.4

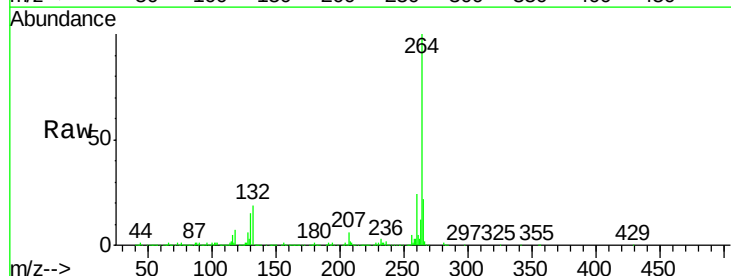

Abundance Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

