


Data Path : Z:\HPCHEM1\BNA G\DATA\BG022717\
 Data File : BG025962.D
 Acq On : 27 Feb 2017 13:55
 Operator : SJ/MA
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG021717.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Feb 17 15:48:21 2017

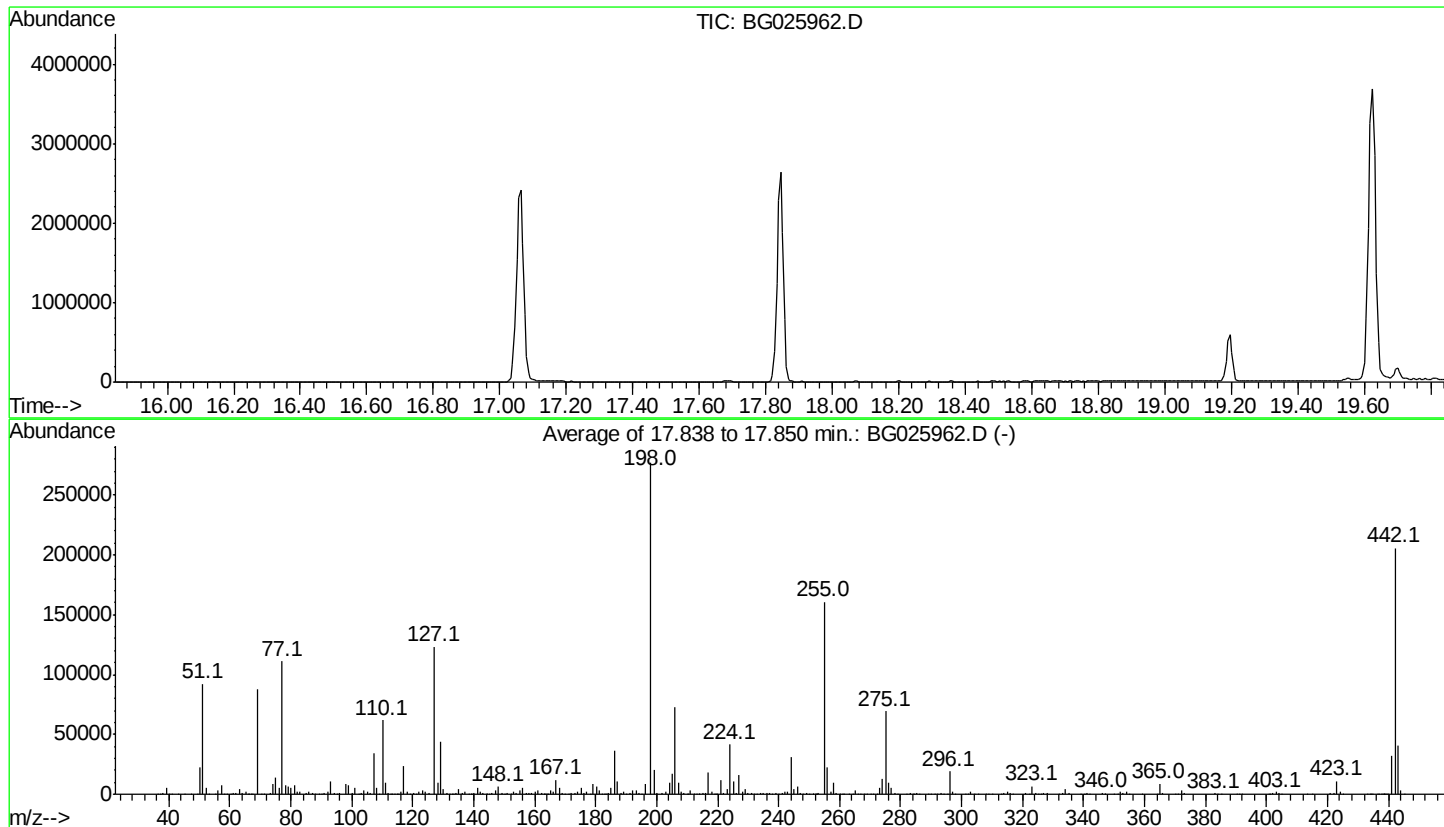

AutoFind: Scans 2468, 2469, 2470; Background Corrected with Scan 2461

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	33.4	92530	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	31.6	87645	PASS
70	69	0.00	2	0.5	458	PASS
127	198	10	80	44.5	123213	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	277034	PASS
199	198	5	9	7.2	19854	PASS
275	198	10	60	25.0	69381	PASS
365	198	1	100	3.2	8996	PASS
441	442	0.01	24	15.8	32541	PASS
442	198	50	100	74.3	205738	PASS
443	442	15	24	19.8	40701	PASS