


Data Path : Z:\HPCHEM1\BNA G\DATA\BG022718\
 Data File : BG032850.D
 Acq On : 27 Feb 2018 12:00
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG022118.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Feb 26 17:50:45 2018

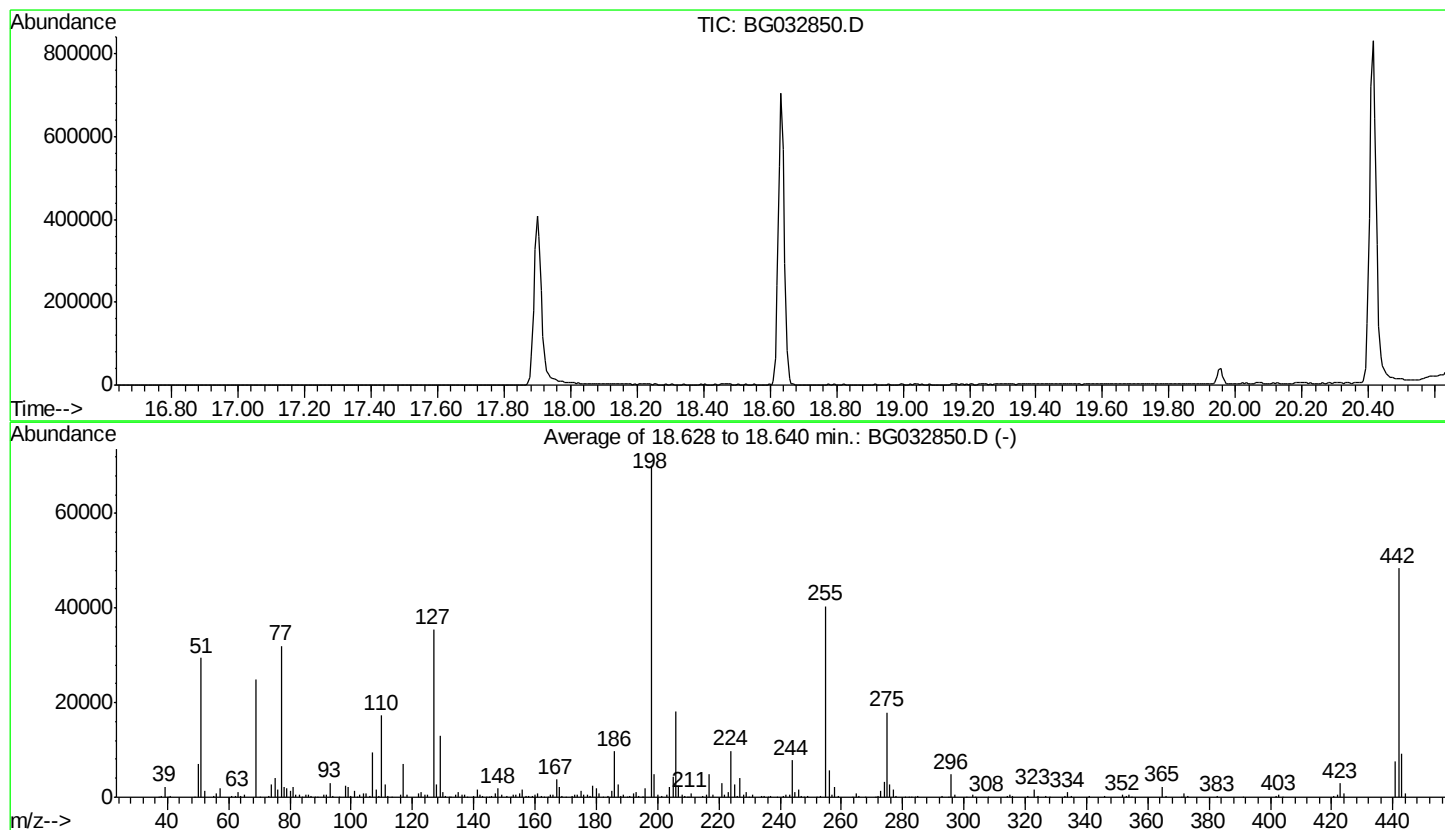

AutoFind: Scans 2611, 2612, 2613; Background Corrected with Scan 2605

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	42.0	29472	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	35.7	25005	PASS
70	69	0.00	2	0.4	108	PASS
127	198	10	80	50.5	35386	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	70101	PASS
199	198	5	9	7.0	4903	PASS
275	198	10	60	25.6	17970	PASS
365	198	1	100	3.2	2245	PASS
441	442	0.01	24	15.5	7520	PASS
442	198	50	100	69.0	48386	PASS
443	442	15	24	19.3	9321	PASS