

Data File : BG026013.D  
Acq On : 1 Mar 2017 1:43  
Operator : SJ/MA  
Sample : PB97225BL  
Misc :  
ALS Vial : 16 Sample Multiplier: 1

Instrument :  
BNA\_G  
ClientSampleId :  
PB97225BL

Quant Time: Mar 01 03:24:11 2017  
Quant Method : Z:\HPCHEM1\BNA\_G\METHODS\8270-BG021717.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Tue Feb 28 15:36:56 2017  
Response via : Initial Calibration

| Internal Standards          | R.T.  | QIon | Response | Conc   | Units | Dev(Min) |
|-----------------------------|-------|------|----------|--------|-------|----------|
| 1) 1,4-Dichlorobenzene-d4   | 8.08  | 152  | 109760   | 20.00  | ng    | 0.00     |
| 21) Naphthalene-d8          | 10.88 | 136  | 501889   | 20.00  | ng    | -0.01    |
| 38) Acenaphthene-d10        | 14.68 | 164  | 329755   | 20.00  | ng    | -0.01    |
| 63) Phenanthrene-d10        | 17.41 | 188  | 898058   | 20.00  | ng    | 0.00     |
| 75) Chrysene-d12            | 21.65 | 240  | 919142   | 20.00  | ng    | -0.03    |
| 86) Perylene-d12            | 24.85 | 264  | 892485   | 20.00  | ng    | -0.03    |
| System Monitoring Compounds |       |      |          |        |       |          |
| 5) 2-Fluorophenol           | 5.65  | 112  | 795534   | 126.19 | ng    | 0.00     |
| 7) Phenol-d6                | 7.23  | 99   | 1105773  | 118.53 | ng    | 0.00     |
| 23) Nitrobenzene-d5         | 9.23  | 82   | 591720   | 74.40  | ng    | -0.01    |
| 41) 2,4,6-Tribromophenol    | 16.16 | 330  | 467737   | 153.53 | ng    | 0.00     |
| 44) 2-Fluorobiphenyl        | 13.31 | 172  | 1527897  | 80.96  | ng    | -0.01    |
| 78) Terphenyl-d14           | 20.00 | 244  | 2316727  | 61.30  | ng    | -0.02    |

| Target Compounds | Qvalue |
|------------------|--------|
|------------------|--------|

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data File : BG026013.D

Acq On : 1 Mar 2017 1:43

Operator : SJ/MA

Sample : PB97225BL

Misc :

ALS Vial : 16 Sample Multiplier: 1

Instrument :

BNA\_G

ClientSampleId :

PB97225BL


Quant Time: Mar 01 03:24:11 2017


Quant Method : Z:\HPCHEM1\BNA\_G\METHODS\8270-BG021717.M

Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

QLast Update : Tue Feb 28 15:36:56 2017

Response via : Initial Calibration

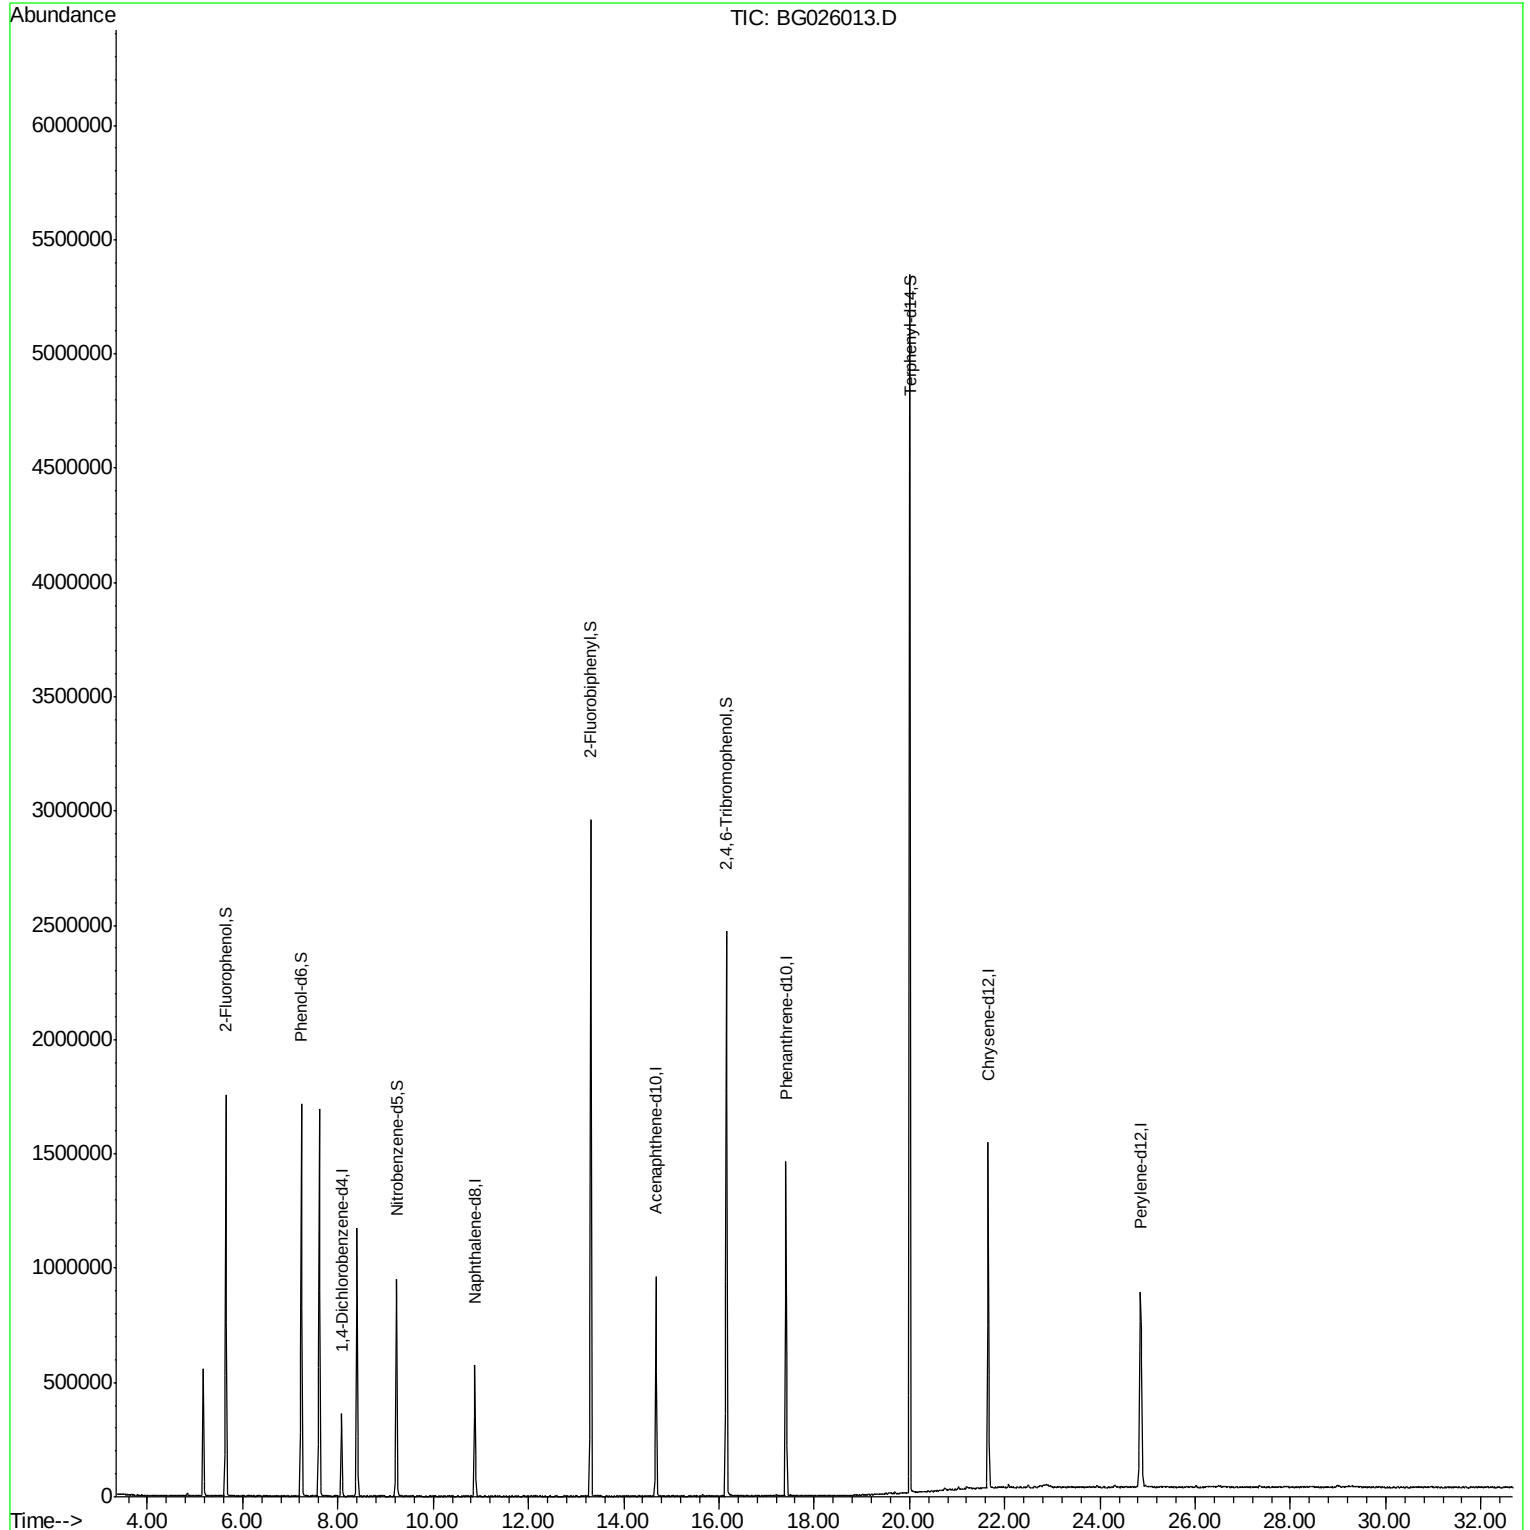

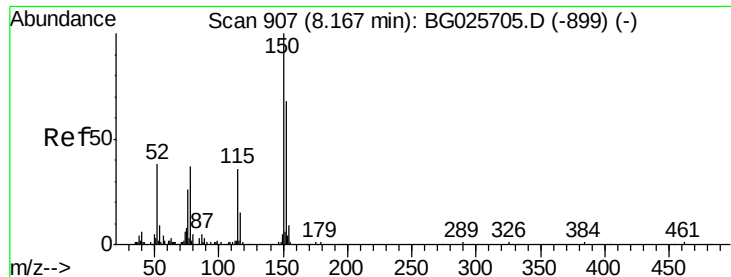

#1

1,4-Dichlorobenzene-d4

Concen: 20.00 ng

RT: 8.08 min Scan# 807

Delta R.T. -0.01 min

Lab File: BG026013.D

Acq: 1 Mar 2017 1:43

Instrument :

BNA\_G

ClientSampleId :

PB97225BL


Tgt Ion:152 Resp: 109760

Ion Ratio Lower Upper

152 100

150 156.4 114.0 171.0




115 55.9 48.1 72.1

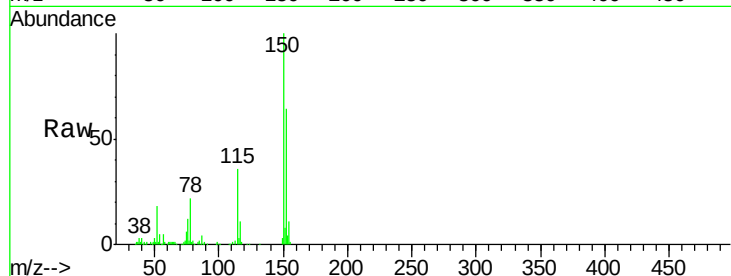

Abundance Ion 152.00 (151.70 to 152.70): E

Ion 150.00 (149.70 to 150.70): E

Ion 115.00 (114.70 to 115.70): E

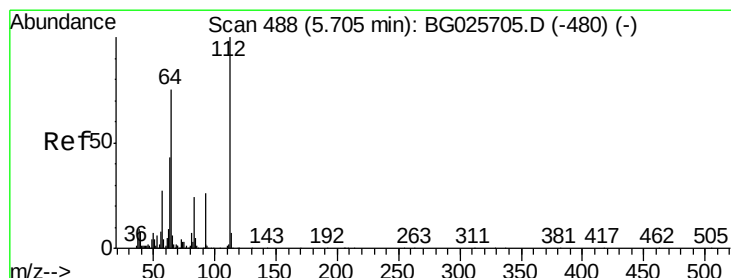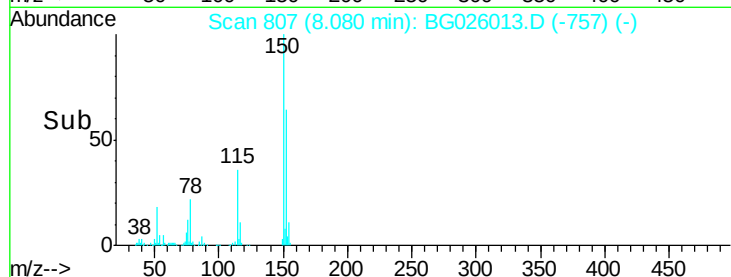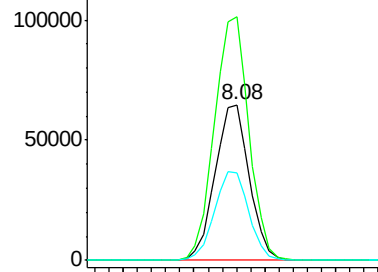

#5

2-Fluorophenol

Concen: 126.19 ng

RT: 5.65 min Scan# 393

Delta R.T. -0.01 min

Lab File: BG026013.D

Acq: 1 Mar 2017 1:43


Tgt Ion:112 Resp: 795534

Ion Ratio Lower Upper

112 100

64 66.2 61.8 92.6



63 32.6 37.2 55.8#

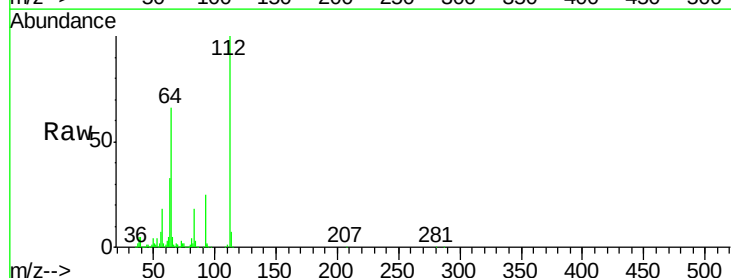


Abundance Ion 112.00 (111.70 to 112.70): E

Ion 64.00 (63.70 to 64.70): BGC

Ion 63.00 (62.70 to 63.70): BGC

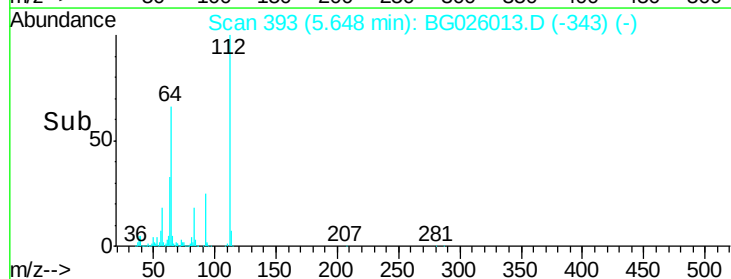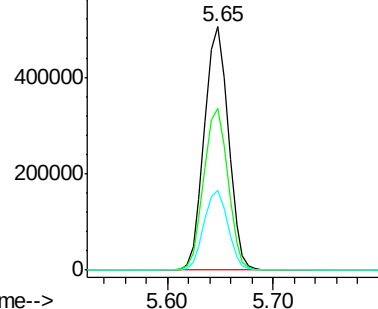

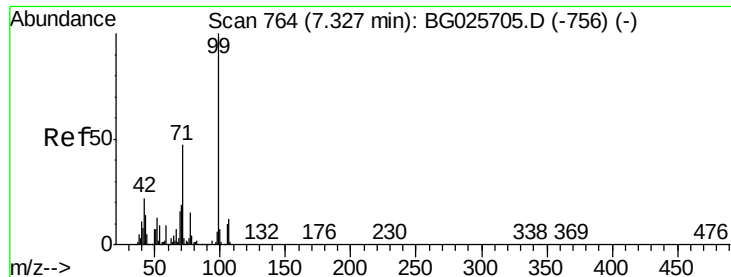

#7

Phenol-d6

Concen: 118.53 ng

RT: 7.23 min Scan# 663

Delta R.T. -0.00 min

Lab File: BG026013.D

Acq: 1 Mar 2017 1:43

Instrument :

BNA\_G

ClientSampleId :

PB97225BL


Tgt Ion: 99 Resp: 1105773

Ion Ratio Lower Upper




99 100

42 14.0 20.5 30.7#

71 29.7 37.6 56.4#

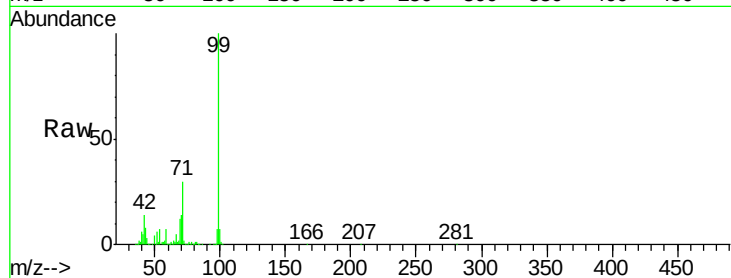

Abundance Ion 99.00 (98.70 to 99.70): BGC  
Ion 42.00 (41.70 to 42.70): BGC  
Ion 71.00 (70.70 to 71.70): BGC

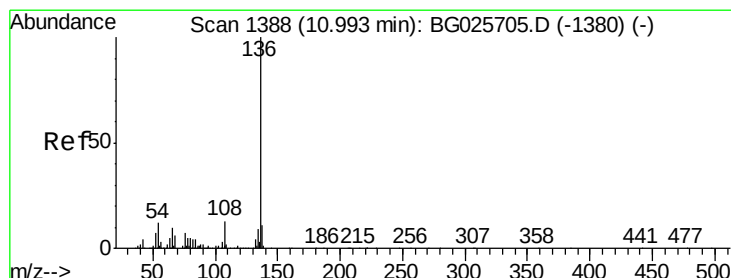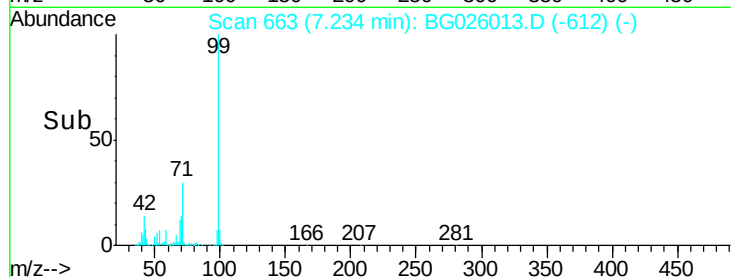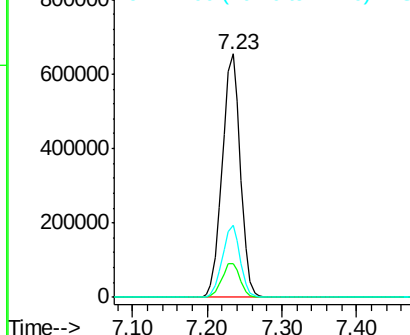

#21

Naphthalene-d8

Concen: 20.00 ng

RT: 10.88 min Scan# 1283

Delta R.T. -0.01 min

Lab File: BG026013.D

Acq: 1 Mar 2017 1:43

Tgt Ion: 136 Resp: 501889


Ion Ratio Lower Upper

136 100



137 11.3 8.9 13.3


54 7.8 9.3 13.9#

68 6.8 5.1 7.7

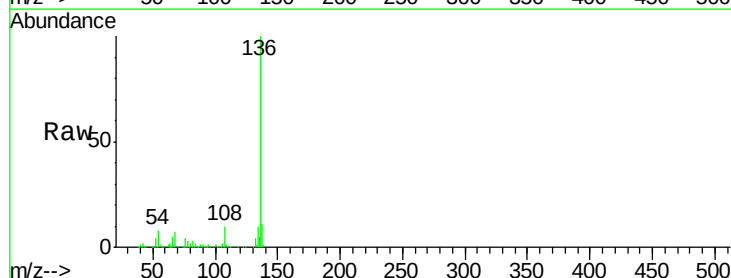

Abundance Ion 136.00 (135.70 to 136.70): BGC  
Ion 137.00 (136.70 to 137.70): BGC  
Ion 54.00 (53.70 to 54.70): BGC  
Ion 68.00 (67.70 to 68.70): BGC



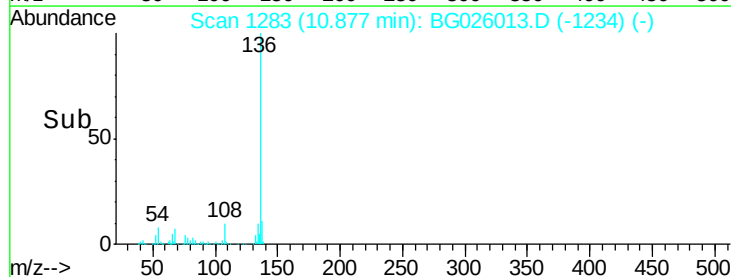
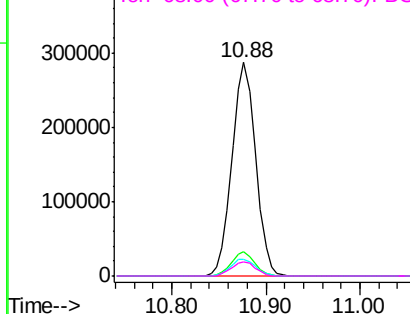


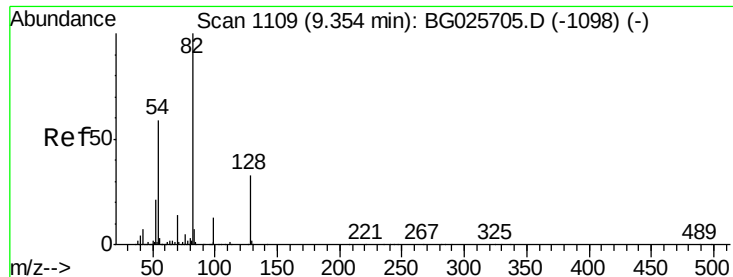

#23  
 Nitrobenzene-d5  
 Concen: 74.40 ng  
 RT: 9.23 min Scan# 1003  
 Delta R.T. -0.01 min  
 Lab File: BG026013.D  
 Acq: 1 Mar 2017 1:43




Instrument :  
 BNA\_G  
 ClientSampleId :  
 PB97225BL


Tgt Ion: 82 Resp: 591720  
 Ion Ratio Lower Upper  
 82 100  
 128 48.7 26.4 39.6#  
 54 49.3 49.4 74.2#

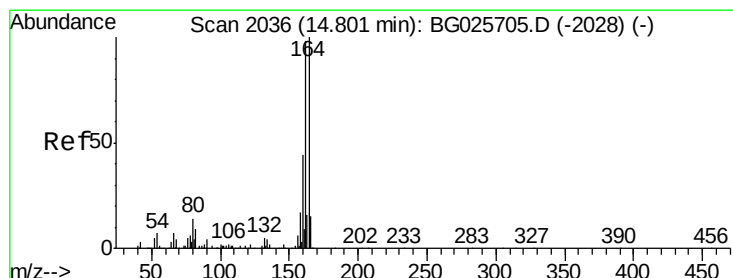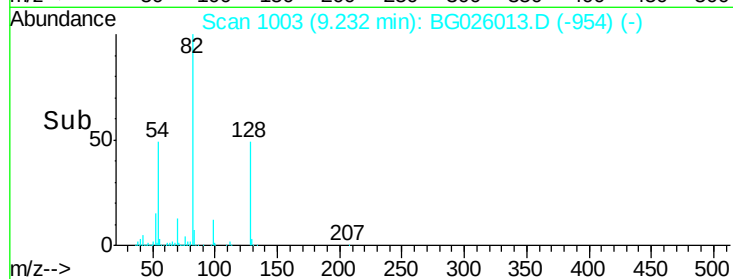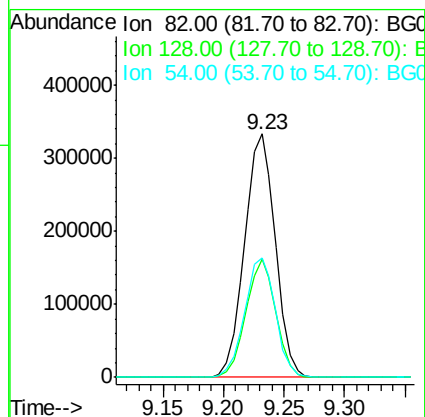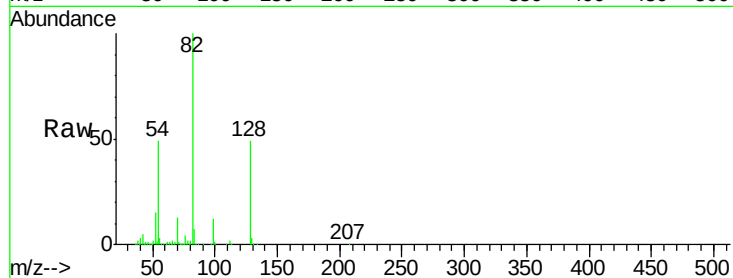

#38  
 Acenaphthene-d10  
 Concen: 20.00 ng  
 RT: 14.68 min Scan# 1930  
 Delta R.T. -0.01 min  
 Lab File: BG026013.D  
 Acq: 1 Mar 2017 1:43

Tgt Ion: 164 Resp: 329755  
 Ion Ratio Lower Upper  
 164 100  
 162 100.9 85.1 127.7  
 160 46.2 34.7 52.1


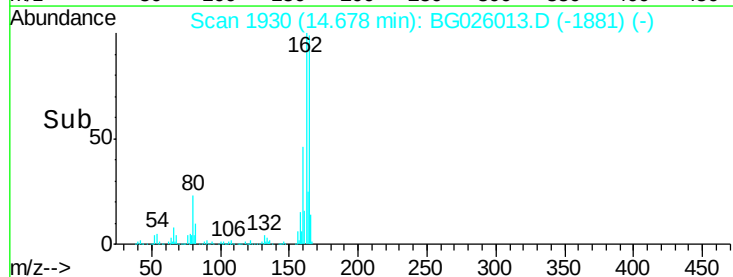
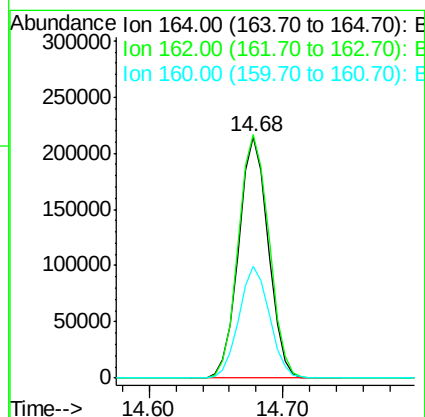
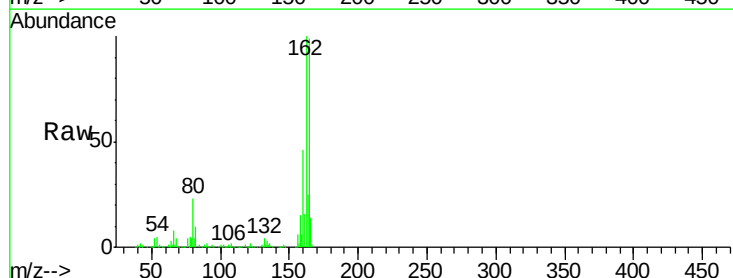


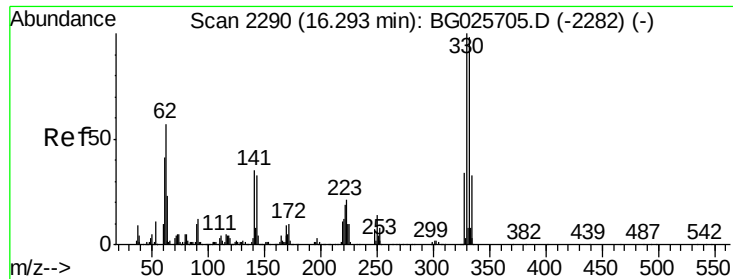

#41  
 2,4,6-Tribromophenol  
 Concen: 153.53 ng  
 RT: 16.16 min Scan# 2182  
 Delta R.T. -0.01 min  
 Lab File: BG026013.D  
 Acq: 1 Mar 2017 1:43




Instrument :  
 BNA\_G  
 ClientSampleId :  
 PB97225BL


Tgt Ion:330 Resp: 467737  
 Ion Ratio Lower Upper  
 330 100  
 332 95.9 77.3 115.9  
 141 39.1 32.1 48.1

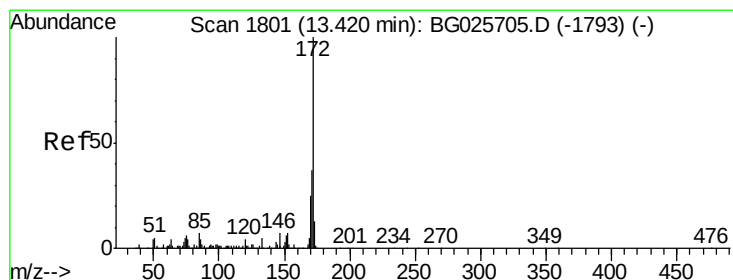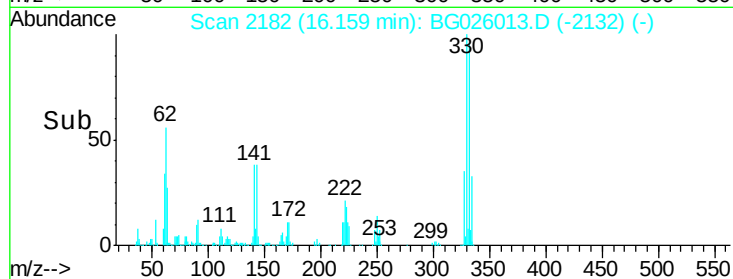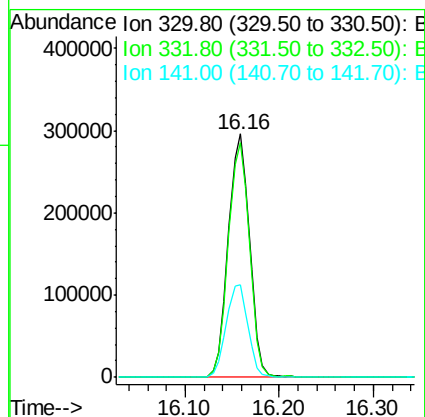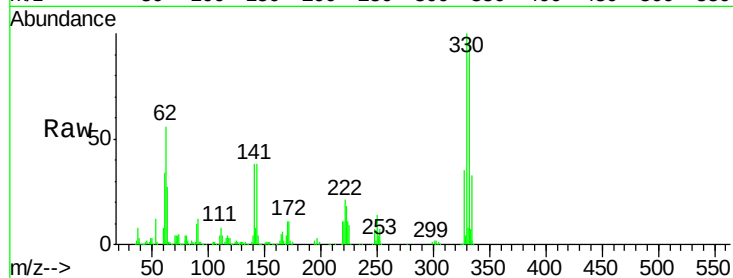

#44  
 2-Fluorobiphenyl  
 Concen: 80.96 ng  
 RT: 13.31 min Scan# 1697  
 Delta R.T. -0.01 min  
 Lab File: BG026013.D  
 Acq: 1 Mar 2017 1:43

Tgt Ion:172 Resp: 1527897  
 Ion Ratio Lower Upper  
 172 100  
 171 38.8 32.2 48.2  
 170 25.7 21.8 32.6

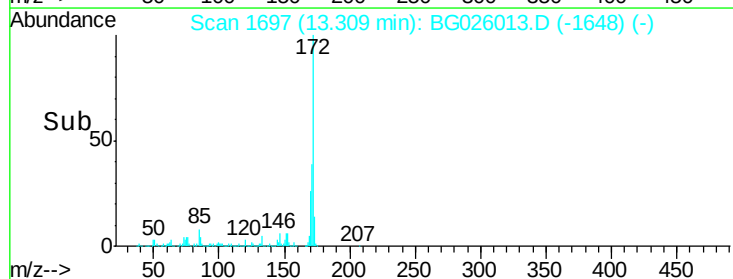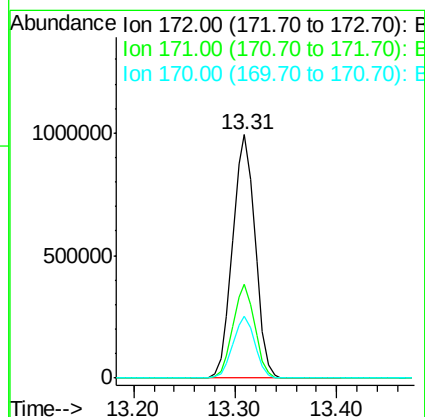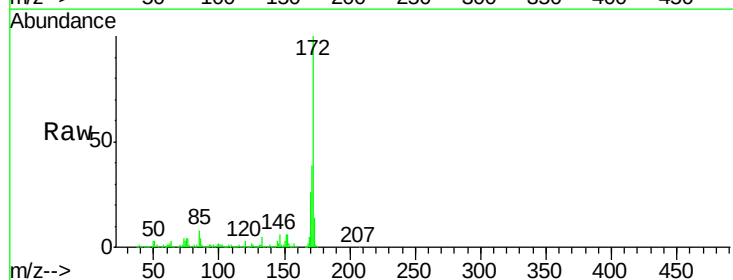

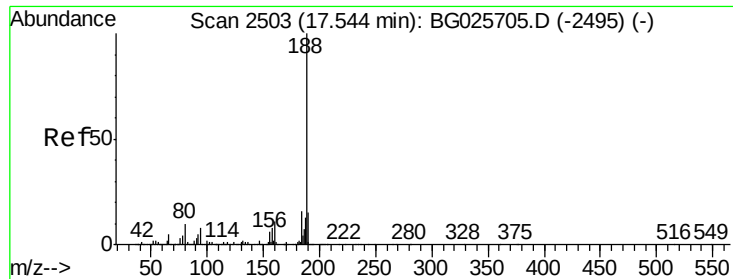

#63

Phenanthrene-d10

Concen: 20.00 ng

RT: 17.41 min Scan# 2395

Delta R.T. -0.01 min

Lab File: BG026013.D

Acq: 1 Mar 2017 1:43

Instrument :

BNA\_G

ClientSampleId :

PB97225BL


Tgt Ion:188 Resp: 898058

Ion Ratio Lower Upper

188 100

94 9.8 5.8 8.8#




80 10.6 7.5 11.3

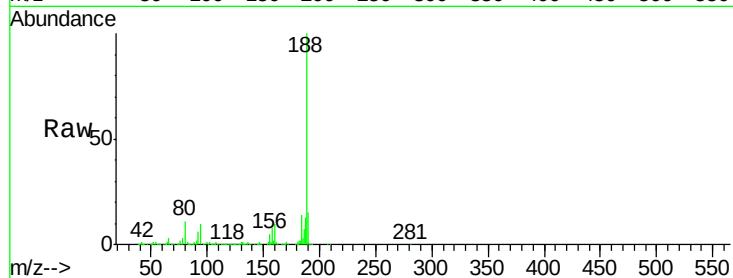

Abundance Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BGC

Ion 80.00 (79.70 to 80.70): BGC

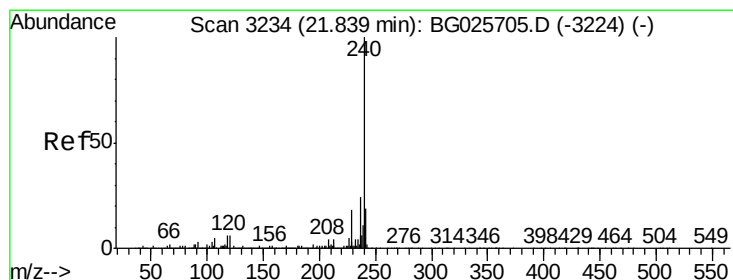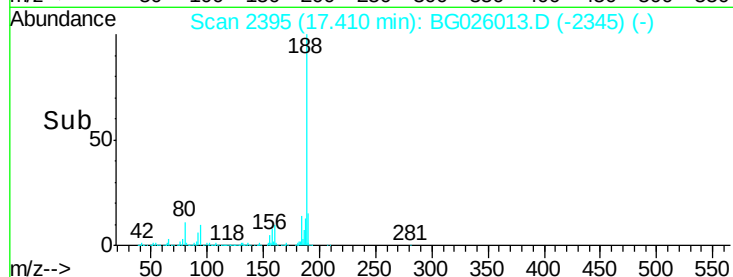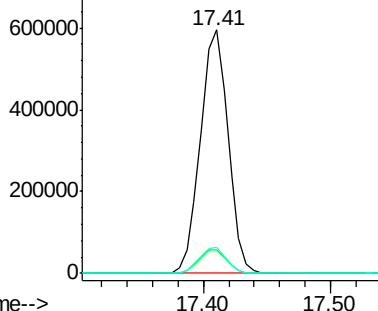

#75

Chrysene-d12

Concen: 20.00 ng

RT: 21.65 min Scan# 3117

Delta R.T. -0.03 min

Lab File: BG026013.D

Acq: 1 Mar 2017 1:43


Tgt Ion:240 Resp: 919142

Ion Ratio Lower Upper

240 100

120 12.0 5.7 8.5#



236 25.3 22.2 33.4

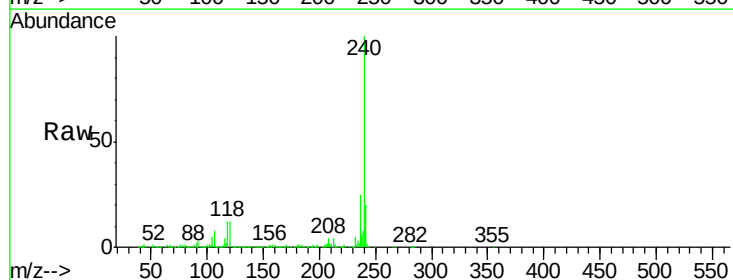


Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

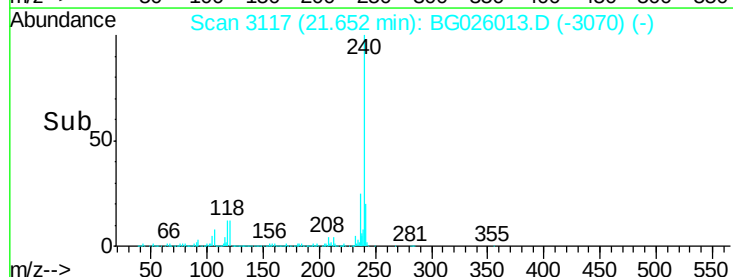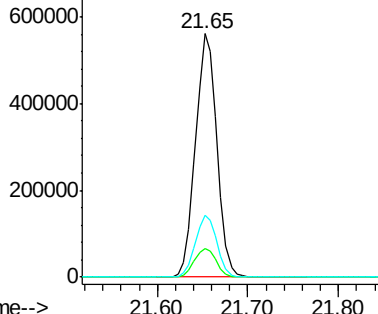

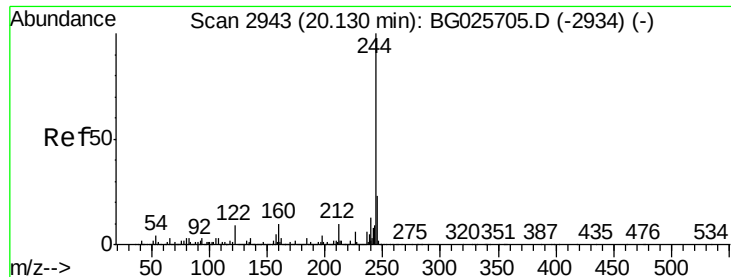

#78

Terphenyl-d14

Concen: 61.30 ng

RT: 20.00 min Scan# 2836

Delta R.T. -0.02 min

Lab File: BG026013.D

Acq: 1 Mar 2017 1:43

Instrument :

BNA\_G

ClientSampleId :

PB97225BL


Tgt Ion:244 Resp: 2316727

Ion Ratio Lower Upper

244 100

212 8.5 10.0 15.0#




122 13.9 8.6 12.8#

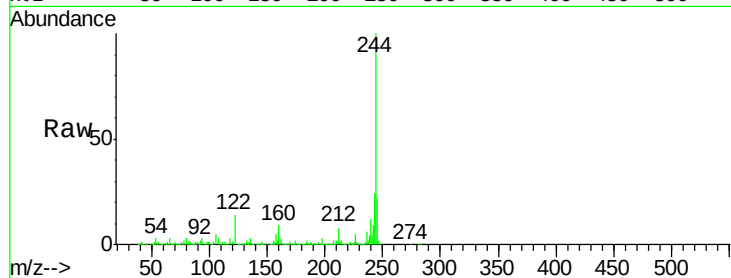

Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

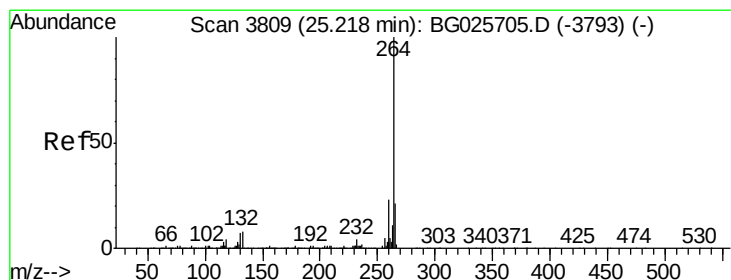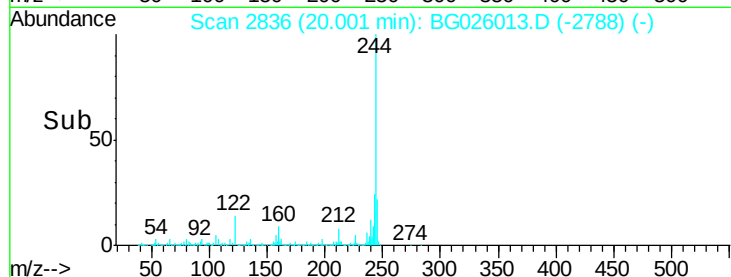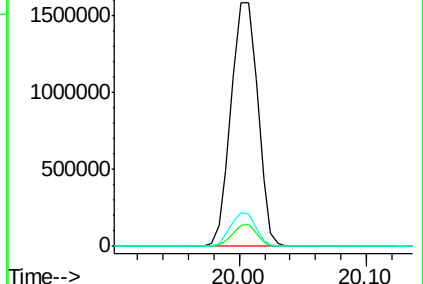

#86

Perylene-d12

Concen: 20.00 ng

RT: 24.85 min Scan# 3662

Delta R.T. -0.03 min

Lab File: BG026013.D

Acq: 1 Mar 2017 1:43


Tgt Ion:264 Resp: 892485

Ion Ratio Lower Upper

264 100

260 23.3 21.8 32.8

265 21.7 18.2 27.4

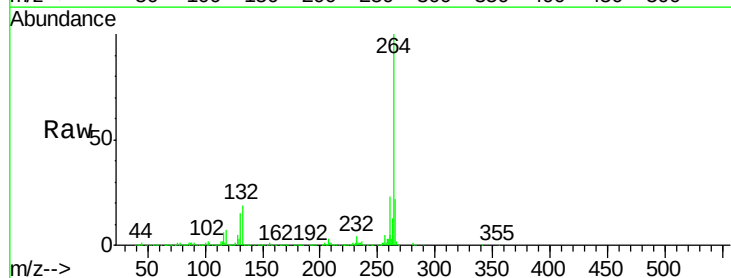

Abundance Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

