
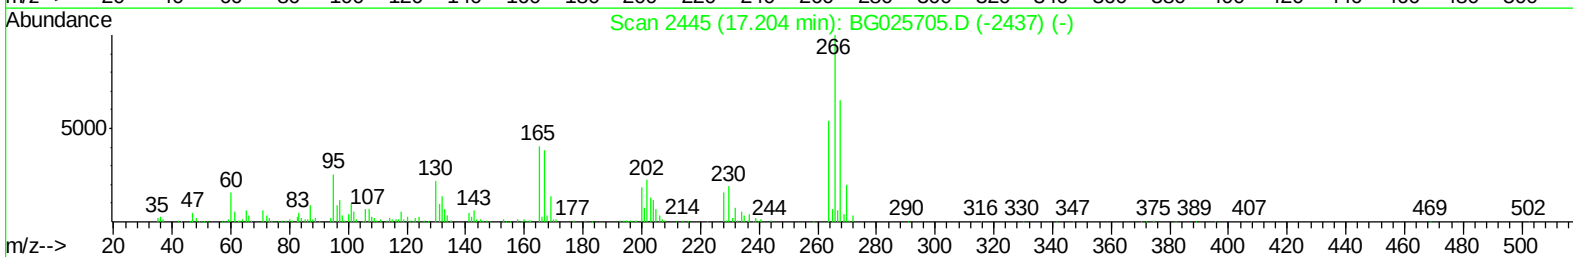
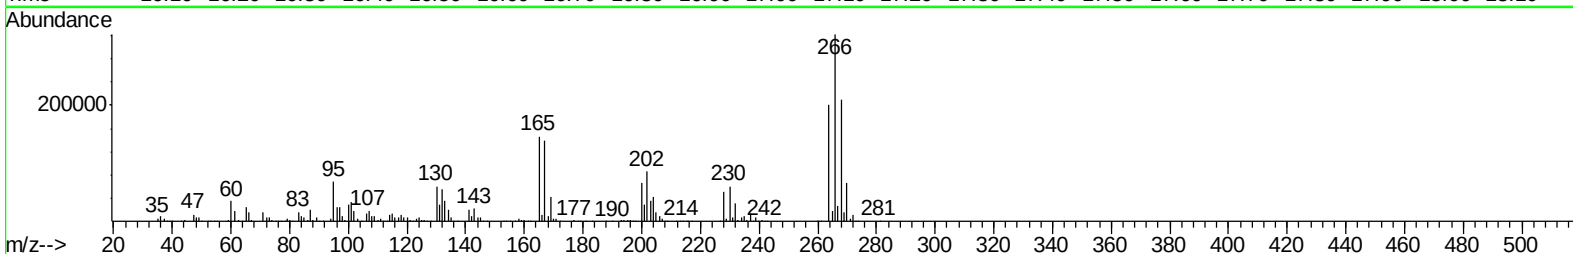


Data File : BG025995.D
Acq On : 28 Feb 2017 12:57
Operator : SJ/MA
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 01 07:13:55 2017
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG021717.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Feb 28 15:36:56 2017
Response via : Initial Calibration

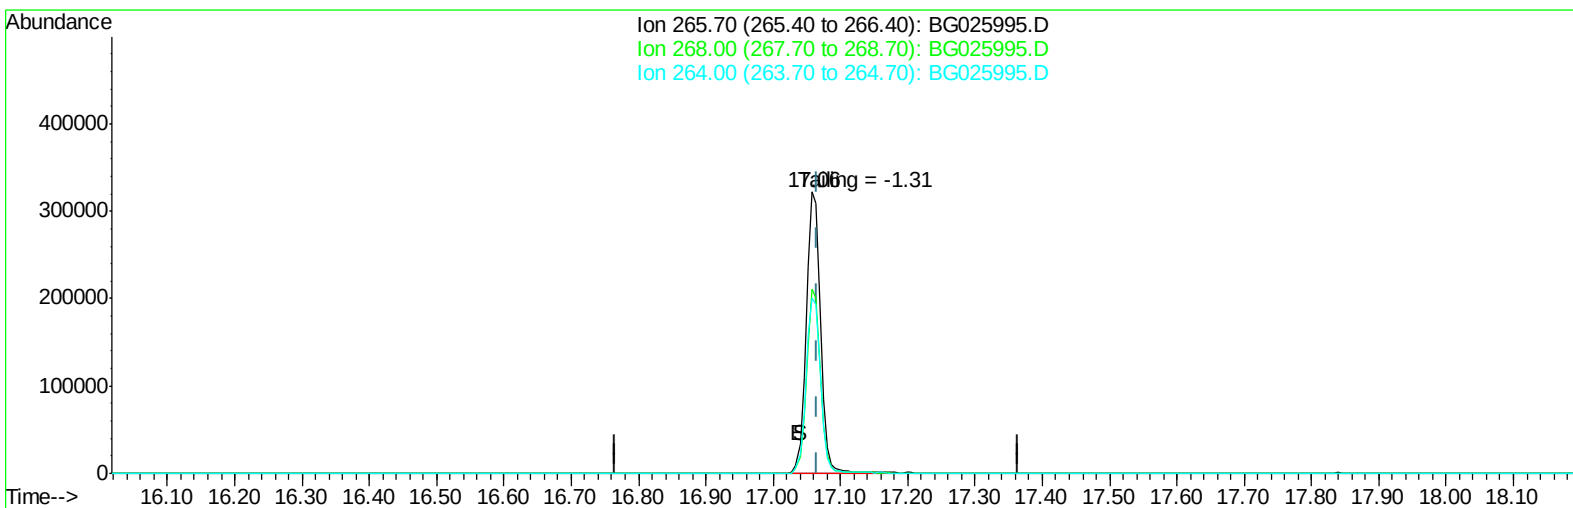

TIC: BG025995.D

(69) Pentachlorophenol (C)




17.057min (-0.008) 1280913.63ng m

response 486512

Ion	Exp%	Act%
265.70	100	100
268.00	60.70	65.40
264.00	62.60	62.24
0.00	0.00	0.00

Data File : BG025995.D
Acq On : 28 Feb 2017 12:57
Operator : SJ/MA
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 01 07:13:55 2017
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG021717.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Feb 28 15:36:56 2017
Response via : Initial Calibration

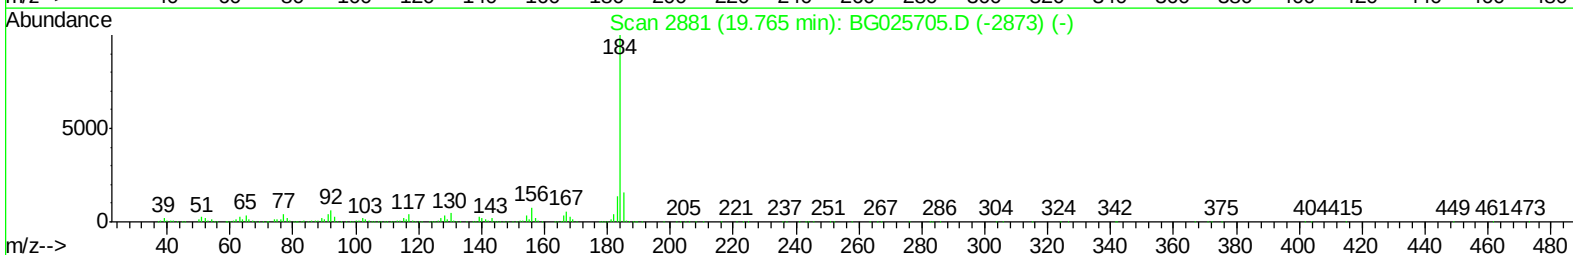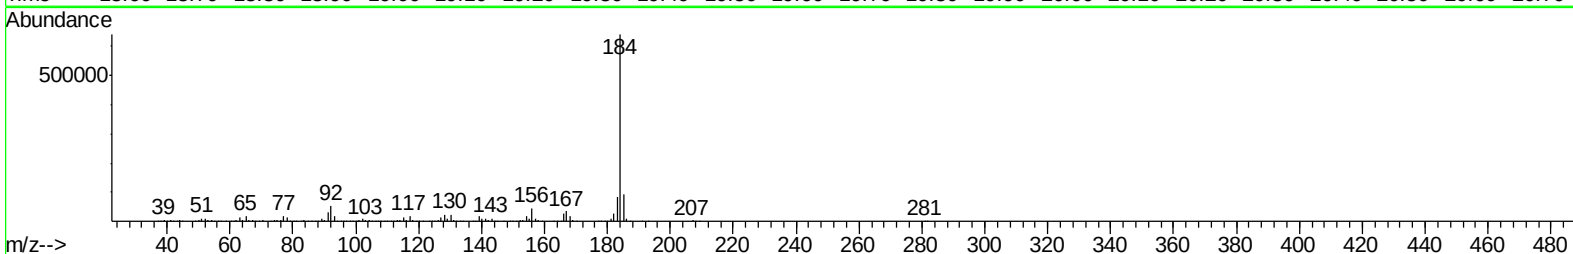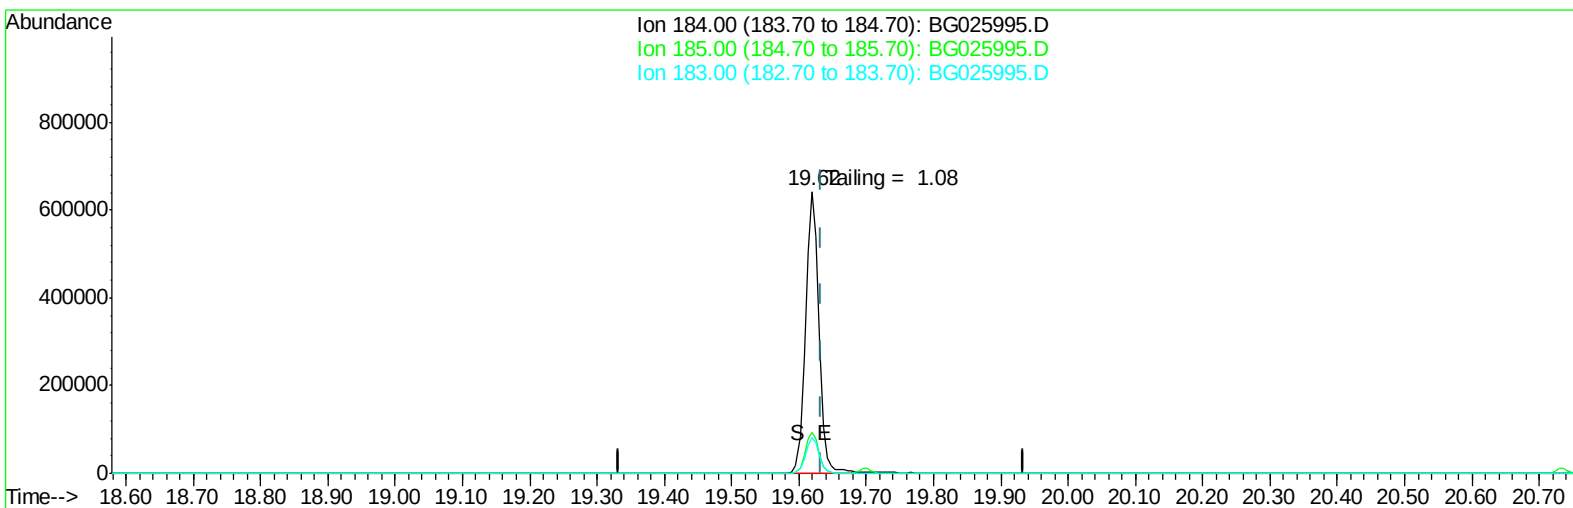

TIC: BG025995.D

(76) Benzidine

19.619min (-0.014) 486411.73ng

response 905929

Ion	Exp%	Act%
184.00	100	100
185.00	16.30	14.66
183.00	13.80	12.93
0.00	0.00	0.00