
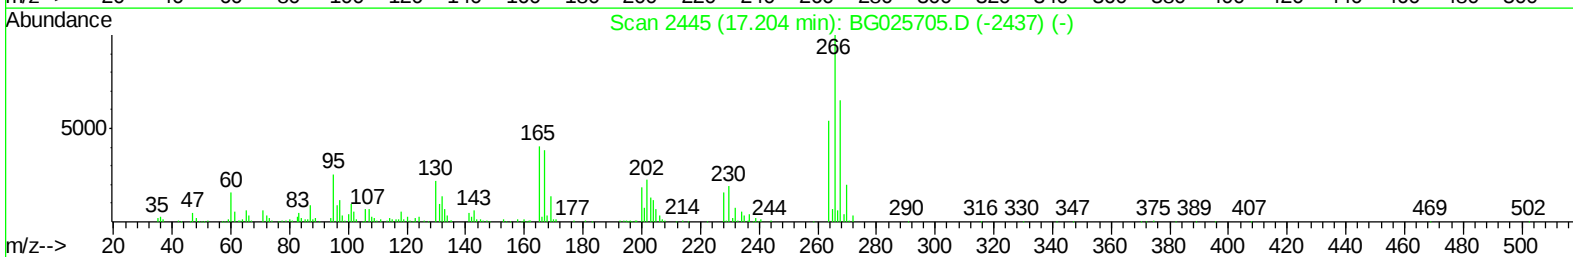
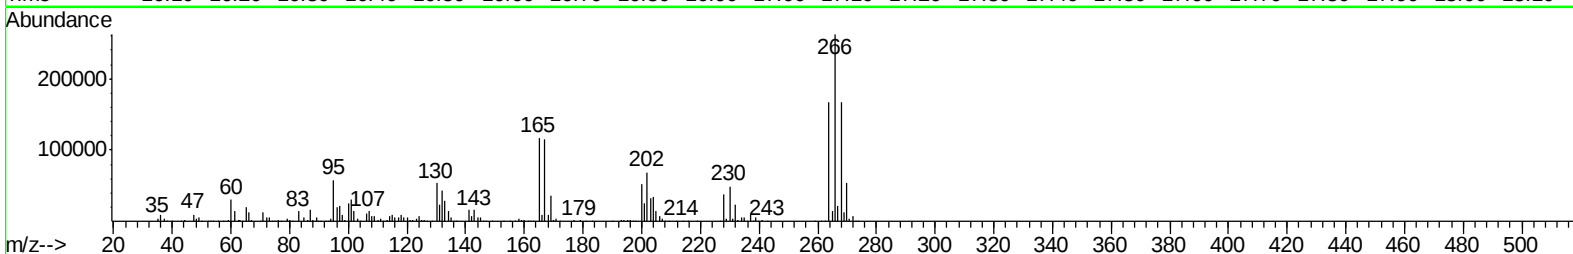


Data File : BG026010.D
Acq On : 28 Feb 2017 23:37
Operator : SJ/MA
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 01 07:14:32 2017
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG021717.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Feb 28 15:36:56 2017
Response via : Initial Calibration

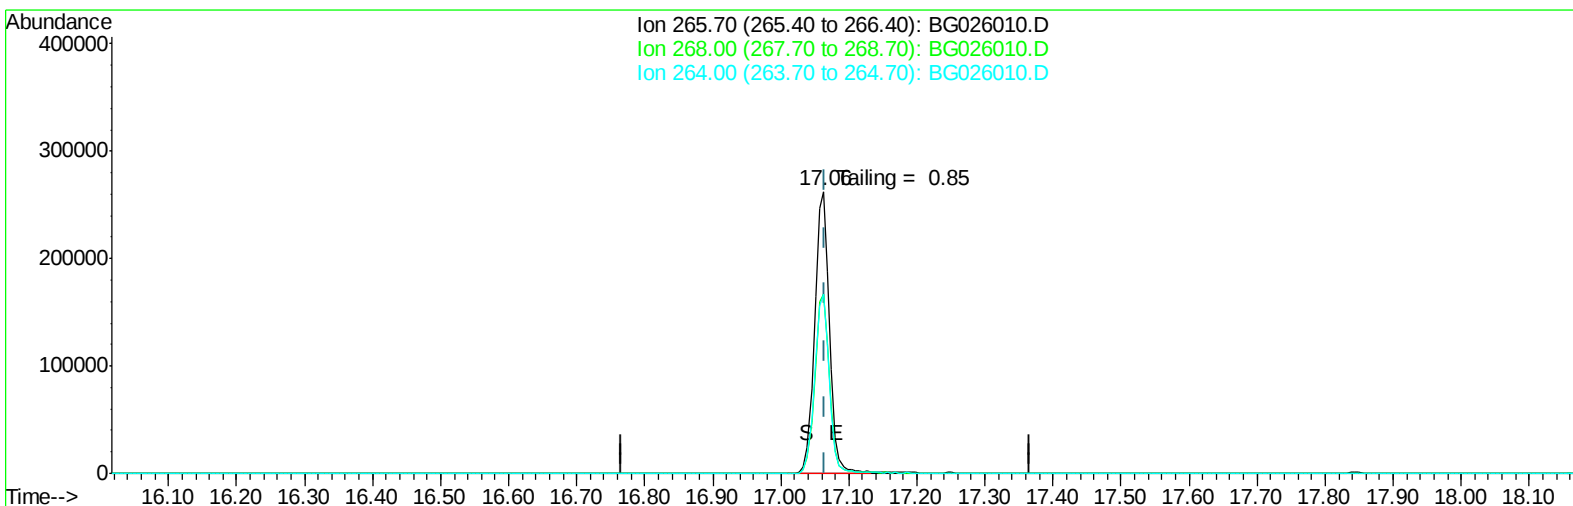

TIC: BG026010.D

(69) Pentachlorophenol (C)




17.063min (-0.003) 392219.38ng

response 402484

Ion	Exp%	Act%
265.70	100	100
268.00	60.70	63.62
264.00	62.60	63.67
0.00	0.00	0.00

Data File : BG026010.D
Acq On : 28 Feb 2017 23:37
Operator : SJ/MA
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 01 07:14:32 2017
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG021717.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Feb 28 15:36:56 2017
Response via : Initial Calibration

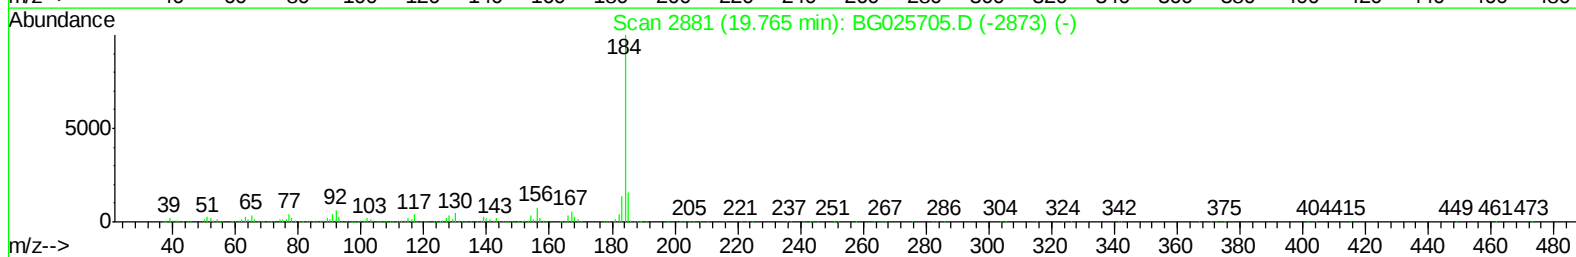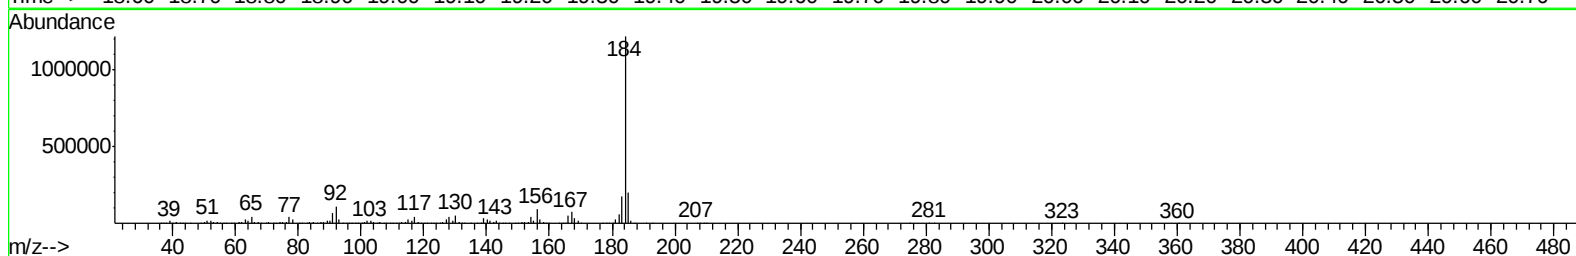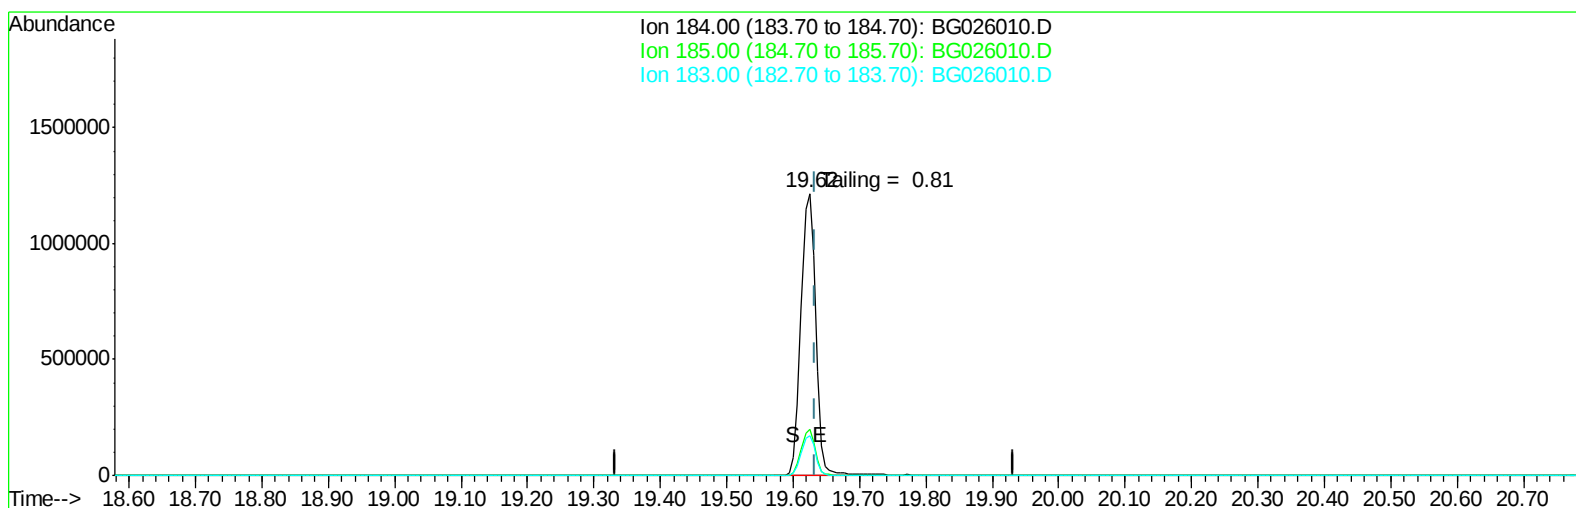

TIC: BG026010.D

(76) Benzidine

19.624min (-0.009) 425368.55ng

response 1826175

Ion	Exp%	Act%
184.00	100	100
185.00	16.30	16.21
183.00	13.80	14.23
0.00	0.00	0.00