

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG022817\
 Data File : BG026018.D
 Acq On : 1 Mar 2017 10:02
 Operator : SJ/MA
 Sample : PB97232BL
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 PB97232BL

Quant Time: Mar 01 12:17:49 2017
 Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG021717.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Feb 28 15:36:56 2017
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.08	152	115696	20.00	ng	0.00
21) Naphthalene-d8	10.88	136	523174	20.00	ng	-0.01
38) Acenaphthene-d10	14.68	164	361357	20.00	ng	-0.01
63) Phenanthrene-d10	17.41	188	1004673	20.00	ng	0.00
75) Chrysene-d12	21.66	240	1038817	20.00	ng	-0.02
86) Perylene-d12	24.86	264	1017296	20.00	ng	-0.03
System Monitoring Compounds						
5) 2-Fluorophenol	5.65	112	770673	115.97	ng	0.00
7) Phenol-d6	7.23	99	1066775	108.48	ng	0.00
23) Nitrobenzene-d5	9.23	82	581140	70.10	ng	-0.01
41) 2,4,6-Tribromophenol	16.16	330	539869	161.71	ng	0.00
44) 2-Fluorobiphenyl	13.31	172	1637809	79.20	ng	-0.01
78) Terphenyl-d14	20.01	244	2594085	60.73	ng	-0.01


Target Compounds	Qvalue
------------------	--------


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG022817\
Data File : BG026018.D
Acq On : 1 Mar 2017 10:02
Operator : SJ/MA
Sample : PB97232BL
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
PB97232BL

Quant Time: Mar 01 12:17:49 2017
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG021717.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Feb 28 15:36:56 2017
Response via : Initial Calibration

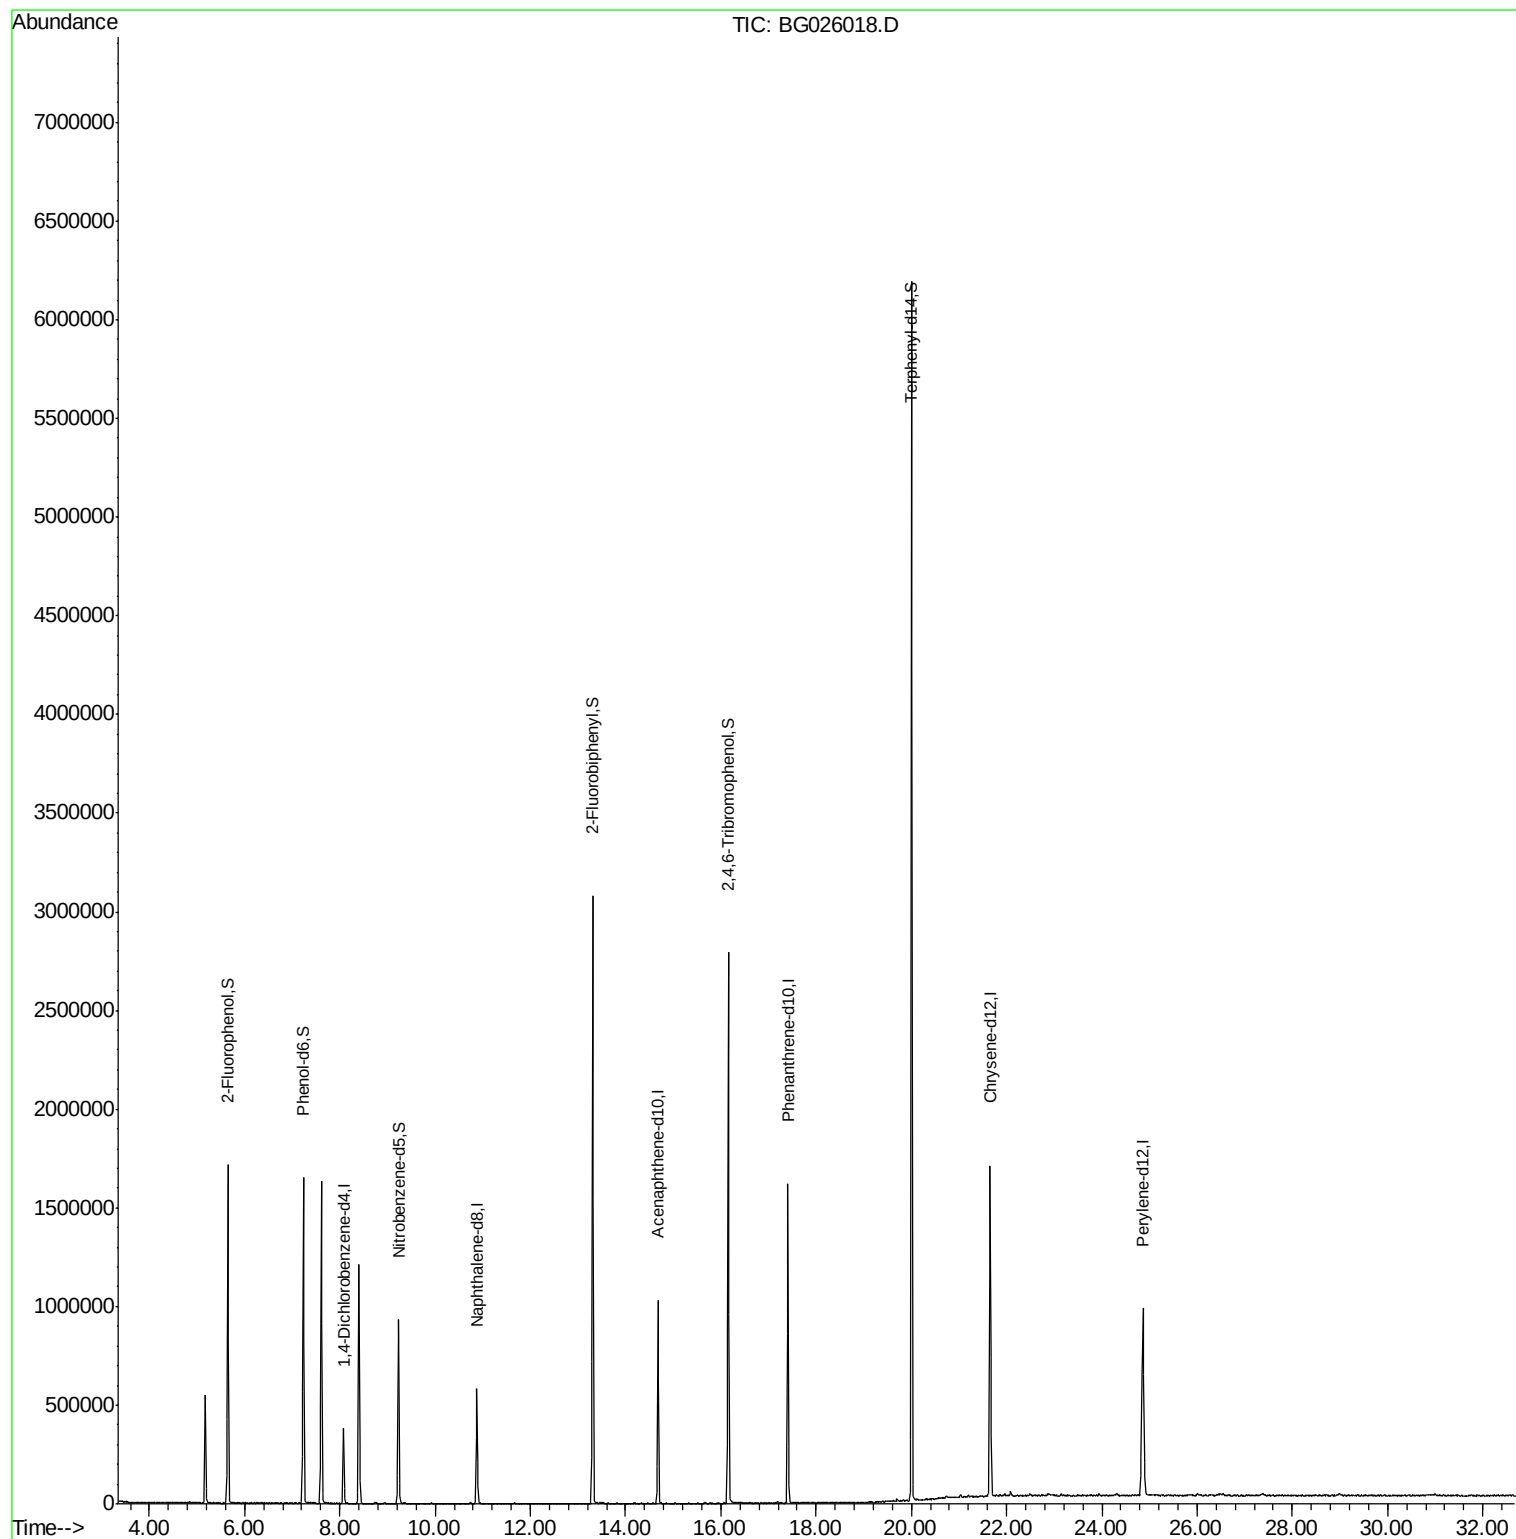

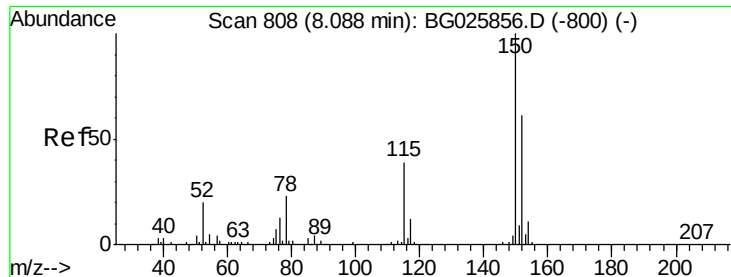


#1


1,4-Dichlorobenzene-d4
Concen: 20.00 ng
RT: 8.08 min Scan# 807
Delta R.T. -0.01 min
Lab File: BG026018.D
Acq: 1 Mar 2017 10:02

Instrument :
BNA_G
ClientSampleId :
PB97232BL



Tgt Ion:152 Resp: 115696
Ion Ratio Lower Upper
152 100
150 152.7 114.0 171.0
115 56.6 48.1 72.1

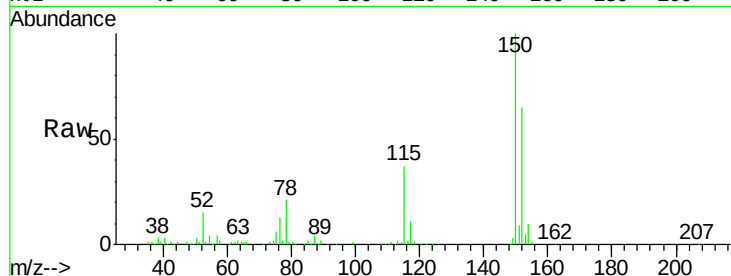

Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

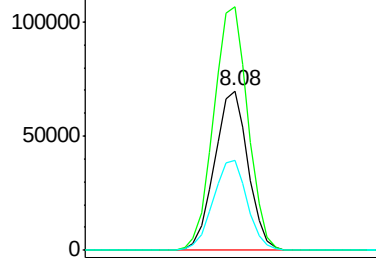


Time-->

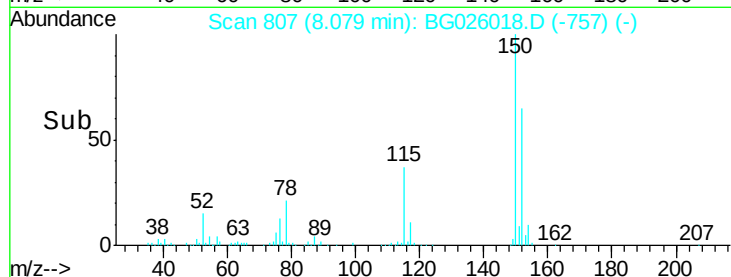


#5

2-Fluorophenol
Concen: 115.97 ng
RT: 5.65 min Scan# 393
Delta R.T. -0.01 min
Lab File: BG026018.D
Acq: 1 Mar 2017 10:02


Tgt Ion:112 Resp: 770673
Ion Ratio Lower Upper
112 100
64 64.0 61.8 92.6
63 32.4 37.2 55.8#




Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BGC
Ion 63.00 (62.70 to 63.70): BGC

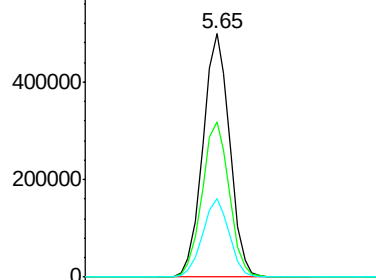

Time-->

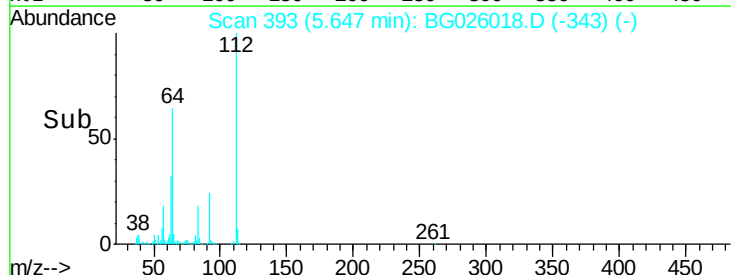

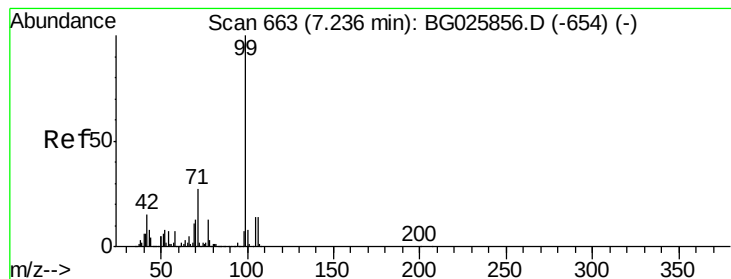

#7

Phenol-d6

Concen: 108.48 ng

RT: 7.23 min Scan# 663

Delta R.T. -0.00 min

Lab File: BG026018.D

Acq: 1 Mar 2017 10:02

Instrument :

BNA_G

ClientSampleId :

PB97232BL


Tgt Ion: 99 Resp: 1066775

Ion Ratio Lower Upper




99 100

42 14.5 20.5 30.7#

71 29.3 37.6 56.4#



Abundance Ion 99.00 (98.70 to 99.70): BGC
Ion 42.00 (41.70 to 42.70): BGC
Ion 71.00 (70.70 to 71.70): BGC

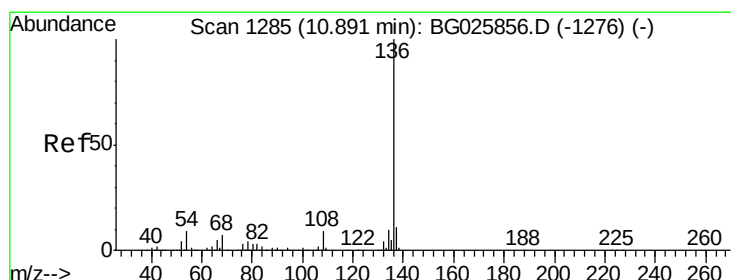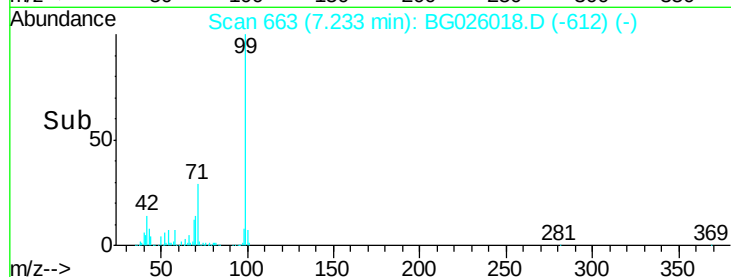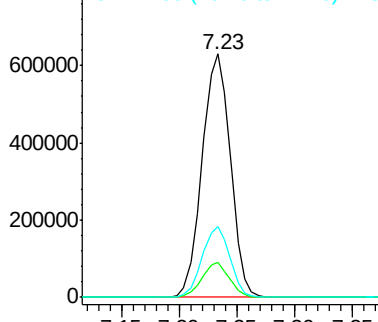

#21

Naphthalene-d8

Concen: 20.00 ng

RT: 10.88 min Scan# 1283

Delta R.T. -0.01 min

Lab File: BG026018.D

Acq: 1 Mar 2017 10:02

Tgt Ion: 136 Resp: 523174


Ion Ratio Lower Upper

136 100



137 10.8 8.9 13.3


54 7.3 9.3 13.9#

68 6.5 5.1 7.7



Abundance Ion 136.00 (135.70 to 136.70): BGC
Ion 137.00 (136.70 to 137.70): BGC
Ion 54.00 (53.70 to 54.70): BGC
Ion 68.00 (67.70 to 68.70): BGC



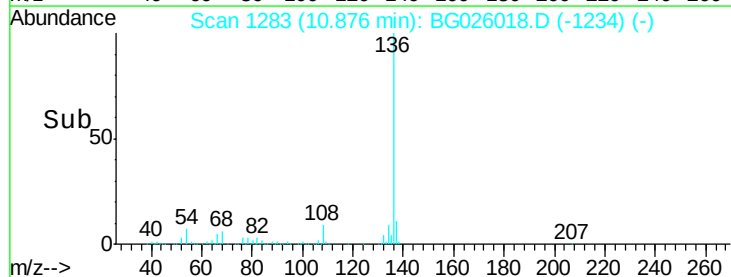
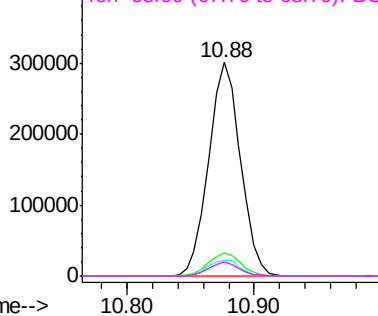


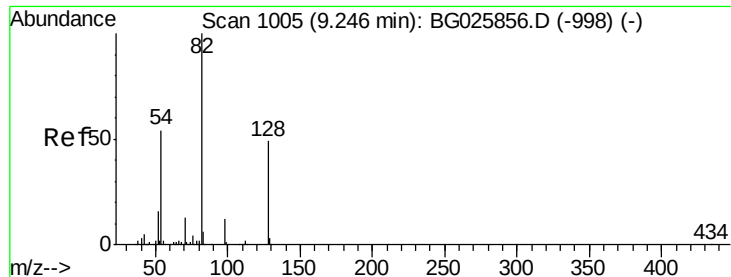

#23
 Nitrobenzene-d5
 Concen: 70.10 ng
 RT: 9.23 min Scan# 1003
 Delta R.T. -0.01 min
 Lab File: BG026018.D
 Acq: 1 Mar 2017 10:02




Instrument :
 BNA_G
 ClientSampleID :
 PB97232BL


Tgt Ion: 82 Resp: 581140
 Ion Ratio Lower Upper
 82 100
 128 49.8 26.4 39.6#
 54 46.9 49.4 74.2#

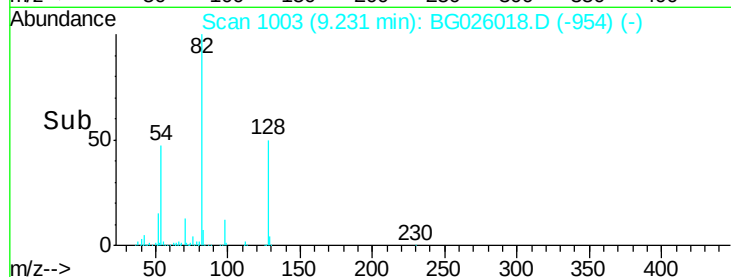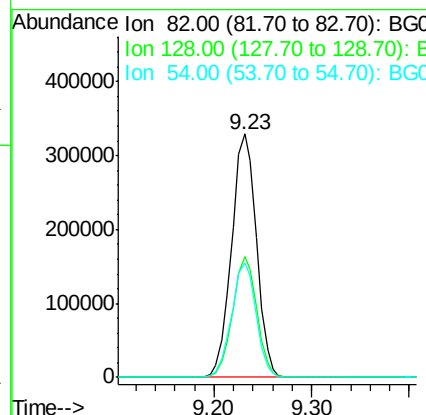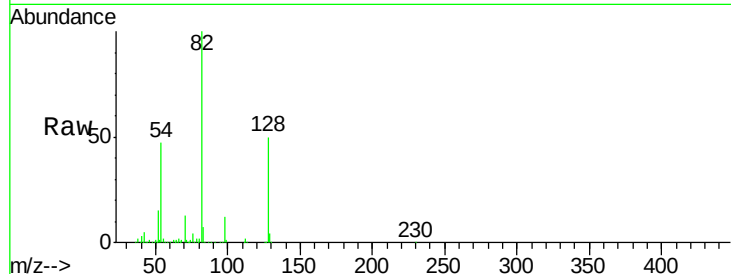

#38
 Acenaphthene-d10
 Concen: 20.00 ng
 RT: 14.68 min Scan# 1930
 Delta R.T. -0.01 min
 Lab File: BG026018.D
 Acq: 1 Mar 2017 10:02

Tgt Ion: 164 Resp: 361357
 Ion Ratio Lower Upper
 164 100
 162 103.2 85.1 127.7
 160 43.4 34.7 52.1


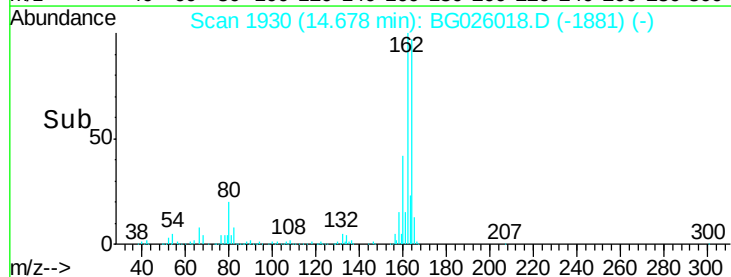
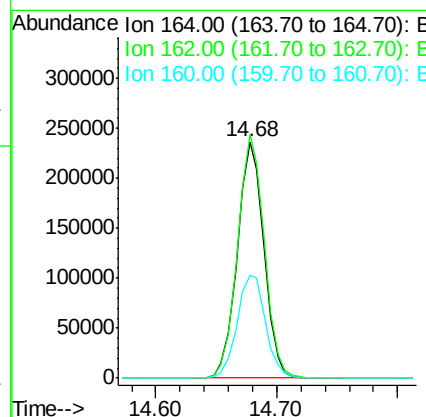
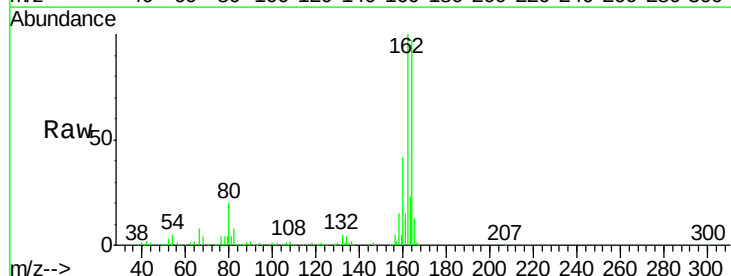


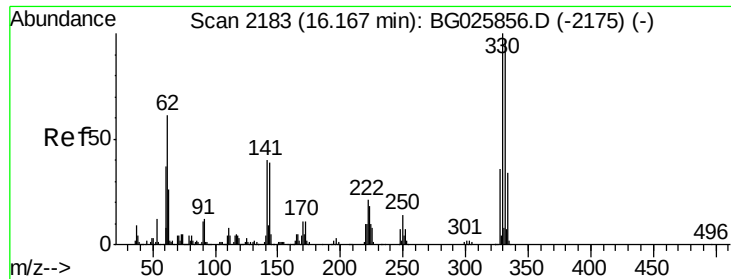

#41
2,4,6-Tribromophenol
Concen: 161.71 ng
RT: 16.16 min Scan# 2182
Delta R.T. -0.01 min
Lab File: BG026018.D
Acq: 1 Mar 2017 10:02




Instrument :
BNA_G
ClientSampleId :
PB97232BL


Tgt Ion	Ratio	Lower	Upper
330	100		
332	95.9	77.3	115.9
141	35.4	32.1	48.1

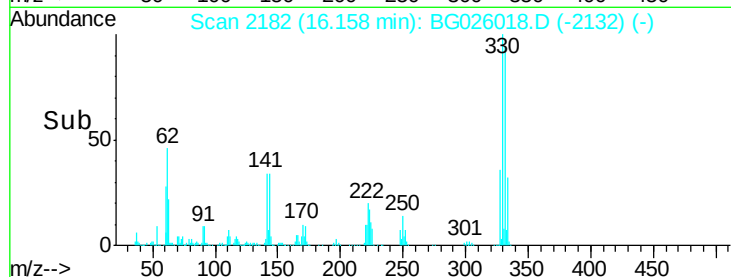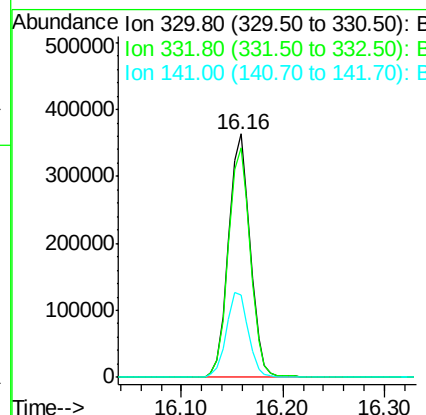

#44
2-Fluorobiphenyl
Concen: 79.20 ng
RT: 13.31 min Scan# 1697
Delta R.T. -0.01 min
Lab File: BG026018.D
Acq: 1 Mar 2017 10:02

Tgt Ion	Ratio	Lower	Upper
172	100		
171	38.2	32.2	48.2
170	25.3	21.8	32.6


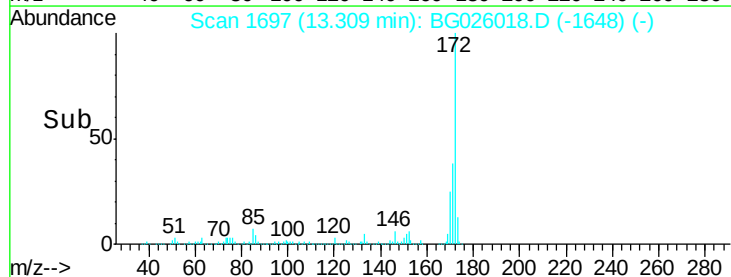
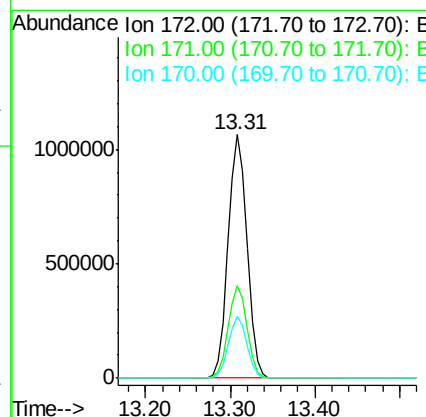



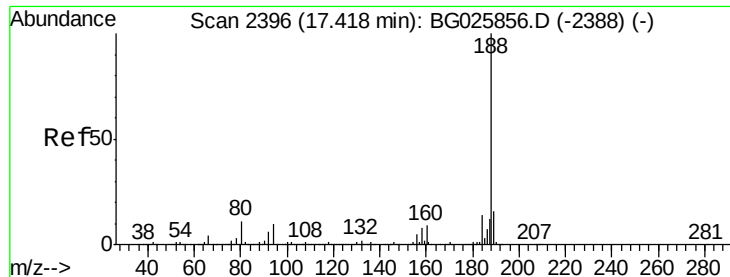

#63
Phenanthrene-d10
Concen: 20.00 ng
RT: 17.41 min Scan# 2395
Delta R.T. -0.01 min
Lab File: BG026018.D
Acq: 1 Mar 2017 10:02




Instrument :
BNA_G
ClientSampleId :
PB97232BL


Tgt Ion:188 Resp: 1004673
Ion Ratio Lower Upper
188 100
94 9.3 5.8 8.8#
80 10.6 7.5 11.3

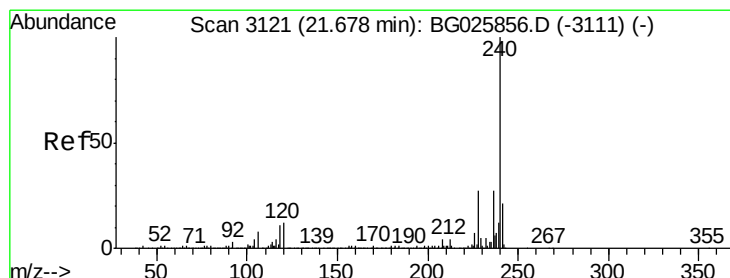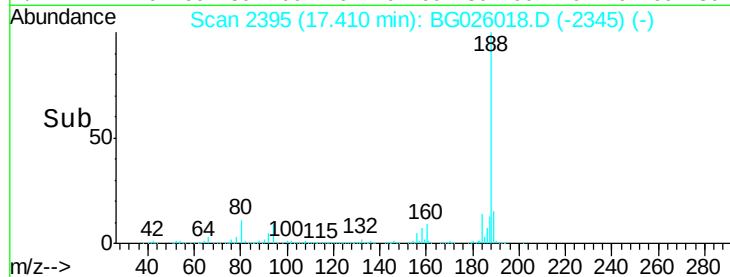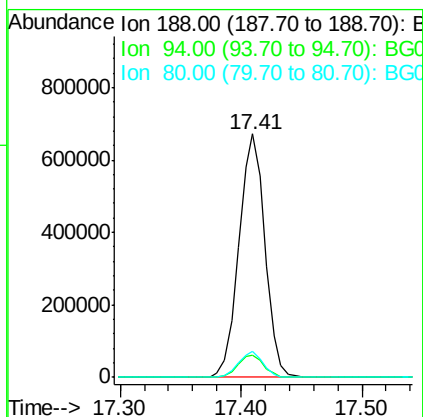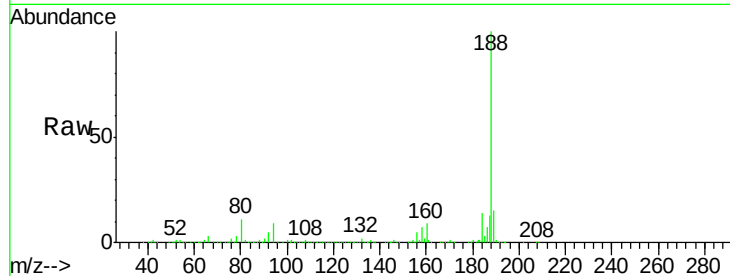

#75
Chrysene-d12
Concen: 20.00 ng
RT: 21.66 min Scan# 3118
Delta R.T. -0.02 min
Lab File: BG026018.D
Acq: 1 Mar 2017 10:02

Tgt Ion:240 Resp: 1038817
Ion Ratio Lower Upper
240 100
120 11.4 5.7 8.5#
236 26.0 22.2 33.4

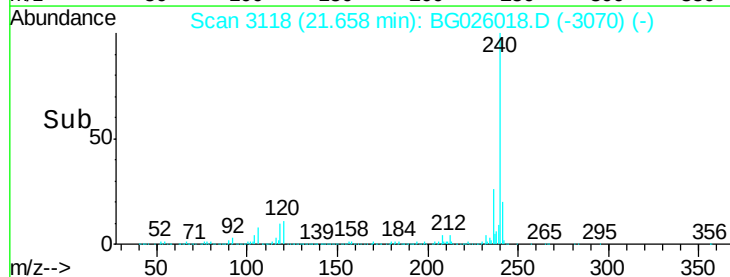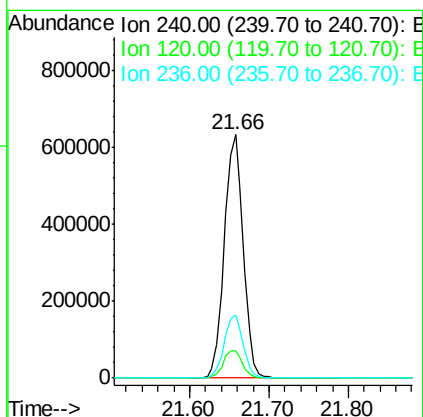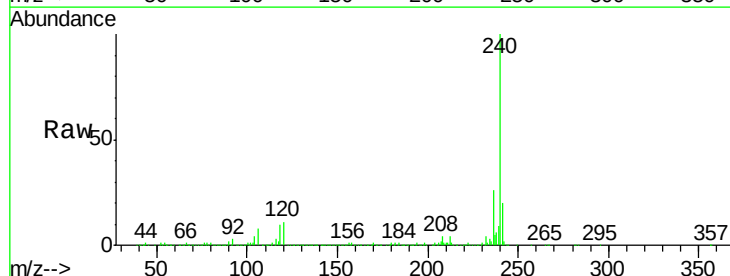

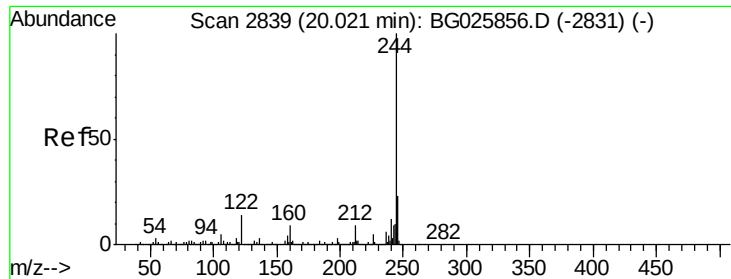

#78

Terphenyl-d14

Concen: 60.73 ng

RT: 20.01 min Scan# 2837

Delta R.T. -0.01 min

Lab File: BG026018.D

Acq: 1 Mar 2017 10:02

Instrument :

BNA_G

ClientSampleId :

PB97232BL


Tgt Ion:244 Resp: 2594085

Ion Ratio Lower Upper

244 100

212 8.9 10.0 15.0#




122 13.3 8.6 12.8#

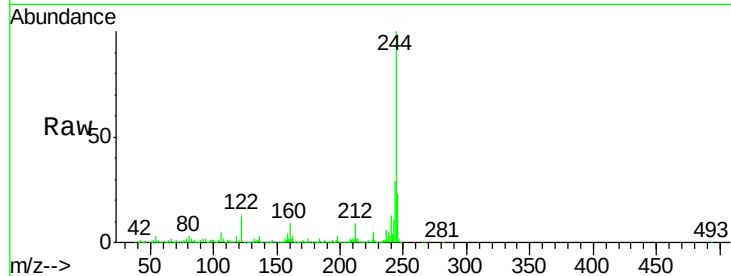

Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

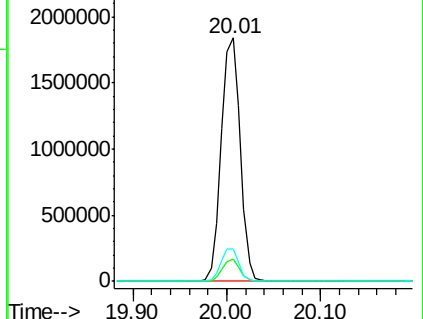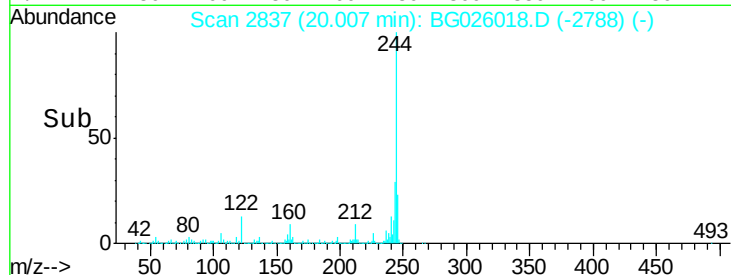

#86

Perylene-d12

Concen: 20.00 ng

RT: 24.86 min Scan# 3663

Delta R.T. -0.03 min

Lab File: BG026018.D

Acq: 1 Mar 2017 10:02


Tgt Ion:264 Resp: 1017296

Ion Ratio Lower Upper

264 100

260 24.3 21.8 32.8

265 21.7 18.2 27.4



Abundance Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

