


Data Path : Z:\HPCHEM1\BNA_G\Data\BG022817\
 Data File : BG025995.D
 Acq On : 28 Feb 2017 12:57
 Operator : SJ/MA
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG021717.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Feb 28 15:36:56 2017

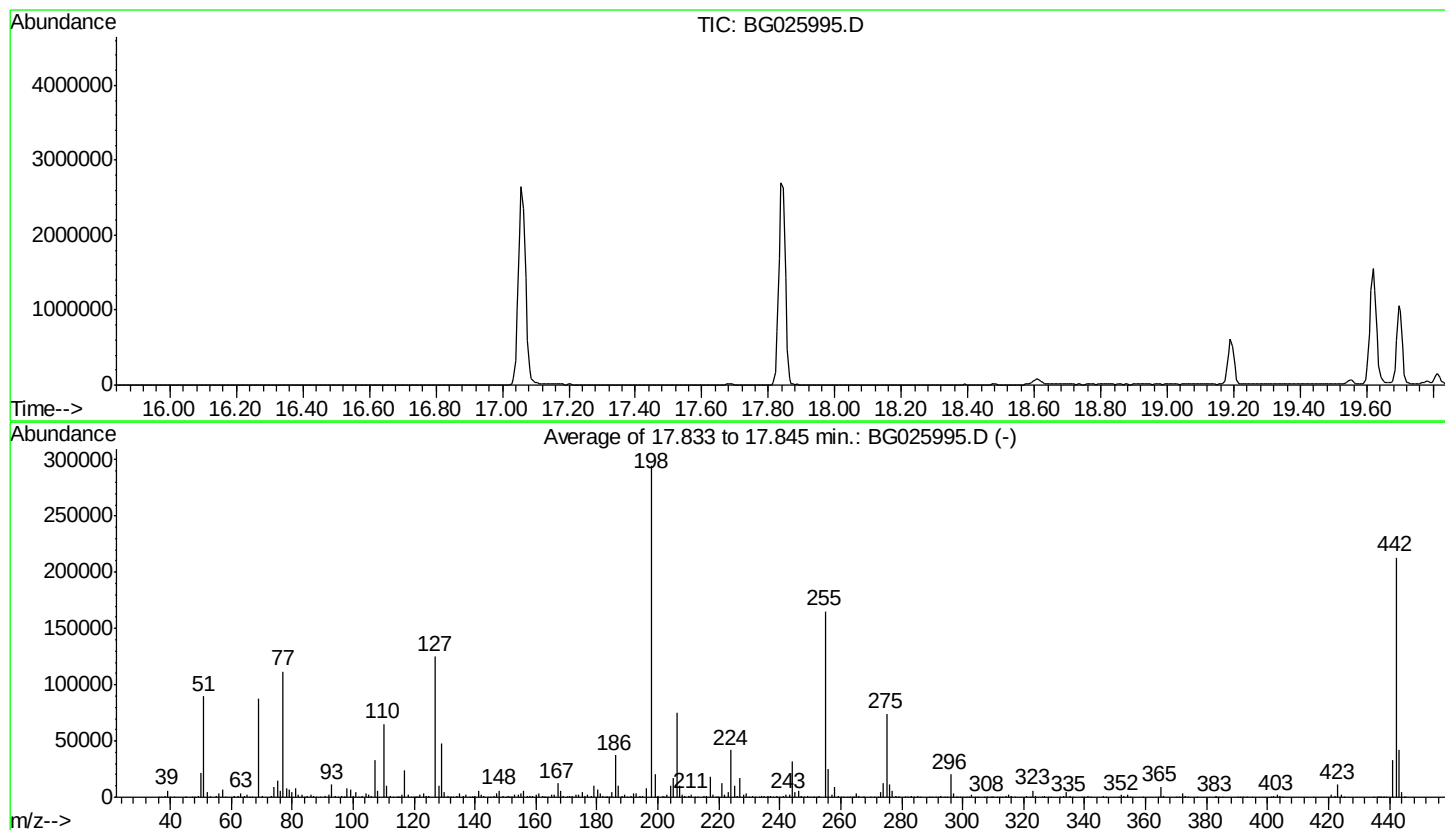

AutoFind: Scans 2467, 2468, 2469; Background Corrected with Scan 2460

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	30.4	89637	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	29.6	87120	PASS
70	69	0.00	2	0.7	627	PASS
127	198	10	80	42.4	125072	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	294762	PASS
199	198	5	9	6.9	20235	PASS
275	198	10	60	25.1	74026	PASS
365	198	1	100	3.1	9218	PASS
441	442	0.01	24	15.8	33570	PASS
442	198	50	100	72.3	213002	PASS
443	442	15	24	19.6	41690	PASS