


Data Path : Z:\HPCHEM1\BNA_G\DATA\BG022817\
 Data File : BG026010.D
 Acq On : 28 Feb 2017 23:37
 Operator : SJ/MA
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG021717.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Feb 28 15:36:56 2017

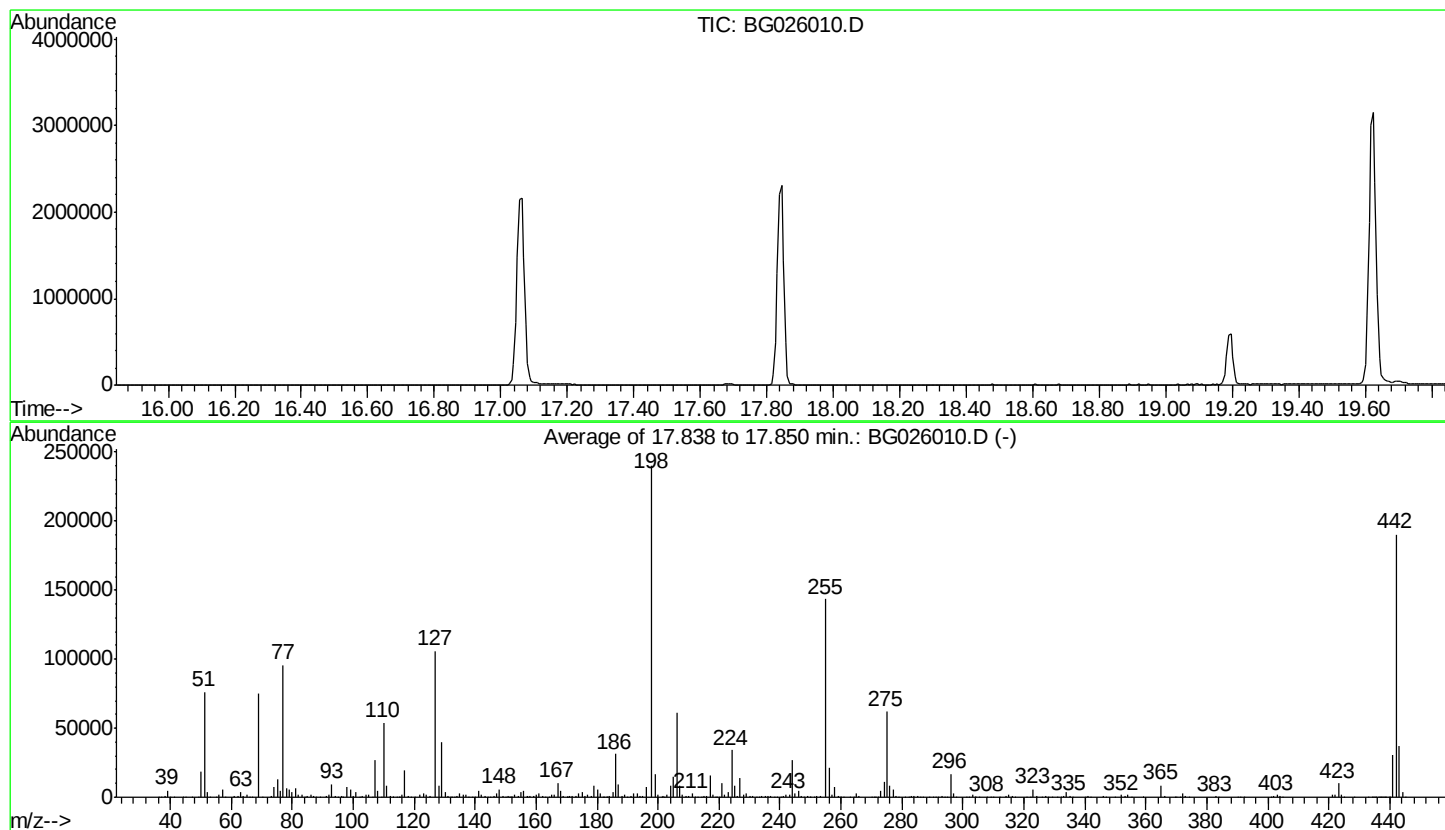

AutoFind: Scans 2468, 2469, 2470; Background Corrected with Scan 2461

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	31.7	76061	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	31.4	75392	PASS
70	69	0.00	2	0.5	407	PASS
127	198	10	80	44.1	105962	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	240256	PASS
199	198	5	9	6.8	16412	PASS
275	198	10	60	25.8	61976	PASS
365	198	1	100	3.5	8436	PASS
441	442	0.01	24	16.0	30434	PASS
442	198	50	100	79.1	190144	PASS
443	442	15	24	19.6	37341	PASS