
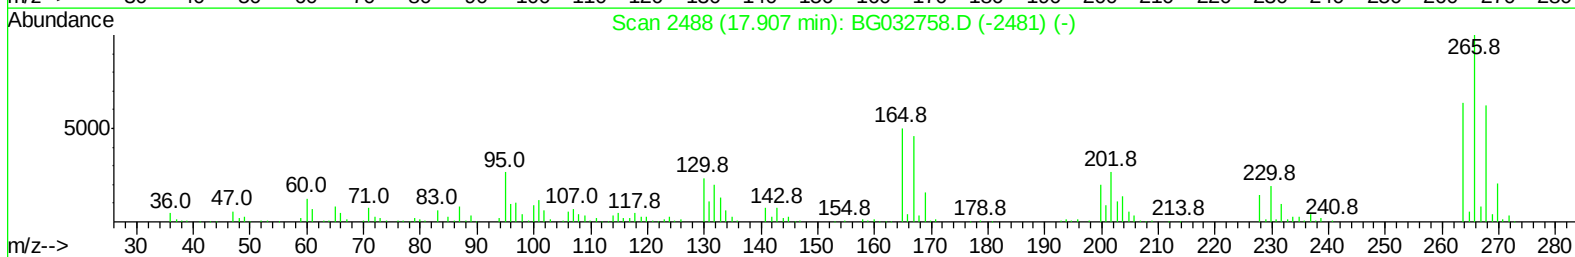
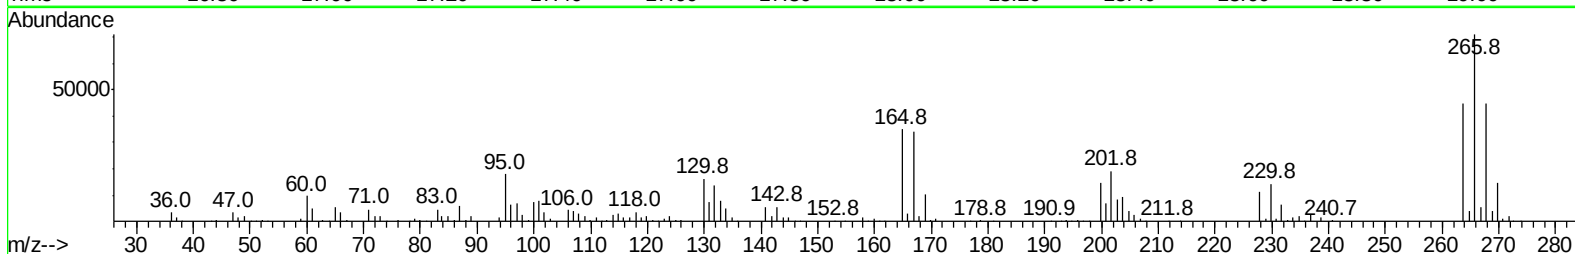


Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA G\DATA\BG022818\
Data File : BG032888.D
Acq On : 28 Feb 2018 14:49
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 01 03:33:38 2018
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG022118.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Feb 26 17:50:45 2018
Response via : Initial Calibration

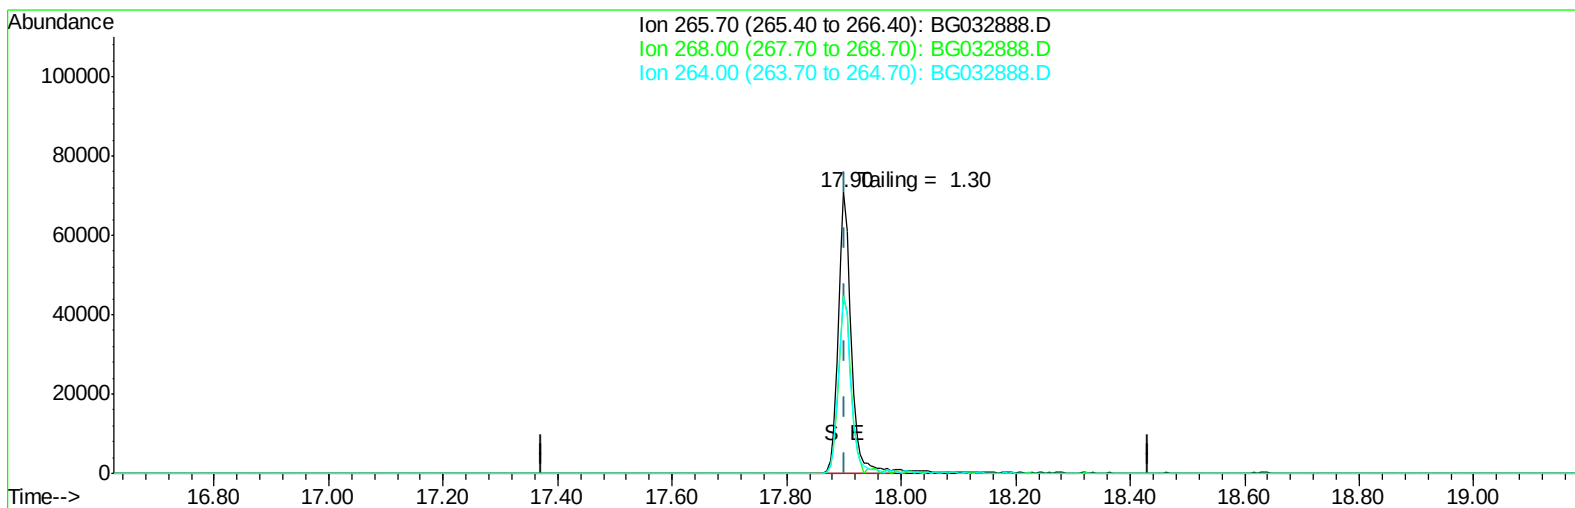

TIC: BG032888.D

(69) Pentachlorophenol (C)




17.899min (-0.003) 27990.11ng

response 112616

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	63.00
264.00	62.00	62.93
0.00	0.00	0.00

Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA G\DATA\BG022818\
Data File : BG032888.D
Acq On : 28 Feb 2018 14:49
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 01 03:33:38 2018
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG022118.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Feb 26 17:50:45 2018
Response via : Initial Calibration

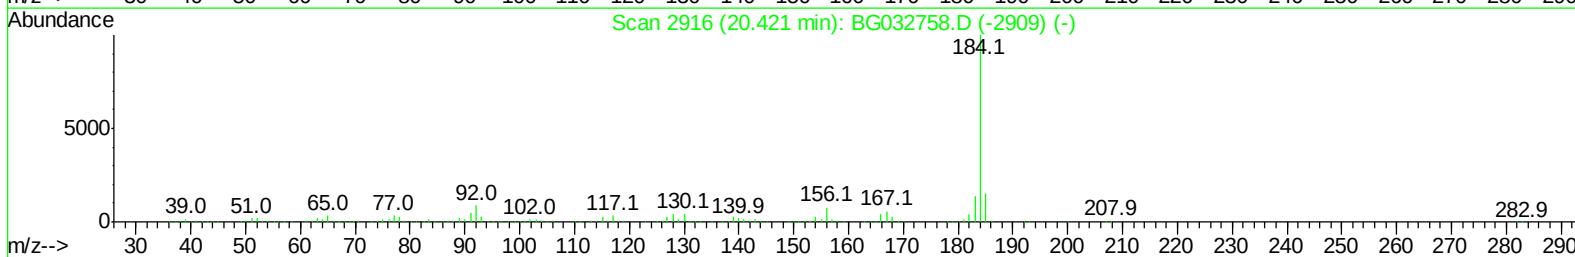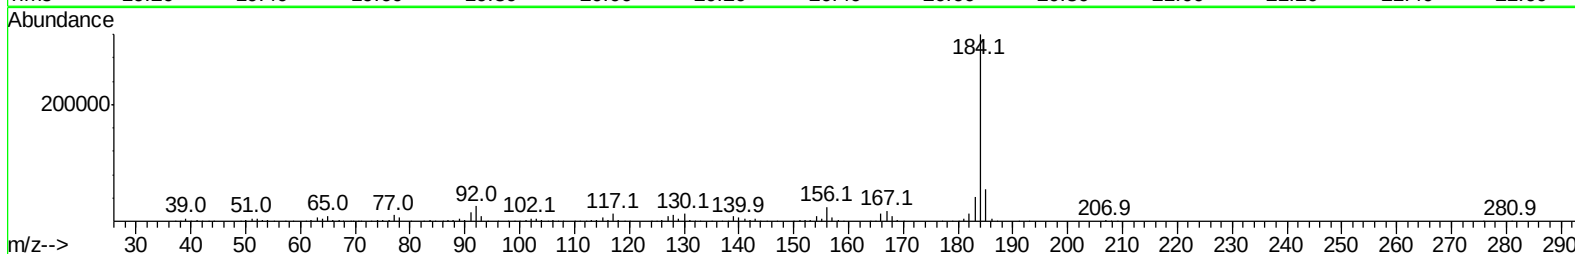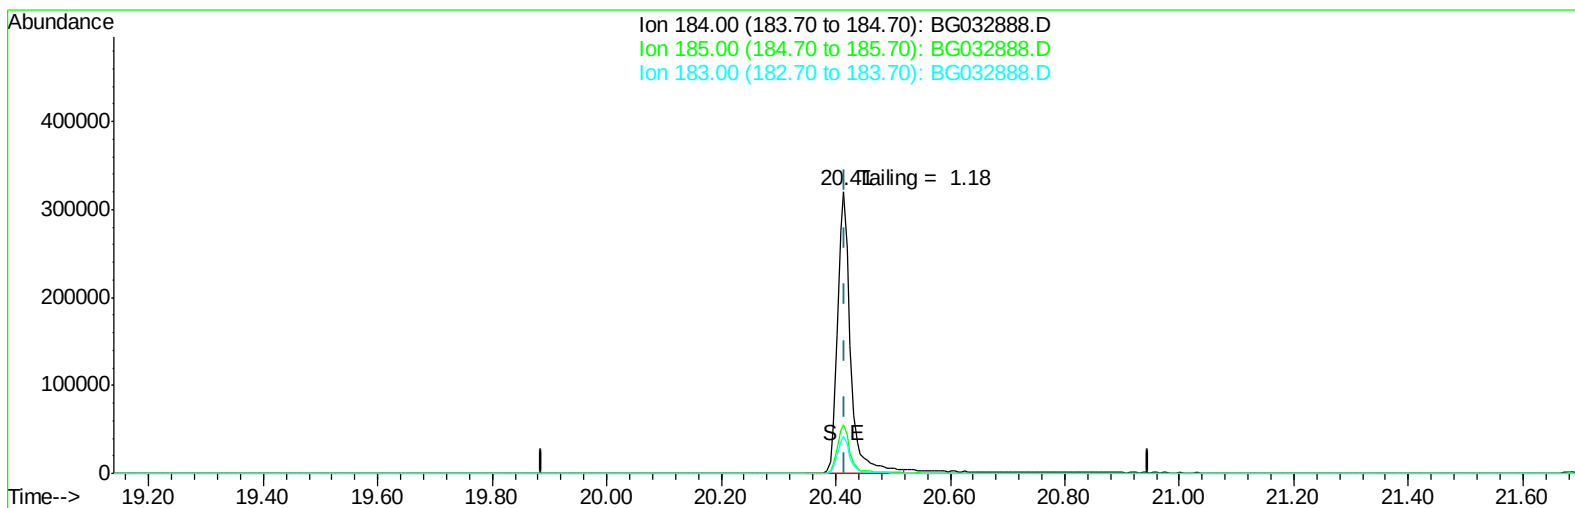

TIC: BG032888.D

(76) Benzidine

20.414min (-0.003) 0.00ng

response 525708

Ion	Exp%	Act%
184.00	100	100
185.00	13.90	17.39#
183.00	13.30	13.06
0.00	0.00	0.00