
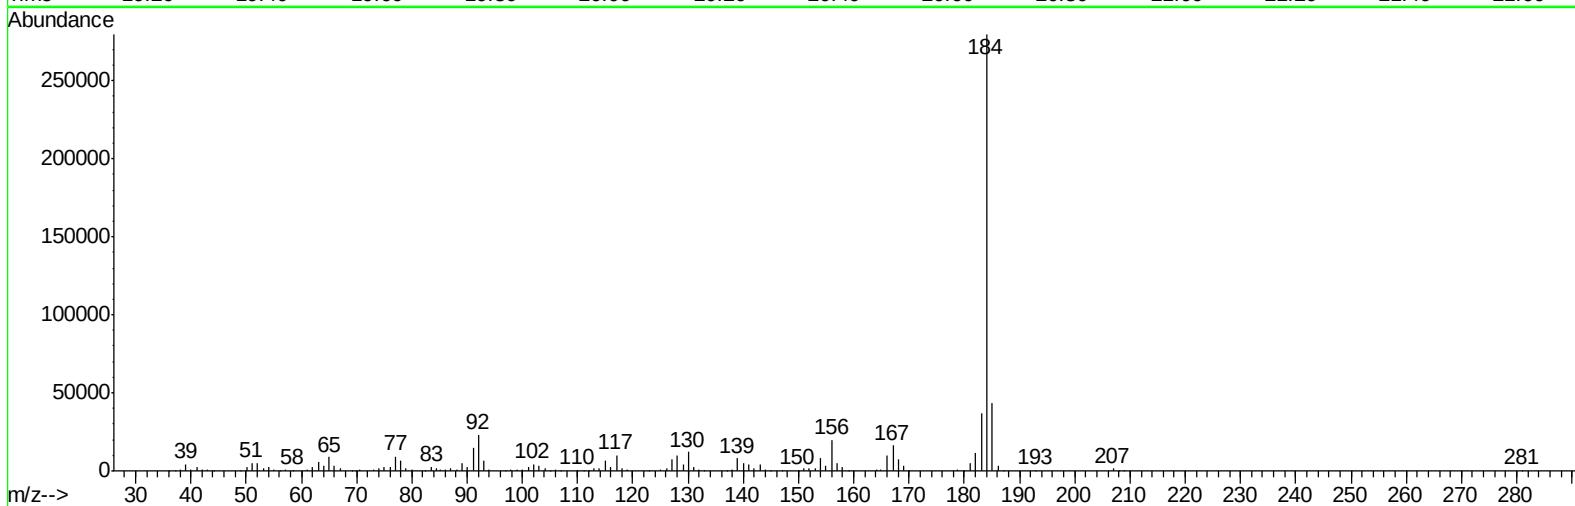


Data Path : Z:\HPCHEM1\BNA G\Data\BG022818\
Data File : BG032906.D
Acq On : 1 Mar 2018 4:00
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 01 08:45:45 2018
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG022118.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Feb 26 17:50:45 2018
Response via : Initial Calibration

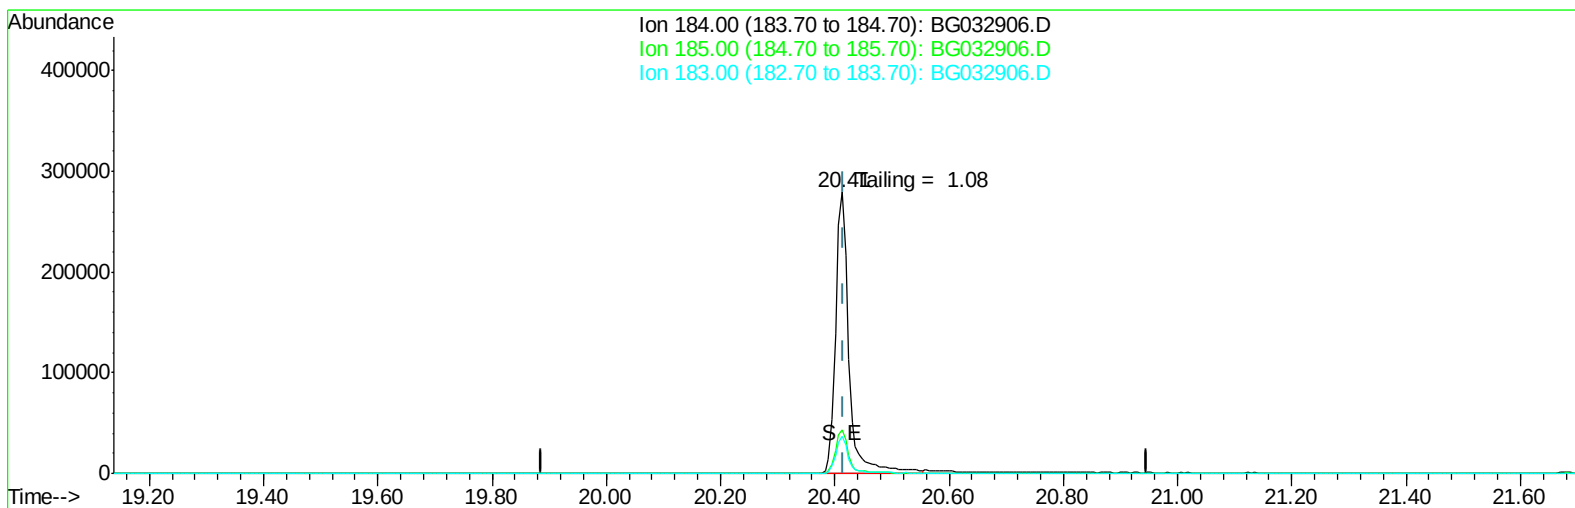

TIC: BG032906.D

(76) Benzidine



20.413min (-0.004) 0.00ng

response 449805

Ion	Exp%	Act%
184.00	100	100
185.00	13.90	15.52
183.00	13.30	13.10
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA G\Data\BG022818\
Data File : BG032906.D
Acq On : 1 Mar 2018 4:00
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 01 08:45:45 2018
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG022118.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Feb 26 17:50:45 2018
Response via : Initial Calibration

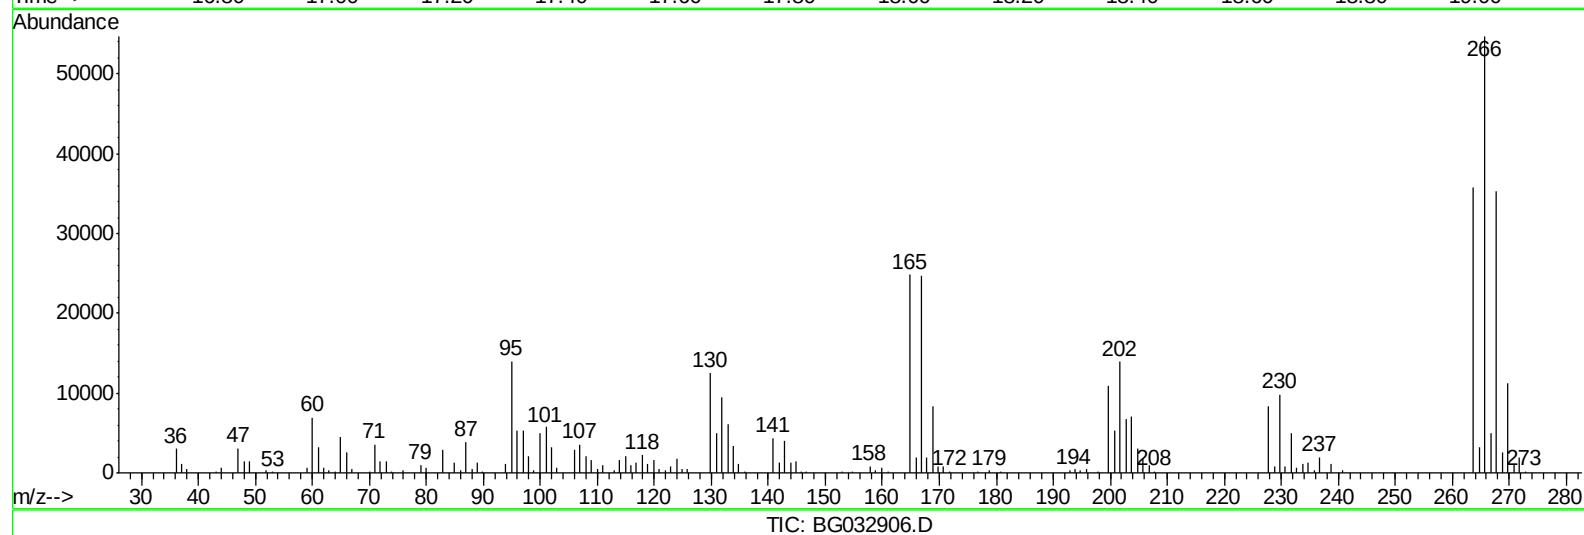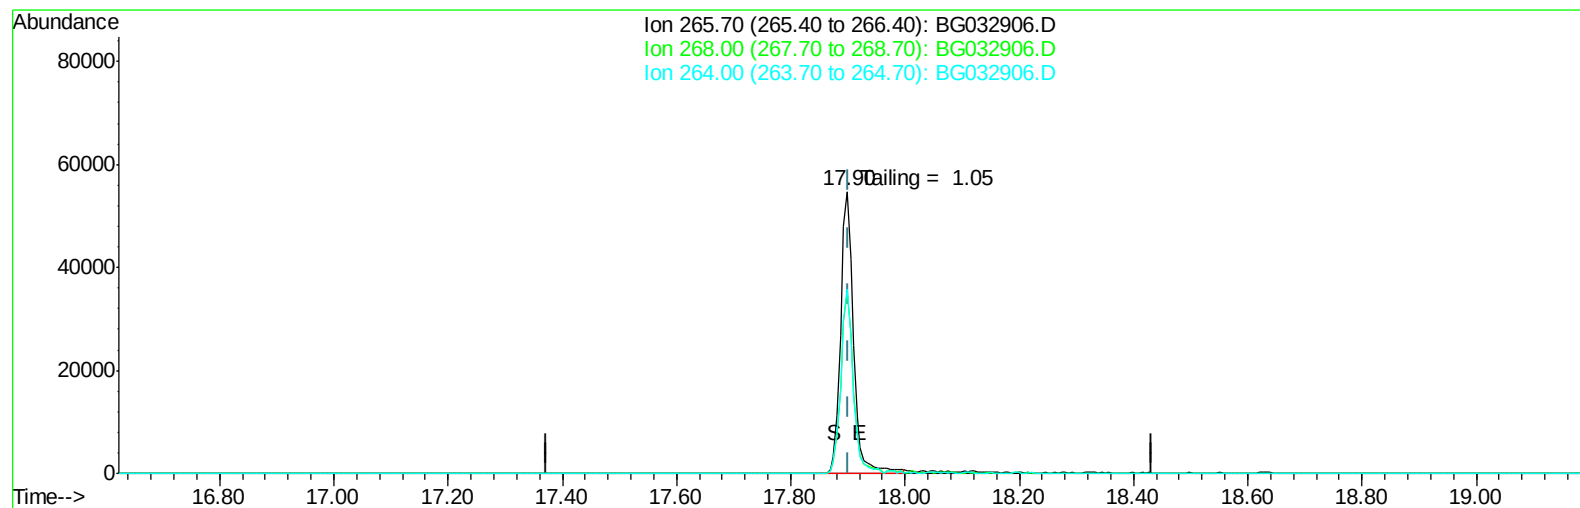

(69) Pentachlorophenol (C)

17.898min (-0.004) 19423.73ng

response 85839

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	64.58
264.00	62.00	65.27
0.00	0.00	0.00