

Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA G\DATA\BG022818\
 Data File : BG032890.D
 Acq On : 28 Feb 2018 16:41
 Operator : SJ/JU
 Sample : J1399-10
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 OR-03-022718-A

Quant Time: Mar 01 02:24:48 2018
 Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG022118.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Feb 26 17:50:45 2018
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.92	152	78218	20.00	ng	0.00
21) Naphthalene-d8	11.81	136	342608	20.00	ng	0.00
38) Acenaphthene-d10	15.54	164	193273	20.00	ng	0.00
63) Phenanthrene-d10	18.26	188	425006	20.00	ng	0.00
75) Chrysene-d12	22.62	240	384769	20.00	ng	-0.01
86) Perylene-d12	26.43	264	367140	20.00	ng	-0.01
System Monitoring Compounds						
5) 2-Fluorophenol	6.34	112	685387	140.19	ng	0.00
7) Phenol-d6	8.02	99	811983	119.15	ng	0.00
23) Nitrobenzene-d5	10.12	82	587931	115.11	ng	0.00
41) 2,4,6-Tribromophenol	17.00	330	315727	155.36	ng	0.00
44) 2-Fluorobiphenyl	14.17	172	1219515	91.00	ng	0.00
78) Terphenyl-d14	20.78	244	1736874	101.42	ng	0.00
Target Compounds						
31) Naphthalene	11.86	128	46733	2.610	ng	Qvalue 99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA G\DATA\BG022818\
Data File : BG032890.D
Acq On : 28 Feb 2018 16:41
Operator : SJ/JU
Sample : J1399-10
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
OR-03-022718-A

Quant Time: Mar 01 02:24:48 2018
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG022118.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Feb 26 17:50:45 2018
Response via : Initial Calibration

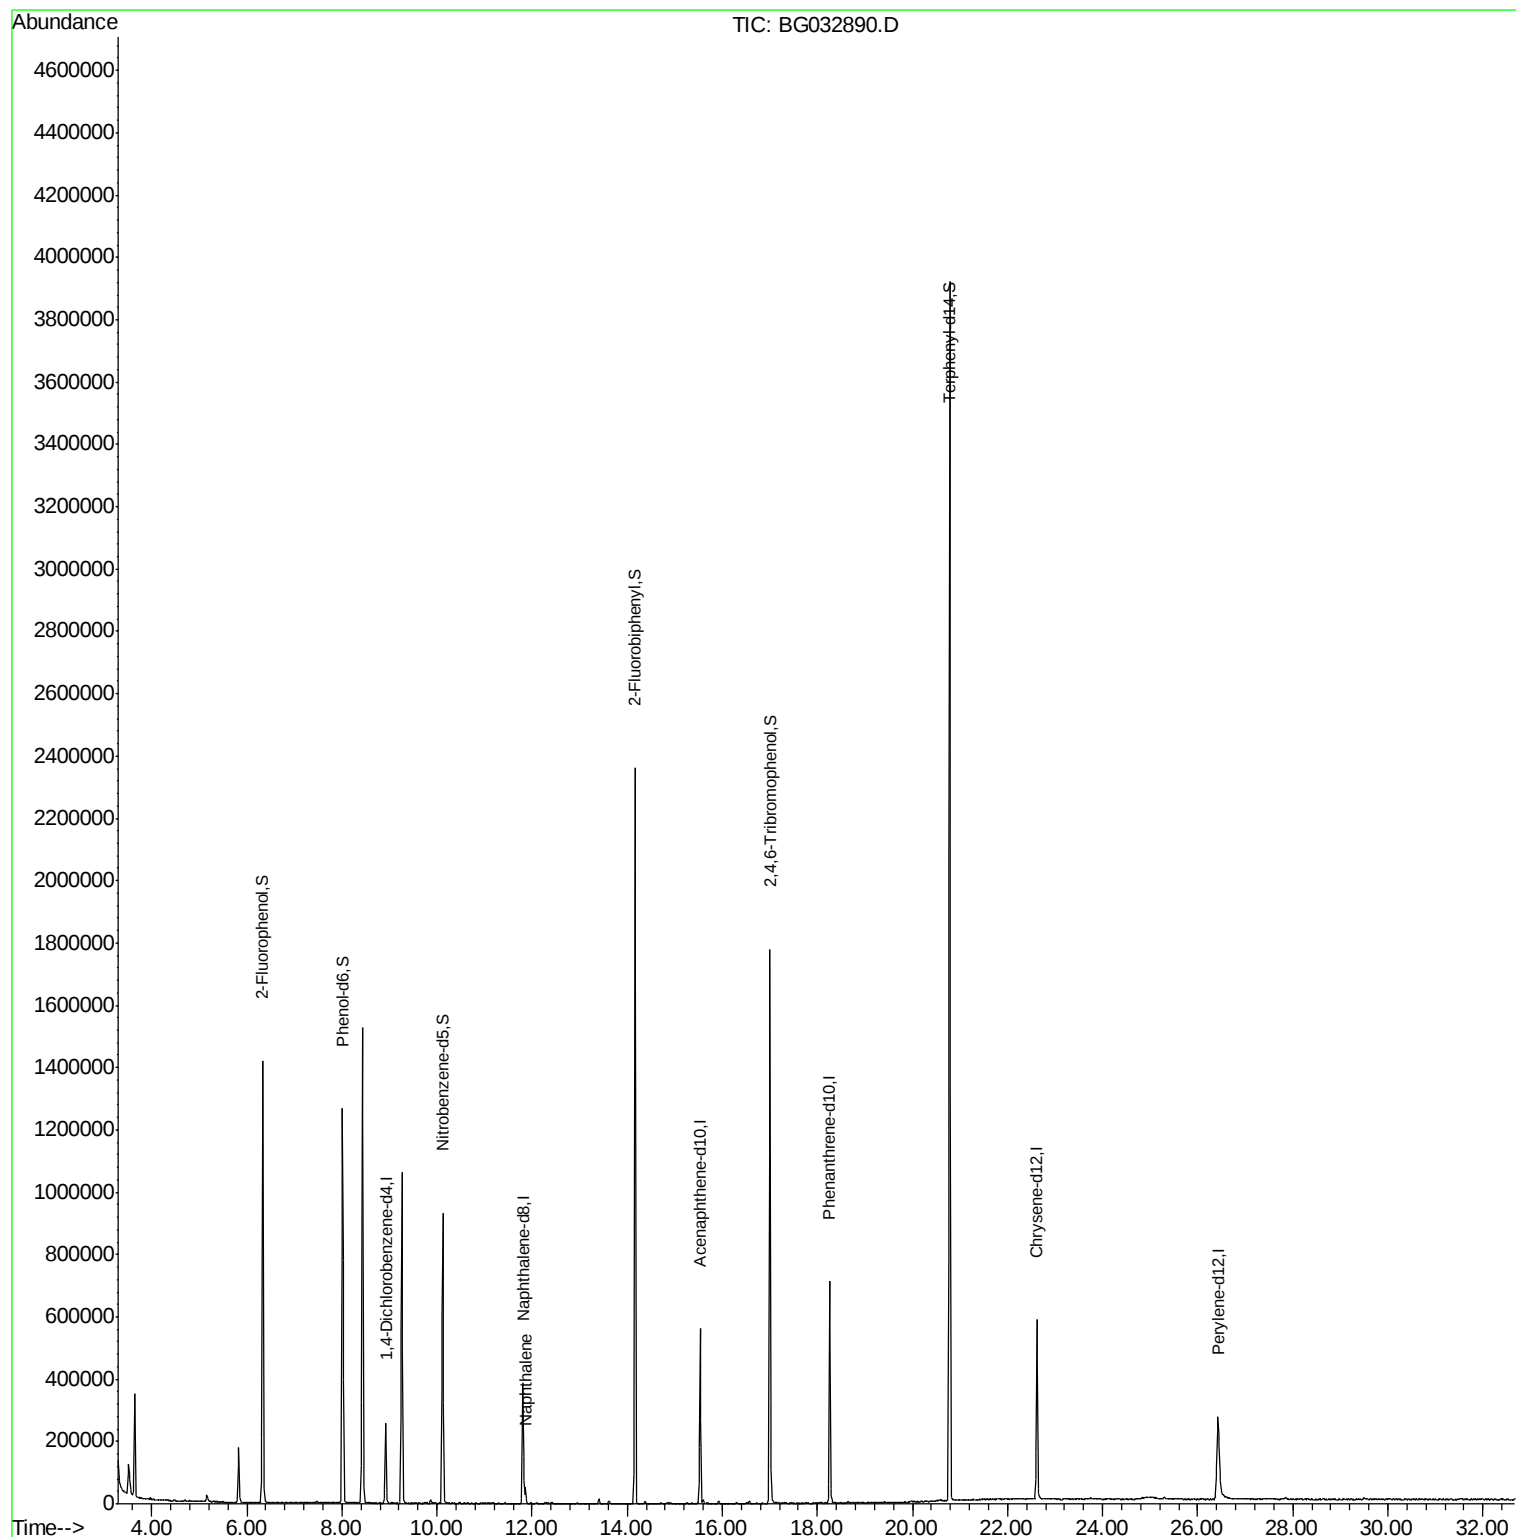

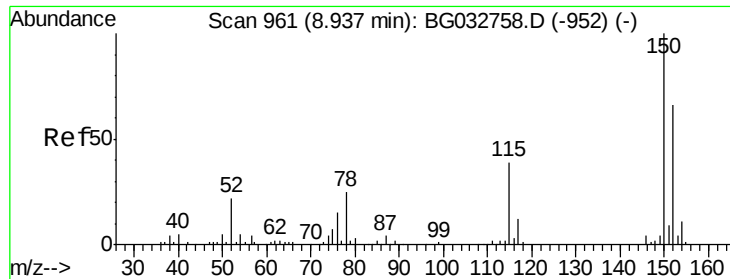


#1




1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 8.92 min Scan# 959
Delta R.T. -0.00 min
Lab File: BG032890.D
Acq: 28 Feb 2018 16:41

Instrument :
BNA_G
ClientSampleId :
OR-03-022718-A

Tot Ion:152 Resp: 78218
Ion Ratio Lower Upper
152 100
150 152.9 126.6 189.8
115 62.3 53.0 79.4

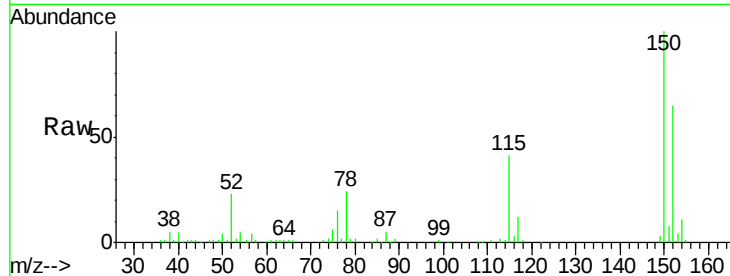


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

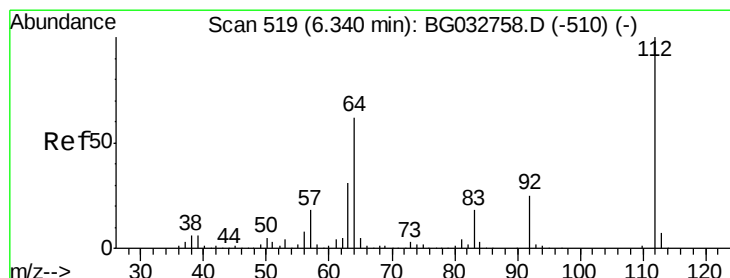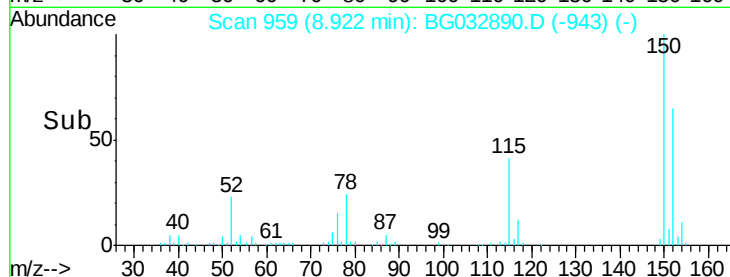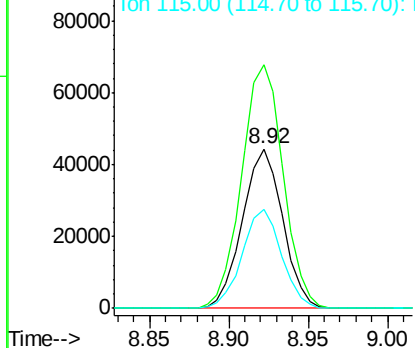



#5

2-Fluorophenol
Concen: 140.188 ng
RT: 6.34 min Scan# 519
Delta R.T. 0.00 min
Lab File: BG032890.D
Acq: 28 Feb 2018 16:41

Tgt Ion:112 Resp: 685387
Ion Ratio Lower Upper
112 100
64 64.9 56.3 84.5
63 32.2 30.1 45.1

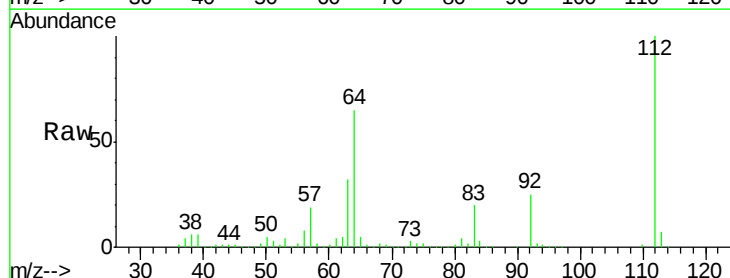

Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BGC
Ion 63.00 (62.70 to 63.70): BGC

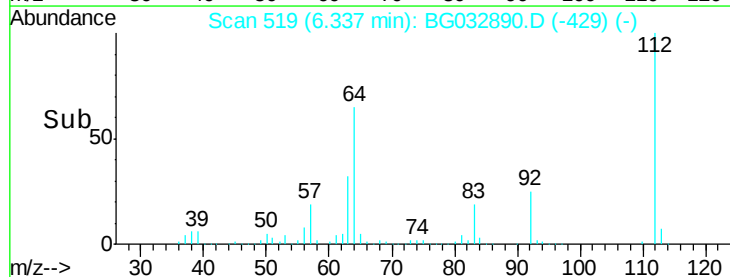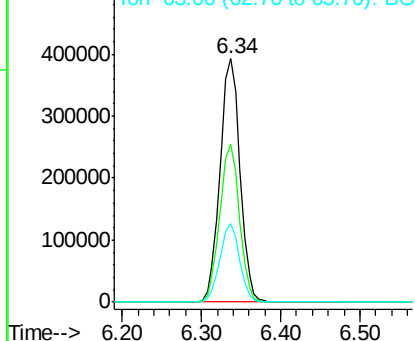



#7

Phenol-d6

Concen: 119.152 ng

RT: 8.02 min Scan# 805

Delta R.T. 0.00 min

Lab File: BG032890.D

Acq: 28 Feb 2018 16:41

Instrument :

BNA_G

ClientSampleId :

OR-03-022718-A


Tot Ion: 99 Resp: 811983

Ion Ratio Lower Upper



99 100

42 19.7 14.1 21.1

71 31.7 26.1 39.1

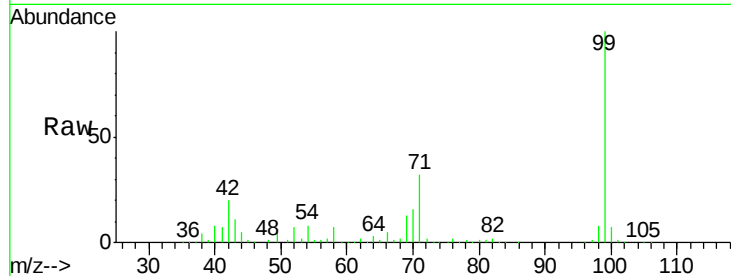

Abundance Ion 99.00 (98.70 to 99.70): BGC
Ion 42.00 (41.70 to 42.70): BGC
Ion 71.00 (70.70 to 71.70): BGC

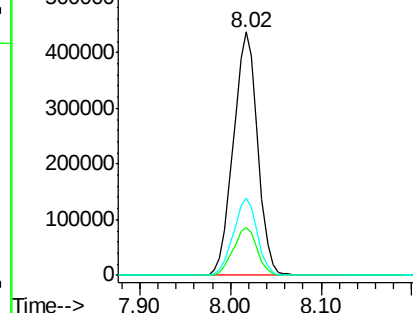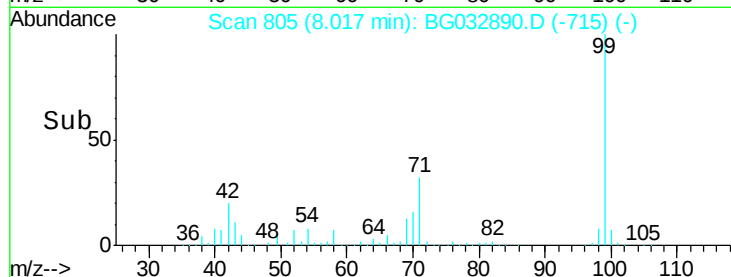

#21

Naphthalene-d8

Concen: 20.000 ng

RT: 11.81 min Scan# 1450

Delta R.T. -0.00 min

Lab File: BG032890.D

Acq: 28 Feb 2018 16:41

Tgt Ion: 136 Resp: 342608


Ion Ratio Lower Upper

136 100



137 11.6 9.2 13.8

54 9.8 10.3 15.5#

68 6.3 4.5 6.7



Abundance Ion 136.00 (135.70 to 136.70): BGC
Ion 137.00 (136.70 to 137.70): BGC
Ion 54.00 (53.70 to 54.70): BGC
Ion 68.00 (67.70 to 68.70): BGC



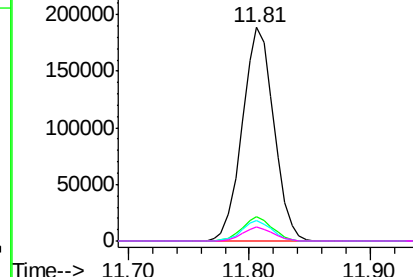
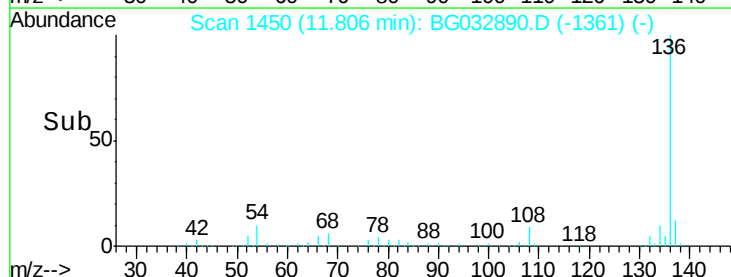




#23
 Nitrobenzene-d5
 Concen: 115.110 ng
 RT: 10.12 min Scan# 1163
 Delta R.T. -0.00 min
 Lab File: BG032890.D
 Acq: 28 Feb 2018 16:41




Instrument :
 BNA_G
 ClientSampleId :
 OR-03-022718-A

Tot Ion	82	Resp	587931
Ion Ratio	Lower	Upper	
82	100		
128	46.4	29.7	44.5#
54	54.8	43.1	64.7

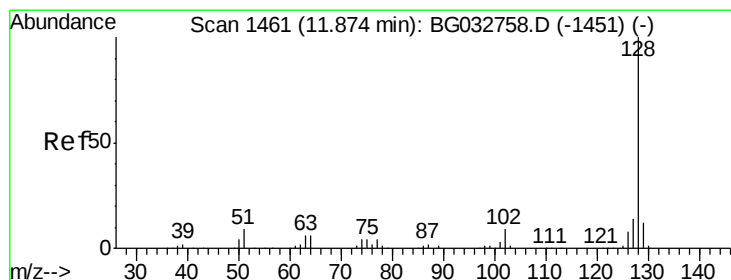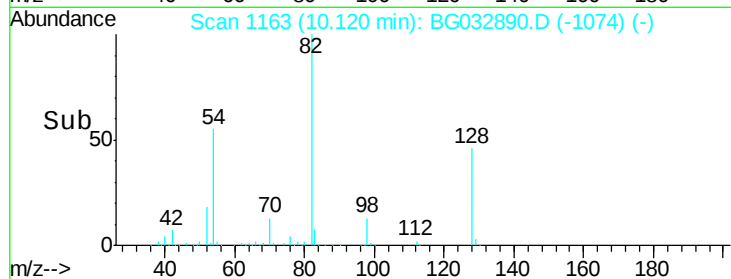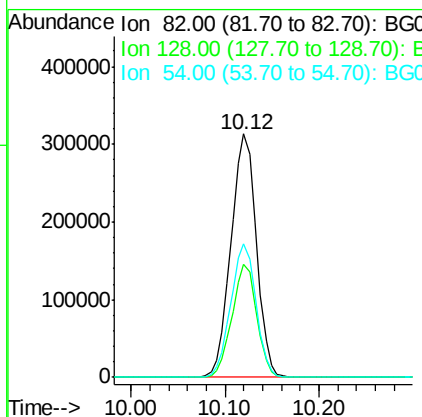

#31
 Naphthalene
 Concen: 2.610 ng
 RT: 11.86 min Scan# 1459
 Delta R.T. -0.00 min
 Lab File: BG032890.D
 Acq: 28 Feb 2018 16:41

Tgt Ion	128	Resp	46733
Ion Ratio <td>Lower</td> <td>Upper</td> <td></td>	Lower	Upper	
128	100		
129	9.8	8.6	12.8
127	14.3	11.6	17.4

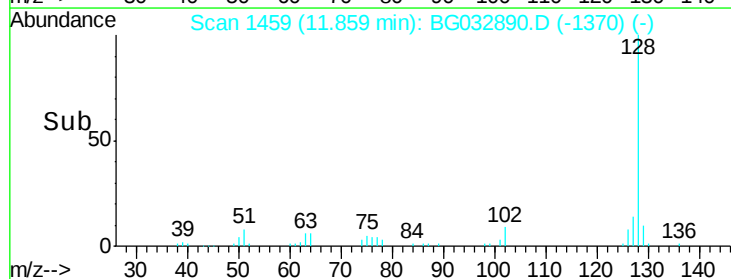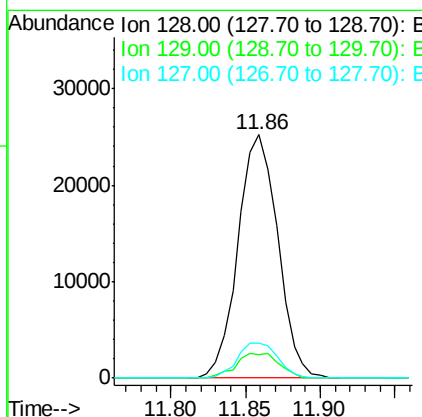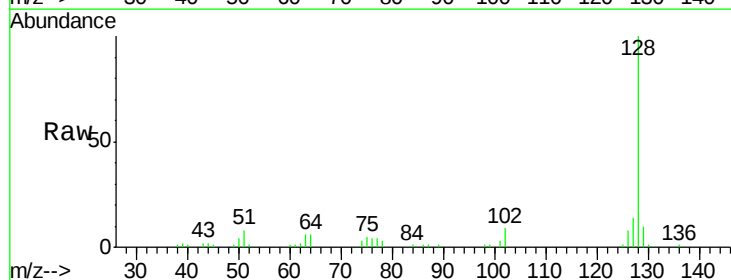



#38

Acenaphthene-d10

Concen: 20.000 ng

RT: 15.54 min Scan# 2085

Delta R.T. -0.00 min

Lab File: BG032890.D

Acq: 28 Feb 2018 16:41

Instrument :

BNA_G

ClientSampleId :

OR-03-022718-A


Tot Ion:164 Resp: 193273

Ion Ratio Lower Upper

164 100

162 105.6 78.8 118.2




160 48.0 35.4 53.0

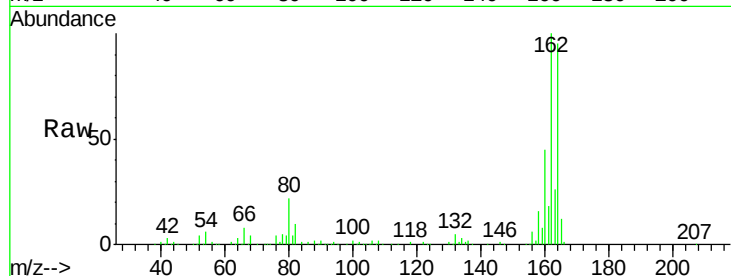

Abundance Ion 164.00 (163.70 to 164.70): E

Ion 162.00 (161.70 to 162.70): E

Ion 160.00 (159.70 to 160.70): E

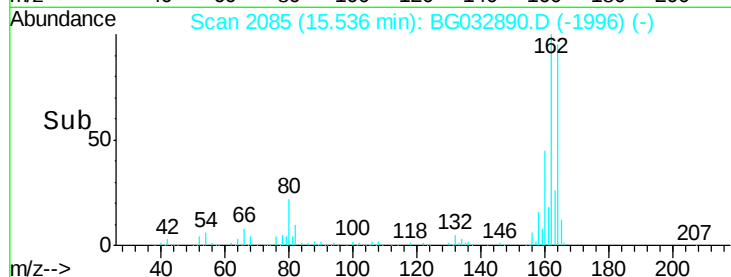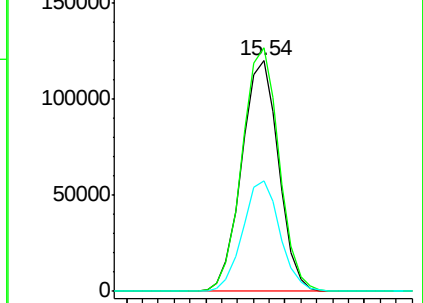

#41

2,4,6-Tribromophenol

Concen: 155.362 ng

RT: 17.00 min Scan# 2335

Delta R.T. -0.00 min

Lab File: BG032890.D

Acq: 28 Feb 2018 16:41


Tgt Ion:330 Resp: 315727

Ion Ratio Lower Upper

330 100

332 96.3 77.0 115.6



141 44.3 25.2 37.8#




Abundance Ion 329.80 (329.50 to 330.50): E

Ion 331.80 (331.50 to 332.50): E

Ion 141.00 (140.70 to 141.70): E

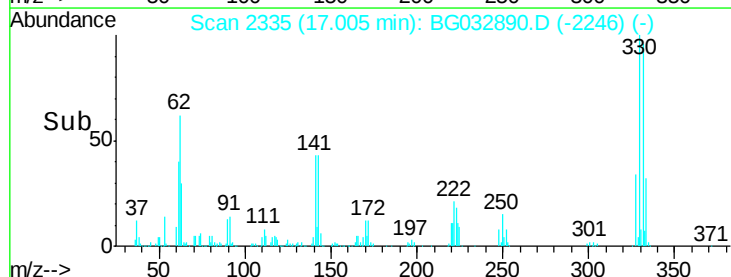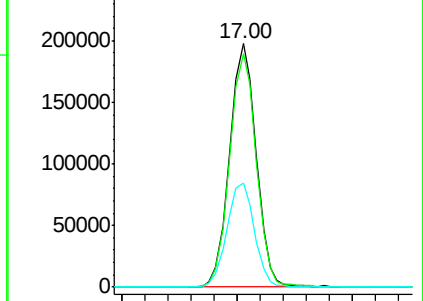

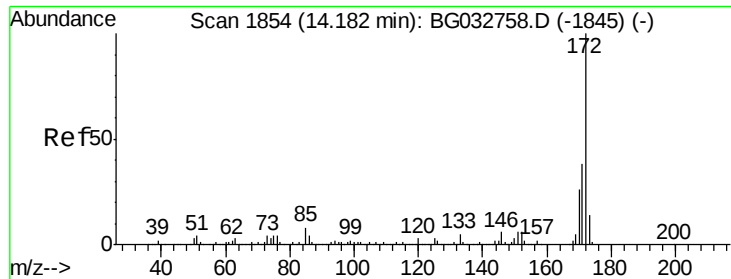


#44
 2-Fluorobiphenyl
 Concen: 91.003 ng
 RT: 14.17 min Scan# 1852
 Delta R.T. -0.00 min
 Lab File: BG032890.D
 Acq: 28 Feb 2018 16:41




Instrument :
 BNA_G
 ClientSampleId :
 OR-03-022718-A

Tot Ion:172 Resp: 1219515

Ion	Ratio	Lower	Upper
172	100		
171	39.5	30.0	45.0
170	26.8	19.5	29.3

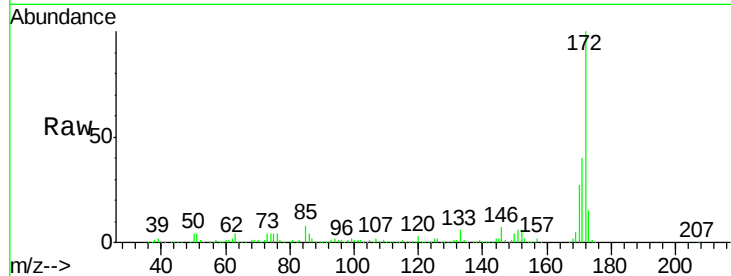


Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E

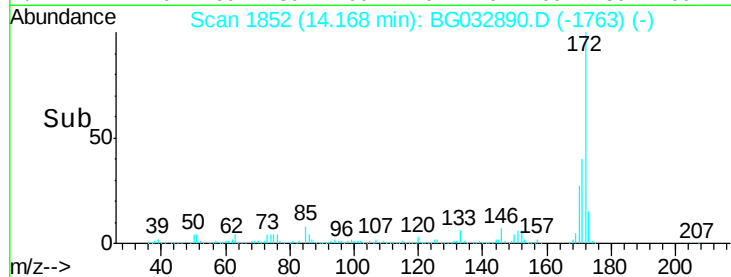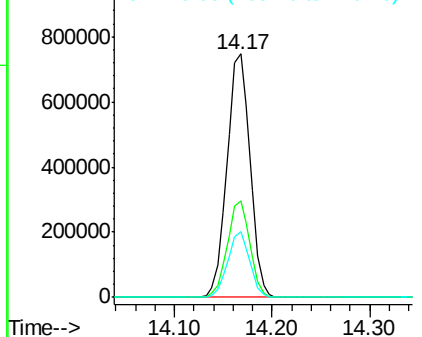



#63
 Phenanthrene-d10
 Concen: 20.000 ng
 RT: 18.26 min Scan# 2549
 Delta R.T. -0.00 min
 Lab File: BG032890.D
 Acq: 28 Feb 2018 16:41

Tgt Ion:188 Resp: 425006

Ion	Ratio	Lower	Upper
188	100		
94	9.7	6.9	10.3
80	11.4	7.7	11.5



Abundance Ion 188.00 (187.70 to 188.70): E
 Ion 94.00 (93.70 to 94.70): BGC
 Ion 80.00 (79.70 to 80.70): BGC

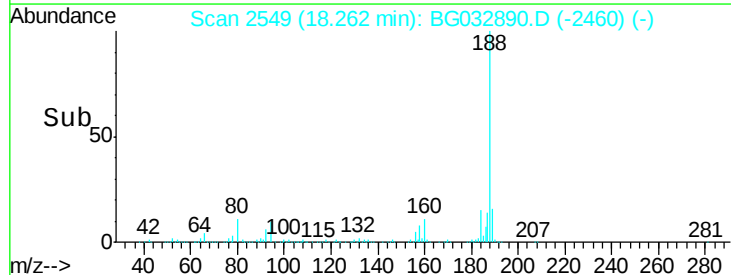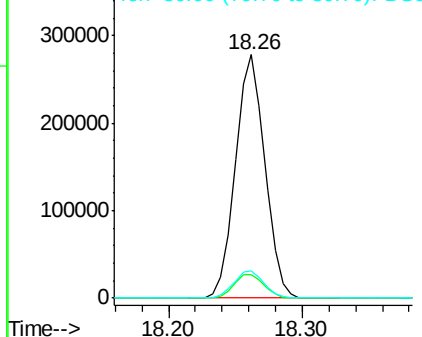



#75

Chrysene-d12

Concen: 20.000 ng

RT: 22.62 min Scan# 3291

Delta R.T. -0.01 min

Lab File: BG032890.D

Acq: 28 Feb 2018 16:41

Instrument :

BNA_G

ClientSampleId :

OR-03-022718-A


Tot Ion:240 Resp: 384769

Ion Ratio Lower Upper

240 100

120 12.7 6.8 10.2#




236 27.6 20.9 31.3



Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

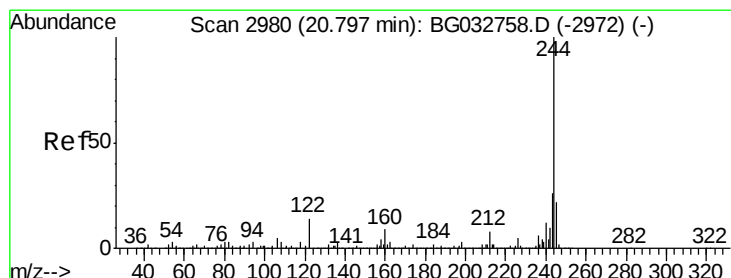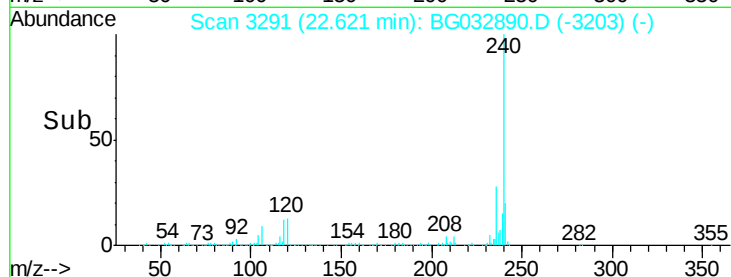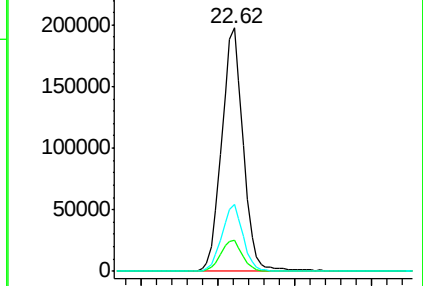

#78

Terphenyl-d14

Concen: 101.419 ng

RT: 20.78 min Scan# 2978

Delta R.T. -0.00 min

Lab File: BG032890.D

Acq: 28 Feb 2018 16:41


Tgt Ion:244 Resp: 1736874

Ion Ratio Lower Upper

244 100

212 8.8 5.8 8.8#



122 14.9 7.0 10.4#






Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

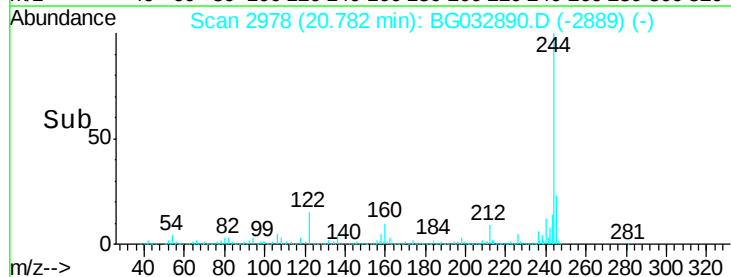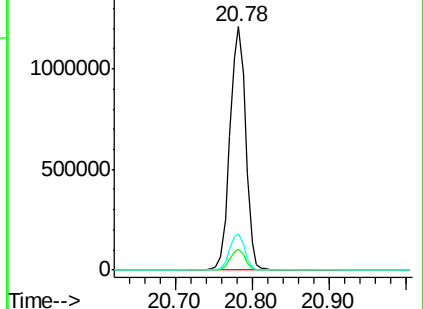

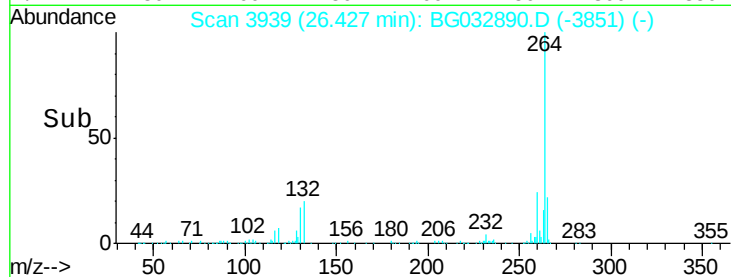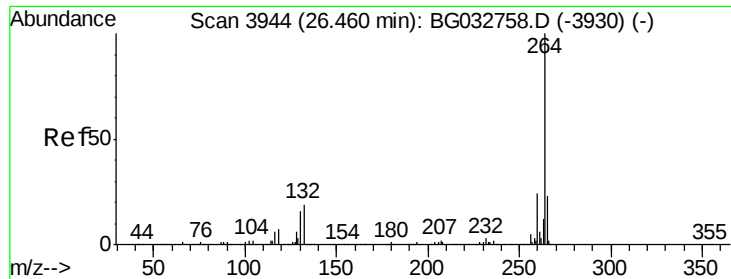

#86

Pervlene-d12

Concen: 20.000 ng

RT: 26.43 min Scan# 3939

Delta R.T. -0.01 min

Lab File: BG032890.D

Acq: 28 Feb 2018 16:41

Instrument :

BNA_G

ClientSampleId :

OR-03-022718-A

Tot Ion:264 Resp: 367140

Ion Ratio Lower Upper

264 100

260 23.9 17.4 26.0

265 21.8 17.7 26.5

