

Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA G\DATA\BG022818\
 Data File : BG032900.D
 Acq On : 28 Feb 2018 22:59
 Operator : SJ/JU
 Sample : J1699-24
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 B2

Quant Time: Mar 01 02:43:36 2018
 Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG022118.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Feb 26 17:50:45 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.92	152	74778	20.00	ng	0.00
21) Naphthalene-d8	11.81	136	334691	20.00	ng	0.00
38) Acenaphthene-d10	15.54	164	187419	20.00	ng	0.00
63) Phenanthrene-d10	18.26	188	406025	20.00	ng	0.00
75) Chrysene-d12	22.62	240	365407	20.00	ng	-0.01
86) Perylene-d12	26.44	264	354005	20.00	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	6.34	112	632958	135.42	ng	0.00
7) Phenol-d6	8.02	99	759407	116.56	ng	0.00
23) Nitrobenzene-d5	10.12	82	532823	107.51	ng	0.00
41) 2,4,6-Tribromophenol	17.00	330	278771	141.46	ng	0.00
44) 2-Fluorobiphenyl	14.17	172	1129958	86.95	ng	0.00
78) Terphenyl-d14	20.78	244	1569286	96.49	ng	0.00


Target Compounds Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA G\DATA\BG022818\
Data File : BG032900.D
Acq On : 28 Feb 2018 22:59
Operator : SJ/JU
Sample : J1699-24
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
B2

Quant Time: Mar 01 02:43:36 2018
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG022118.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Feb 26 17:50:45 2018
Response via : Initial Calibration

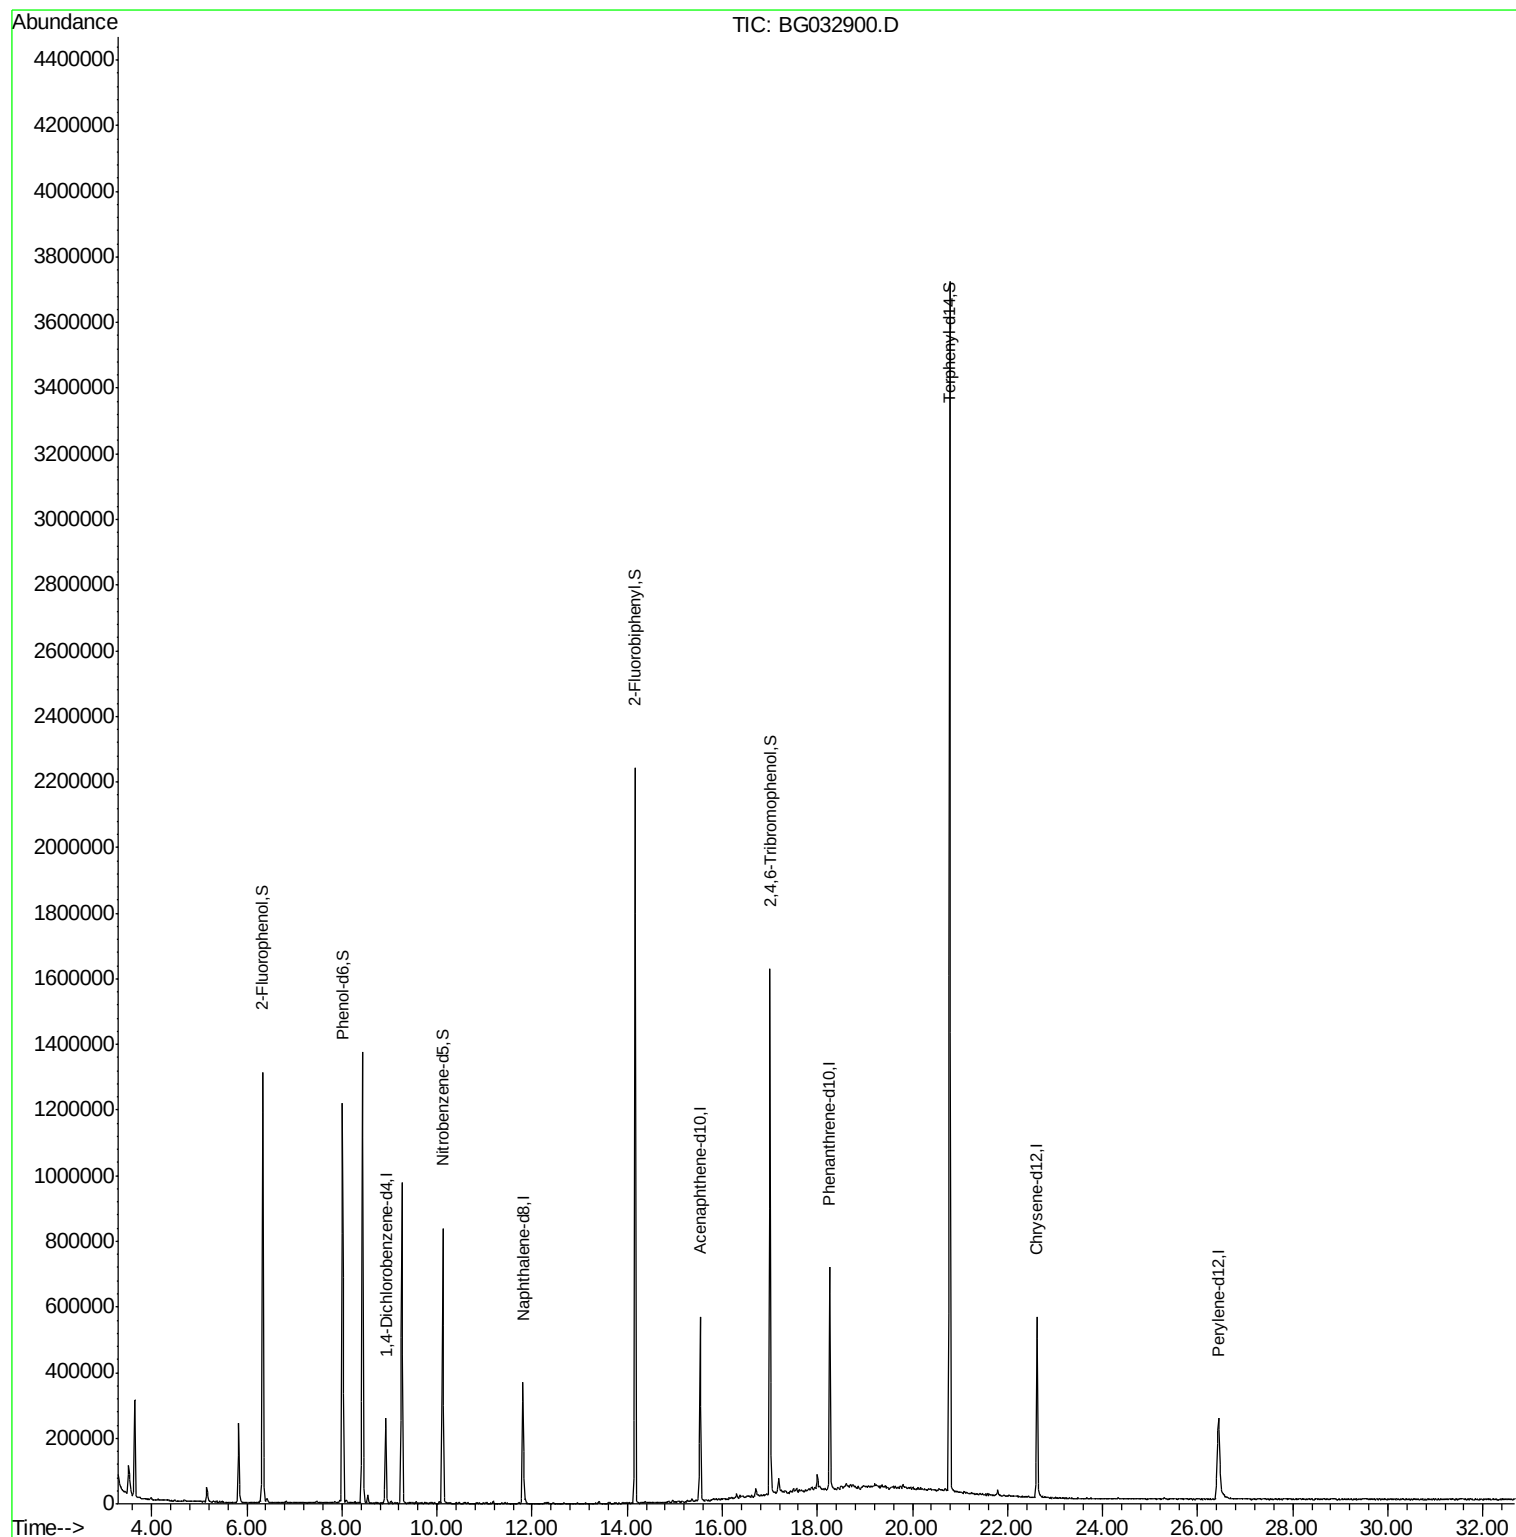




#1




1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 8.92 min Scan# 959
Delta R.T. -0.01 min
Lab File: BG032900.D
Acq: 28 Feb 2018 22:59

Instrument :
BNA_G
ClientSampled :
B2

Tot Ion:152 Resp: 74778
Ion Ratio Lower Upper
152 100
150 159.4 126.6 189.8
115 60.4 53.0 79.4

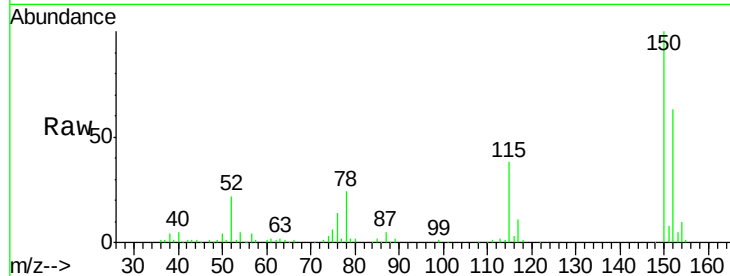


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

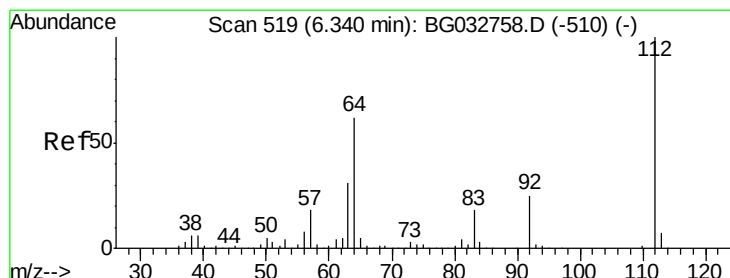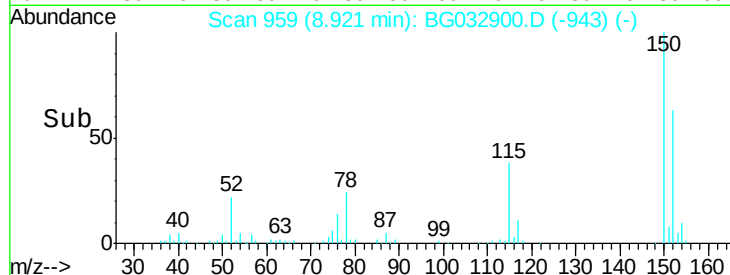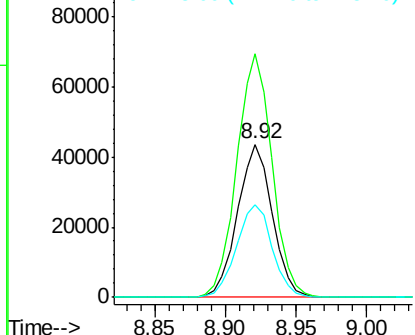



#5


2-Fluorophenol
Concen: 135.420 ng
RT: 6.34 min Scan# 519
Delta R.T. 0.00 min
Lab File: BG032900.D
Acq: 28 Feb 2018 22:59

Tgt Ion:112 Resp: 632958
Ion Ratio Lower Upper
112 100
64 65.3 56.3 84.5
63 32.3 30.1 45.1

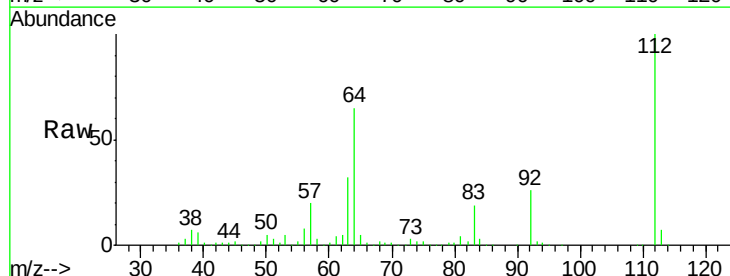

Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BGC
Ion 63.00 (62.70 to 63.70): BGC

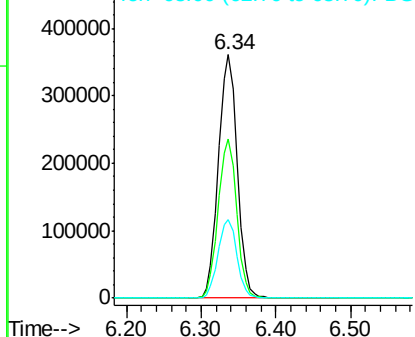

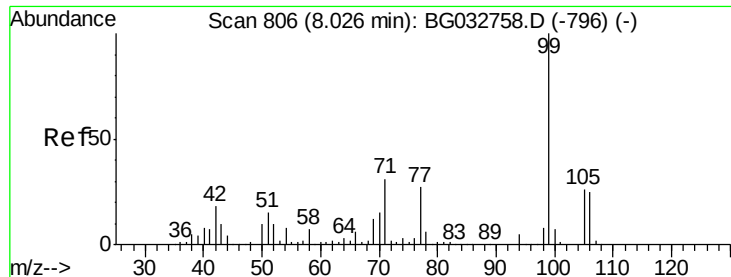

#7

Phenol-d6

Concen: 116.563 ng

RT: 8.02 min Scan# 805

Delta R.T. 0.00 min

Lab File: BG032900.D

Acq: 28 Feb 2018 22:59

Instrument :

BNA_G

ClientSampled :

B2


Tot Ion: 99 Resp: 759407

Ion Ratio Lower Upper




99 100

42 19.7 14.1 21.1

71 32.6 26.1 39.1

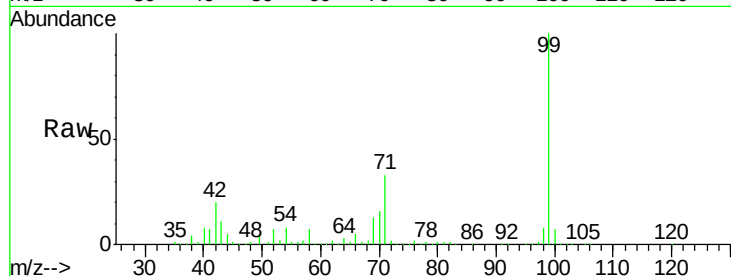

Abundance Ion 99.00 (98.70 to 99.70): BGC
Ion 42.00 (41.70 to 42.70): BGC
Ion 71.00 (70.70 to 71.70): BGC

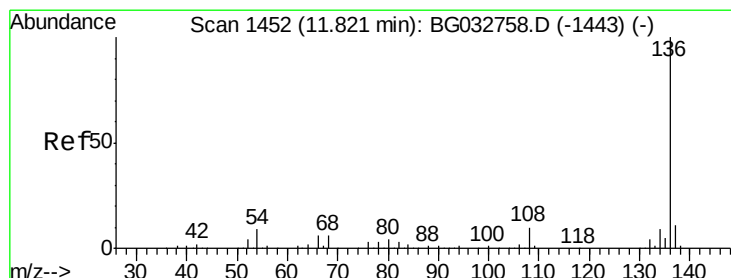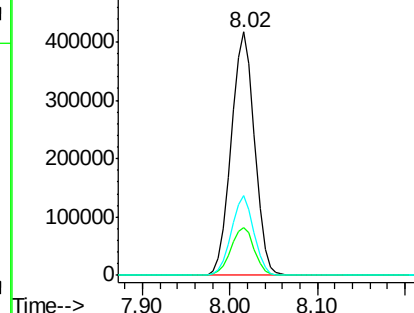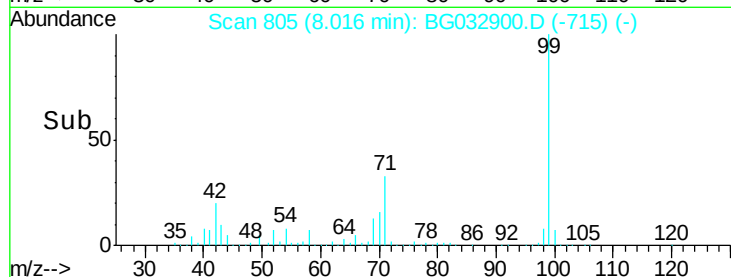

#21

Naphthalene-d8

Concen: 20.000 ng

RT: 11.81 min Scan# 1450

Delta R.T. -0.01 min

Lab File: BG032900.D

Acq: 28 Feb 2018 22:59

Tgt Ion: 136 Resp: 334691


Ion Ratio Lower Upper

136 100



137 11.0 9.2 13.8


54 9.6 10.3 15.5#

68 6.0 4.5 6.7

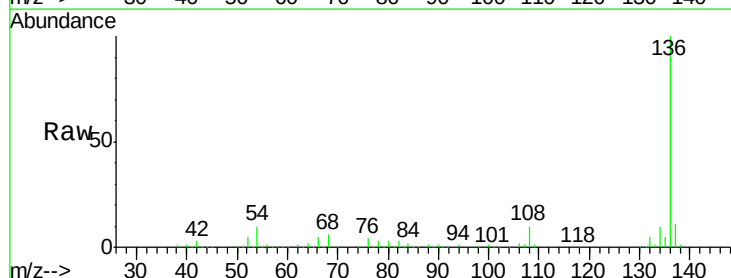

Abundance Ion 136.00 (135.70 to 136.70): BGC
Ion 137.00 (136.70 to 137.70): BGC
Ion 54.00 (53.70 to 54.70): BGC
Ion 68.00 (67.70 to 68.70): BGC



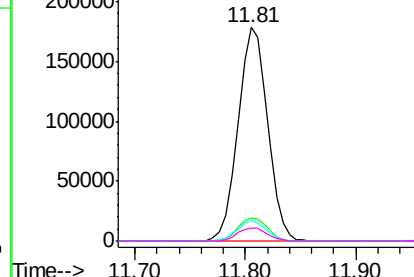
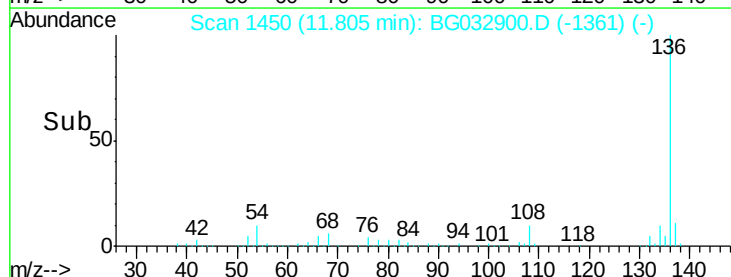


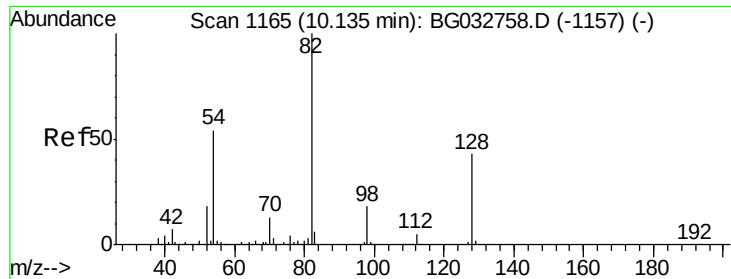

#23
Nitrobenzene-d5
Concen: 107.505 ng
RT: 10.12 min Scan# 1163
Delta R.T. -0.01 min
Lab File: BG032900.D
Acq: 28 Feb 2018 22:59




Instrument :
BNA_G
ClientSampleId :
B2


Tot Ion	82	Resp	532823
Ion Ratio	Lower	Upper	
82	100		
128	45.1	29.7	44.5#
54	54.3	43.1	64.7

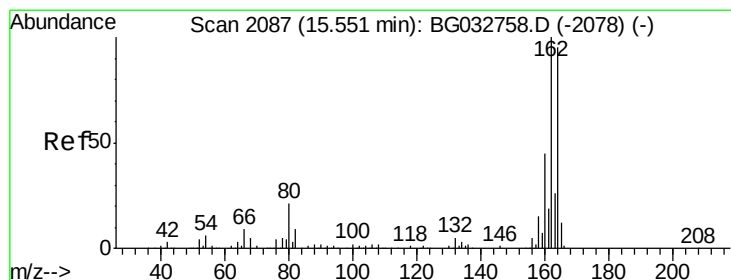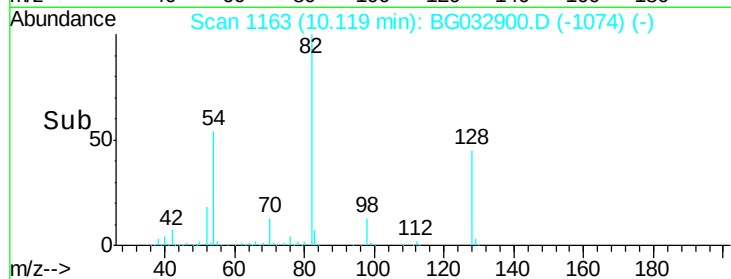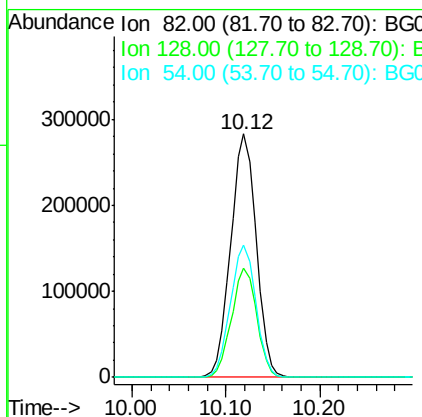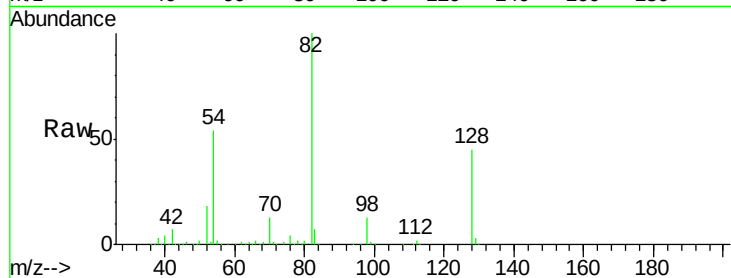

#38
Acenaphthene-d10
Concen: 20.000 ng
RT: 15.54 min Scan# 2085
Delta R.T. -0.01 min
Lab File: BG032900.D
Acq: 28 Feb 2018 22:59

Tgt Ion	164	Resp	187419
Ion Ratio	Lower	Upper	
164	100		
162	106.2	78.8	118.2
160	48.9	35.4	53.0

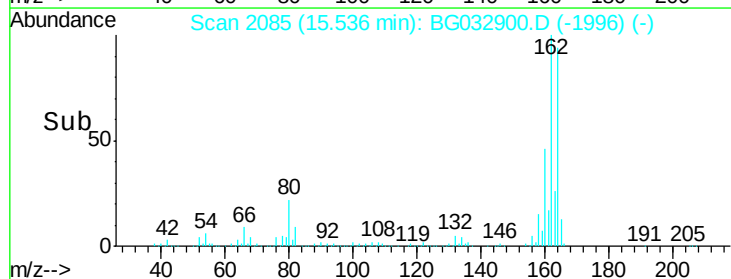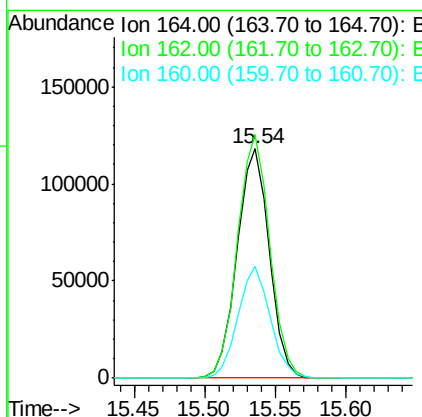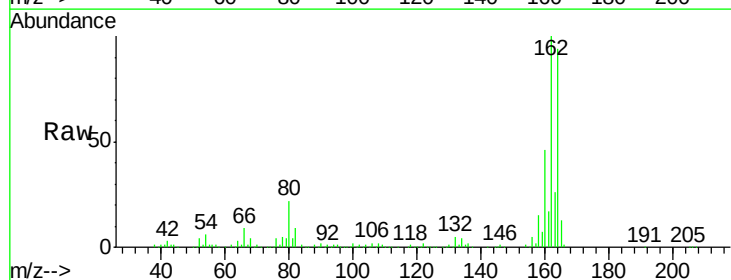







#41
 2,4,6-Tribromophenol
 Concen: 141.462 ng
 RT: 17.00 min Scan# 2335
 Delta R.T. -0.01 min
 Lab File: BG032900.D
 Acq: 28 Feb 2018 22:59

Instrument :
 BNA_G
 ClientSampled :
 B2

Tot Ion:330 Resp: 278771
 Ion Ratio Lower Upper
 330 100
 332 95.6 77.0 115.6
 141 44.8 25.2 37.8#

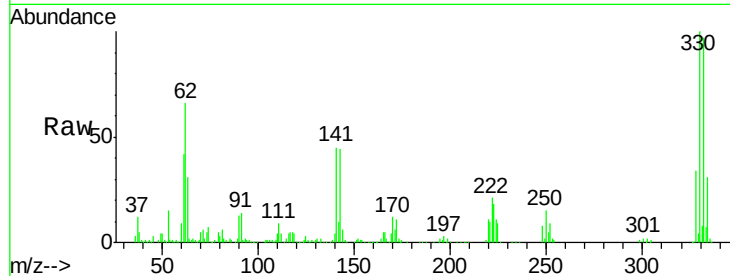


Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E

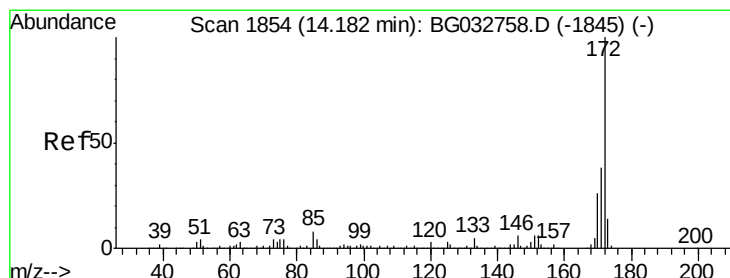
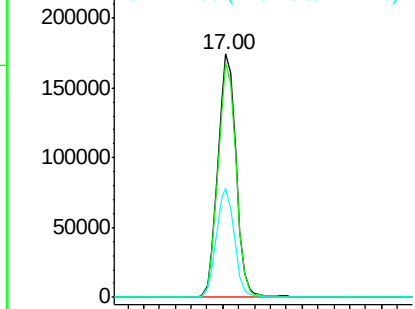



#44
 2-Fluorobiphenyl
 Concen: 86.954 ng
 RT: 14.17 min Scan# 1852
 Delta R.T. -0.01 min
 Lab File: BG032900.D
 Acq: 28 Feb 2018 22:59

Tgt Ion:172 Resp: 1129958
 Ion Ratio Lower Upper
 172 100
 171 39.5 30.0 45.0
 170 26.9 19.5 29.3

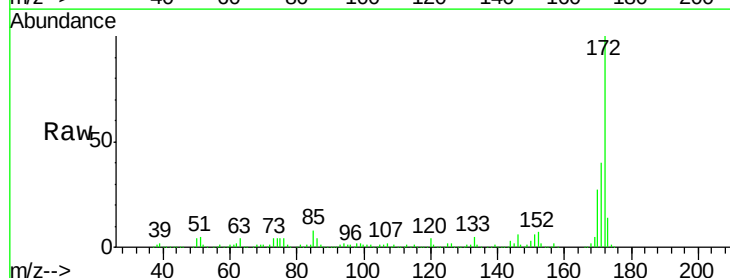

Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E

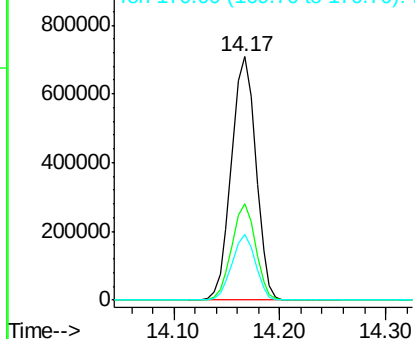



#63

Phenanthrene-d10

Concen: 20.000 ng

RT: 18.26 min Scan# 2549

Delta R.T. -0.01 min

Lab File: BG032900.D

Acq: 28 Feb 2018 22:59

Instrument :

BNA_G

ClientSampleId :

B2


Tot Ion:188 Resp: 406025

Ion Ratio Lower Upper

188 100

94 10.7 6.9 10.3#




80 12.1 7.7 11.5#

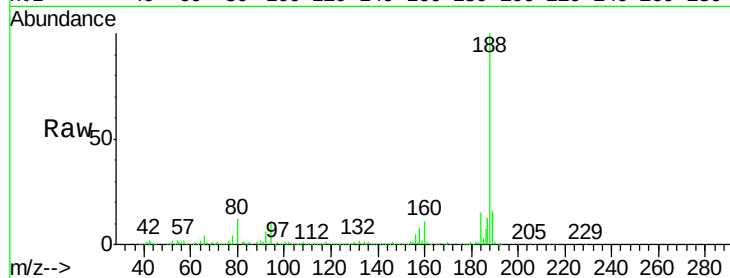

Abundance Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BGC

Ion 80.00 (79.70 to 80.70): BGC

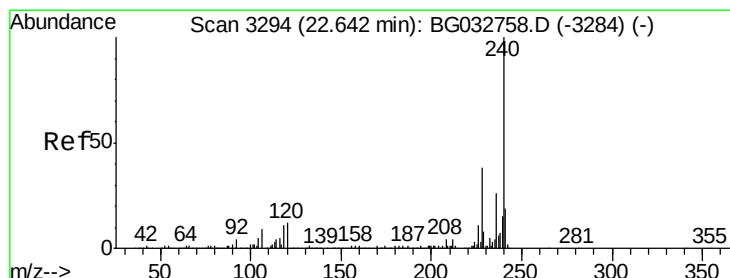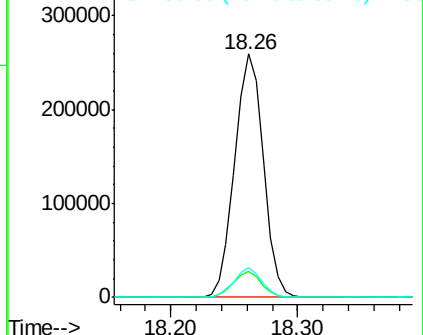

#75

Chrysene-d12

Concen: 20.000 ng

RT: 22.62 min Scan# 3291

Delta R.T. -0.01 min

Lab File: BG032900.D

Acq: 28 Feb 2018 22:59


Tgt Ion:240 Resp: 365407

Ion Ratio Lower Upper

240 100

120 12.9 6.8 10.2#



236 26.2 20.9 31.3

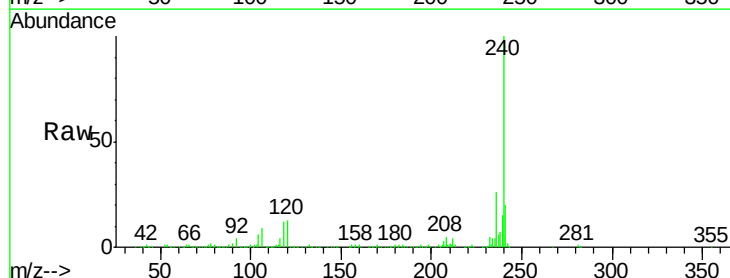


Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

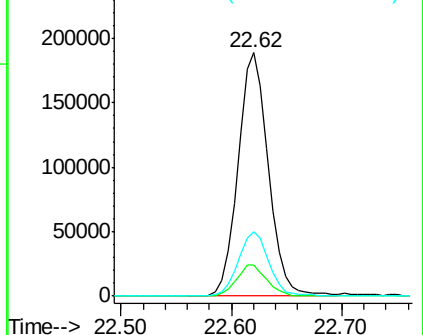



#78

Terphenyl-d14

Concen: 96.489 ng

RT: 20.78 min Scan# 2978

Delta R.T. -0.01 min

Lab File: BG032900.D

Acq: 28 Feb 2018 22:59

Instrument :

BNA_G

ClientSampleId :

B2


Tot Ion:244 Resp: 1569286

Ion Ratio Lower Upper

244 100

212 8.8 5.8 8.8#




122 14.7 7.0 10.4#

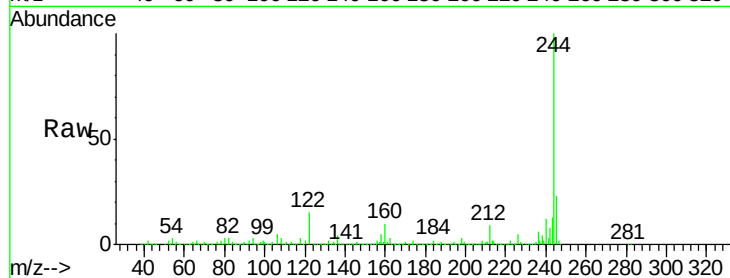

Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

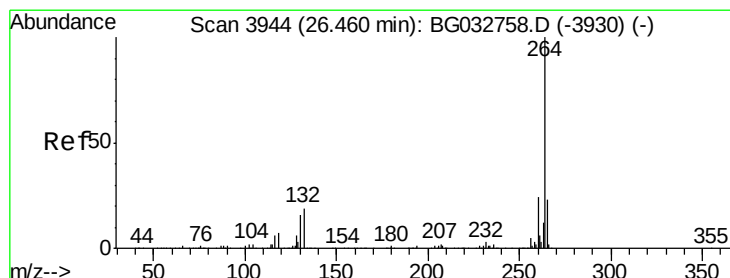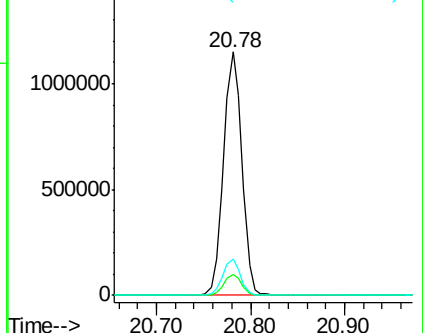

#86

Perylene-d12

Concen: 20.000 ng

RT: 26.44 min Scan# 3941

Delta R.T. 0.00 min

Lab File: BG032900.D

Acq: 28 Feb 2018 22:59


Tgt Ion:264 Resp: 354005

Ion Ratio Lower Upper

264 100

260 22.2 17.4 26.0

265 22.0 17.7 26.5

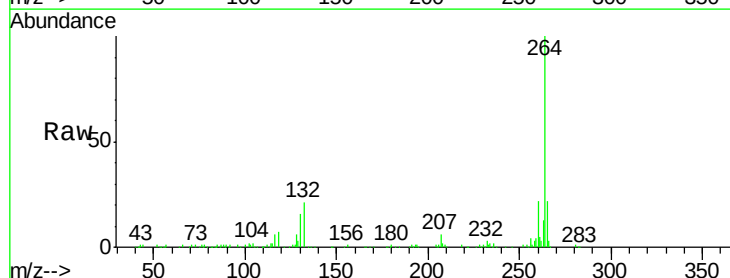

Abundance Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

