
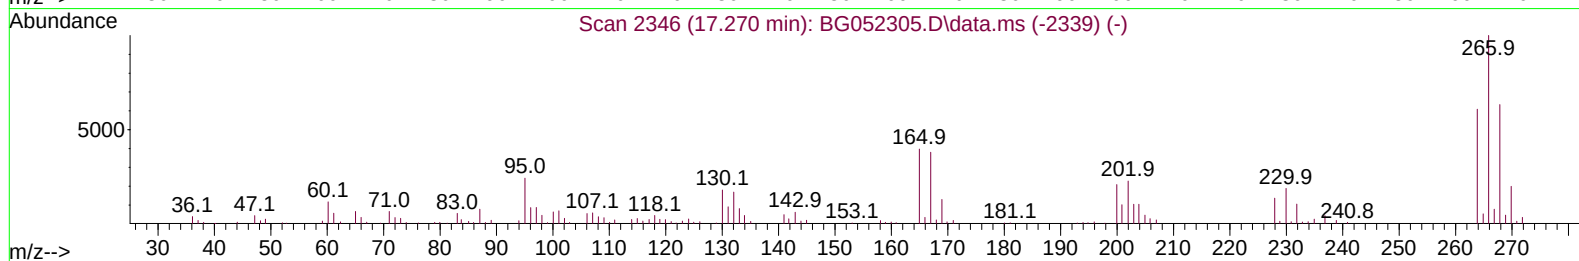
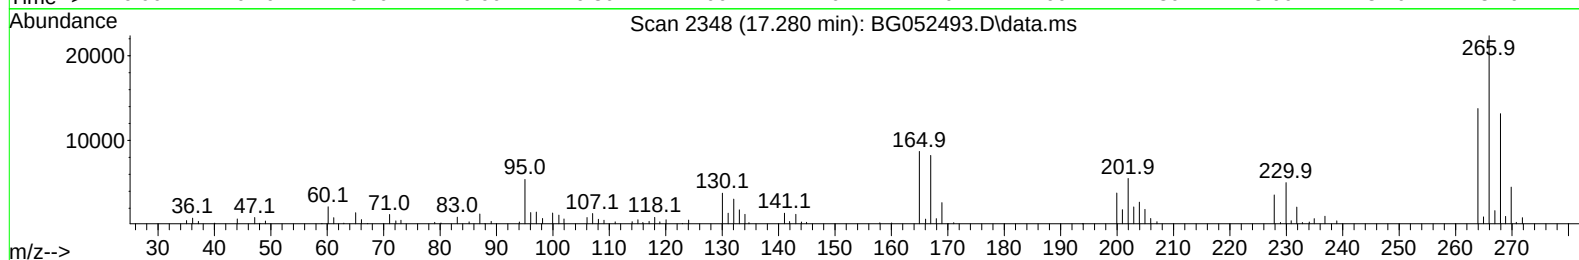


Data Path : Z:\svoasrv\HPCHEM1\BNA\_G\Data\BG022822\  
Data File : BG052493.D  
Acq On : 28 Feb 2022 9:38  
Operator : CG/JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 01 04:23:44 2022  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_G\Methods\8270-BG020722.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Tue Feb 08 01:21:20 2022  
Response via : Initial Calibration

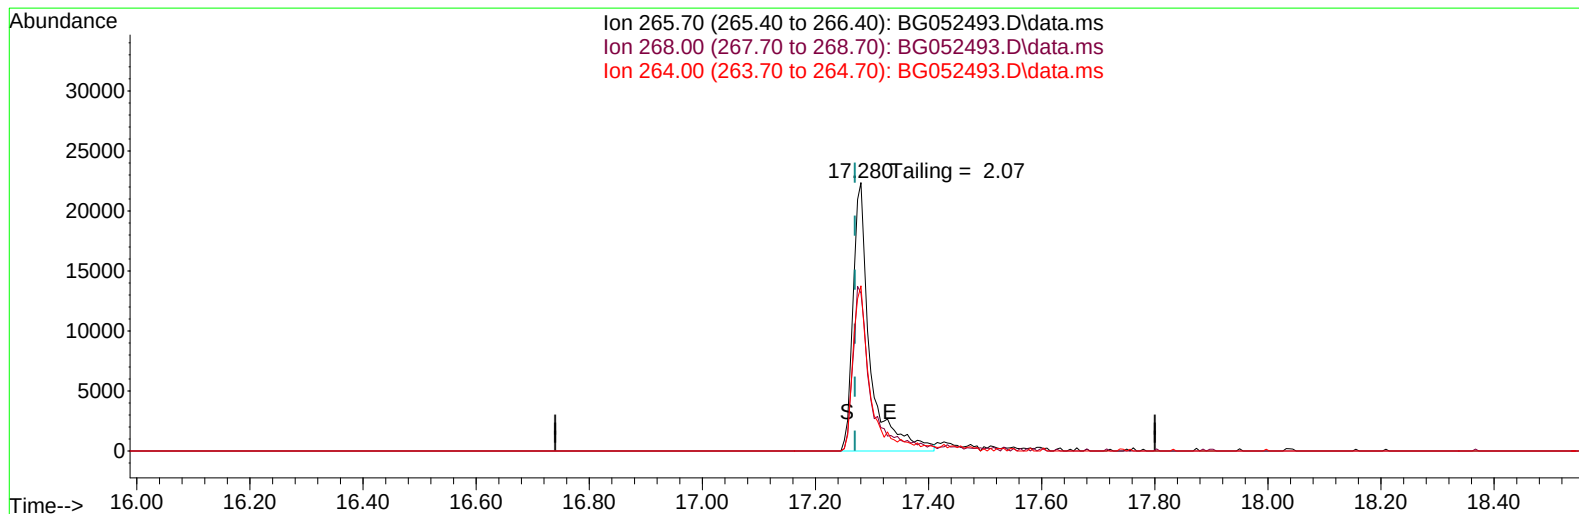

TIC: BG052493.D\data.ms

**(70) Pentachlorophenol (C)**




**17.280min (+ 0.010) 113993.12 ng**

**response 47077**

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 265.70 | 100.00 | 100.00 |
| 268.00 | 63.20  | 58.84  |
| 264.00 | 65.20  | 61.53  |
| 0.00   | 0.00   | 0.00   |

Data Path : Z:\svoasrv\HPCHEM1\BNA\_G\Data\BG022822\  
Data File : BG052493.D  
Acq On : 28 Feb 2022 9:38  
Operator : CG/JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 01 04:23:44 2022  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_G\Methods\8270-BG020722.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Tue Feb 08 01:21:20 2022  
Response via : Initial Calibration

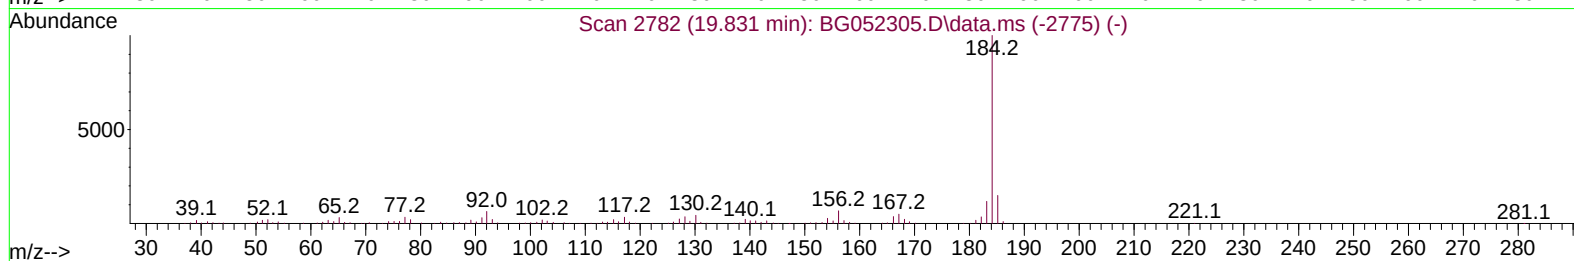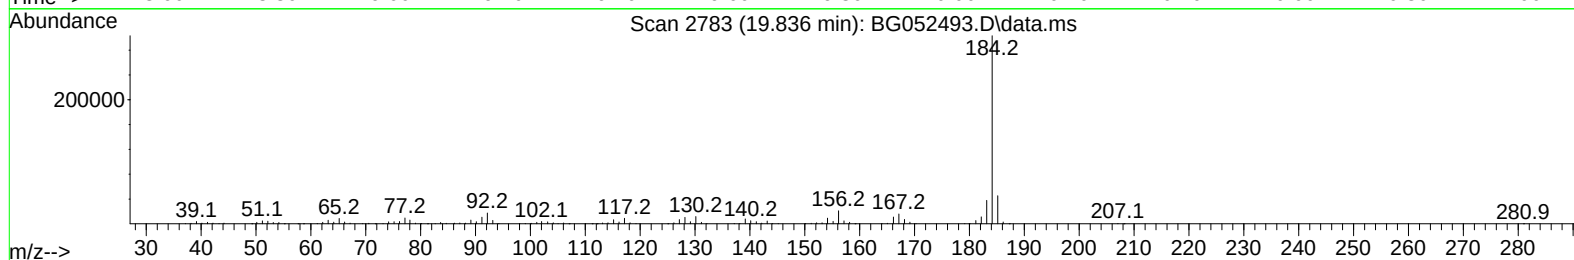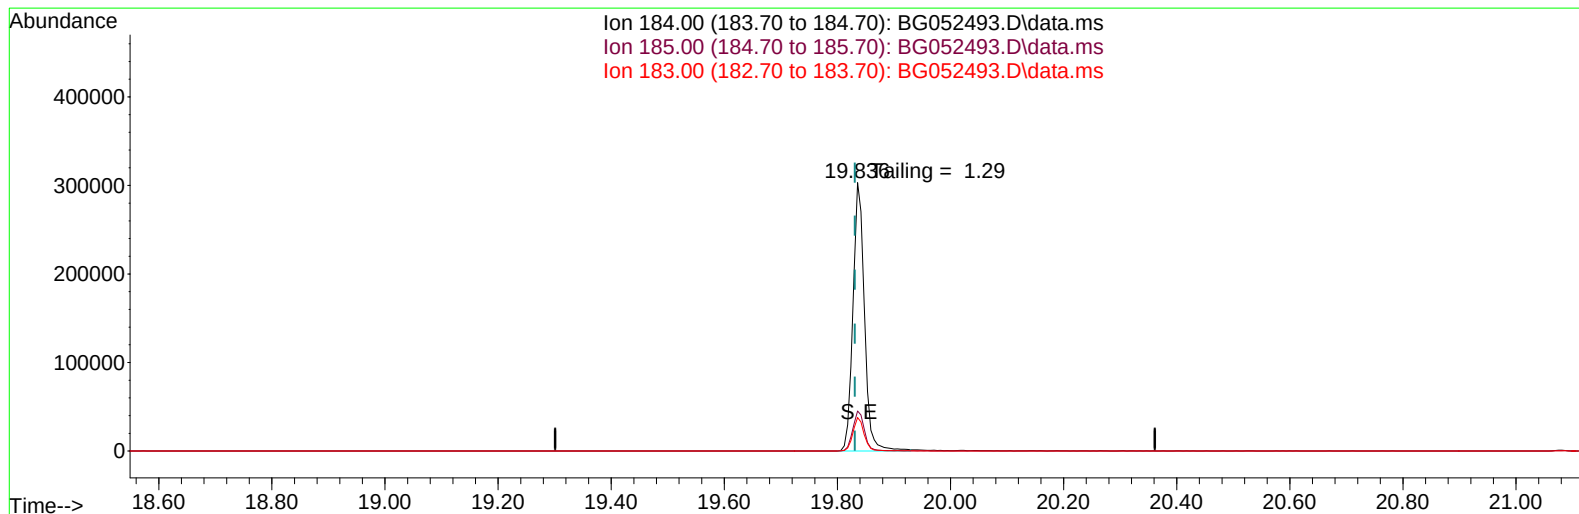

TIC: BG052493.D\data.ms

**(77) Benzidine**

19.836min (+ 0.005) 76966.05 ng

response 430883

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 184.00 | 100.00 | 100.00 |
| 185.00 | 14.80  | 14.93  |
| 183.00 | 12.20  | 12.45  |
| 0.00   | 0.00   | 0.00   |