

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG022822\
 Data File : BG052511.D
 Acq On : 28 Feb 2022 21:17
 Operator : CG/JU
 Sample : N1664-04
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 TP-2

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG020722.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BG052511.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.749	379	385	400	rVB	310481	508310	19.53%	5.559%
2	7.364	652	660	670	rBV	354018	617279	23.72%	6.751%
3	8.216	796	805	814	rBV	116826	200248	7.69%	2.190%
4	9.391	997	1005	1013	rBV	234380	419917	16.13%	4.592%
5	11.054	1281	1288	1300	rBV	155289	288239	11.07%	3.152%
6	13.486	1695	1702	1714	rBV	862386	1287078	49.45%	14.076%
7	14.860	1930	1936	1944	rBV	257182	415703	15.97%	4.546%
8	16.352	2183	2190	2204	rBV	654798	1079241	41.46%	11.803%
9	17.615	2398	2405	2411	rBV	349753	533901	20.51%	5.839%
10	20.206	2841	2846	2853	rVB	1893722	2602874	100.00%	28.465%
11	21.522	3067	3070	3078	rVB5	24950	36120	1.39%	0.395%
12	21.927	3131	3139	3146	rBV	325501	580413	22.30%	6.347%
13	25.387	3718	3728	3742	rVB2	187952	574778	22.08%	6.286%




Sum of corrected areas: 9144101

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG022822\
Data File : BG052511.D
Acq On : 28 Feb 2022 21:17
Operator : CG/JU
Sample : N1664-04
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
TP-2

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG020722.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

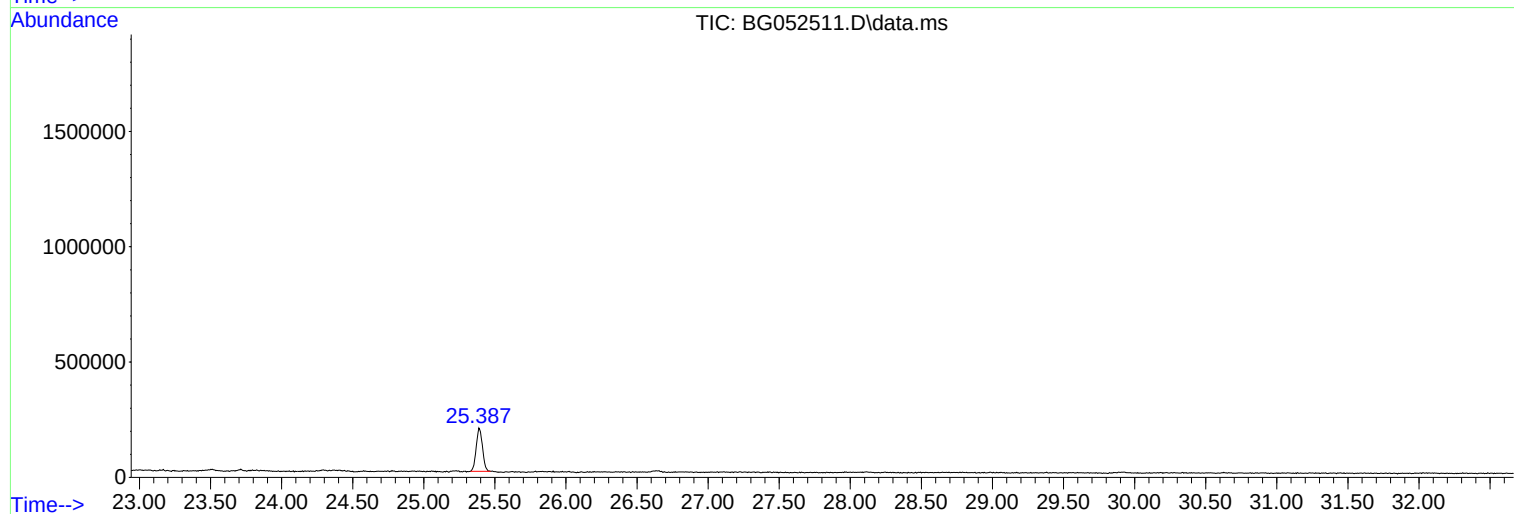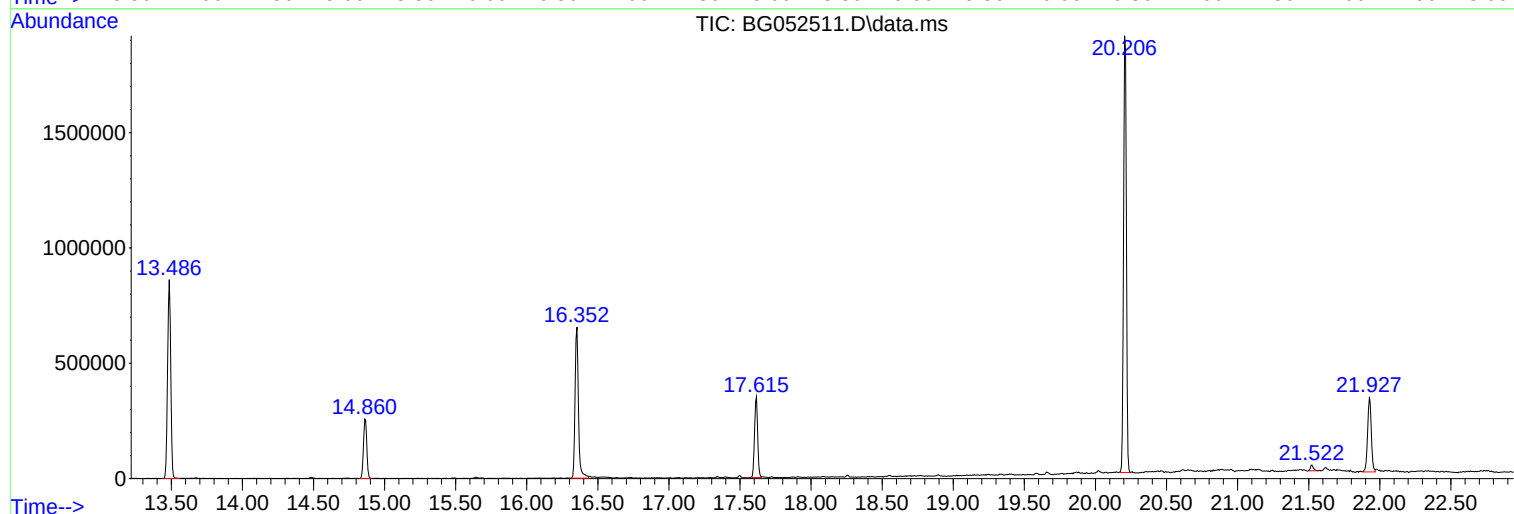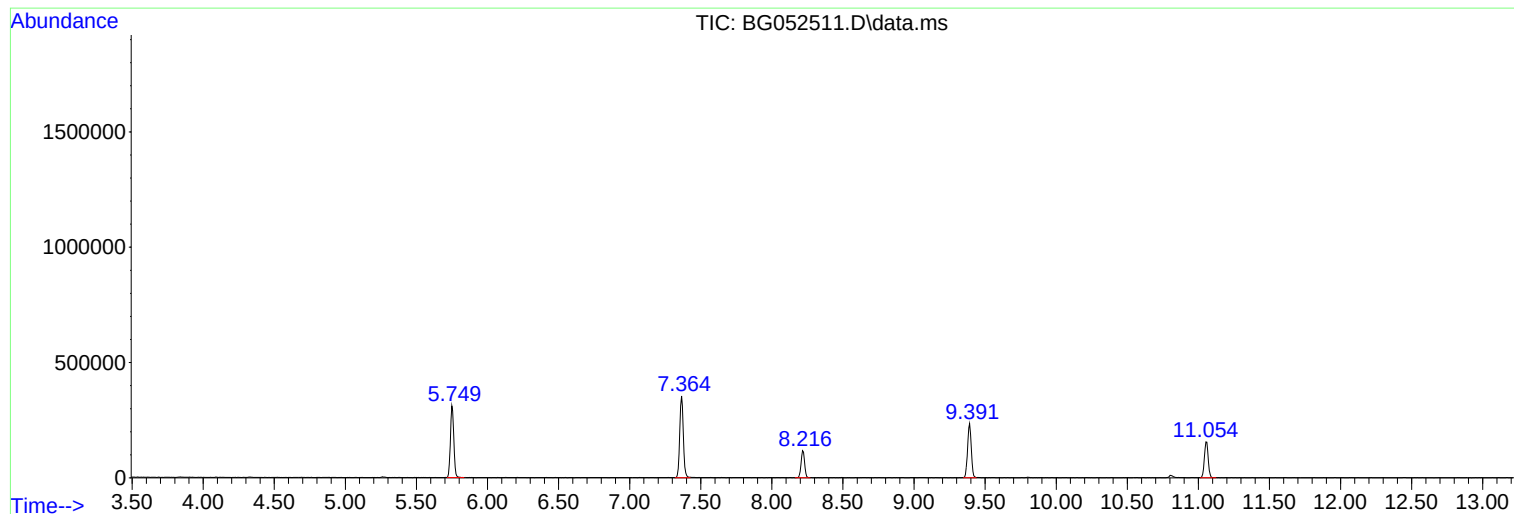

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG022822\
Data File : BG052511.D
Acq On : 28 Feb 2022 21:17
Operator : CG/JU
Sample : N1664-04
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
TP-2

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG020722.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG022822\
Data File : BG052511.D
Acq On : 28 Feb 2022 21:17
Operator : CG/JU
Sample : N1664-04
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
TP-2

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG020722.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------