


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG022822\
 Data File : BG052493.D
 Acq On : 28 Feb 2022 9:38
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG020722.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Feb 08 01:21:20 2022

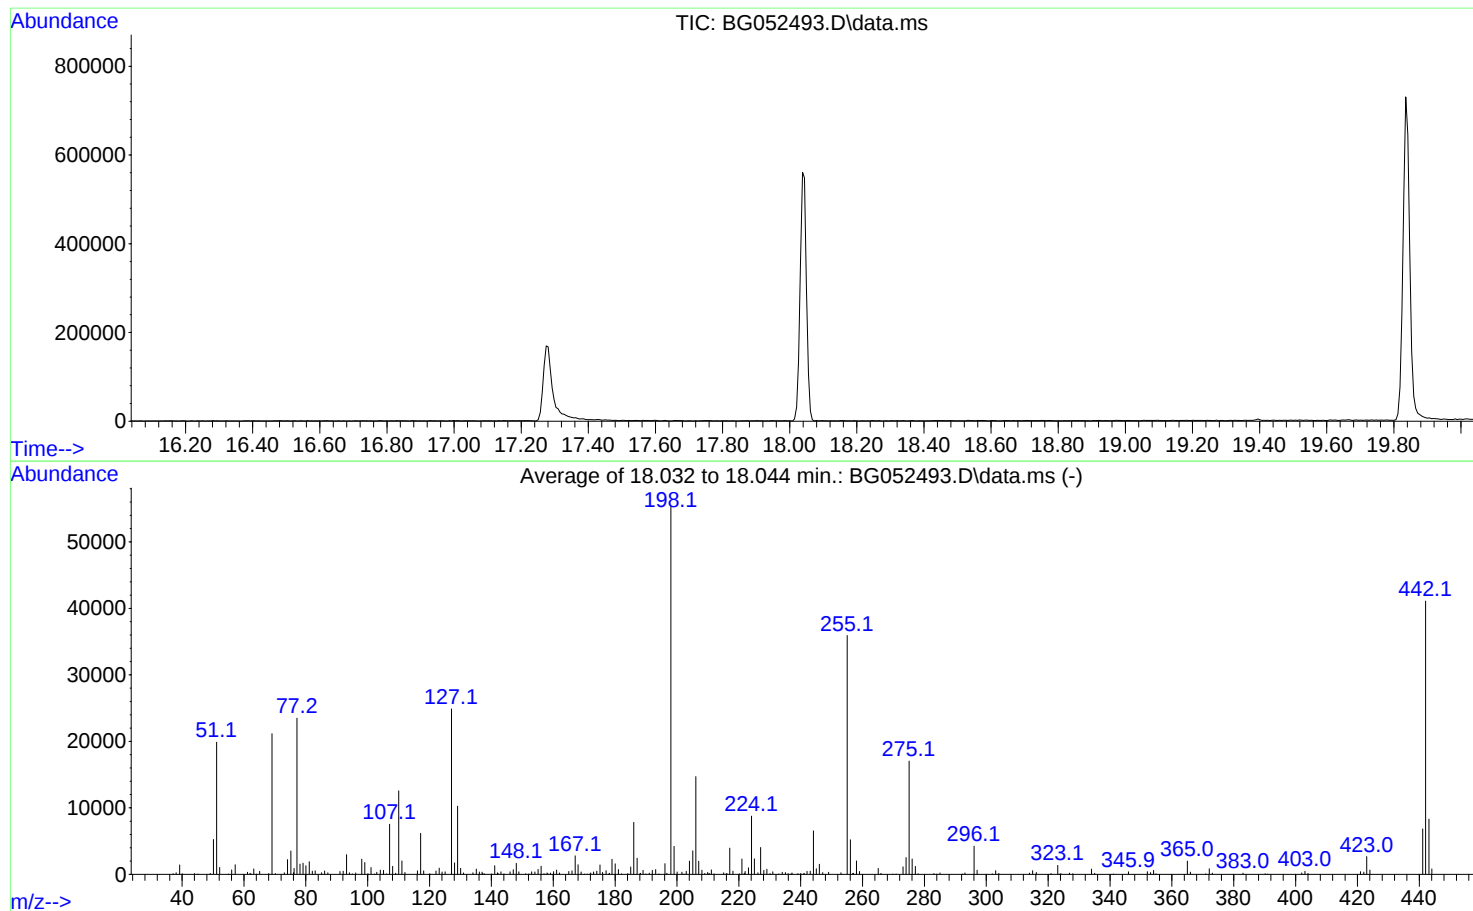




AutoFind: Scans 2476, 2477, 2478; Background Corrected with Scan 2470

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	35.9	19880	PASS
68	69	0.00	2	0.6	128	PASS
69	198	0.00	100	38.2	21147	PASS
70	69	0.00	2	0.6	120	PASS
127	198	10	80	45.0	24893	PASS
197	198	0.00	2	0.3	179	PASS
198	198	100	100	100.0	55325	PASS
199	198	5	9	7.6	4221	PASS
275	198	10	60	30.8	17029	PASS
365	198	1	100	3.6	1990	PASS
441	198	0.01	100	12.4	6844	PASS
442	442	50	100	100.0	41109	PASS
443	442	15	24	20.2	8309	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG022822\
Data File : BG052493.D
Acq On : 28 Feb 2022 9:38
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Mar 01 04:23:44 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG020722.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Feb 08 01:21:20 2022
Response via : Initial Calibration

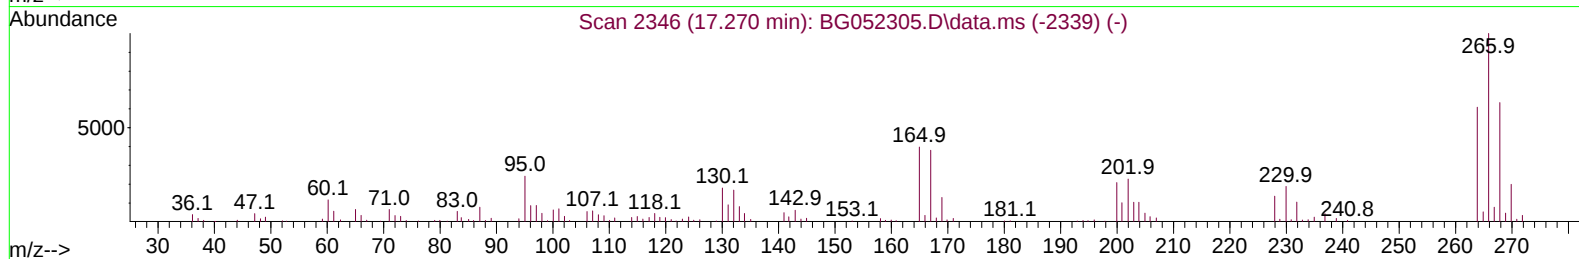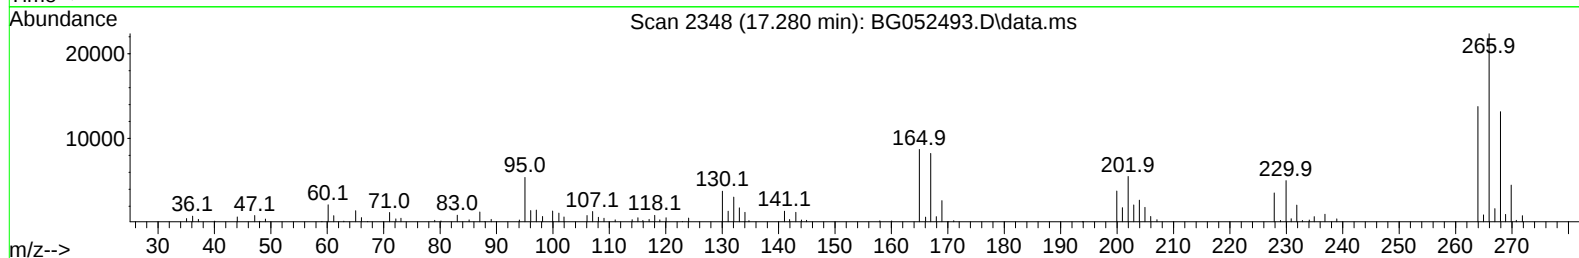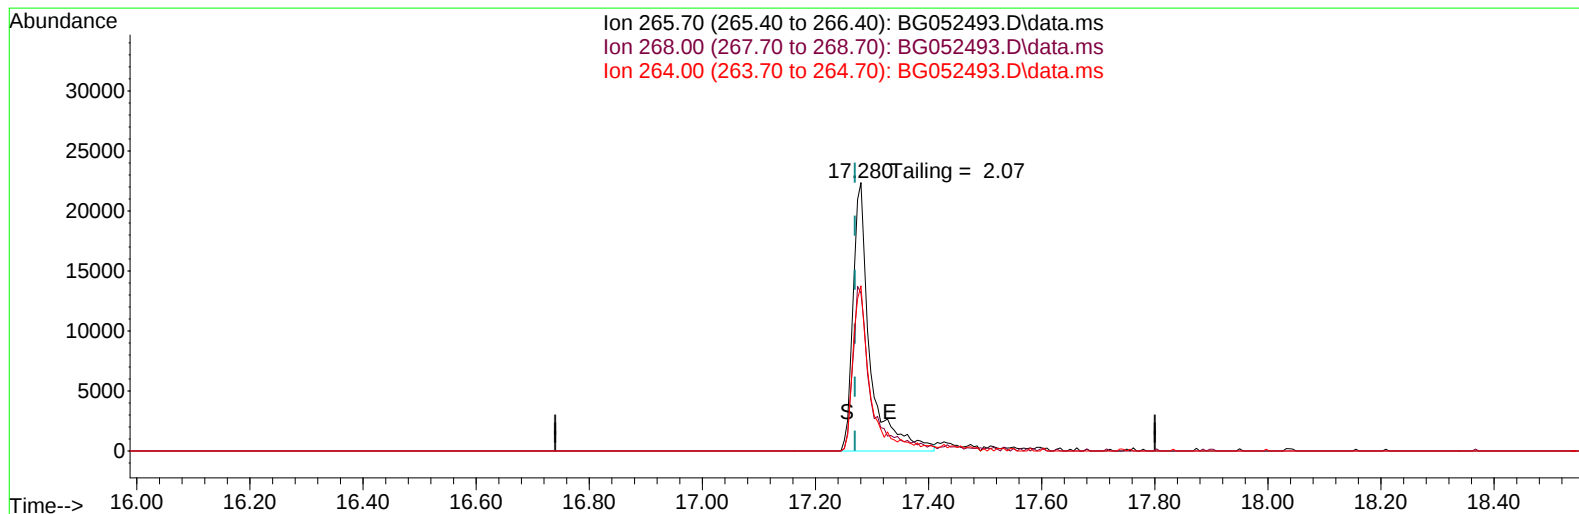

TIC: BG052493.D\data.ms

(70) Pentachlorophenol (C)

17.280min (+ 0.010) 113993.12 ng




response 47077

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.20	58.84
264.00	65.20	61.53
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG022822\
Data File : BG052493.D
Acq On : 28 Feb 2022 9:38
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Mar 01 04:23:44 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG020722.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Feb 08 01:21:20 2022
Response via : Initial Calibration

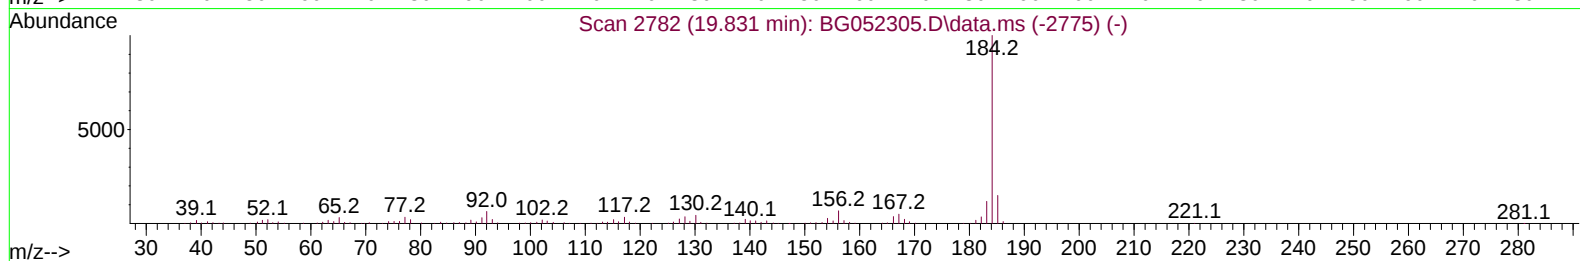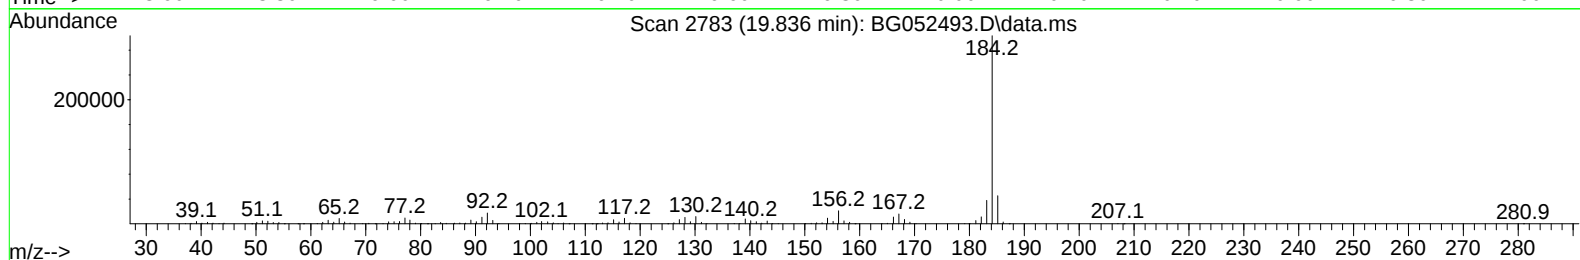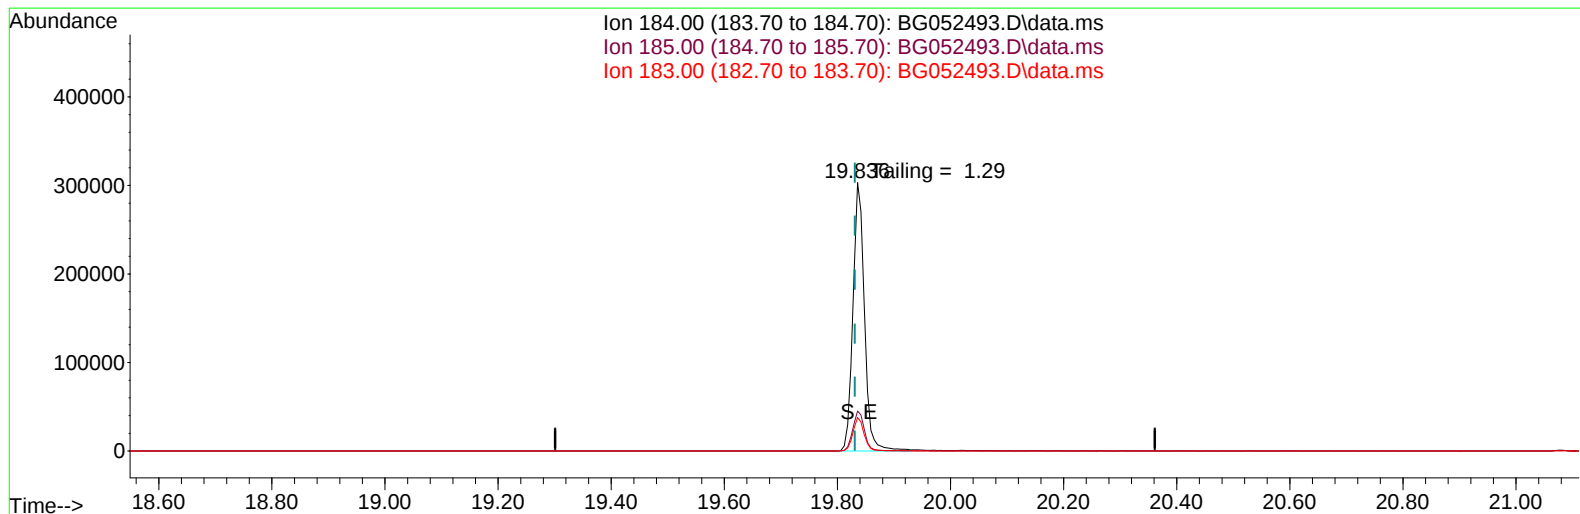

TIC: BG052493.D\data.ms

(77) Benzidine

19.836min (+ 0.005) 76966.05 ng

response 430883

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.80	14.93
183.00	12.20	12.45
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
2/28/2022	BNA_G	BG052493.D
Compound Name	Response	Retention Time
DDT	224466	21.081
DDD	3198	20.629
DDE	0	20.118
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
3198	227664	1.40

Instrument :
BNA_G
ClientSampleId :
DFTPP