
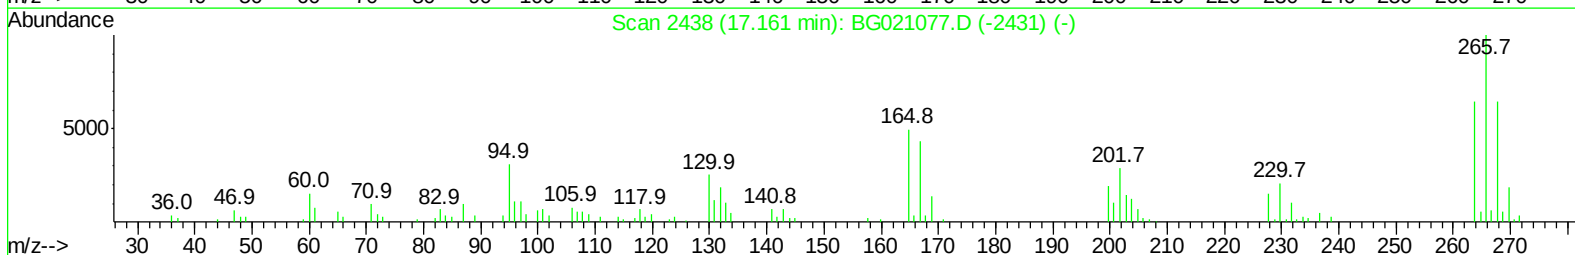
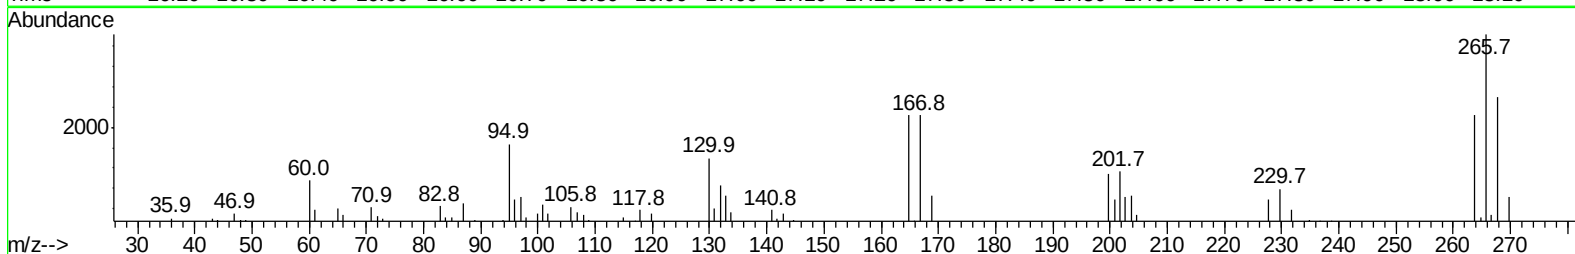


Data Path : Z:\HPCHEM1\BNA G\DATA\BG022916\
Data File : BG021150.D
Acq On : 29 Feb 2016 11:32
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 01 03:47:33 2016
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG022616.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Feb 26 16:39:44 2016
Response via : Initial Calibration

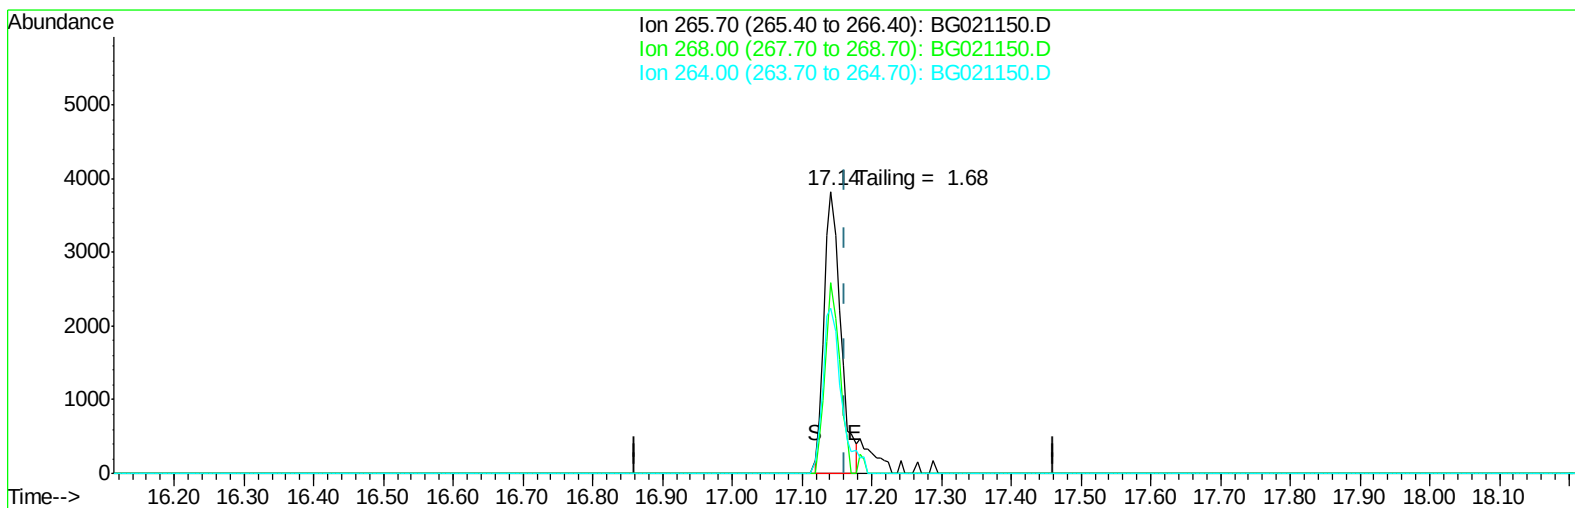

TIC: BG021150.D

(69) Pentachlorophenol (C)




17.142min (-0.020) 0.00ng m

response 6188

Ion	Exp%	Act%
265.70	100	100
268.00	63.80	67.73
264.00	59.80	58.84
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA G\DATA\BG022916\
 Data File : BG021150.D
 Acq On : 29 Feb 2016 11:32
 Operator : UM/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 01 03:47:33 2016
 Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG022616.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Feb 26 16:39:44 2016
 Response via : Initial Calibration

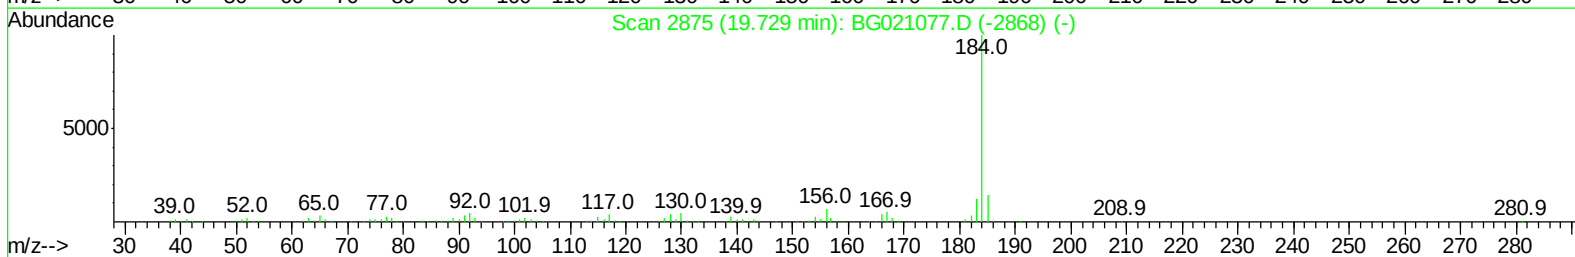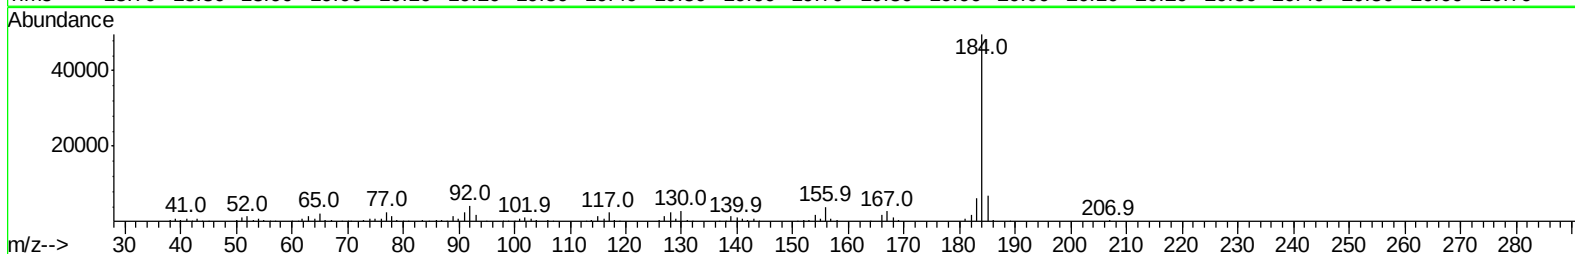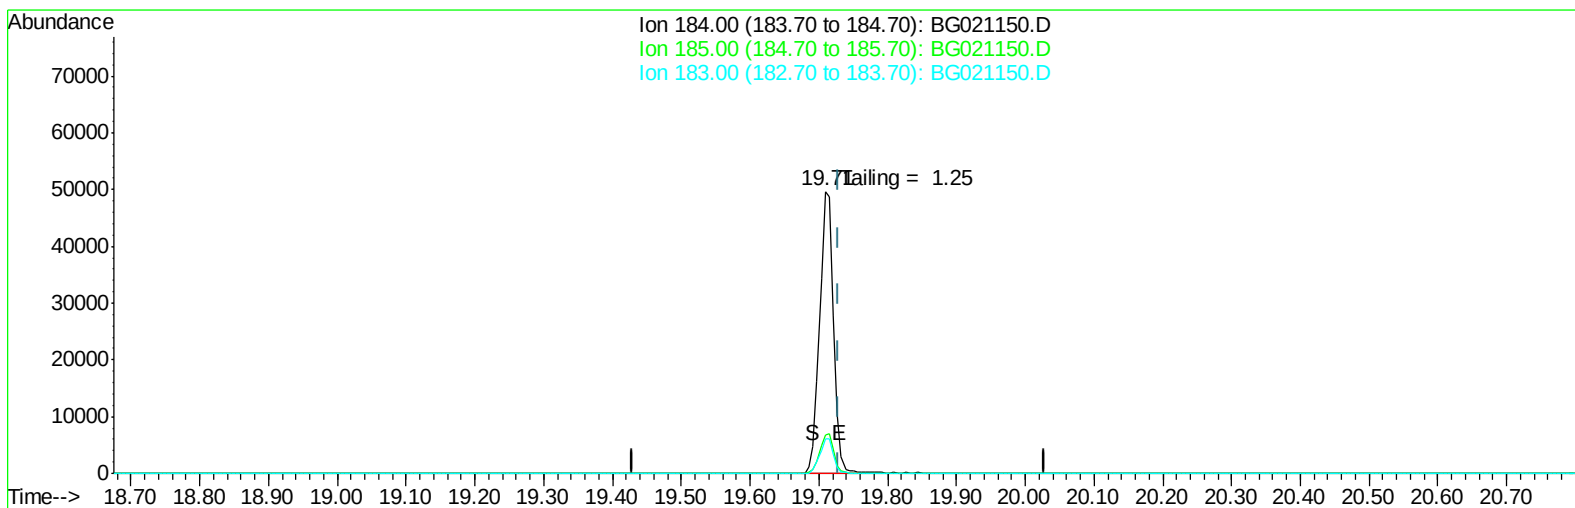

TIC: BG021150.D

(76) Benzidine

19.709min (-0.020) 0.00ng

response 70318

Ion	Exp%	Act%
184.00	100	100
185.00	14.40	13.76
183.00	12.60	12.43
0.00	0.00	0.00