
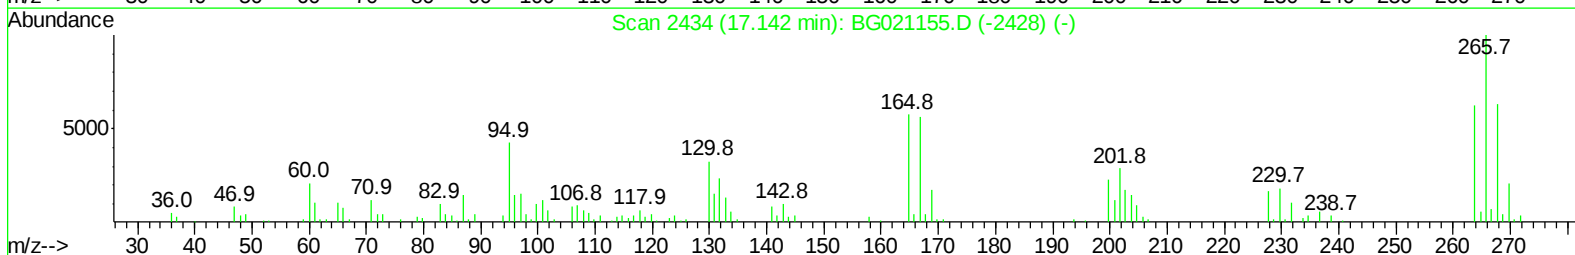
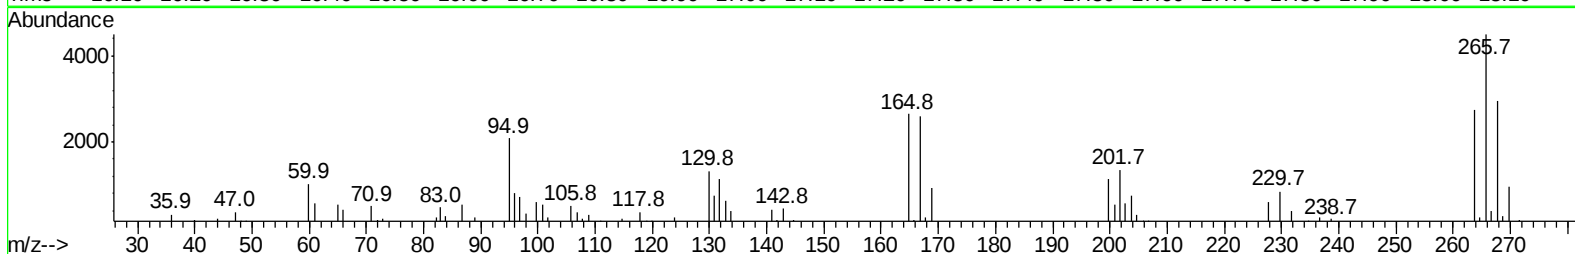


Data Path : Z:\HPCHEM1\BNA G\DATA\BG022916\
Data File : BG021160.D
Acq On : 29 Feb 2016 18:14
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 01 03:55:05 2016
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG022916.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Feb 29 17:40:25 2016
Response via : Initial Calibration

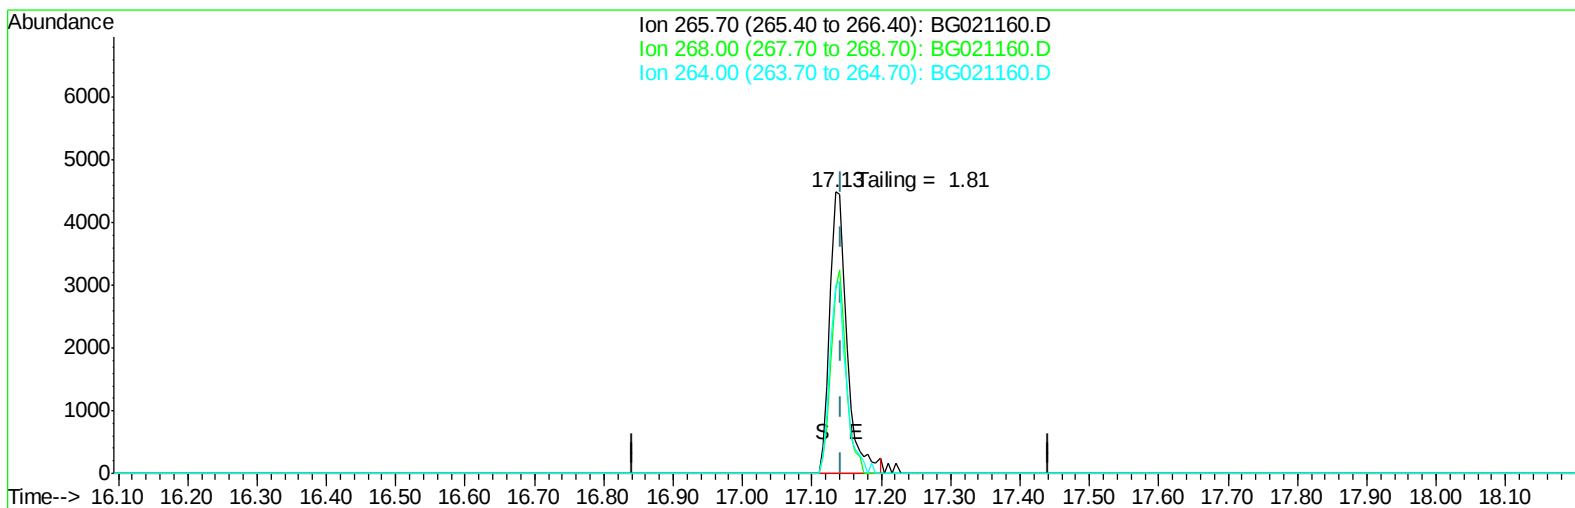

TIC: BG021160.D

(69) Pentachlorophenol (C)




17.133min (-0.009) 0.00ng

response 7759

Ion	Exp%	Act%
265.70	100	100
268.00	63.80	71.66
264.00	59.80	66.66
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA G\DATA\BG022916\
Data File : BG021160.D
Acq On : 29 Feb 2016 18:14
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 01 03:55:05 2016
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG022916.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Feb 29 17:40:25 2016
Response via : Initial Calibration

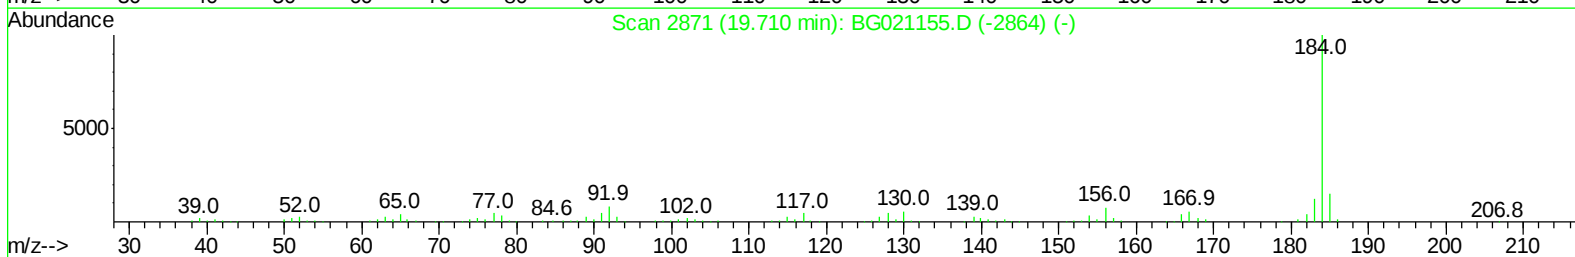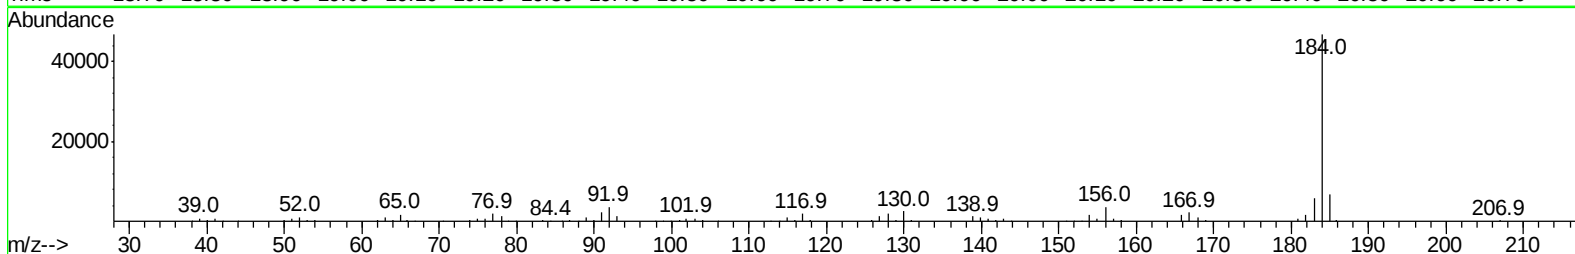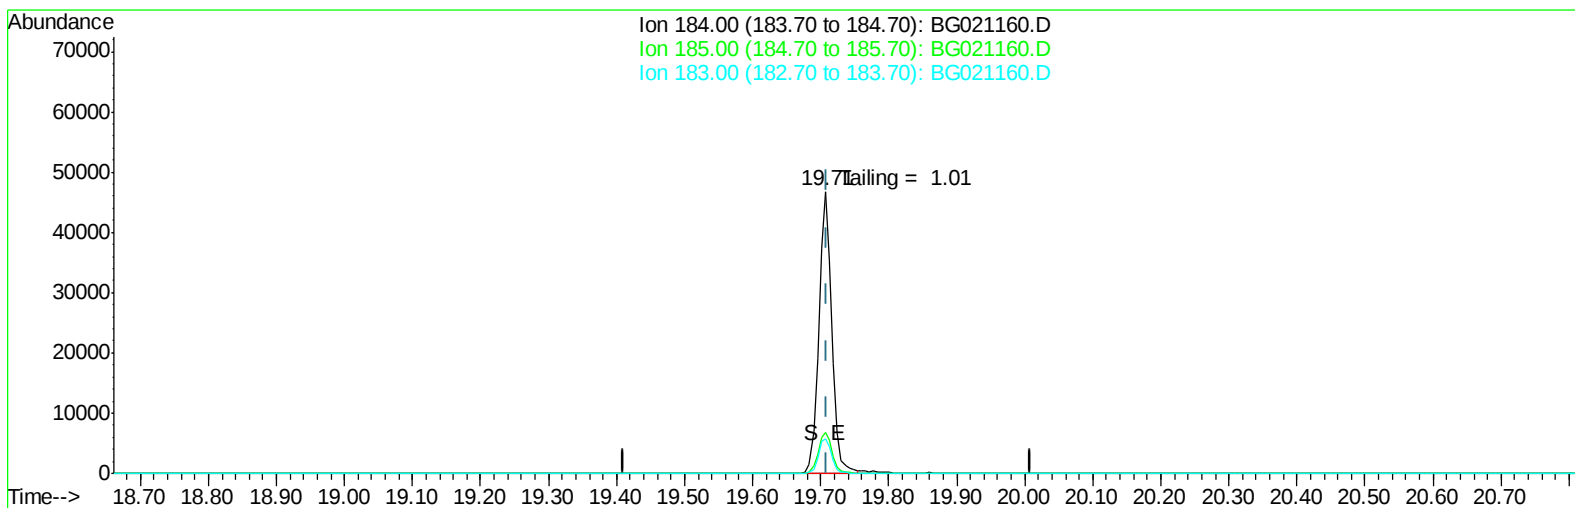

TIC: BG021160.D

(76) Benzidine

19.707min (-0.003) 0.00ng

response 63405

Ion	Exp%	Act%
184.00	100	100
185.00	14.40	14.72
183.00	12.60	12.39
0.00	0.00	0.00