


Data Path : Z:\HPCHEM1\BNA G\Data\BG022916\
 Data File : BG021150.D
 Acq On : 29 Feb 2016 11:32
 Operator : UM/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG022916.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Feb 29 17:40:25 2016

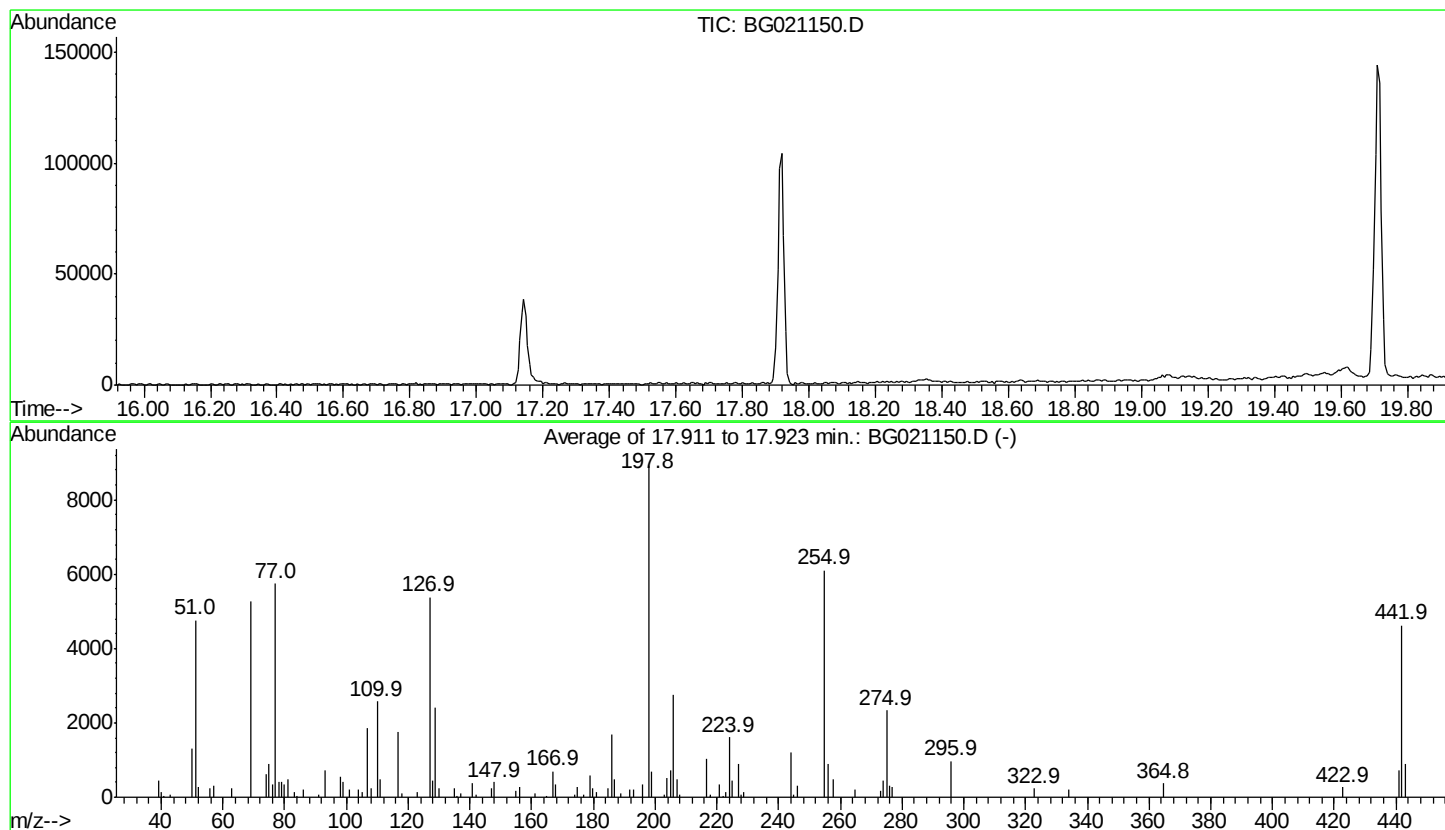

AutoFind: Scans 2565, 2566, 2567; Background Corrected with Scan 2559

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	53.3	4758	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	59.3	5287	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	60.3	5380	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	8921	PASS
199	198	5	9	7.6	681	PASS
275	198	10	60	26.2	2335	PASS
365	198	1	100	4.1	367	PASS
441	442	0.01	24	16.0	740	PASS
442	198	50	100	51.8	4625	PASS
443	442	15	24	19.4	899	PASS