


Data Path : Z:\HPCHEM1\BNA G\DATA\BG022916\
 Data File : BG021160.D
 Acq On : 29 Feb 2016 18:14
 Operator : UM/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG022916.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Feb 29 17:40:25 2016

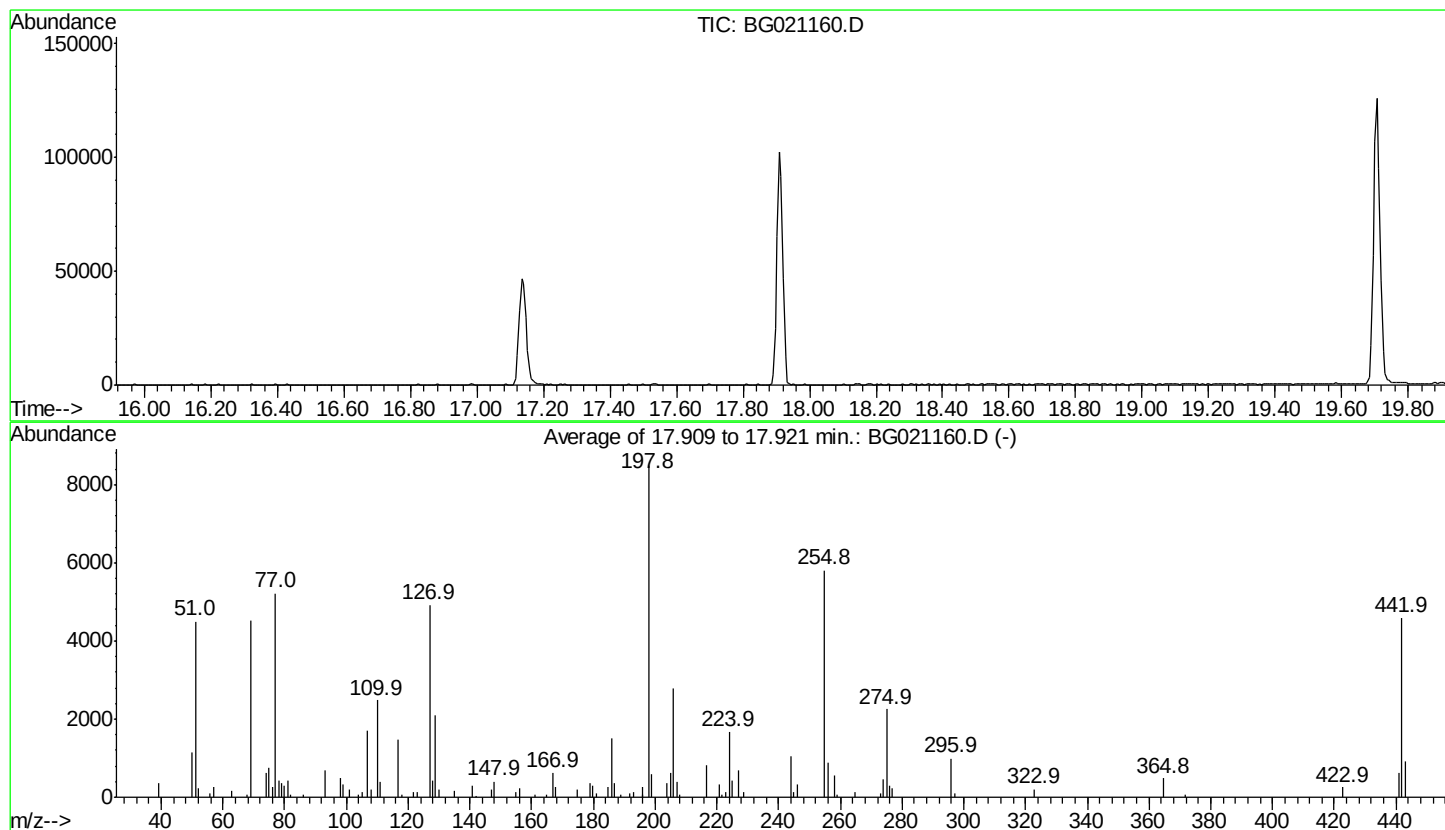

AutoFind: Scans 2565, 2566, 2567; Background Corrected with Scan 2559

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	53.1	4504	PASS
68	69	0.00	2	1.3	57	PASS
69	198	0.00	100	53.5	4536	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	57.9	4916	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	8484	PASS
199	198	5	9	6.9	582	PASS
275	198	10	60	26.6	2254	PASS
365	198	1	100	5.6	476	PASS
441	442	0.01	24	13.8	632	PASS
442	198	50	100	54.1	4587	PASS
443	442	15	24	19.9	913	PASS