
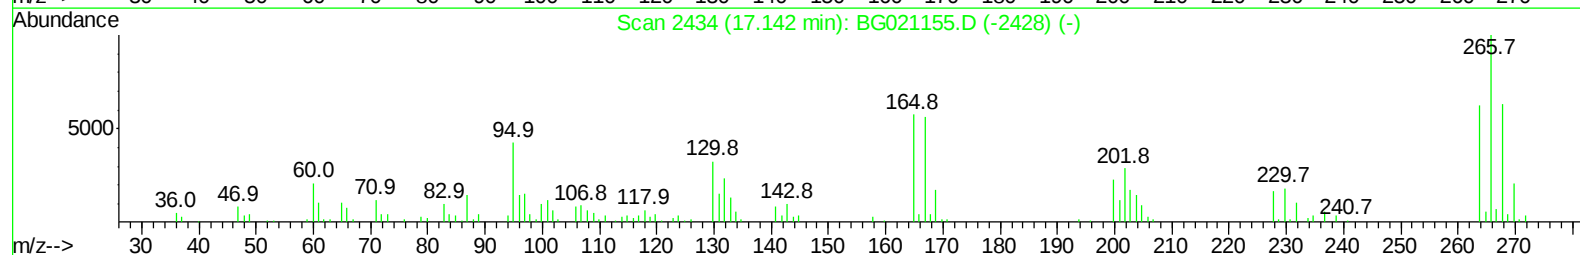
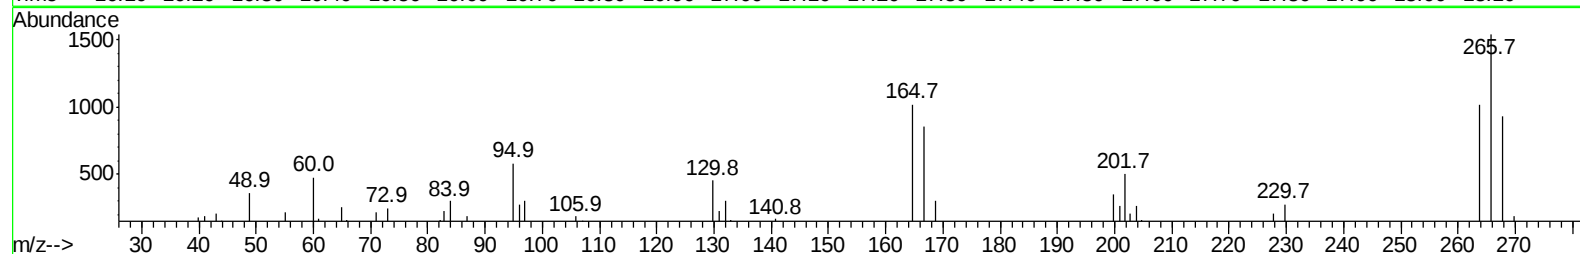


Data Path : Z:\HPCHEM1\BNA G\DATA\BG030116\
Data File : BG021190.D
Acq On : 1 Mar 2016 17:59
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 02 03:02:06 2016
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG022916.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Feb 29 17:40:25 2016
Response via : Initial Calibration

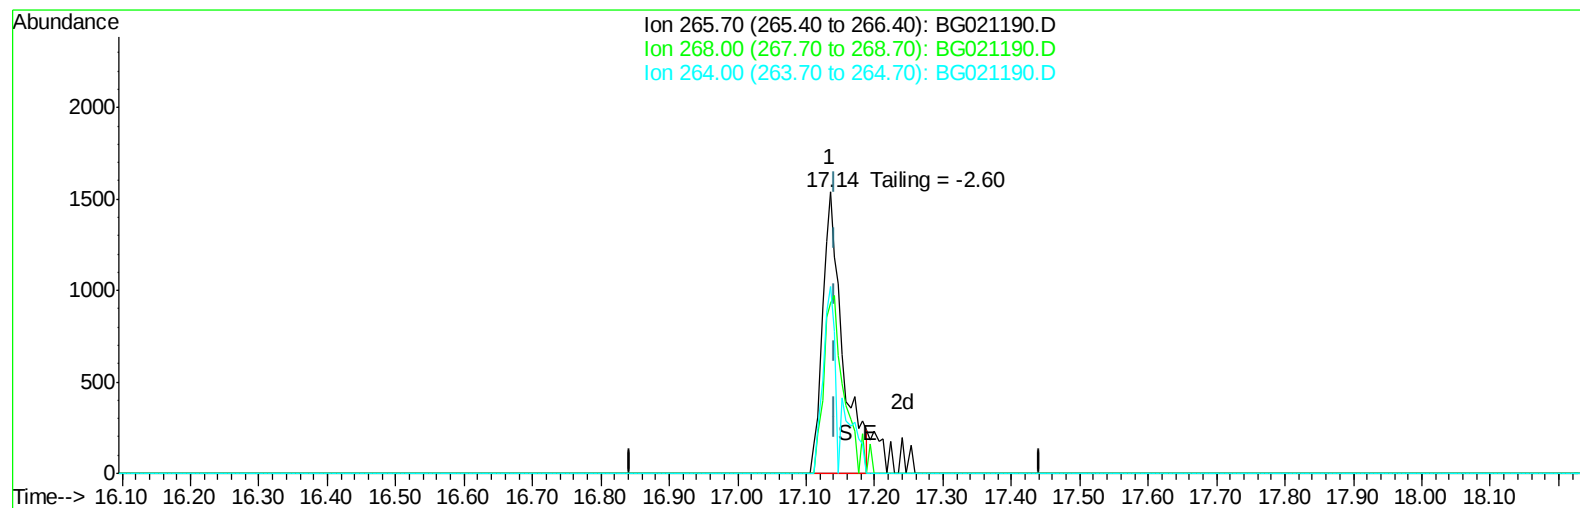

TIC: BG021190.D

(69) Pentachlorophenol (C)




17.135min (-0.007) 0.00ng m

response 3171

Ion	Exp%	Act%
265.70	100	100
268.00	63.80	60.58
264.00	59.80	66.17
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA G\DATA\BG030116\
Data File : BG021190.D
Acq On : 1 Mar 2016 17:59
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 02 03:02:06 2016
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG022916.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Feb 29 17:40:25 2016
Response via : Initial Calibration

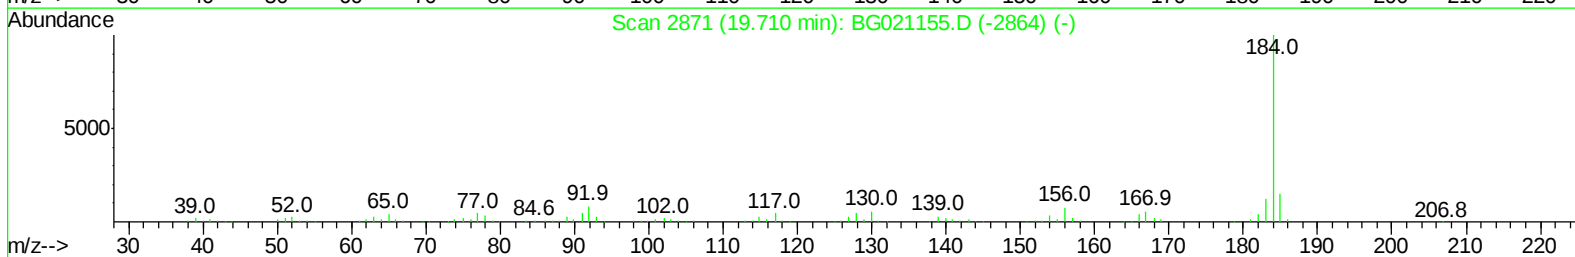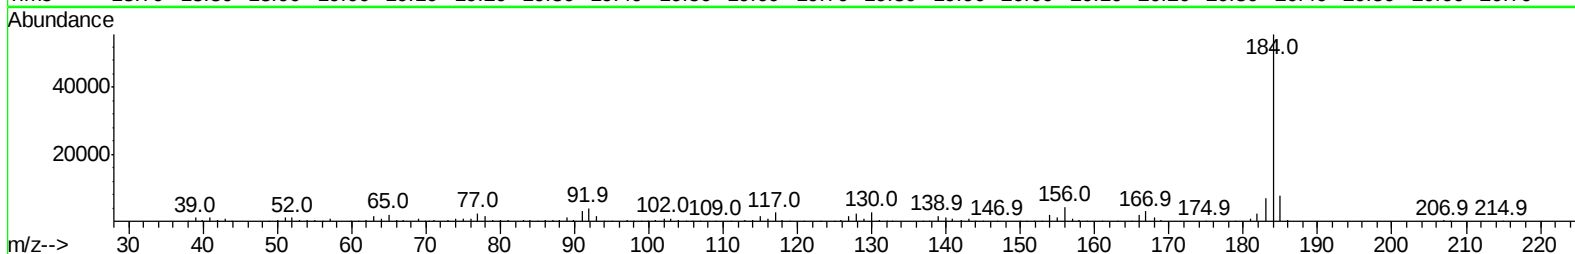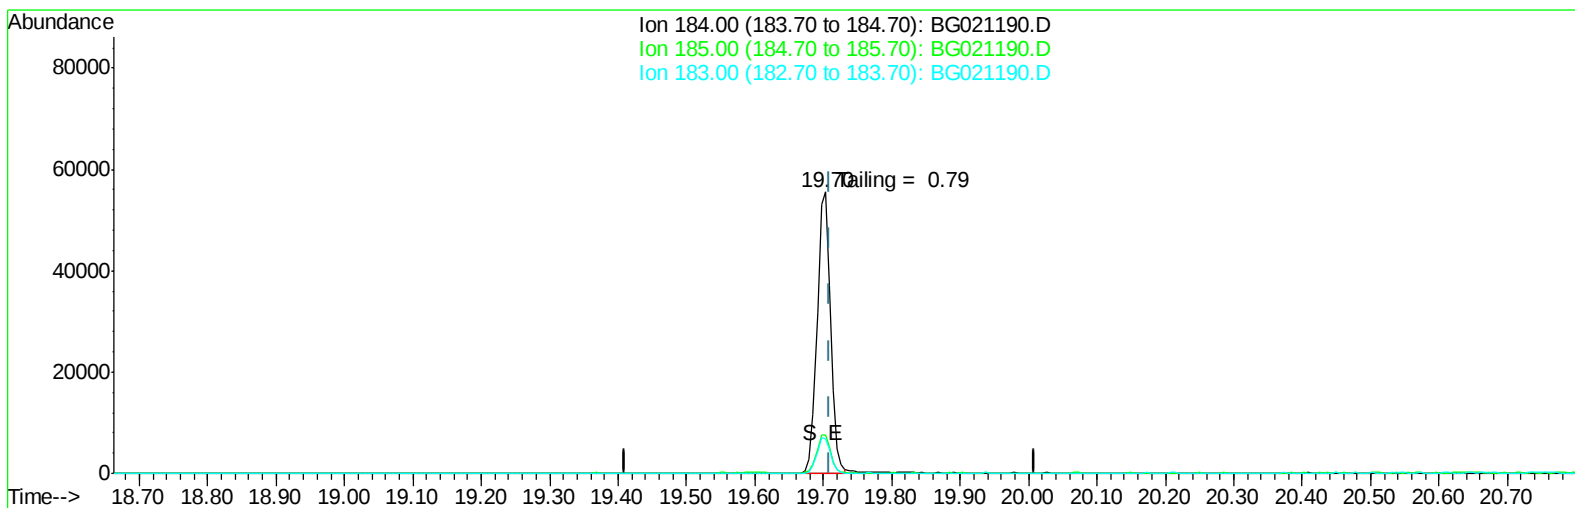

TIC: BG021190.D

(76) Benzidine

19.703min (-0.007) 0.00ng

response 77585

Ion	Exp%	Act%
184.00	100	100
185.00	14.40	13.72
183.00	12.60	12.40
0.00	0.00	0.00