


Data Path : Z:\HPCHEM1\BNA G\Data\BG030116\
 Data File : BG021190.D
 Acq On : 1 Mar 2016 17:59
 Operator : UM/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG022916.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Mar 02 11:46:16 2016

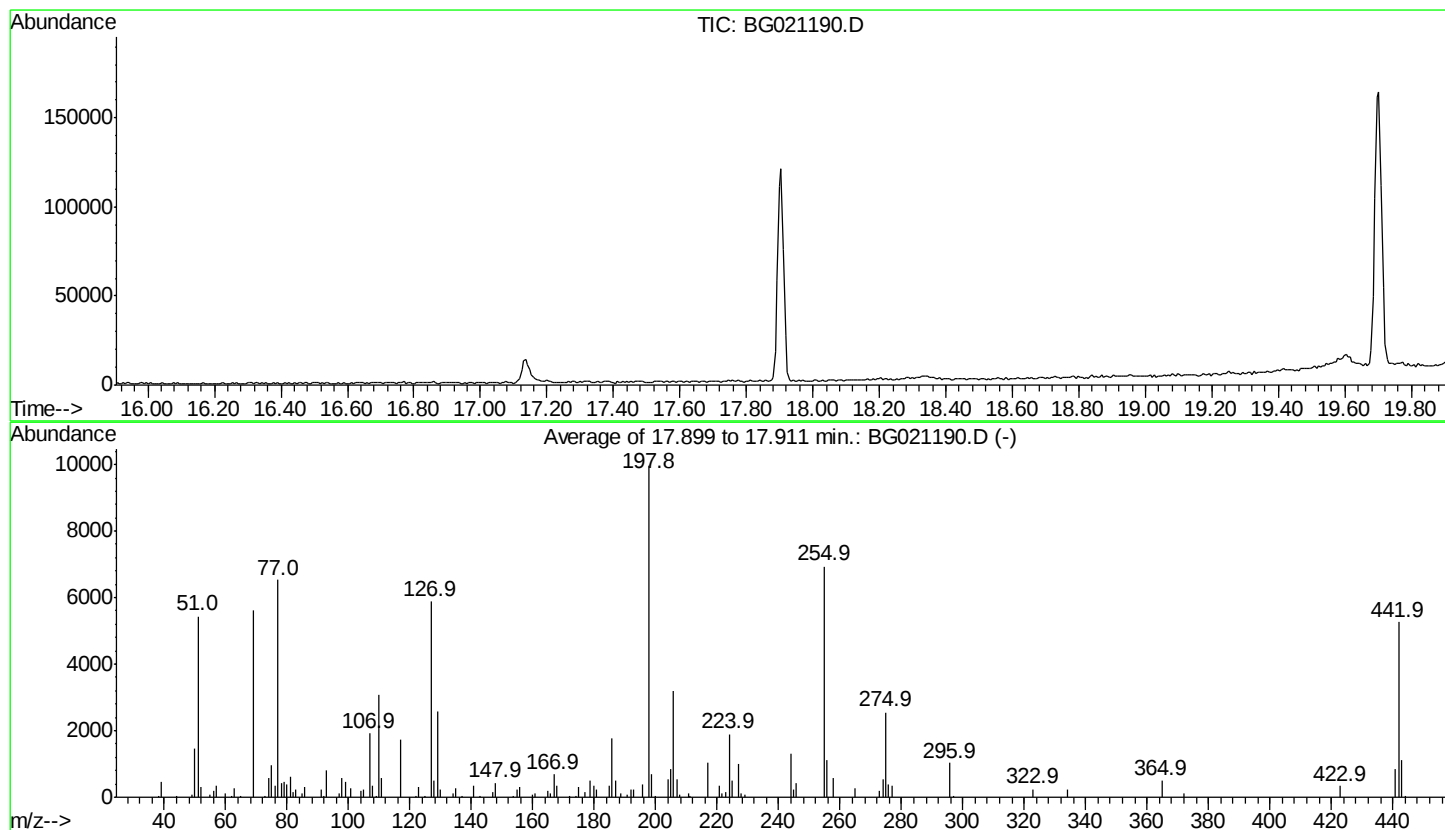

AutoFind: Scans 2563, 2564, 2565; Background Corrected with Scan 2557

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	54.5	5432	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	56.4	5622	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	59.1	5886	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	9967	PASS
199	198	5	9	6.8	676	PASS
275	198	10	60	25.6	2550	PASS
365	198	1	100	5.0	499	PASS
441	442	0.01	24	16.0	841	PASS
442	198	50	100	52.8	5260	PASS
443	442	15	24	21.2	1113	PASS