

Data Path : Z:\HPCHEM1\BNA G\DATA\BG030118\
 Data File : BG032919.D
 Acq On : 1 Mar 2018 16:20
 Operator : SJ/JU
 Sample : J1402-08
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 PL-01-022818-A

Quant Time: Mar 01 17:44:10 2018
 Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG022118.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Mar 01 17:38:52 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.92	152	67193	20.00	ng	0.00
21) Naphthalene-d8	11.81	136	293222	20.00	ng	0.00
38) Acenaphthene-d10	15.53	164	163698	20.00	ng	0.00
63) Phenanthrene-d10	18.26	188	366728	20.00	ng	0.00
75) Chrysene-d12	22.61	240	334426	20.00	ng	0.00
86) Perylene-d12	26.42	264	316784	20.00	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	6.34	112	568657	135.40	ng	0.00
7) Phenol-d6	8.02	99	680133	116.18	ng	0.00
23) Nitrobenzene-d5	10.12	82	527080	120.11	ng	0.00
41) 2,4,6-Tribromophenol	17.00	330	259101	150.53	ng	0.00
44) 2-Fluorobiphenyl	14.17	172	1154473	101.71	ng	0.00
78) Terphenyl-d14	20.78	244	1584787	106.47	ng	0.00


Target Compounds Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA G\DATA\BG030118\
Data File : BG032919.D
Acq On : 1 Mar 2018 16:20
Operator : SJ/JU
Sample : J1402-08
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
PL-01-022818-A

Quant Time: Mar 01 17:44:10 2018
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG022118.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Mar 01 17:38:52 2018
Response via : Initial Calibration

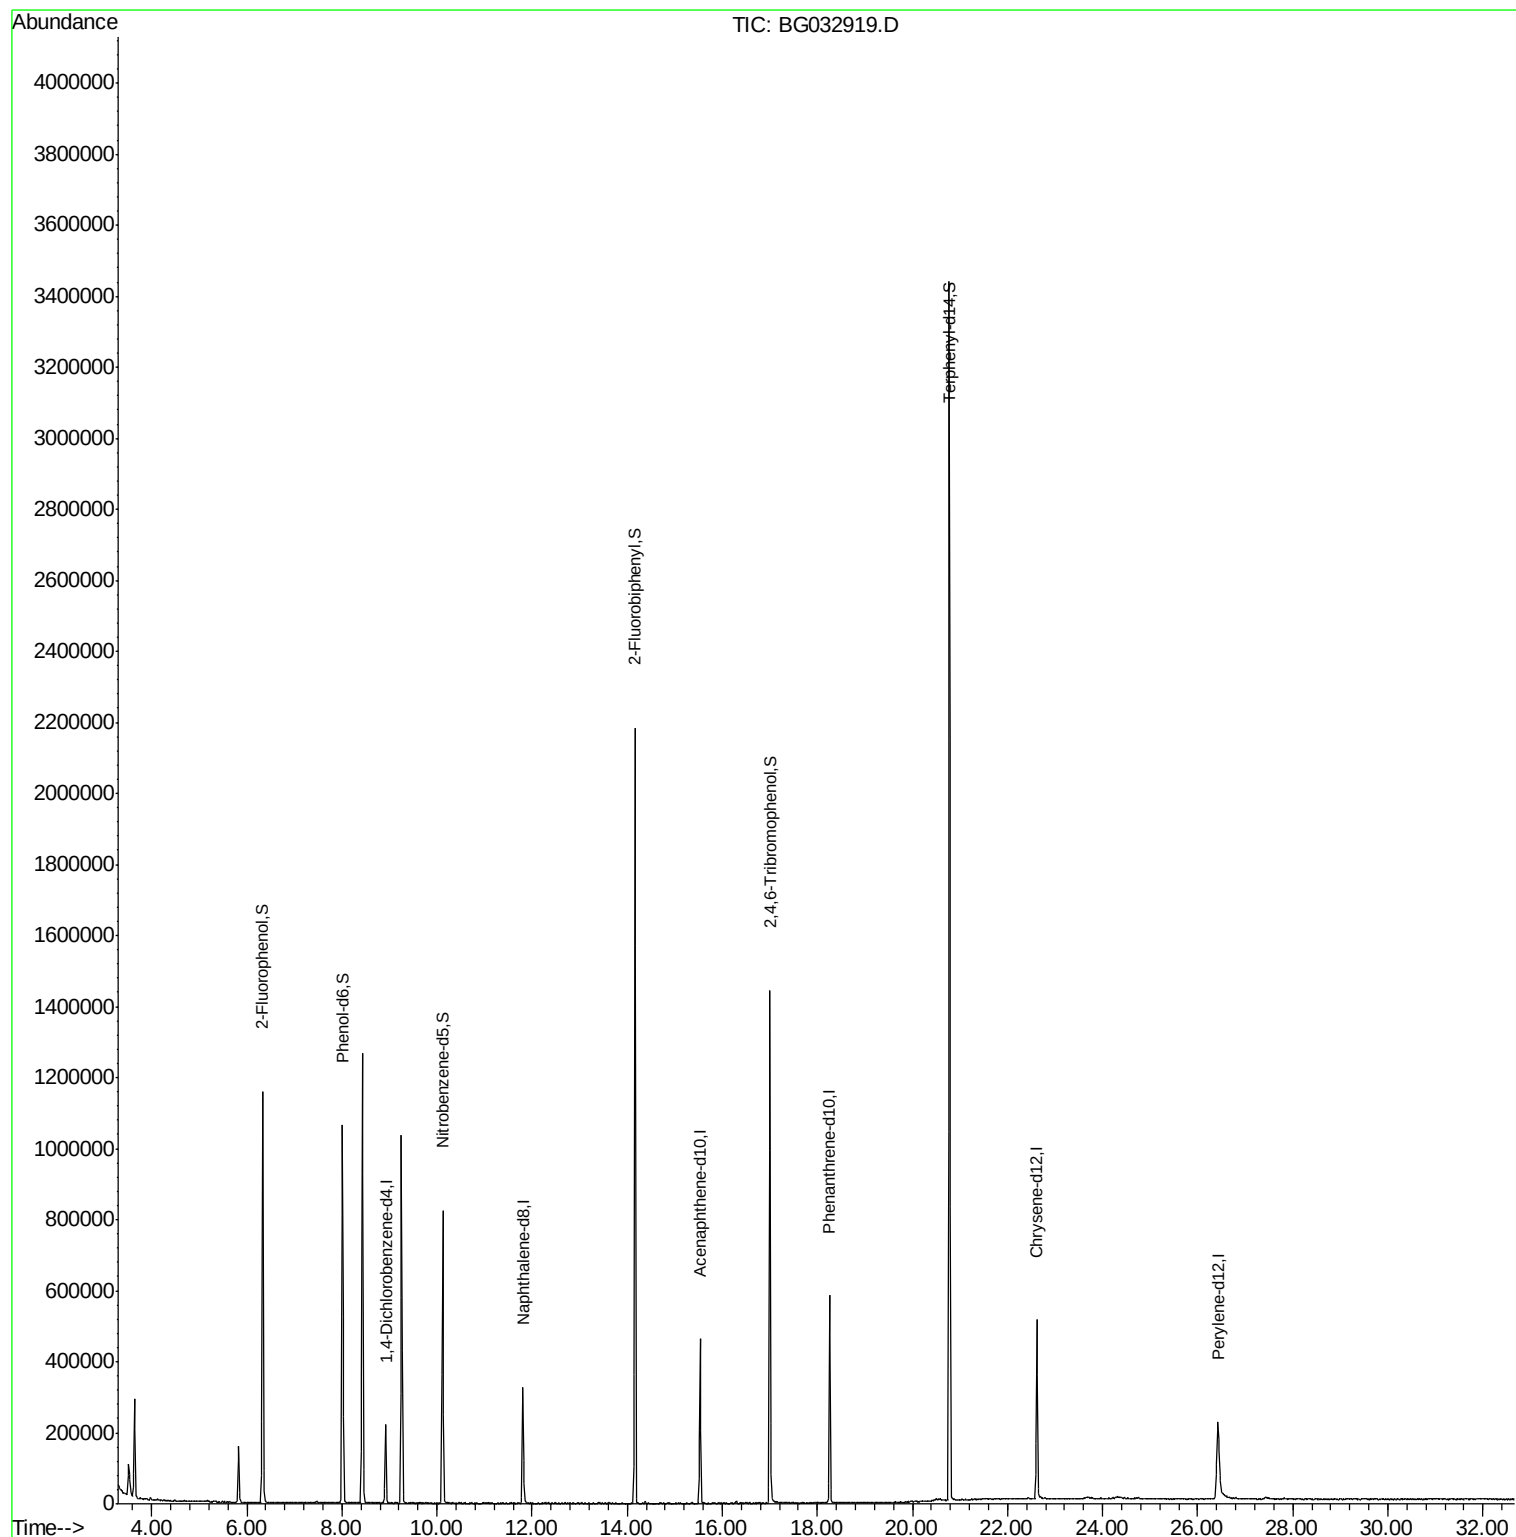

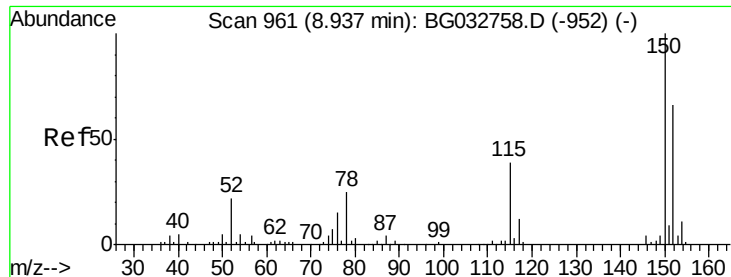


#1




1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 8.92 min Scan# 959
Delta R.T. 0.00 min
Lab File: BG032919.D
Acq: 1 Mar 2018 16:20

Instrument :
BNA_G
ClientSampleId :
PL-01-022818-A

Tot Ion:152 Resp: 67193
Ion Ratio Lower Upper
152 100
150 153.9 126.6 189.8
115 61.1 53.0 79.4

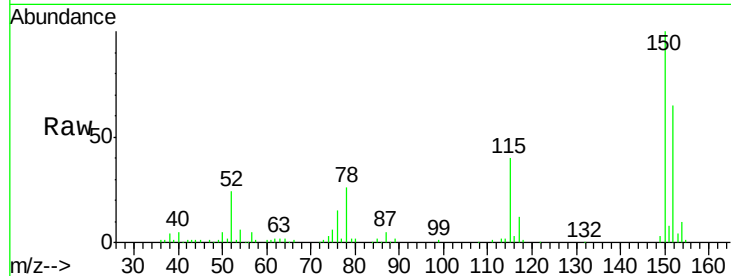


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

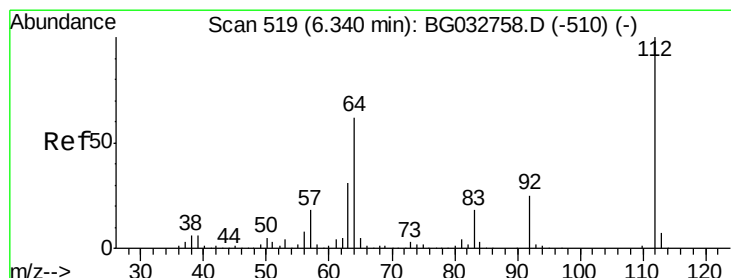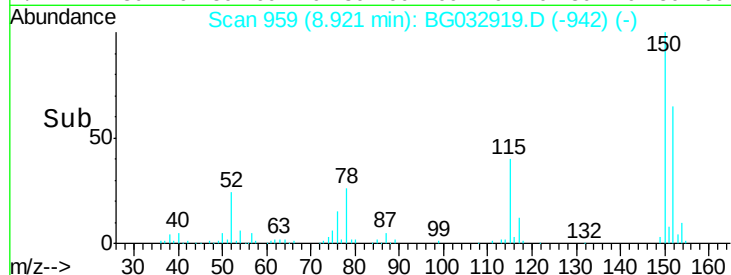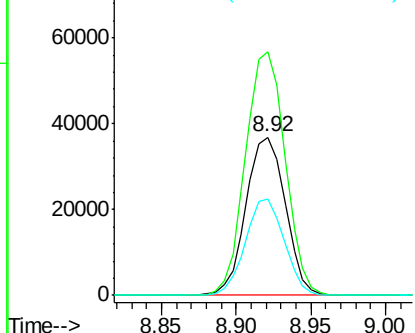



#5


2-Fluorophenol
Concen: 135.396 ng
RT: 6.34 min Scan# 519
Delta R.T. 0.01 min
Lab File: BG032919.D
Acq: 1 Mar 2018 16:20

Tgt Ion:112 Resp: 568657
Ion Ratio Lower Upper
112 100
64 65.9 56.3 84.5
63 31.8 30.1 45.1

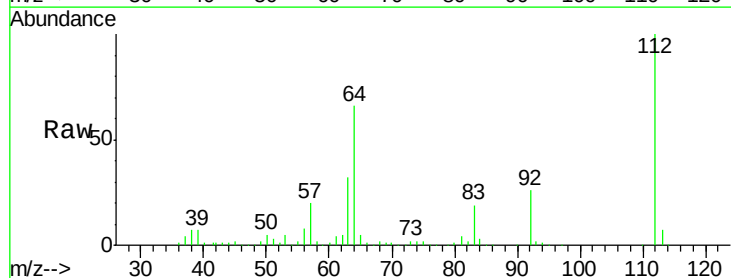

Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BGC
Ion 63.00 (62.70 to 63.70): BGC

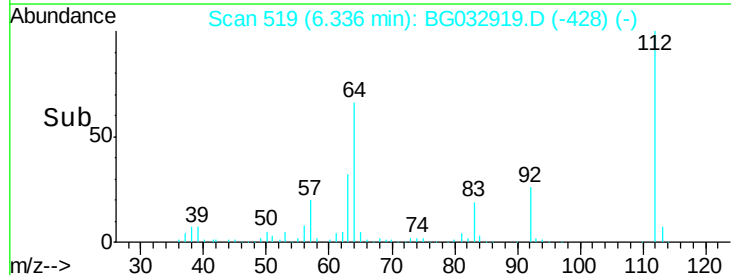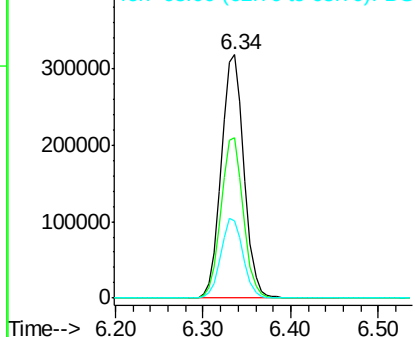

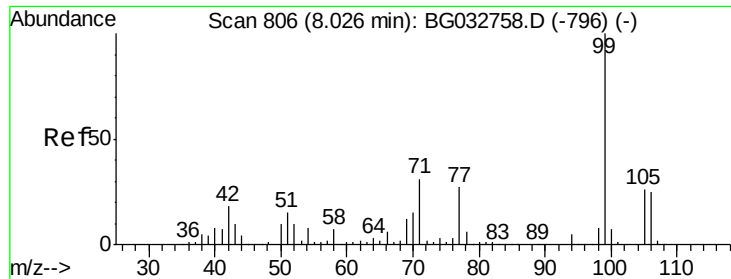

#7

Phenol-d6

Concen: 116.180 ng

RT: 8.02 min Scan# 805

Delta R.T. 0.00 min

Lab File: BG032919.D

Acq: 1 Mar 2018 16:20

Instrument :

BNA_G

ClientSampleId :

PL-01-022818-A


Tot Ion: 99 Resp: 680133

Ion Ratio Lower Upper




99 100

42 20.3 14.1 21.1

71 32.1 26.1 39.1

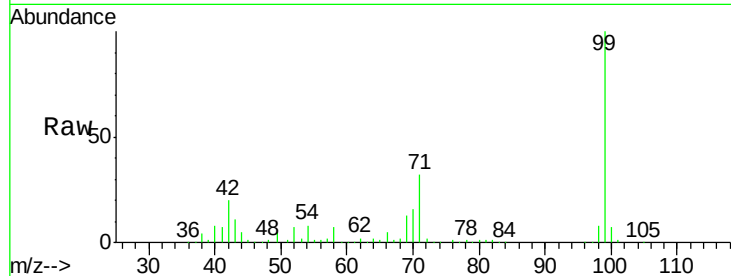

Abundance Ion 99.00 (98.70 to 99.70): BGC
Ion 42.00 (41.70 to 42.70): BGC
Ion 71.00 (70.70 to 71.70): BGC

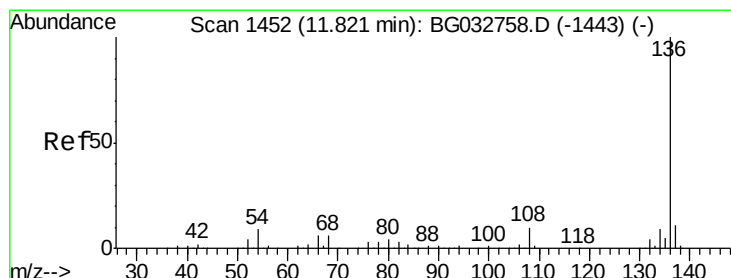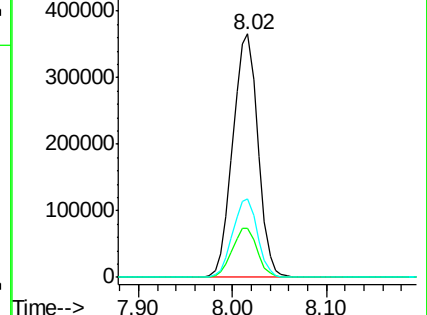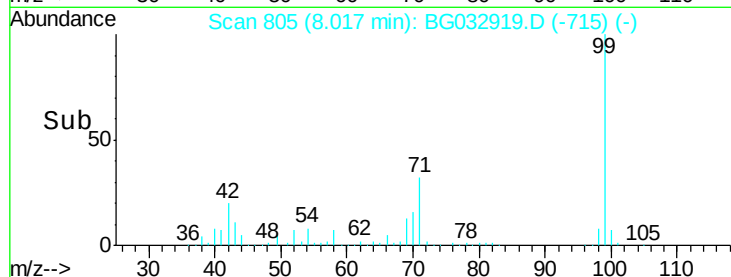

#21

Naphthalene-d8

Concen: 20.000 ng

RT: 11.81 min Scan# 1450

Delta R.T. 0.00 min

Lab File: BG032919.D

Acq: 1 Mar 2018 16:20

Tgt Ion: 136 Resp: 293222


Ion Ratio Lower Upper

136 100



137 11.3 9.2 13.8


54 8.9 10.3 15.5#

68 6.6 4.5 6.7

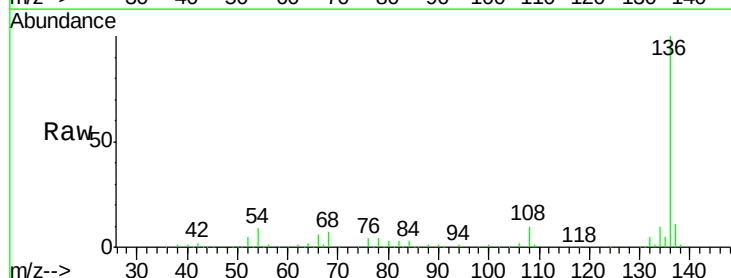

Abundance Ion 136.00 (135.70 to 136.70): BGC
Ion 137.00 (136.70 to 137.70): BGC
Ion 54.00 (53.70 to 54.70): BGC
Ion 68.00 (67.70 to 68.70): BGC

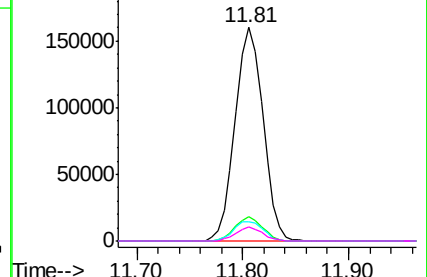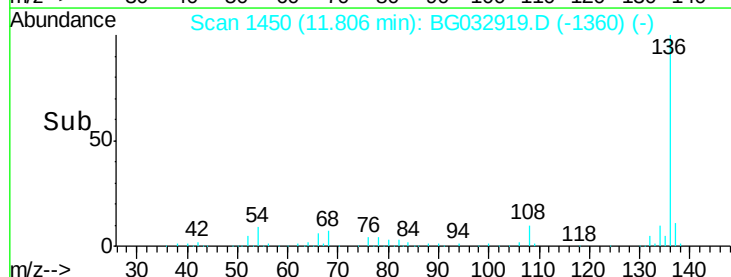


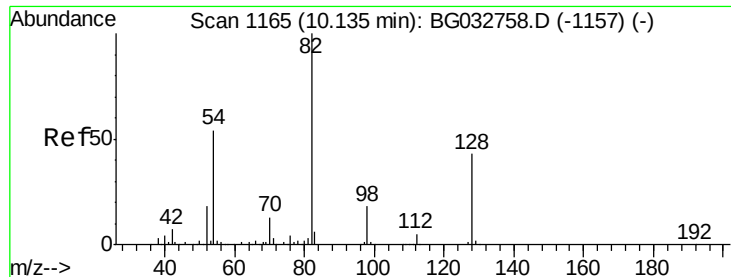




#23
 Nitrobenzene-d5
 Concen: 120.106 ng
 RT: 10.12 min Scan# 1163
 Delta R.T. 0.00 min
 Lab File: BG032919.D
 Acq: 1 Mar 2018 16:20

Instrument :
 BNA_G
 ClientSampleId :
 PL-01-022818-A

Tot Ion: 82 Resp: 527080
 Ion Ratio Lower Upper
 82 100
 128 44.3 29.7 44.5
 54 55.7 43.1 64.7

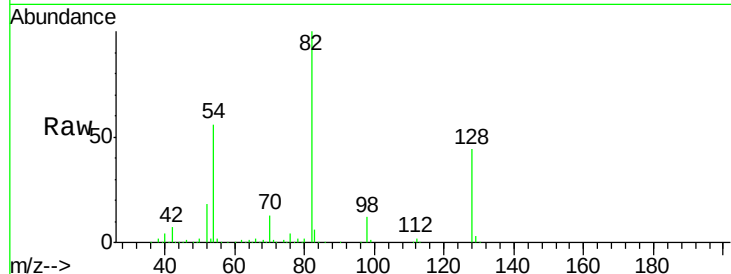


Abundance Ion 82.00 (81.70 to 82.70): BG032758.D (-1157) (-)
 Ion 128.00 (127.70 to 128.70): BG032758.D (-1157) (-)
 Ion 54.00 (53.70 to 54.70): BG032758.D (-1157) (-)

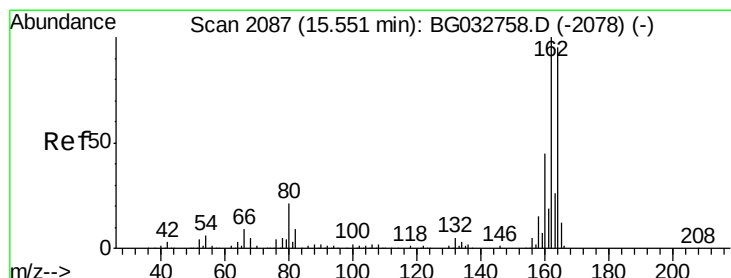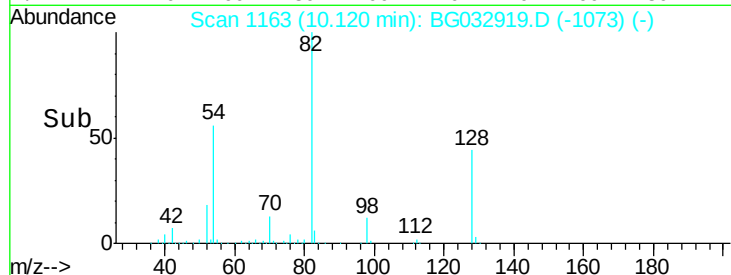
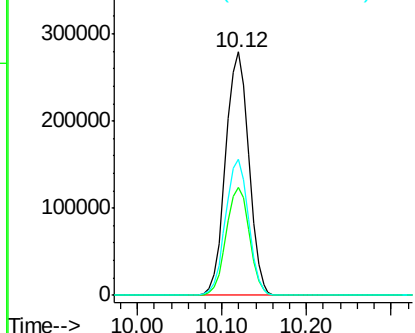



#38
 Acenaphthene-d10
 Concen: 20.000 ng
 RT: 15.53 min Scan# 2084
 Delta R.T. -0.01 min
 Lab File: BG032919.D
 Acq: 1 Mar 2018 16:20

Tgt Ion:164 Resp: 163698
 Ion Ratio Lower Upper
 164 100
 162 105.3 78.8 118.2
 160 46.9 35.4 53.0

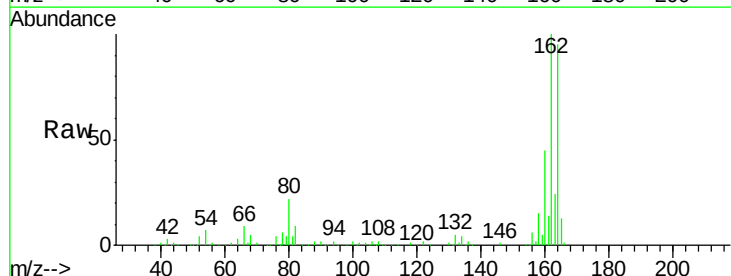

Abundance Ion 164.00 (163.70 to 164.70): BG032758.D (-2078) (-)
 Ion 162.00 (161.70 to 162.70): BG032758.D (-2078) (-)
 Ion 160.00 (159.70 to 160.70): BG032758.D (-2078) (-)

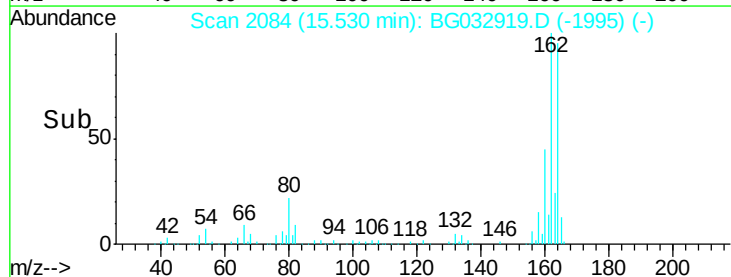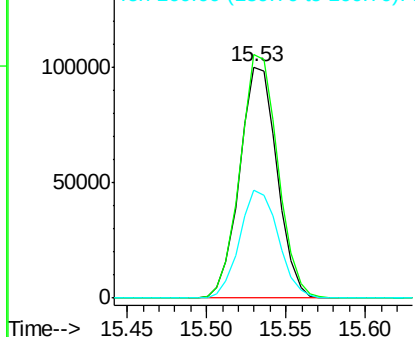


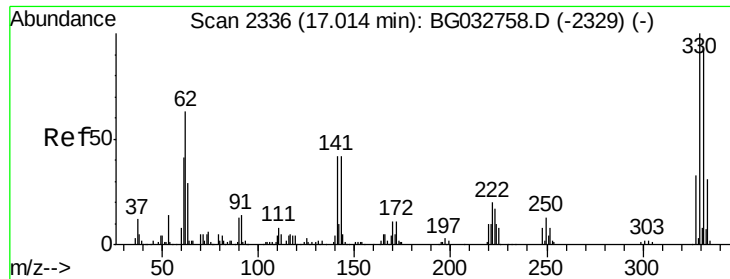




#41
 2,4,6-Tribromophenol
 Concen: 150.533 ng
 RT: 17.00 min Scan# 2335
 Delta R.T. 0.00 min
 Lab File: BG032919.D
 Acq: 1 Mar 2018 16:20

Instrument :
 BNA_G
 ClientSampleId :
 PL-01-022818-A

Tot Ion:330 Resp: 259101
 Ion Ratio Lower Upper
 330 100
 332 95.5 77.0 115.6
 141 44.6 25.2 37.8#

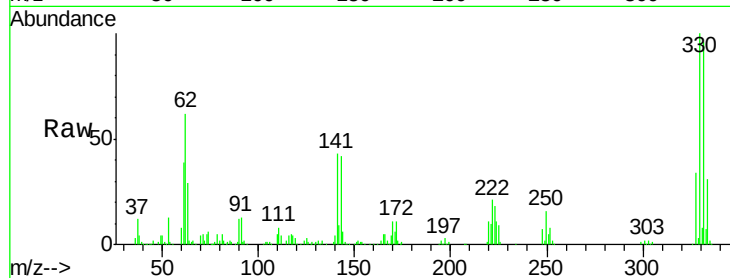


Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E

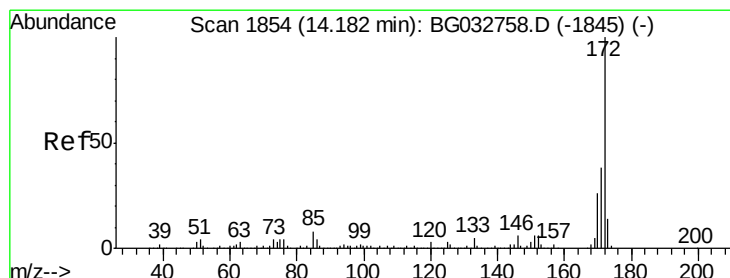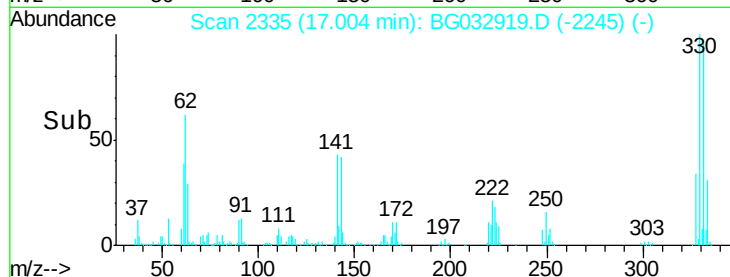
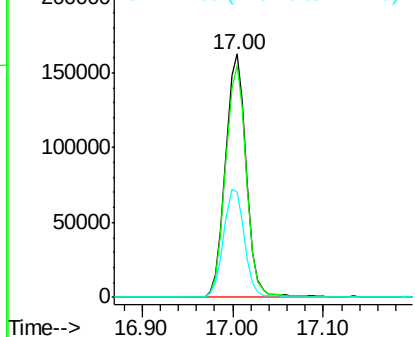



#44
 2-Fluorobiphenyl
 Concen: 101.714 ng
 RT: 14.17 min Scan# 1852
 Delta R.T. 0.00 min
 Lab File: BG032919.D
 Acq: 1 Mar 2018 16:20

Tgt Ion:172 Resp: 1154473
 Ion Ratio Lower Upper
 172 100
 171 38.6 30.0 45.0
 170 25.9 19.5 29.3

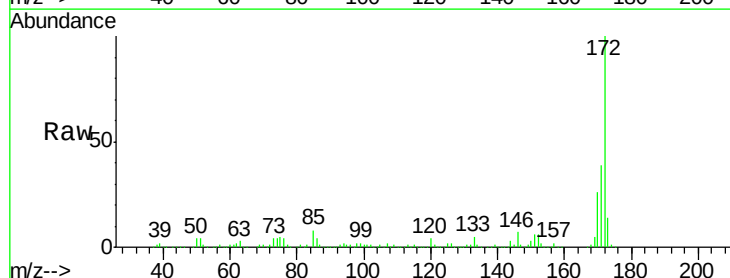

Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E

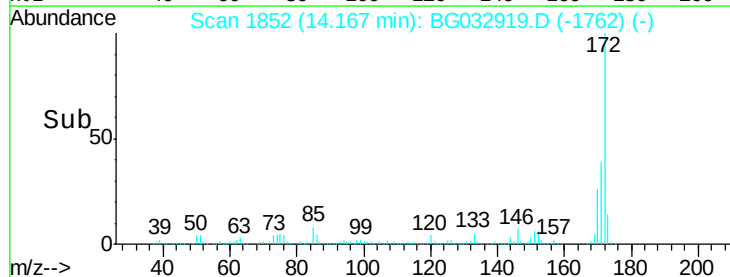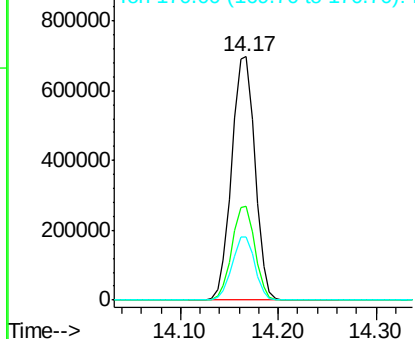

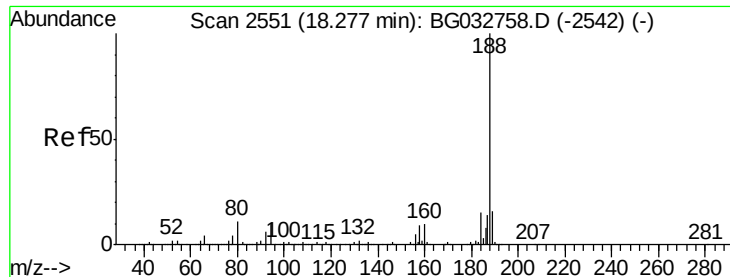

#63

Phenanthrene-d10

Concen: 20.000 ng

RT: 18.26 min Scan# 2549

Delta R.T. 0.00 min

Lab File: BG032919.D

Acq: 1 Mar 2018 16:20

Instrument :

BNA_G

ClientSampleId :

PL-01-022818-A


Tot Ion:188 Resp: 366728

Ion Ratio Lower Upper

188 100

94 9.9 6.9 10.3




80 11.1 7.7 11.5

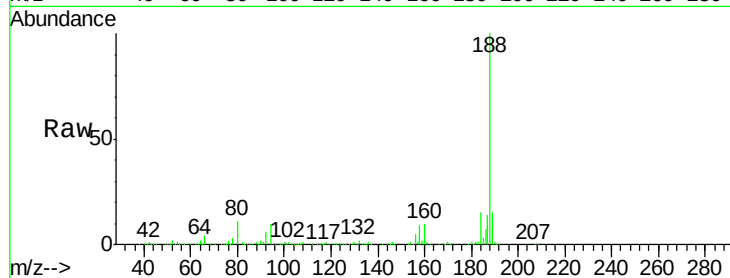

Abundance Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BGC

Ion 80.00 (79.70 to 80.70): BGC

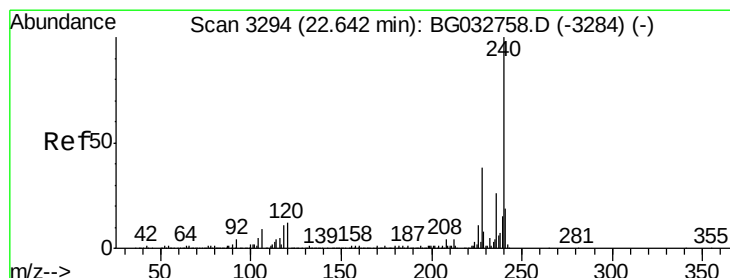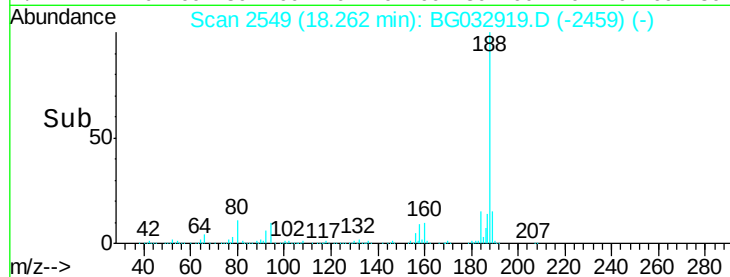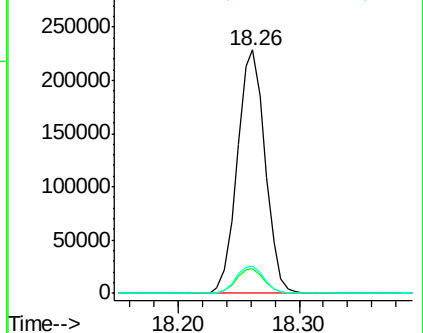

#75

Chrysene-d12

Concen: 20.000 ng

RT: 22.61 min Scan# 3290

Delta R.T. -0.01 min

Lab File: BG032919.D

Acq: 1 Mar 2018 16:20


Tgt Ion:240 Resp: 334426

Ion Ratio Lower Upper

240 100

120 13.0 6.8 10.2#



236 26.9 20.9 31.3

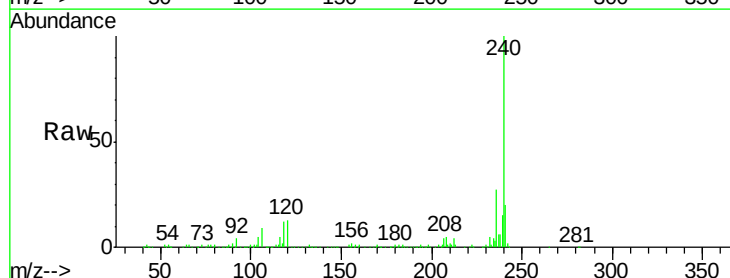


Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

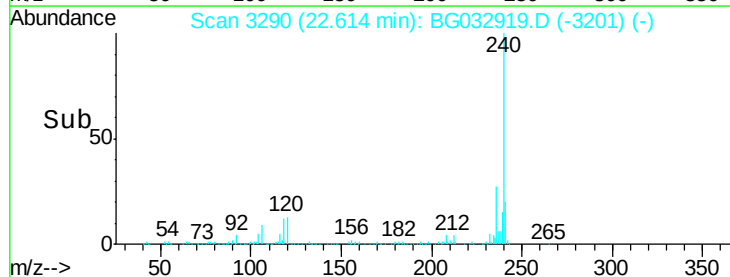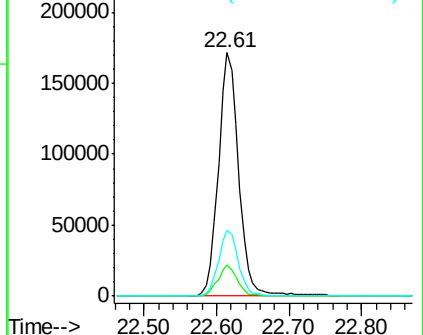

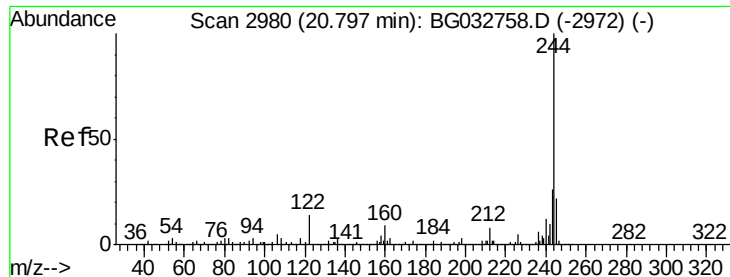

#78

Terphenyl-d14

Concen: 106.469 ng

RT: 20.78 min Scan# 2978

Delta R.T. 0.01 min

Lab File: BG032919.D

Acq: 1 Mar 2018 16:20

Instrument :

BNA_G

ClientSampleId :

PL-01-022818-A


Tot Ion:244 Resp: 1584787

Ion Ratio Lower Upper




244 100

212 8.7 5.8 8.8

122 13.8 7.0 10.4#

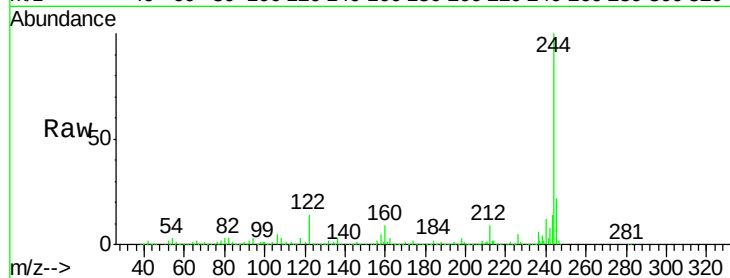

Abundance Ion 244.00 (243.70 to 244.70): E
Ion 212.00 (211.70 to 212.70): E
Ion 122.00 (121.70 to 122.70): E

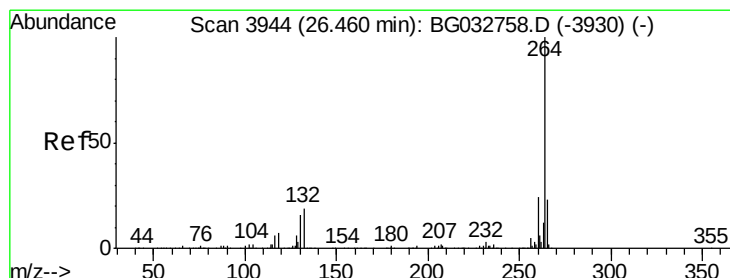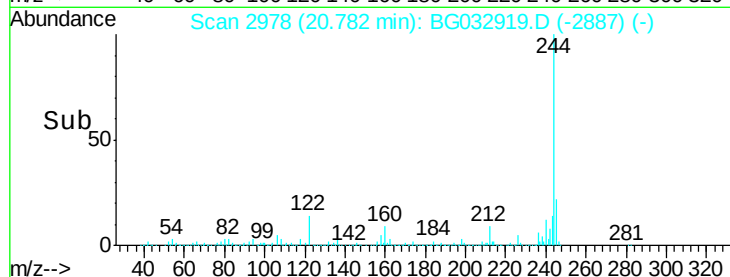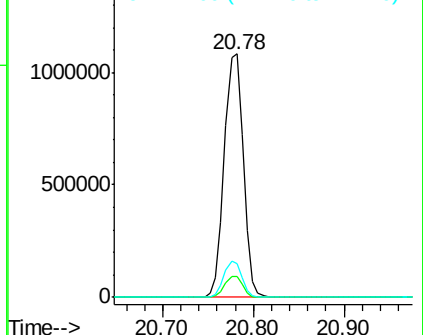

#86

Perylene-d12

Concen: 20.000 ng

RT: 26.42 min Scan# 3938

Delta R.T. -0.01 min

Lab File: BG032919.D

Acq: 1 Mar 2018 16:20


Tgt Ion:264 Resp: 316784

Ion Ratio Lower Upper

264 100

260 22.2 17.4 26.0

265 22.8 17.7 26.5

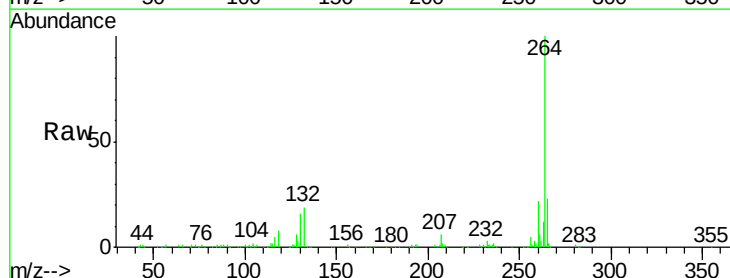

Abundance Ion 264.00 (263.70 to 264.70): E
Ion 260.00 (259.70 to 260.70): E
Ion 265.00 (264.70 to 265.70): E

