


Data Path : Z:\HPCHEM1\BNA G\Data\BG030118\
 Data File : BG032917.D
 Acq On : 1 Mar 2018 15:05
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG022118.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Mar 01 17:38:52 2018

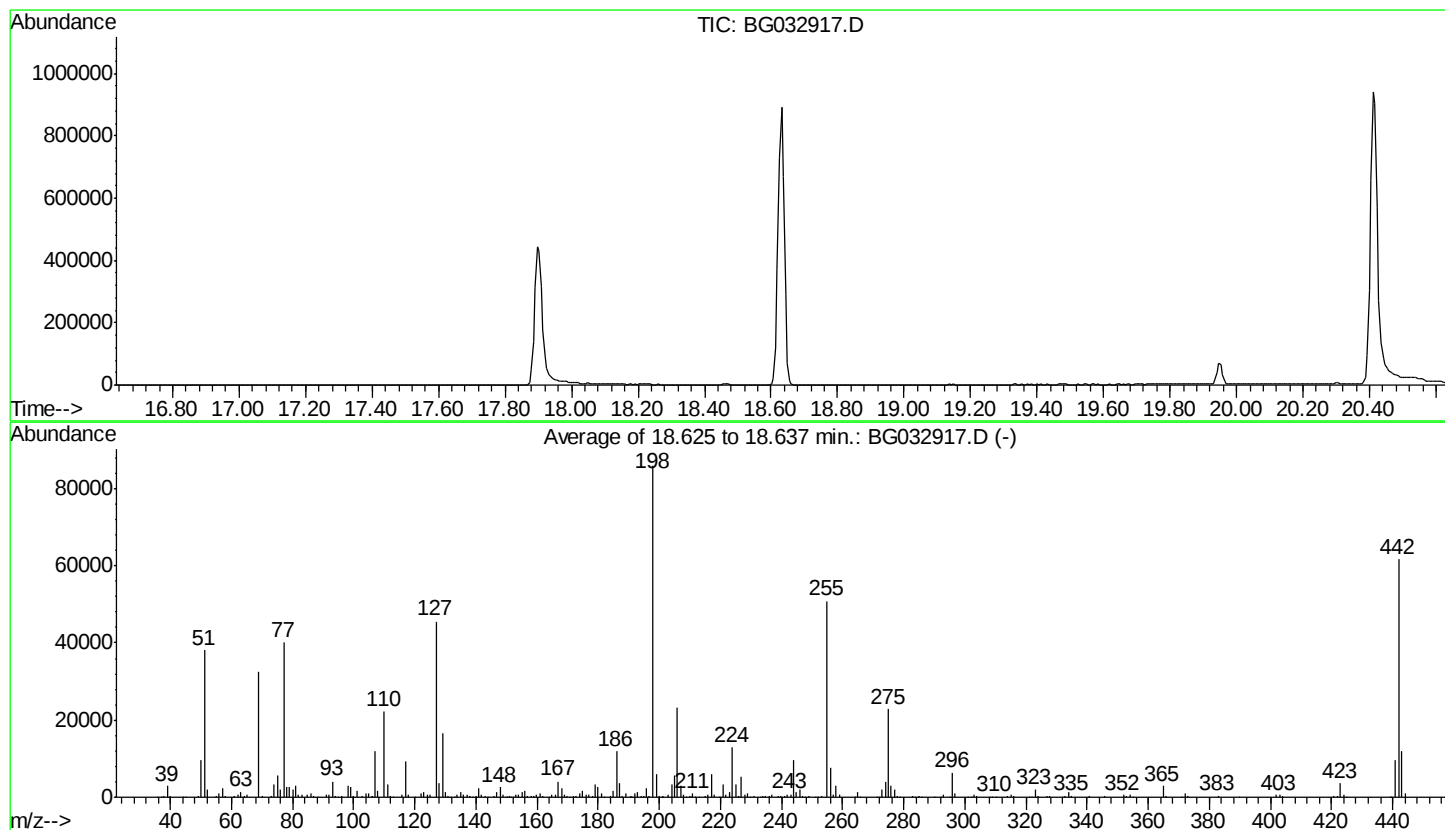

AutoFind: Scans 2611, 2612, 2613; Background Corrected with Scan 2604

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	44.3	38098	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	37.7	32384	PASS
70	69	0.00	2	0.9	297	PASS
127	198	10	80	53.0	45525	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	85968	PASS
199	198	5	9	6.9	5974	PASS
275	198	10	60	26.5	22768	PASS
365	198	1	100	3.5	2974	PASS
441	442	0.01	24	15.7	9659	PASS
442	198	50	100	71.8	61693	PASS
443	442	15	24	19.5	12014	PASS