


Data Path : Z:\HPCHEM1\BNA G\Data\BG030118\
 Data File : BG032936.D
 Acq On : 2 Mar 2018 4:18
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG022118.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Mar 01 17:38:52 2018

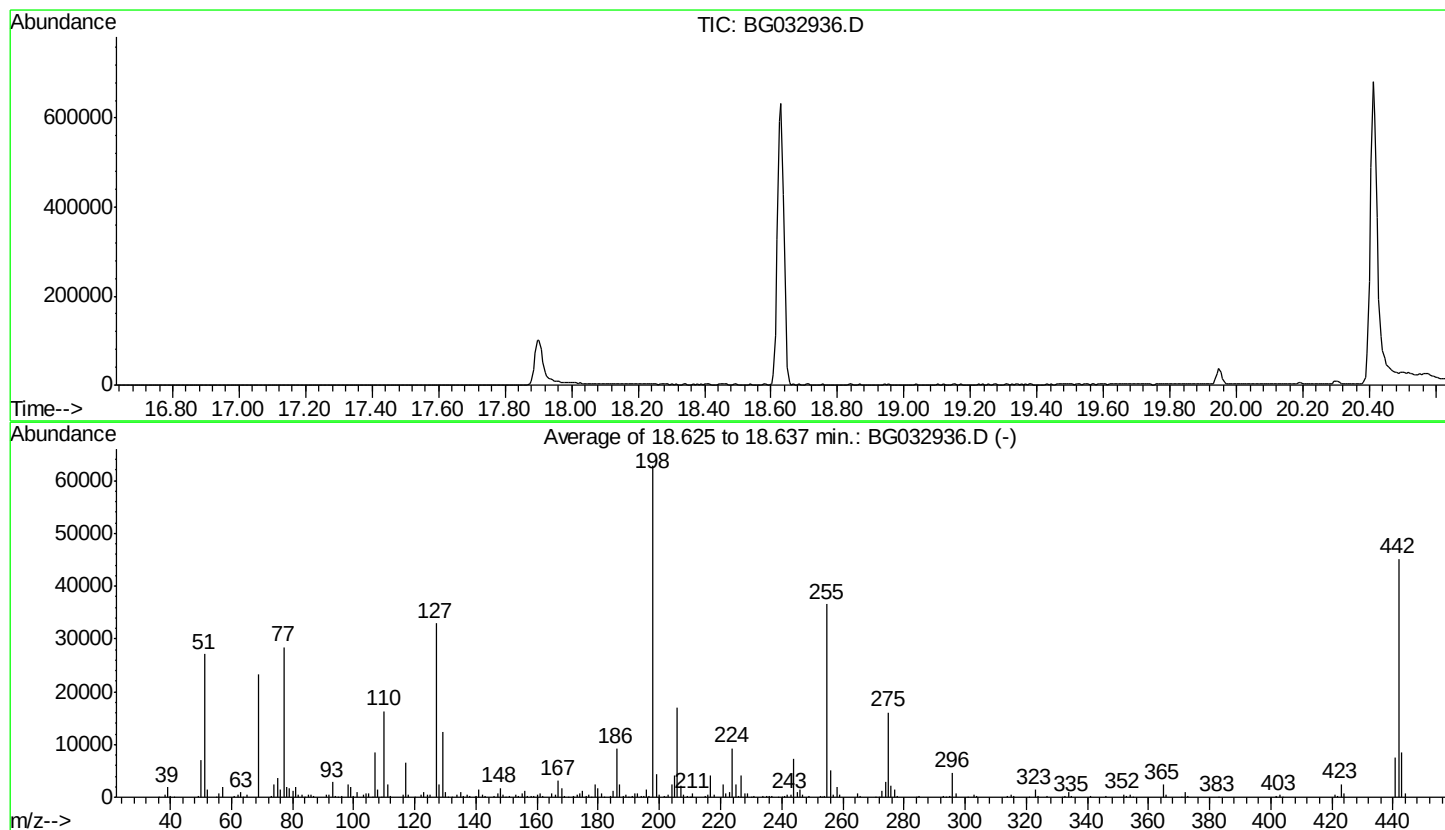

AutoFind: Scans 2611, 2612, 2613; Background Corrected with Scan 2604

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	43.1	27096	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	36.9	23204	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	52.4	32957	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	62842	PASS
199	198	5	9	7.0	4407	PASS
275	198	10	60	25.6	16118	PASS
365	198	1	100	3.7	2339	PASS
441	442	0.01	24	16.4	7434	PASS
442	198	50	100	72.0	45237	PASS
443	442	15	24	19.0	8579	PASS