

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG030122\
 Data File : BG052524.D
 Acq On : 1 Mar 2022 18:18
 Operator : CG/JU
 Sample : N1688-20
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 MW-37

Quant Time: Mar 02 01:52:32 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG020722.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Feb 08 01:21:20 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.217	152	30587	20.000	ng	0.00
21) Naphthalene-d8	11.054	136	119281	20.000	ng	#-0.01
39) Acenaphthene-d10	14.867	164	82716	20.000	ng	0.00
64) Phenanthrene-d10	17.616	188	186343	20.000	ng	0.00
76) Chrysene-d12	21.928	240	195328	20.000	ng	-0.01
86) Perylene-d12	25.394	264	203738	20.000	ng	-0.01
System Monitoring Compounds						
5) 2-Fluorophenol	5.756	112	115099	65.584	ng	0.00
7) Phenol-d6	7.365	99	95485	35.262	ng	0.00
23) Nitrobenzene-d5	9.392	82	237934	86.693	ng	0.00
42) 2,4,6-Tribromophenol	16.353	330	157713	132.716	ng	0.00
45) 2-Fluorobiphenyl	13.486	172	539219	90.583	ng	0.00
79) Terphenyl-d14	20.213	244	884408	79.955	ng	0.00
Target Compounds						
						Qvalue
19) n-Nitroso-di-n-propyla...	9.392	70	32709	16.023	ng	# 74
51) 2,6-Dinitrotoluene	14.867	165	10967	8.020	ng	# 16
57) 2,4-Dinitrotoluene	14.867	165	10967	5.635	ng	# 15
67) 4-Bromophenyl-phenylether	16.353	248	10042	4.431	ng	# 1
77) Benzidine	20.207	184	12857	3.080	ng	# 90


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG030122\
Data File : BG052524.D
Acq On : 1 Mar 2022 18:18
Operator : CG/JU
Sample : N1688-20
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
MW-37

Quant Time: Mar 02 01:52:32 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG020722.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Feb 08 01:21:20 2022
Response via : Initial Calibration




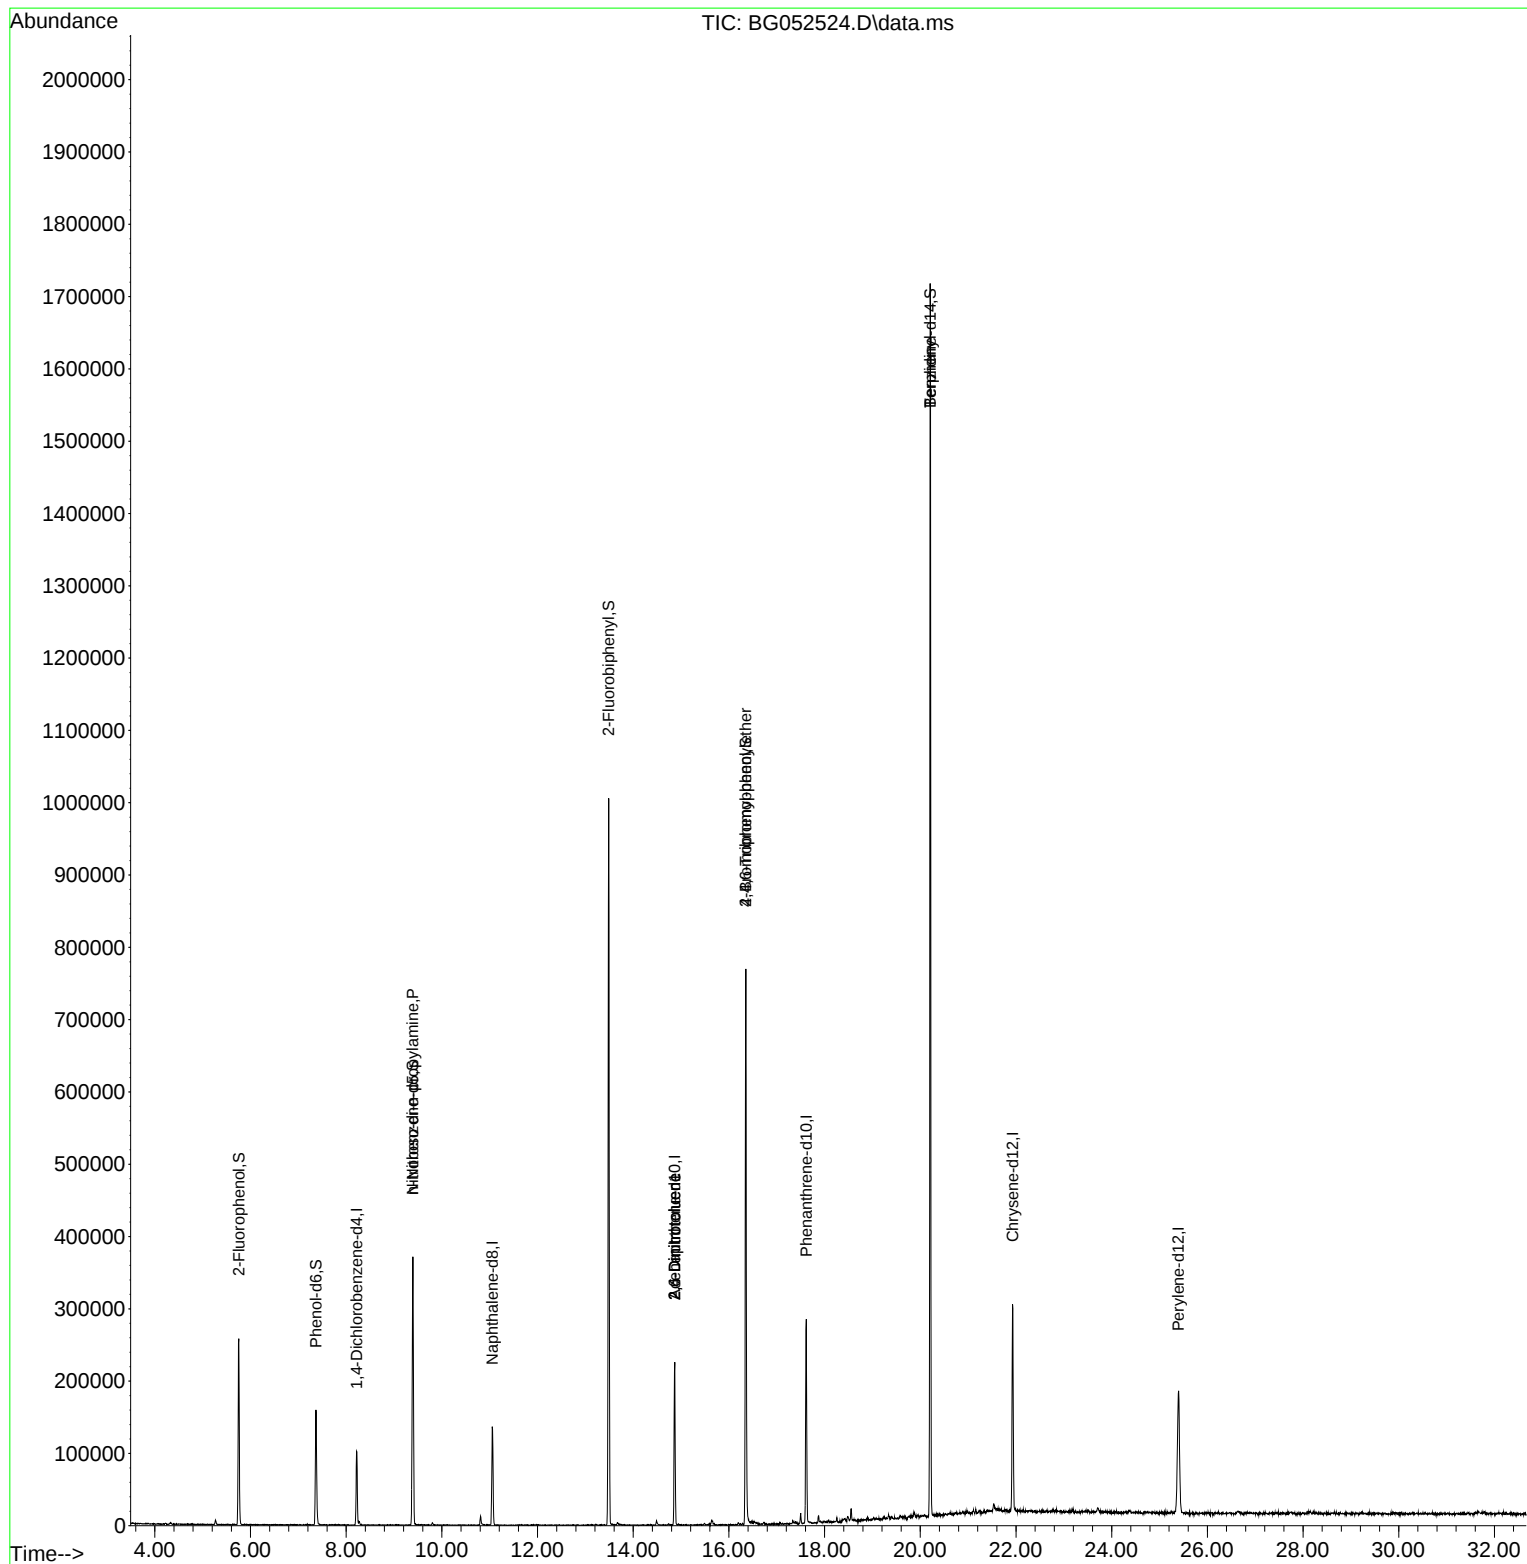




#1
1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 8.217 min Scan# 806
Delta R.T. -0.006 min
Lab File: BG052524.D
Acq: 1 Mar 2022 18:18




Instrument :
BNA_G
ClientSampleId :
MW-37


Tgt Ion:152 Resp: 30587
Ion Ratio Lower Upper
152 100
150 159.1 117.8 176.8
115 57.1 50.2 75.2

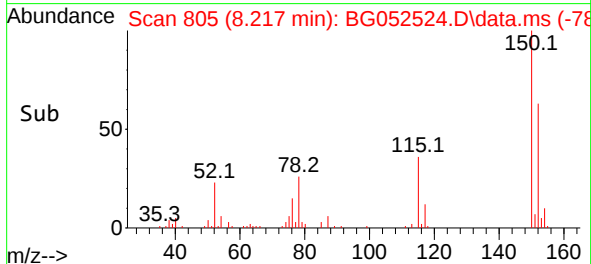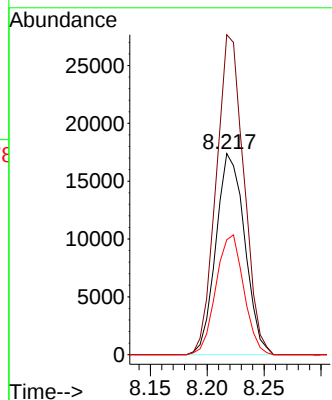

#5
2-Fluorophenol
Concen: 65.584 ng
RT: 5.756 min Scan# 386
Delta R.T. 0.006 min
Lab File: BG052524.D
Acq: 1 Mar 2022 18:18

Tgt Ion:112 Resp: 115099
Ion Ratio Lower Upper
112 100
64 62.0 60.4 90.6
63 35.0 33.3 49.9


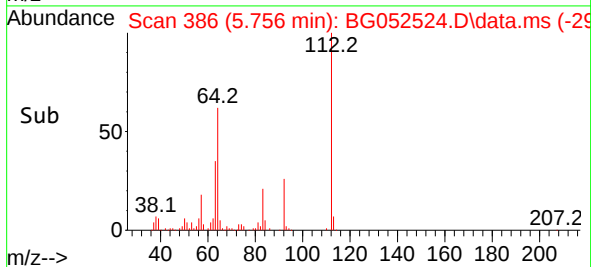
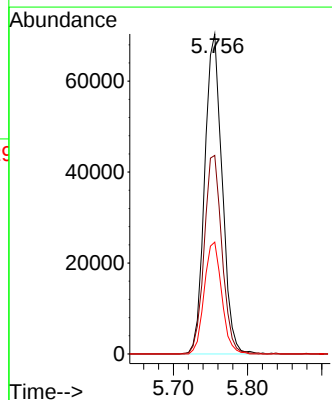
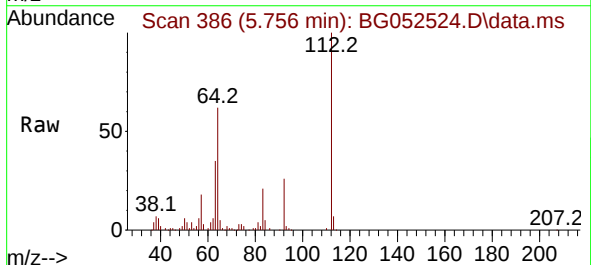


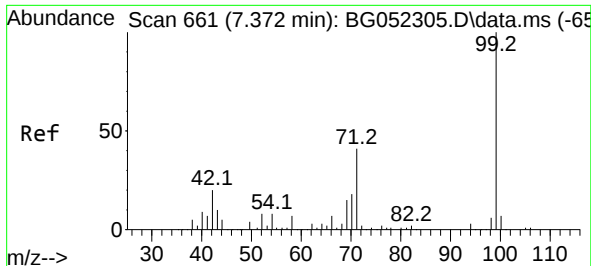

#7
Phenol-d6
Concen: 35.262 ng
RT: 7.365 min Scan# 60
Delta R.T. -0.006 min
Lab File: BG052524.D
Acq: 1 Mar 2022 18:18




Instrument :
BNA_G
ClientSampleId :
MW-37


Tgt Ion: 99 Resp: 95485
Ion Ratio Lower Upper
99 100
42 17.9 19.1 28.7#
71 37.3 33.4 50.2

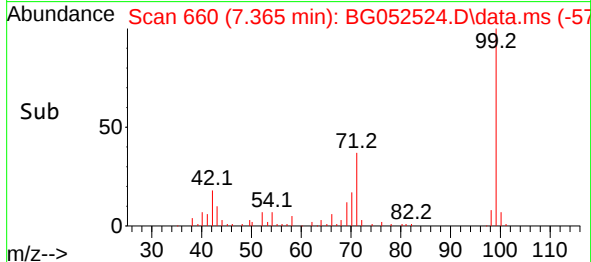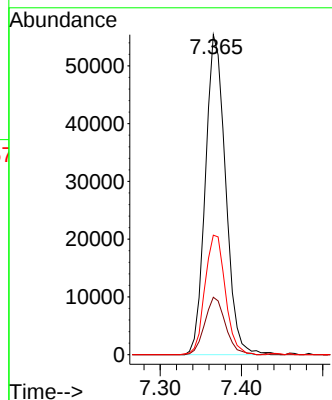

#19
n-Nitroso-di-n-propylamine
Concen: 16.023 ng
RT: 9.392 min Scan# 1005
Delta R.T. 0.364 min
Lab File: BG052524.D
Acq: 1 Mar 2022 18:18

Tgt Ion: 70 Resp: 32709
Ion Ratio Lower Upper
70 100
42 46.1 51.8 77.6#
101 0.0 6.6 10.0#
130 2.9 14.7 22.1#

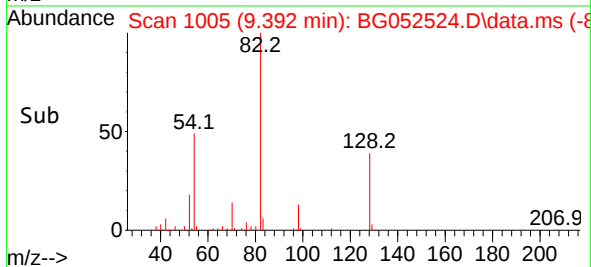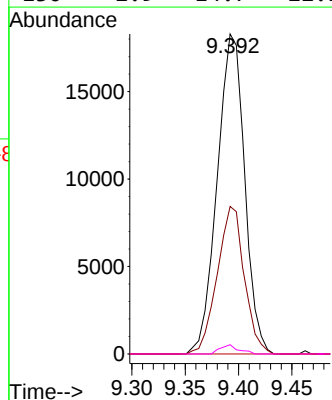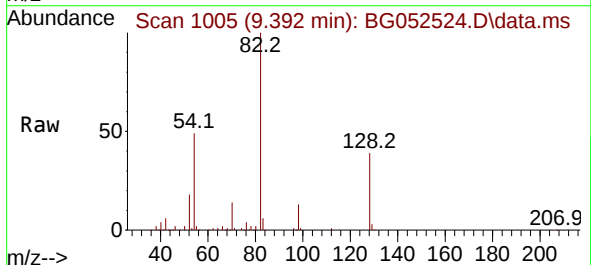



#21

Naphthalene-d8

Concen: 20.000 ng

RT: 11.054 min Scan# 11

Delta R.T. -0.013 min

Lab File: BG052524.D

Acq: 1 Mar 2022 18:18

Instrument :

BNA_G

ClientSampleId :

MW-37

Tgt Ion:136 Resp: 119281





Ion Ratio Lower Upper

136 100

137 10.5 9.1 13.7

54 7.9 8.3 12.5#

68 6.2 4.5 6.7

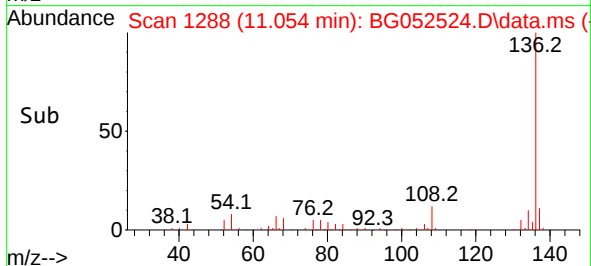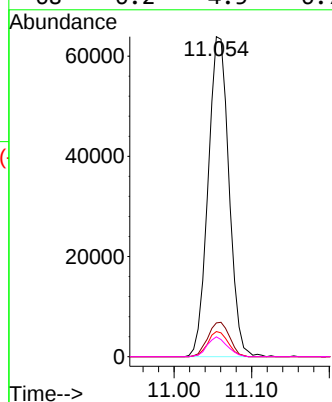

#23

Nitrobenzene-d5

Concen: 86.693 ng

RT: 9.392 min Scan# 1005

Delta R.T. -0.006 min

Lab File: BG052524.D

Acq: 1 Mar 2022 18:18




Tgt Ion: 82 Resp: 237934


Ion Ratio Lower Upper

82 100

128 39.1 27.0 40.4

54 48.8 41.0 61.6


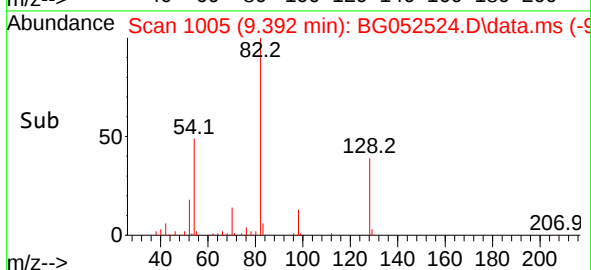
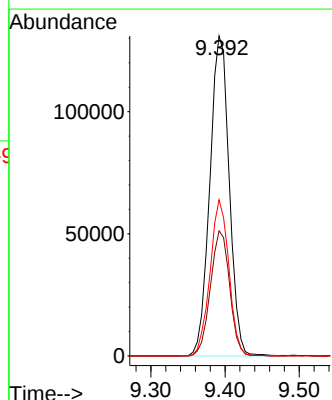
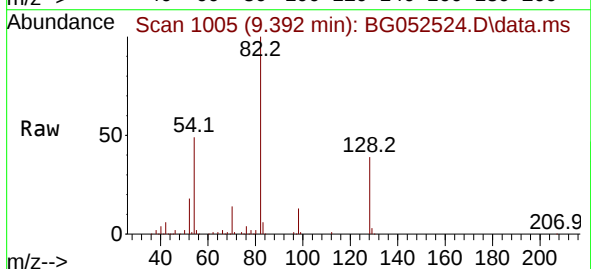


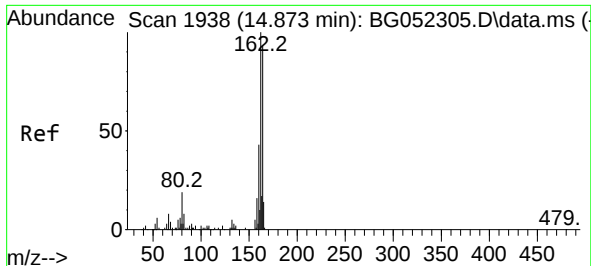

#39
Acenaphthene-d10
Concen: 20.000 ng
RT: 14.867 min Scan# 1937
Delta R.T. -0.006 min
Lab File: BG052524.D
Acq: 1 Mar 2022 18:18




Instrument :
BNA_G
ClientSampleId :
MW-37


Tgt Ion:164 Resp: 82716
Ion Ratio Lower Upper
164 100
162 101.0 82.2 123.2
160 44.2 36.2 54.2

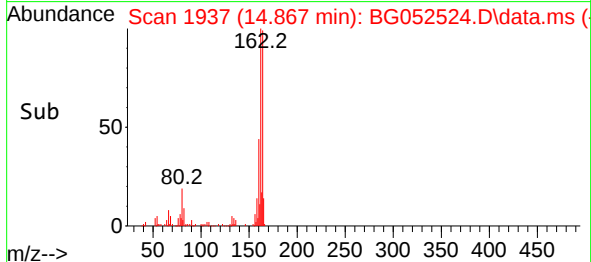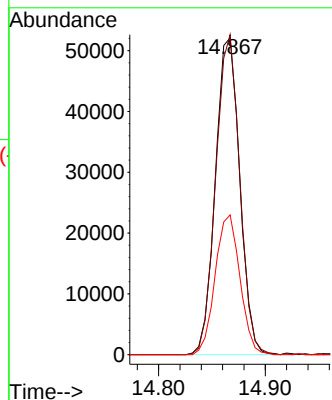

#42
2,4,6-Tribromophenol
Concen: 132.716 ng
RT: 16.353 min Scan# 2190
Delta R.T. -0.006 min
Lab File: BG052524.D
Acq: 1 Mar 2022 18:18

Tgt Ion:330 Resp: 157713
Ion Ratio Lower Upper
330 100
332 96.8 78.6 117.8
141 32.1 28.8 43.2

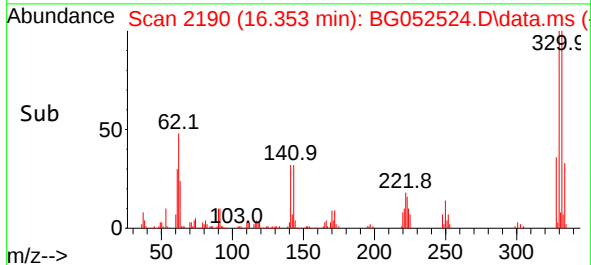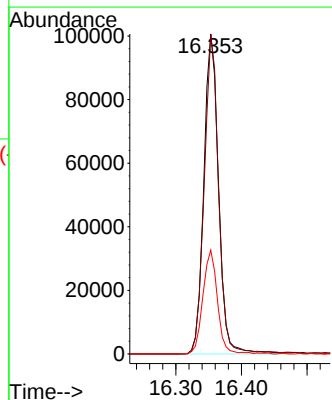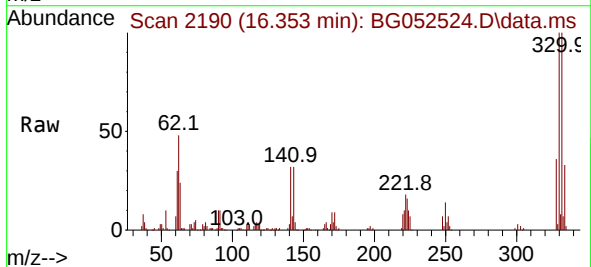



#45

2-Fluorobiphenyl

Concen: 90.583 ng

RT: 13.486 min Scan# 1

Delta R.T. -0.006 min

Lab File: BG052524.D

Acq: 1 Mar 2022 18:18

Instrument :

BNA_G

ClientSampleId :

MW-37





Tgt Ion:172 Resp: 539219

Ion Ratio Lower Upper

172 100

171 34.9 28.3 42.5

170 23.2 18.3 27.5

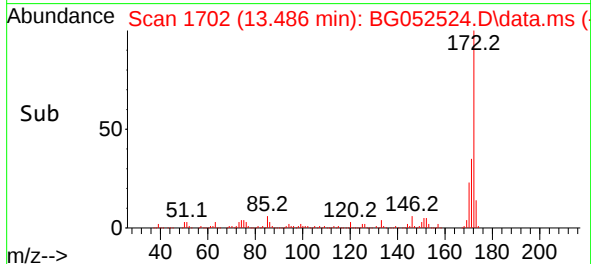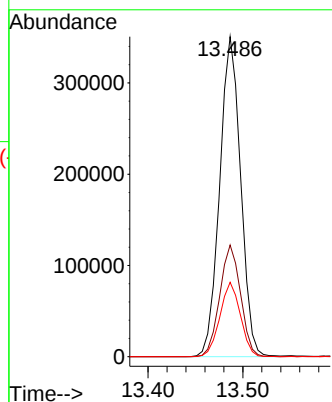

#51

2,6-Dinitrotoluene

Concen: 8.020 ng

RT: 14.867 min Scan# 1937

Delta R.T. 0.434 min

Lab File: BG052524.D

Acq: 1 Mar 2022 18:18




Tgt Ion:165 Resp: 10967


Ion Ratio Lower Upper

165 100

63 0.0 59.0 88.4#

89 0.0 49.4 74.0#

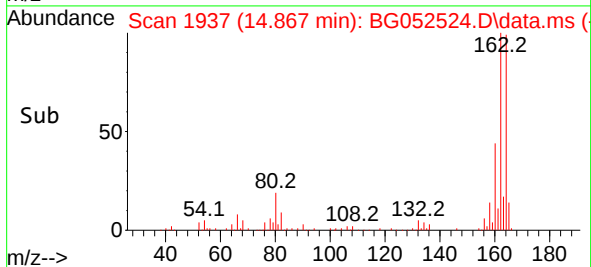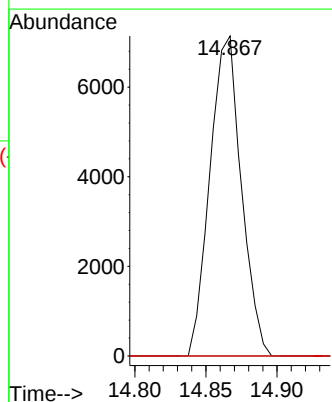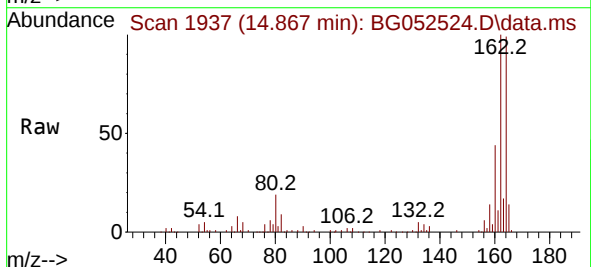

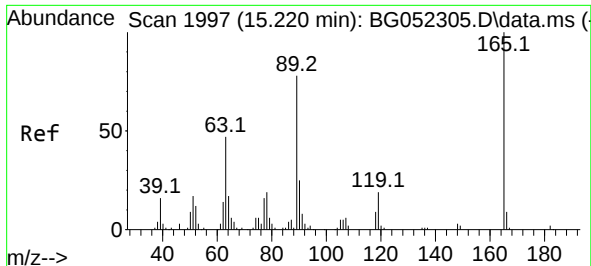

#57

2,4-Dinitrotoluene

Concen: 5.635 ng

RT: 14.867 min Scan# 19

Delta R.T. -0.353 min

Lab File: BG052524.D


Acq: 1 Mar 2022 18:18

Instrument :

BNA_G

ClientSampleId :

MW-37

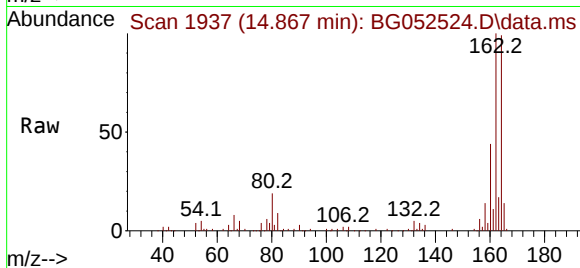

Tgt Ion:165 Resp: 10967




Ion Ratio Lower Upper

165 100

63 0.0 44.6 66.8#

89 0.0 67.4 101.0#

182 0.0 1.6 2.4#

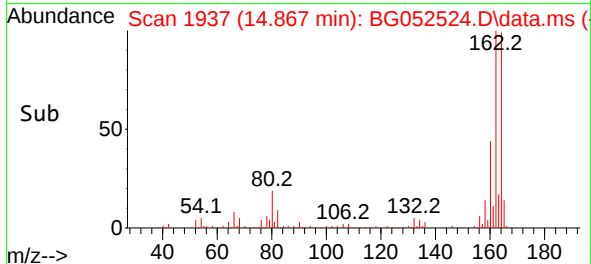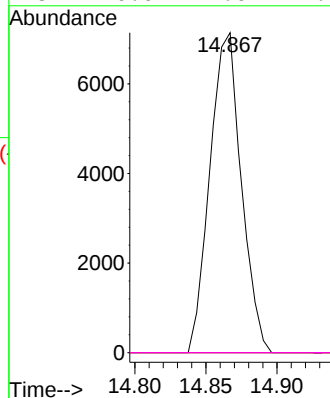

#64

Phenanthrene-d10

Concen: 20.000 ng

RT: 17.616 min Scan# 2405

Delta R.T. -0.006 min

Lab File: BG052524.D

Acq: 1 Mar 2022 18:18




Tgt Ion:188 Resp: 186343


Ion Ratio Lower Upper

188 100

94 6.5 5.9 8.9

80 8.8 6.6 10.0


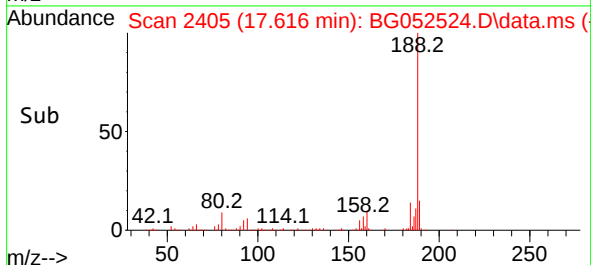
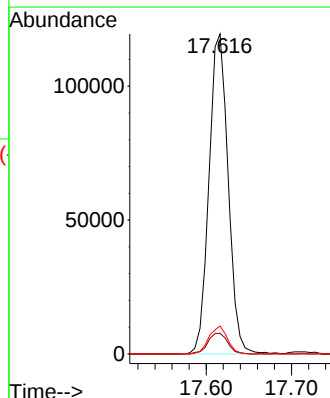
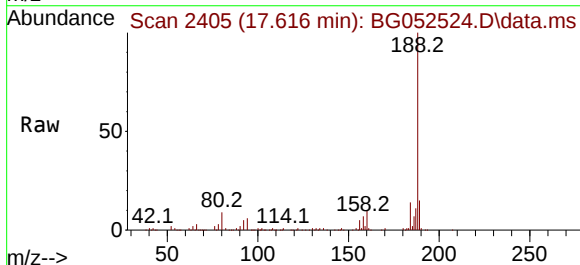




#67
4-Bromophenyl-phenylether
Concen: 4.431 ng
RT: 16.353 min Scan# 2190
Delta R.T. -0.447 min
Lab File: BG052524.D
Acq: 1 Mar 2022 18:18




Instrument :
BNA_G
ClientSampleId :
MW-37


Tgt Ion:248 Resp: 10042
Ion Ratio Lower Upper
248 100
250 189.6 79.6 119.4#
141 455.7 54.6 81.8#

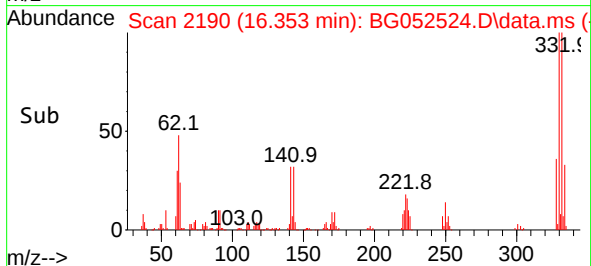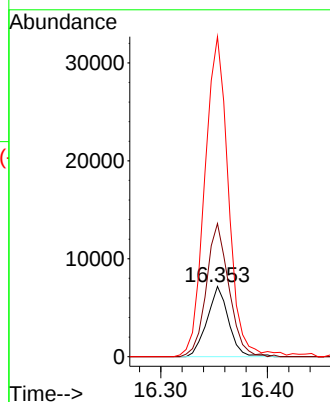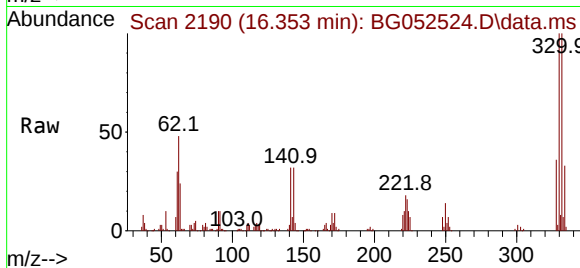

#76
Chrysene-d12
Concen: 20.000 ng
RT: 21.928 min Scan# 3139
Delta R.T. -0.012 min
Lab File: BG052524.D
Acq: 1 Mar 2022 18:18

Tgt Ion:240 Resp: 195328
Ion Ratio Lower Upper
240 100
120 6.4 4.4 6.6
236 24.2 20.8 31.2



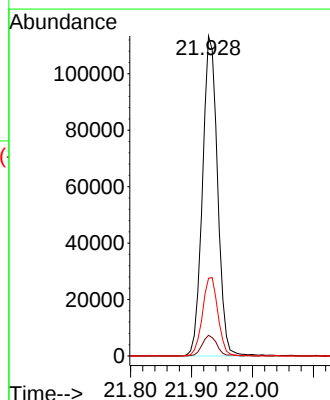
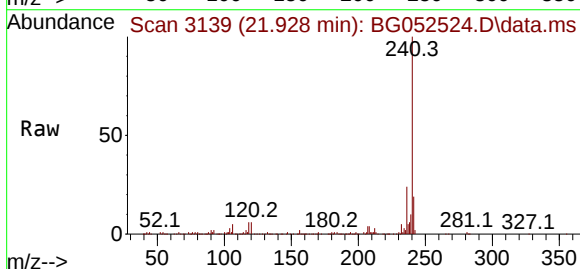


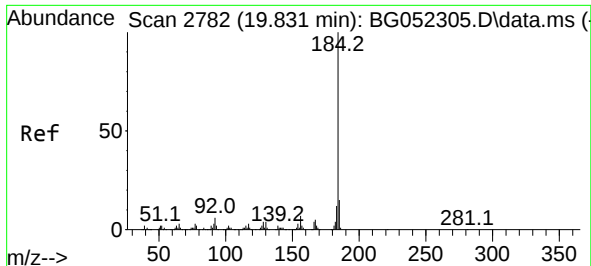

#77
Benzidine
Concen: 3.080 ng
RT: 20.207 min Scan# 21
Delta R.T. 0.376 min
Lab File: BG052524.D
Acq: 1 Mar 2022 18:18




Instrument :
BNA_G
ClientSampleId :
MW-37


Tgt Ion:184 Resp: 12857
Ion Ratio Lower Upper
184 100
185 17.1 11.8 17.8
183 6.1 9.8 14.6#

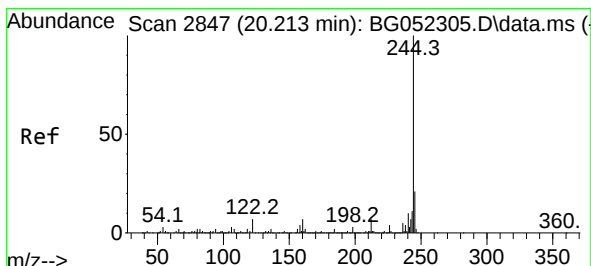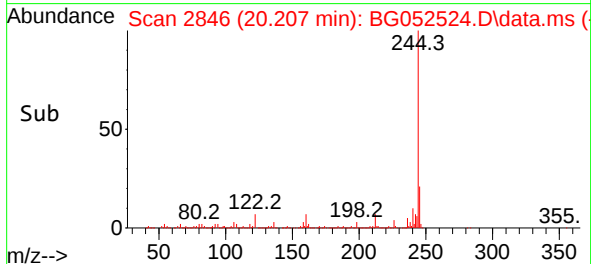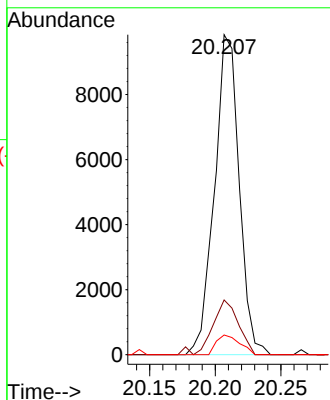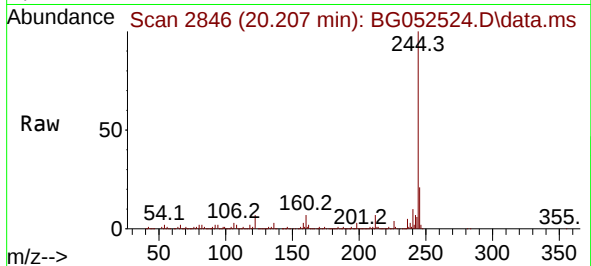

#79
Terphenyl-d14
Concen: 79.955 ng
RT: 20.213 min Scan# 2847
Delta R.T. -0.000 min
Lab File: BG052524.D
Acq: 1 Mar 2022 18:18

Tgt Ion:244 Resp: 884408
Ion Ratio Lower Upper
244 100
212 6.6 6.0 9.0
122 6.7 6.2 9.4

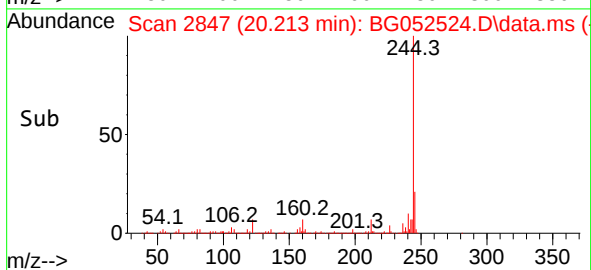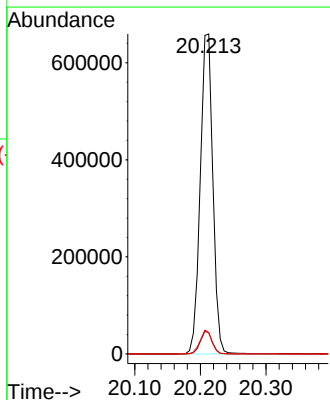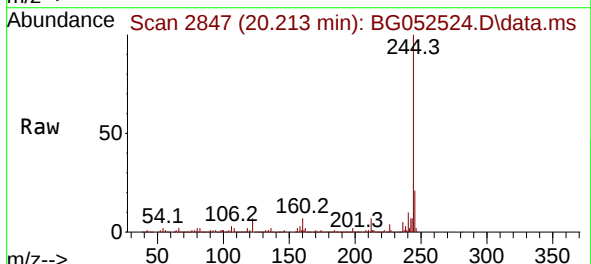



#86
 Perylene-d12
 Concen: 20.000 ng
 RT: 25.394 min Scan# 31
 Delta R.T. -0.012 min
 Lab File: BG052524.D
 Acq: 1 Mar 2022 18:18

Instrument :
 BNA_G
 ClientSampleId :
 MW-37

Tgt Ion:264 Resp: 203738
 Ion Ratio Lower Upper
 264 100
 260 23.1 18.5 27.7
 265 21.8 17.8 26.6

