

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG030122\
 Data File : BG052526.D
 Acq On : 1 Mar 2022 19:36
 Operator : CG/JU
 Sample : N1709-01
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 PPSP-B18-18.0-18.5

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG020722.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BG052526.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.756	379	386	396	rBV	395257	640131	39.05%	8.519%
2	7.371	654	661	674	rVB	398979	703632	42.93%	9.364%
3	8.217	799	805	811	rBV	98287	170189	10.38%	2.265%
4	9.392	996	1005	1015	rBV2	256511	456165	27.83%	6.071%
5	10.808	1240	1246	1255	rBV2	12618	23393	1.43%	0.311%
6	11.060	1282	1289	1296	rBV	131853	241411	14.73%	3.213%
7	13.486	1695	1702	1711	rBV	679797	1043260	63.65%	13.884%
8	14.068	1795	1801	1812	rBV2	18107	28675	1.75%	0.382%
9	14.867	1930	1937	1945	rVB	215389	332924	20.31%	4.431%
10	16.353	2183	2190	2203	rBV	468179	763252	46.57%	10.158%
11	17.616	2398	2405	2414	rBV	276356	423409	25.83%	5.635%
12	20.207	2840	2846	2854	rVB	1253759	1639080	100.00%	21.813%
13	21.523	3066	3070	3075	rBV6	12387	23806	1.45%	0.317%
14	21.928	3131	3139	3147	rBV	287228	503039	30.69%	6.695%
15	25.394	3718	3729	3742	rBV3	166079	521782	31.83%	6.944%




Sum of corrected areas: 7514148

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG030122\
Data File : BG052526.D
Acq On : 1 Mar 2022 19:36
Operator : CG/JU
Sample : N1709-01
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
PPSP-B18-18.0-18.5

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG020722.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

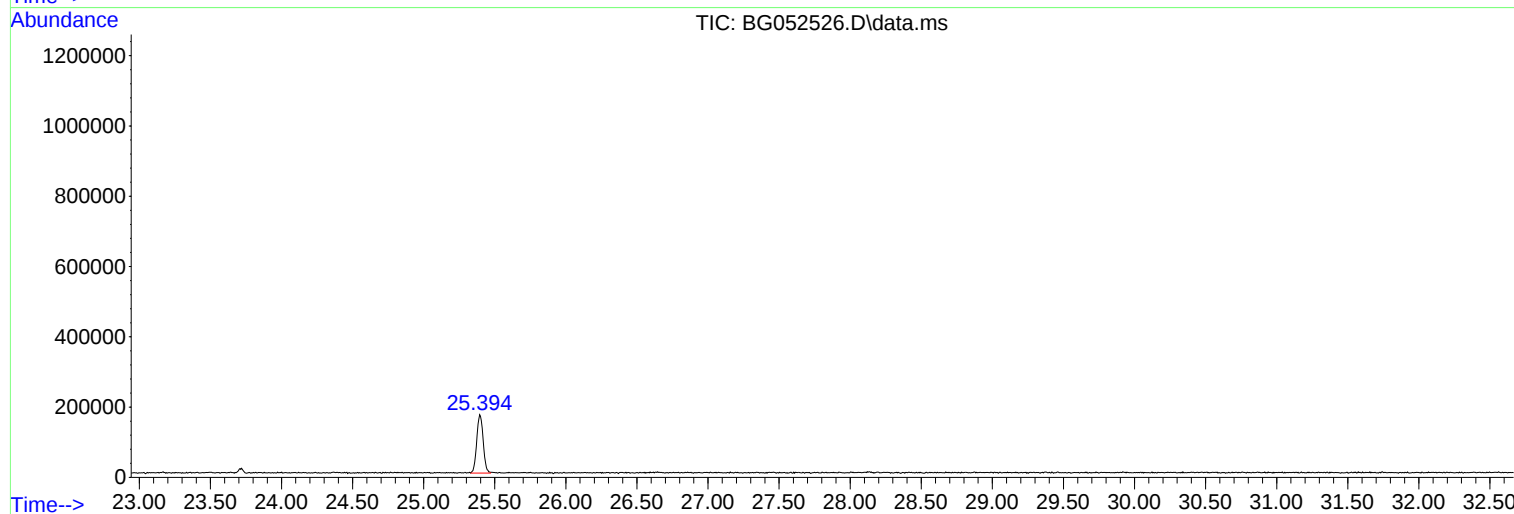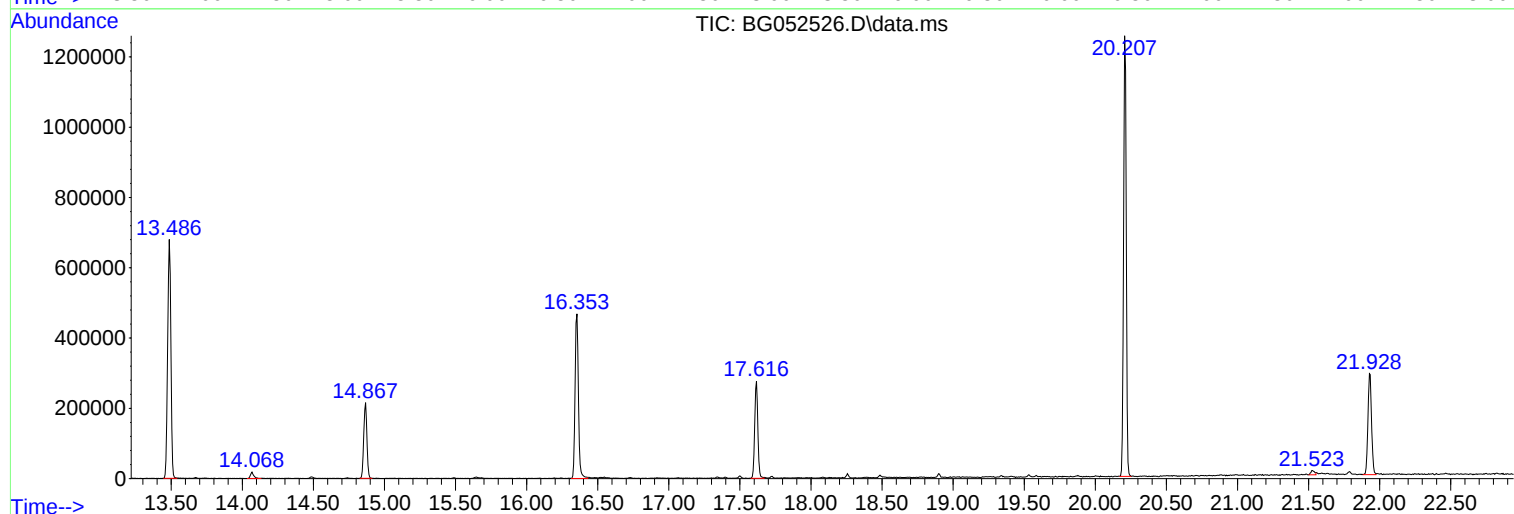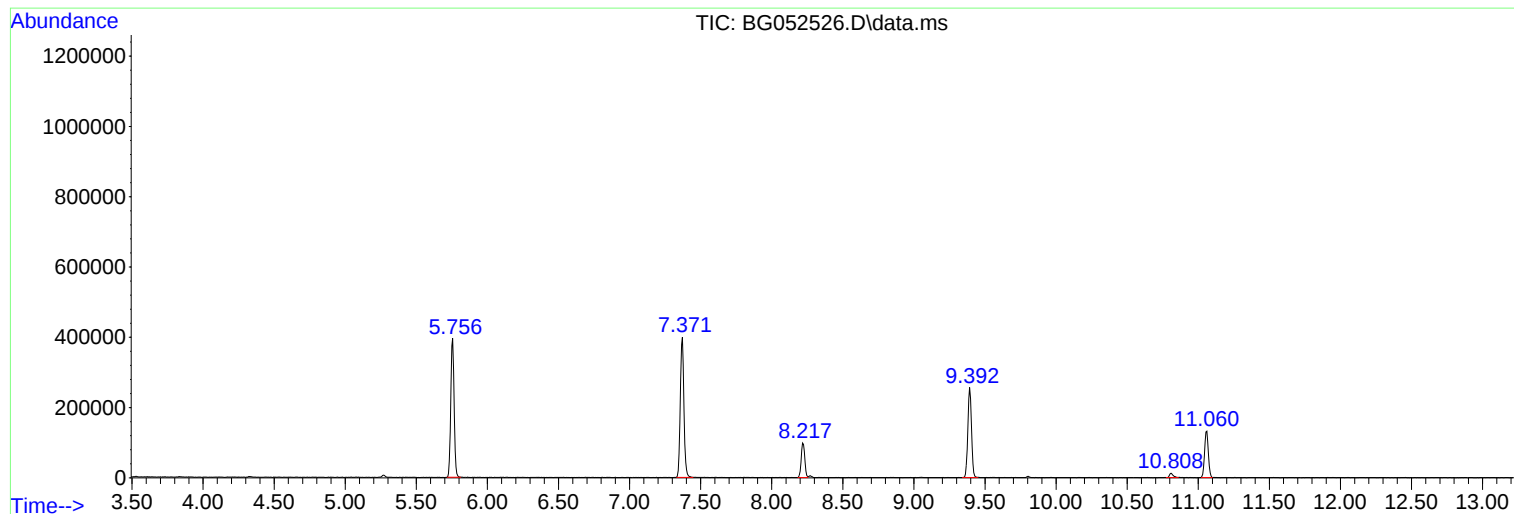

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG030122\
Data File : BG052526.D
Acq On : 1 Mar 2022 19:36
Operator : CG/JU
Sample : N1709-01
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
PPSP-B18-18.0-18.5

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG020722.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG030122\
Data File : BG052526.D
Acq On : 1 Mar 2022 19:36
Operator : CG/JU
Sample : N1709-01
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
PPSP-B18-18.0-18.5

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG020722.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------