


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG030122\
 Data File : BG052512.D
 Acq On : 1 Mar 2022 10:28
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG020722.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Feb 08 01:21:20 2022

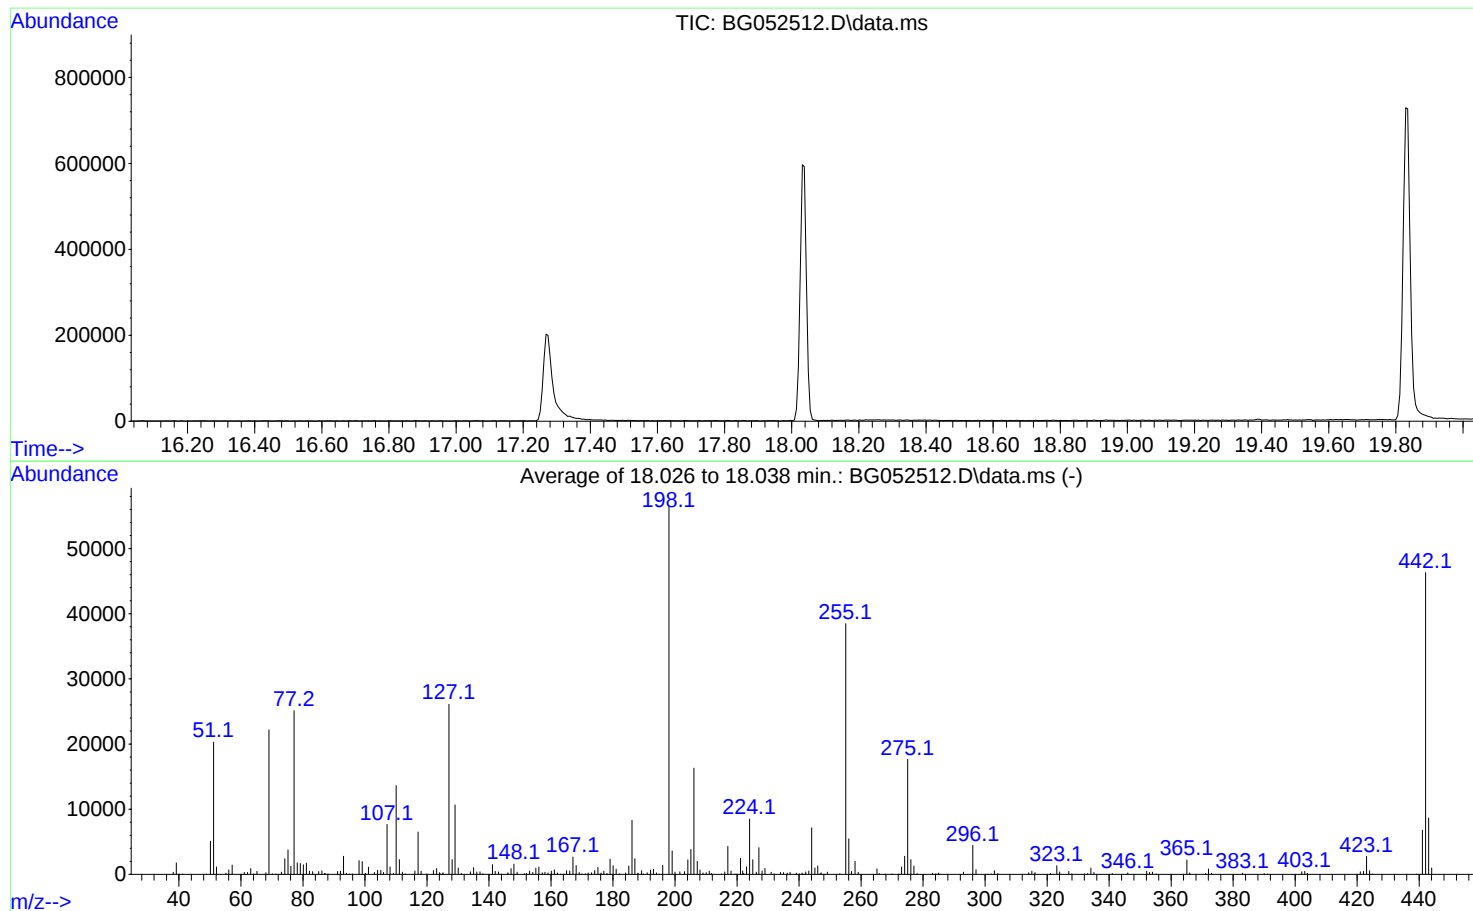




AutoFind: Scans 2475, 2476, 2477; Background Corrected with Scan 2469

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	35.9	20283	PASS
68	69	0.00	2	1.1	239	PASS
69	198	0.00	100	39.3	22168	PASS
70	69	0.00	2	0.3	69	PASS
127	198	10	80	46.3	26112	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	56453	PASS
199	198	5	9	6.4	3609	PASS
275	198	10	60	31.3	17644	PASS
365	198	1	100	3.9	2222	PASS
441	198	0.01	100	12.0	6773	PASS
442	442	50	100	100.0	46301	PASS
443	442	15	24	18.6	8632	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG030122\
Data File : BG052512.D
Acq On : 1 Mar 2022 10:28
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Mar 02 03:41:12 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG020722.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Feb 08 01:21:20 2022
Response via : Initial Calibration

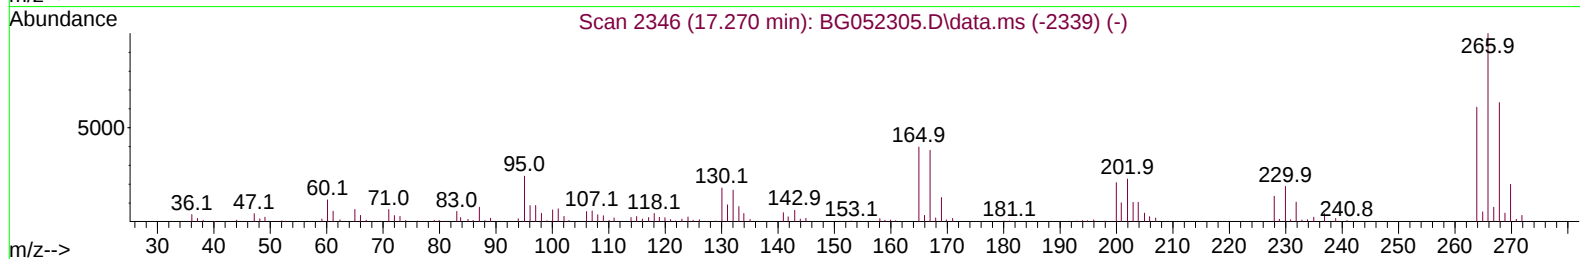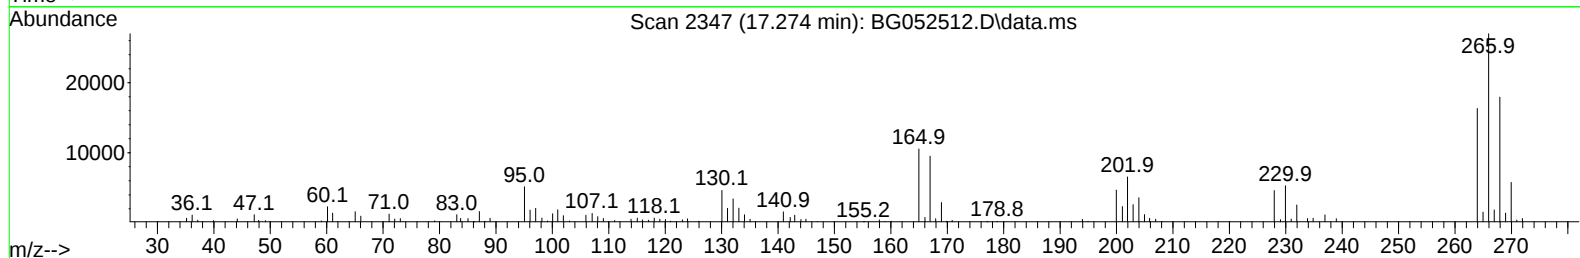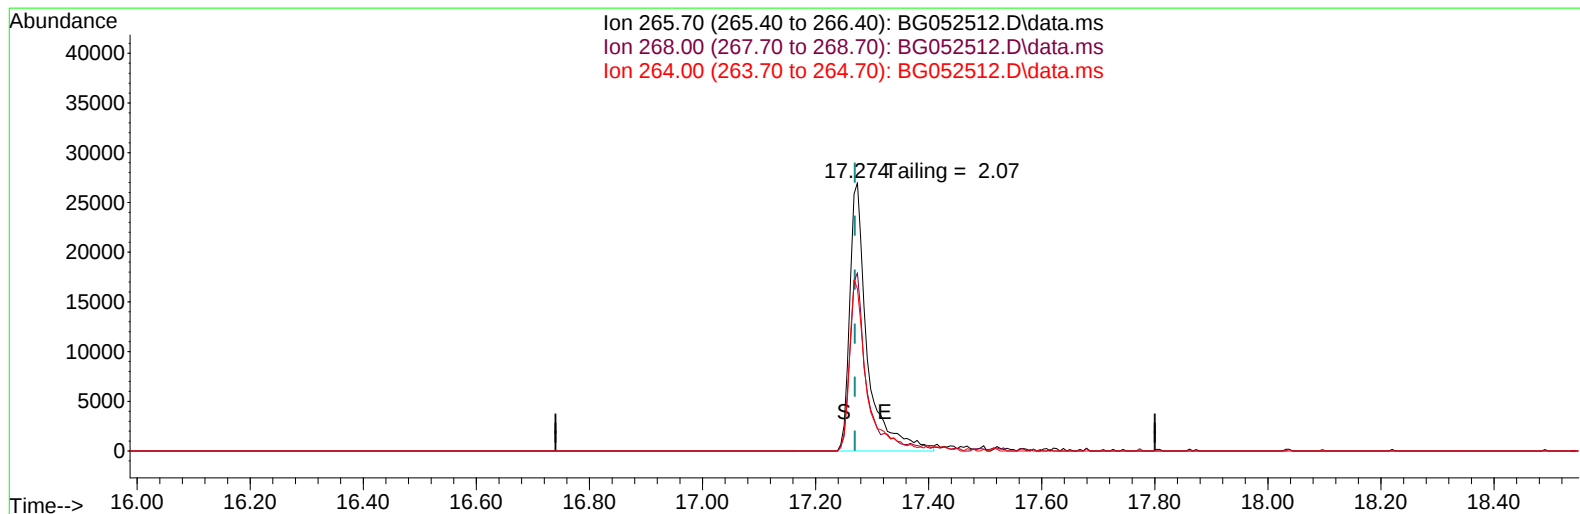

TIC: BG052512.D\data.ms

(70) Pentachlorophenol (C)

17.274min (+ 0.004) 26397.74 ng




response 58597

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.20	66.45
264.00	65.20	60.49
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG030122\
Data File : BG052512.D
Acq On : 1 Mar 2022 10:28
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Mar 02 03:41:12 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG020722.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Feb 08 01:21:20 2022
Response via : Initial Calibration

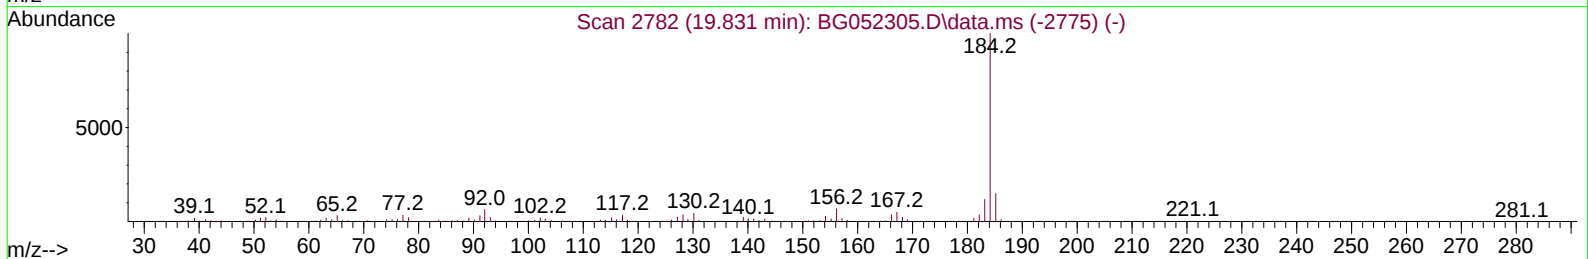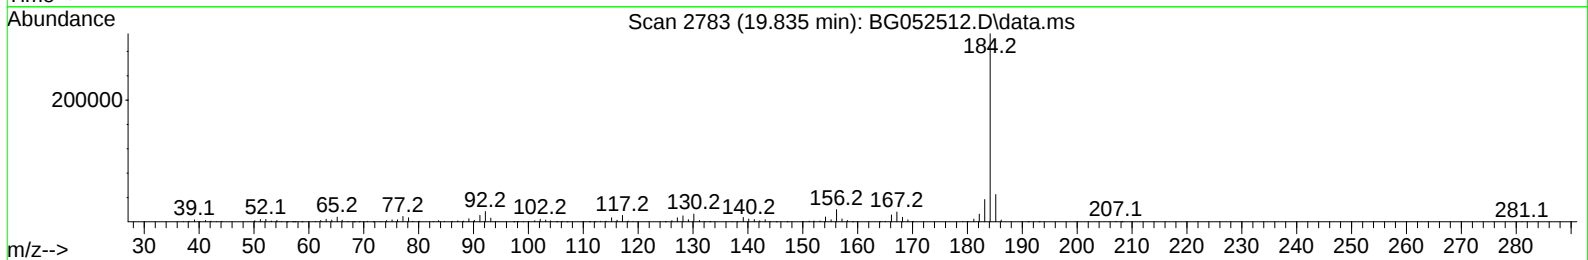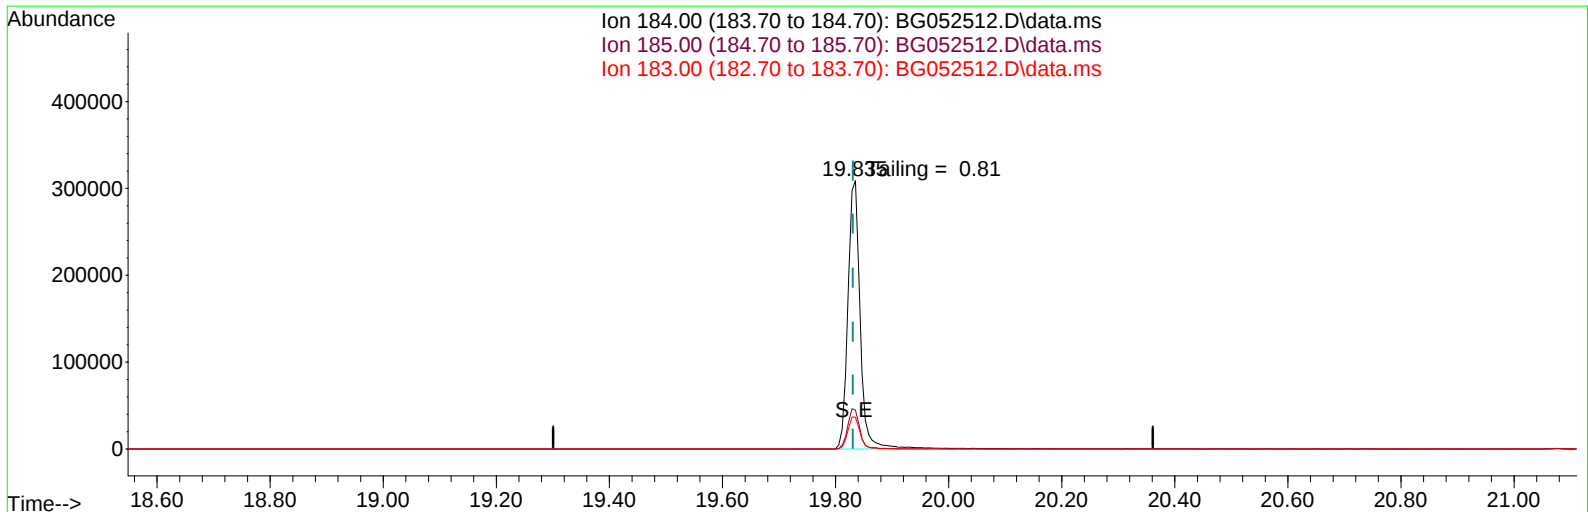

TIC: BG052512.D\data.ms

(77) Benzidine

19.835min (+ 0.004) 0.00 ng

response 466215

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.80	14.49
183.00	12.20	11.87
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
3/1/2022	BNA_G	<u>BG052512.D</u>
Compound Name	Response	Retention Time
DDT	242000	21.075
DDD	5872	20.622
DDE	0	20.146
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
5872	247872	2.37

Instrument :
BNA_G
ClientSampleId :
DFTPP