
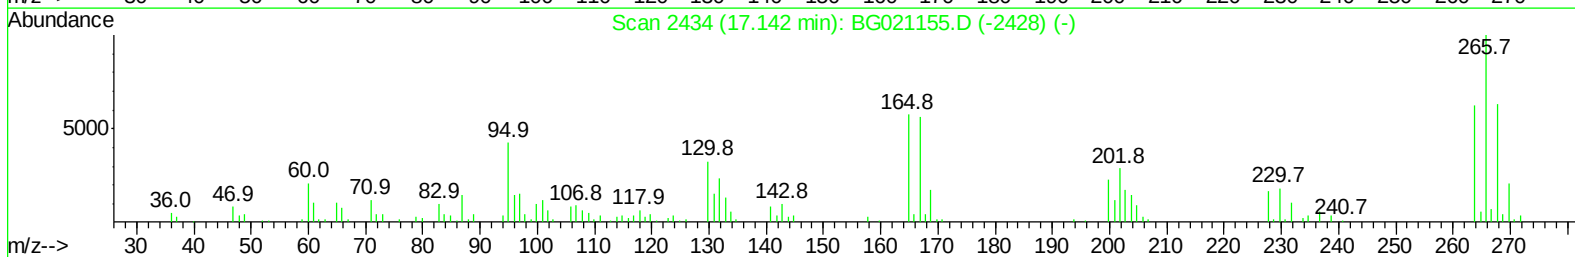
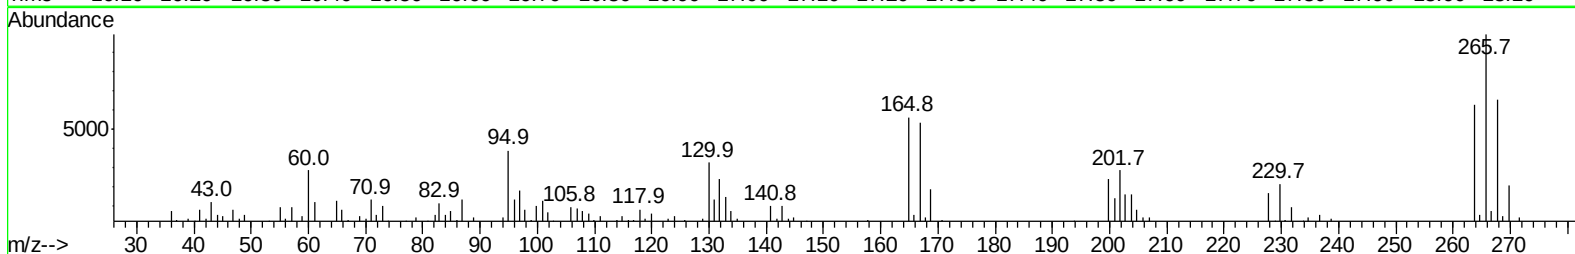


Data Path : Z:\HPCHEM1\BNA G\Data\BG030216\
Data File : BG021209.D
Acq On : 2 Mar 2016 11:38
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 03 07:26:15 2016
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG022916.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Mar 02 11:46:16 2016
Response via : Initial Calibration

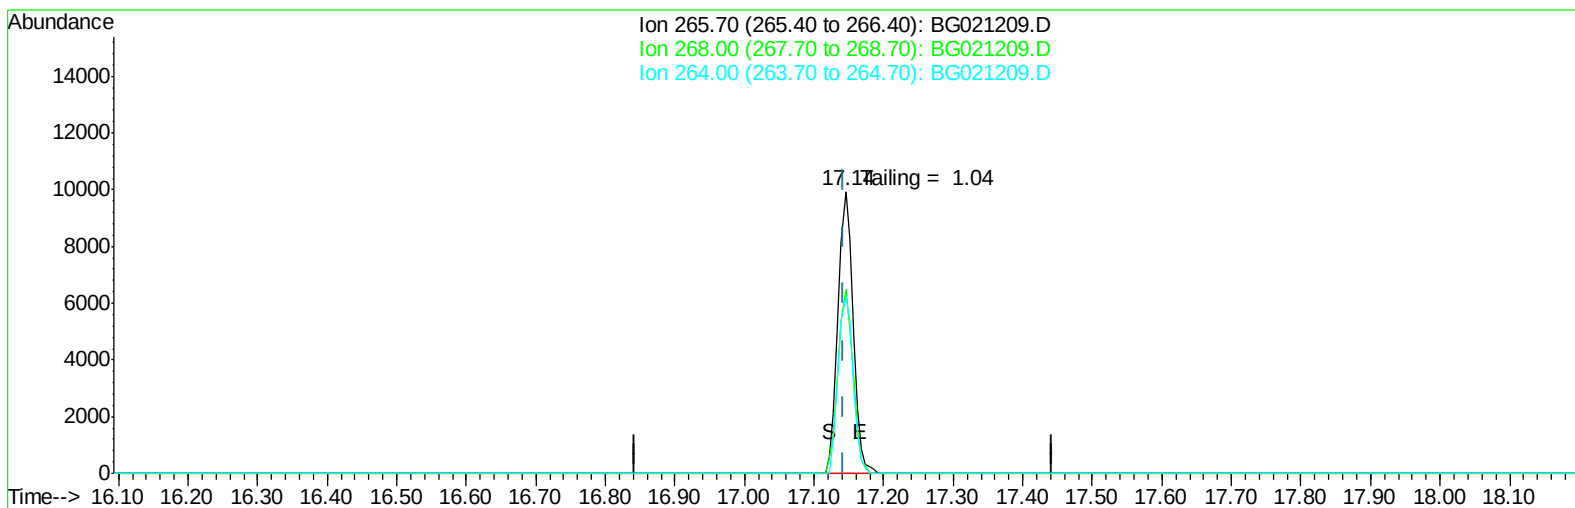

TIC: BG021209.D

(69) Pentachlorophenol (C)




17.145min (+0.003) 4360.16ng

response 15054

Ion	Exp%	Act%
265.70	100	100
268.00	63.80	69.67
264.00	59.80	68.07
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA G\Data\BG030216\
Data File : BG021209.D
Acq On : 2 Mar 2016 11:38
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 03 07:26:15 2016
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG022916.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Mar 02 11:46:16 2016
Response via : Initial Calibration

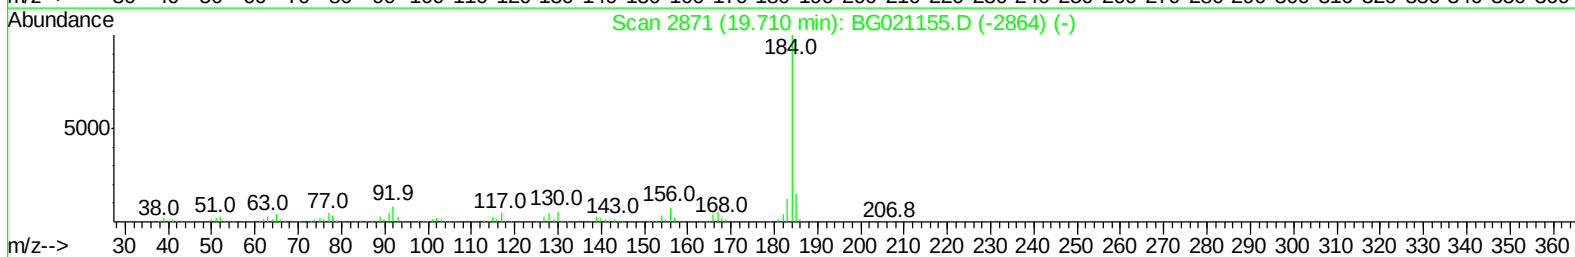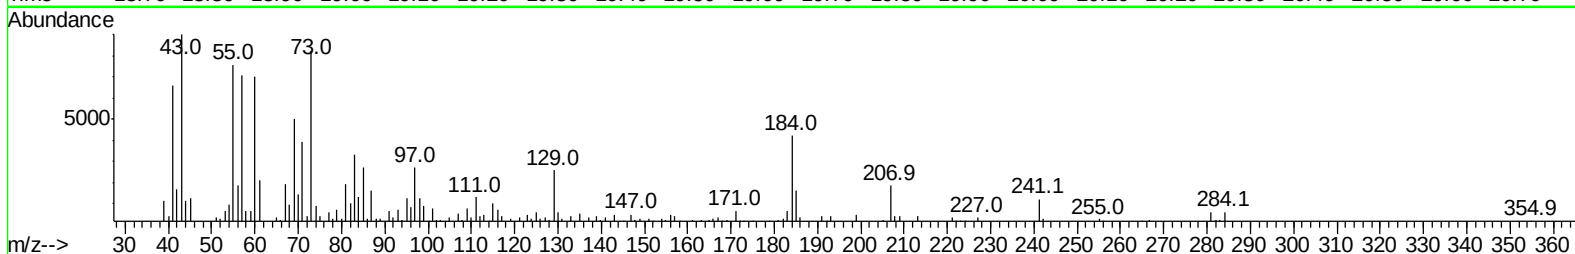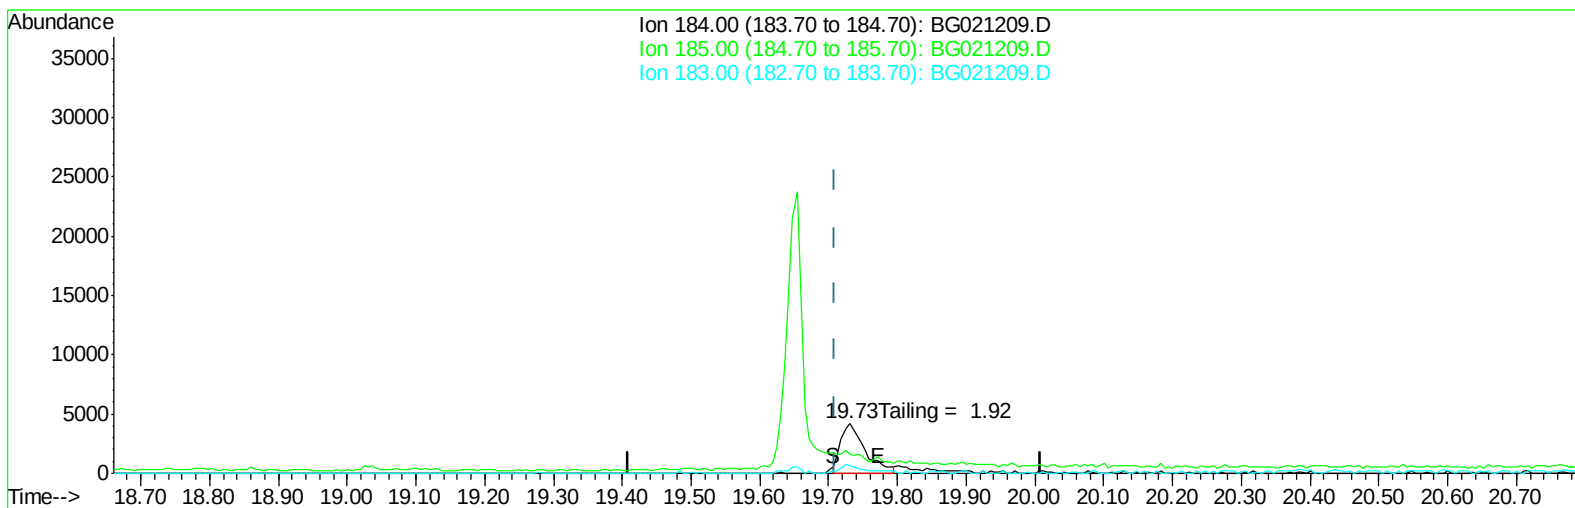

TIC: BG021209.D

(76) Benzidine

19.730min (+0.020) 592.44ng m

response 10427

Ion	Exp%	Act%
184.00	100	100
185.00	14.40	38.18#
183.00	12.60	14.77
0.00	0.00	0.00