


Data Path : Z:\HPCHEM1\BNA G\DATA\BG030216\
 Data File : BG021225.D
 Acq On : 2 Mar 2016 22:58
 Operator : UM/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG022916.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Mar 02 11:46:16 2016

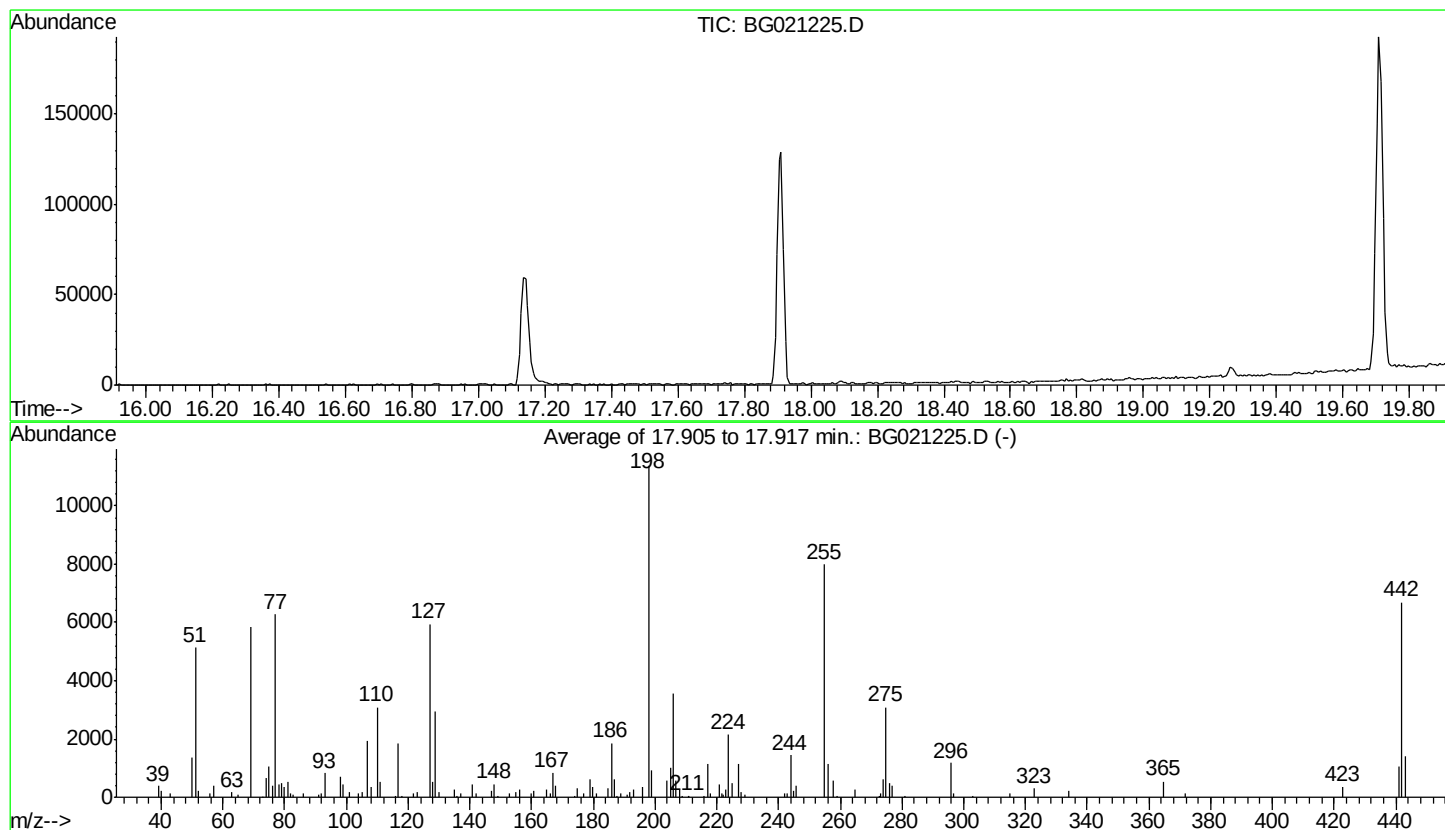

AutoFind: Scans 2564, 2565, 2566; Background Corrected with Scan 2558

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	45.1	5133	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	51.5	5864	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	52.3	5953	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	11384	PASS
199	198	5	9	8.3	941	PASS
275	198	10	60	27.1	3088	PASS
365	198	1	100	4.7	534	PASS
441	442	0.01	24	15.8	1056	PASS
442	198	50	100	58.7	6681	PASS
443	442	15	24	21.0	1401	PASS