

Data Path : Z:\HPCHEM1\BNA G\Data\BG030217\
 Data File : BG026032.D
 Acq On : 2 Mar 2017 16:39
 Operator : SJ/MA
 Sample : I2056-01
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 1B-18

Quant Time: Mar 02 17:38:45 2017
 Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG021717.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Feb 28 15:36:56 2017
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.07	152	112051	20.00	ng	-0.02
21) Naphthalene-d8	10.87	136	463660	20.00	ng	-0.02
38) Acenaphthene-d10	14.67	164	252583	20.00	ng	-0.02
63) Phenanthrene-d10	17.41	188	582373	20.00	ng	-0.01
75) Chrysene-d12	21.65	240	547561	20.00	ng	-0.02
86) Perylene-d12	24.85	264	503460	20.00	ng	-0.04
System Monitoring Compounds						
5) 2-Fluorophenol	5.64	112	830405	129.03	ng	-0.01
7) Phenol-d6	7.23	99	1101294	115.63	ng	0.00
23) Nitrobenzene-d5	9.23	82	615120	83.72	ng	-0.02
41) 2,4,6-Tribromophenol	16.15	330	341372	146.29	ng	-0.01
44) 2-Fluorobiphenyl	13.30	172	1461758	101.12	ng	-0.02
78) Terphenyl-d14	20.00	244	1858913	82.57	ng	-0.02
Target Compounds						
49) Dimethylphthalate	14.12	163	311660	17.99	ng	Qvalue 98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA G\Data\BG030217\
Data File : BG026032.D
Acq On : 2 Mar 2017 16:39
Operator : SJ/MA
Sample : I2056-01
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
1B-18

Quant Time: Mar 02 17:38:45 2017
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG021717.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Feb 28 15:36:56 2017
Response via : Initial Calibration

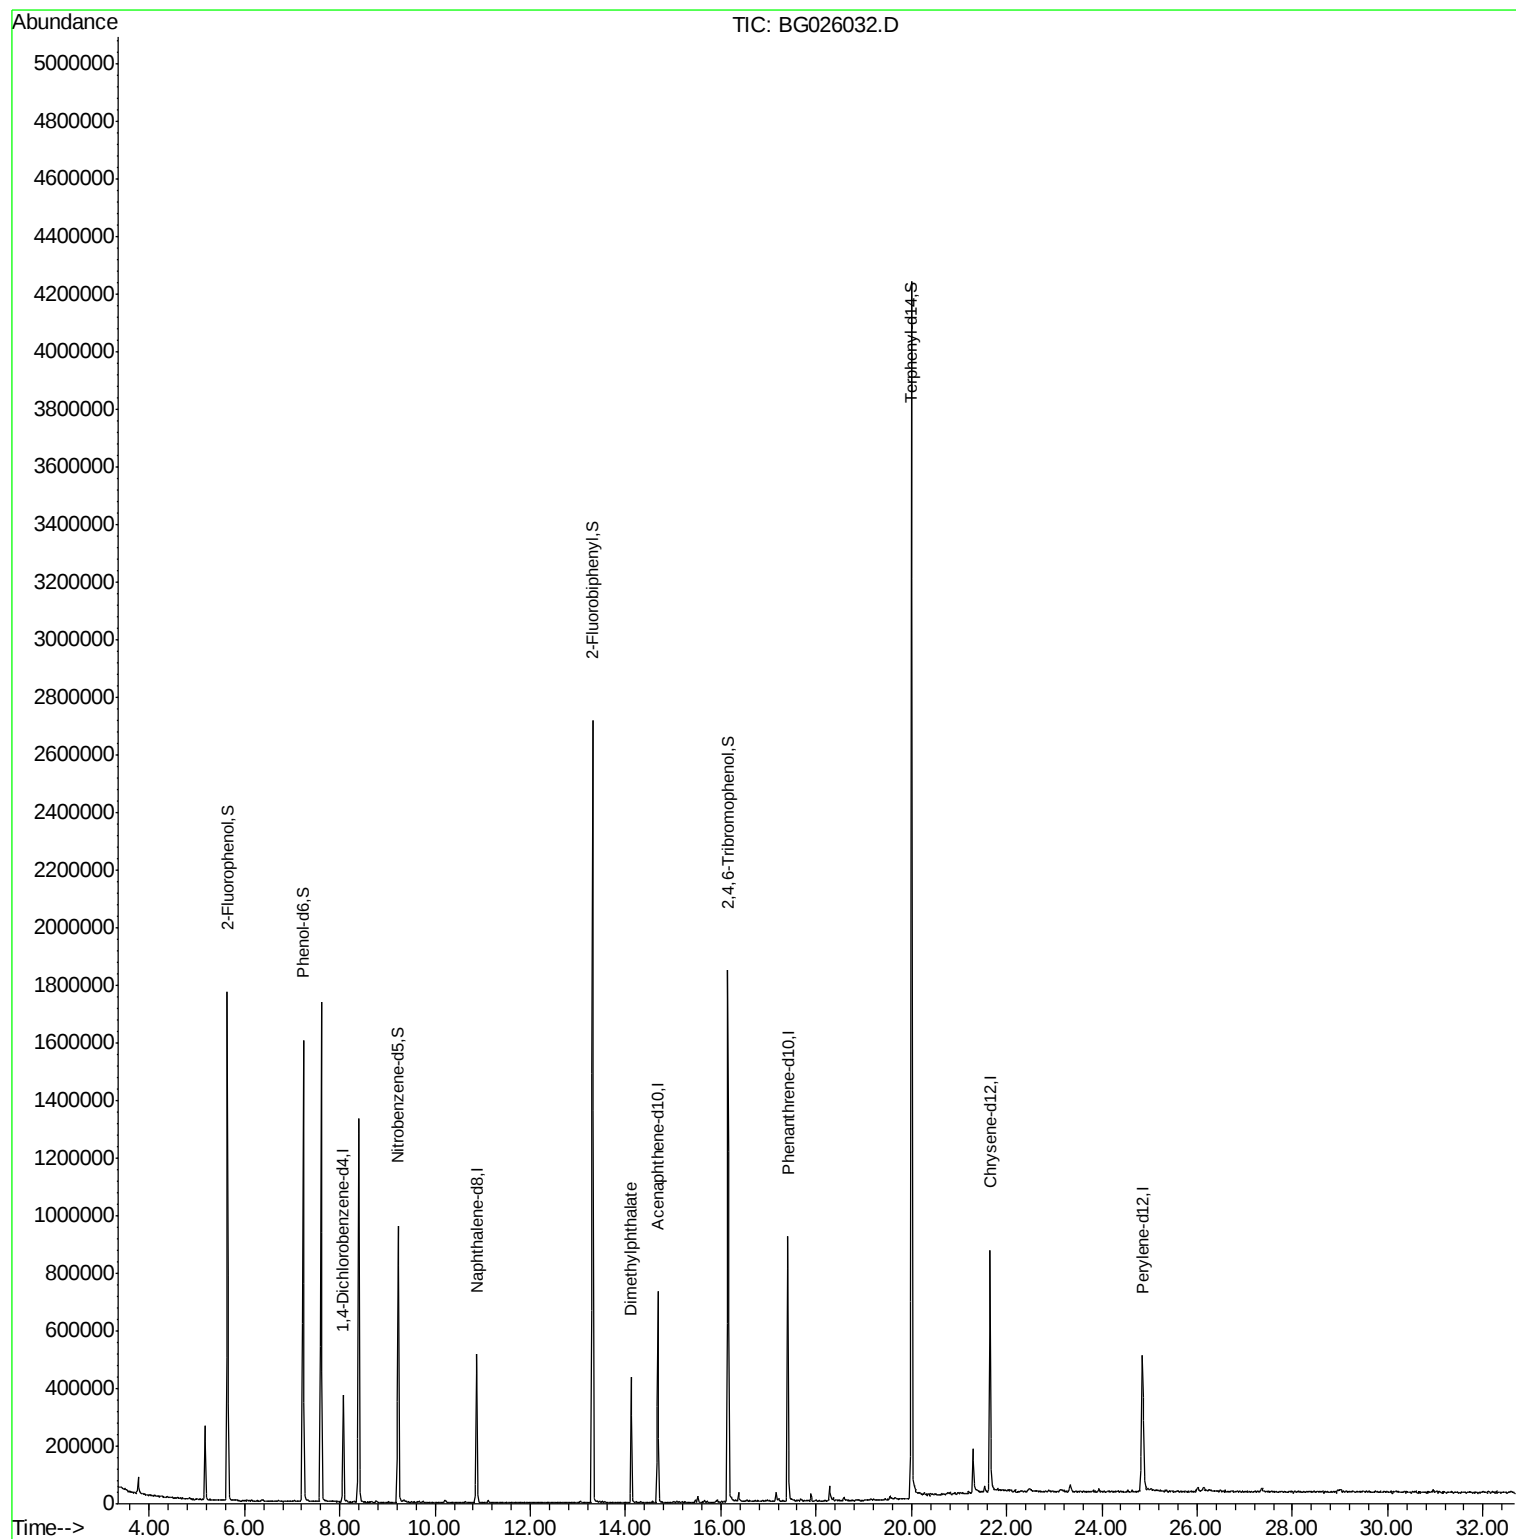

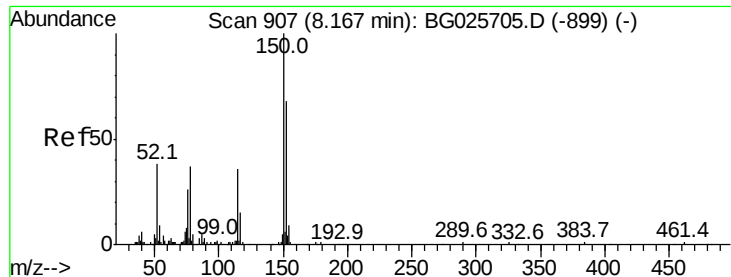

#1

1,4-Dichlorobenzene-d4

Concen: 20.00 ng

RT: 8.07 min Scan# 805

Delta R.T. -0.02 min

Lab File: BG026032.D

Acq: 2 Mar 2017 16:39

Instrument :

BNA_G

ClientSampleId :

1B-18


Tot Ion:152 Resp: 112051

Ion Ratio Lower Upper

152 100

150 159.1 114.0 171.0




115 57.1 48.1 72.1

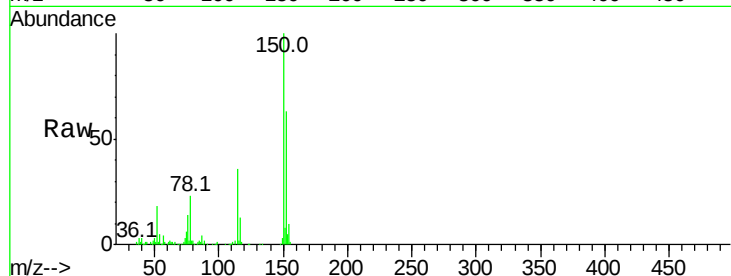

Abundance Ion 152.00 (151.70 to 152.70): E

Ion 150.00 (149.70 to 150.70): E

Ion 115.00 (114.70 to 115.70): E

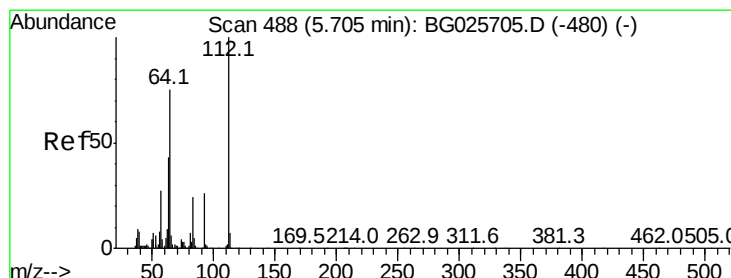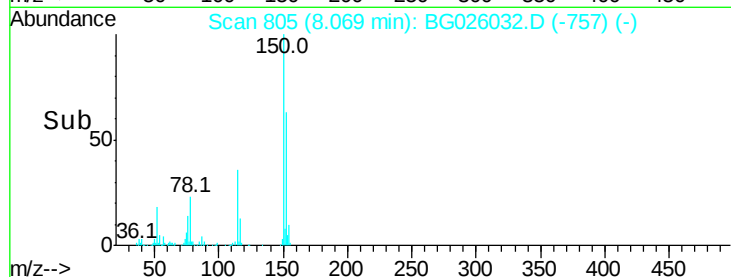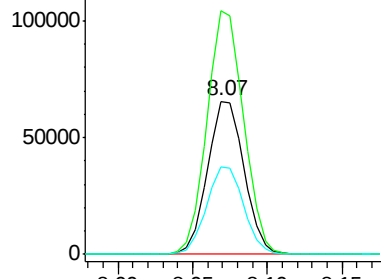

#5

2-Fluorophenol

Concen: 129.03 ng

RT: 5.64 min Scan# 392

Delta R.T. -0.01 min

Lab File: BG026032.D

Acq: 2 Mar 2017 16:39


Tgt Ion:112 Resp: 830405

Ion Ratio Lower Upper

112 100

64 60.4 61.8 92.6#



63 30.7 37.2 55.8#

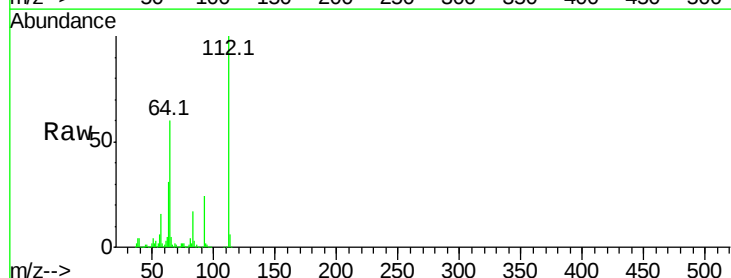


Abundance Ion 112.00 (111.70 to 112.70): E

Ion 64.00 (63.70 to 64.70): BGC

Ion 63.00 (62.70 to 63.70): BGC

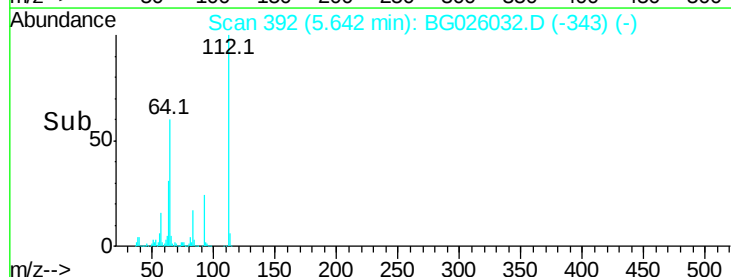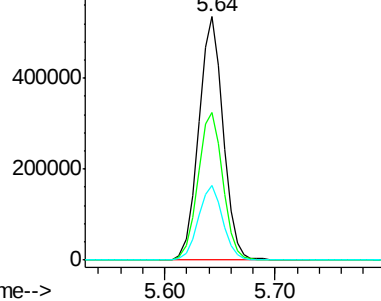

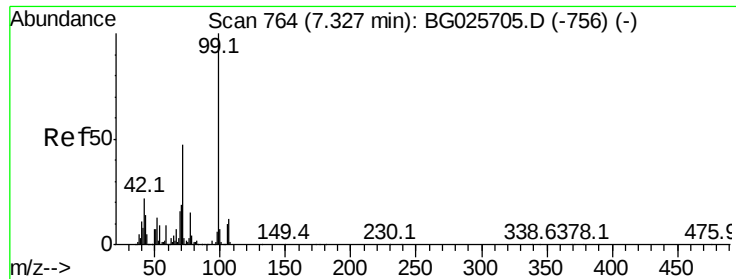

#7

Phenol-d6

Concen: 115.63 ng

RT: 7.23 min Scan# 662

Delta R.T. -0.01 min

Lab File: BG026032.D

Acq: 2 Mar 2017 16:39

Instrument :





BNA_G

ClientSampleId :

1B-18

Tot Ion: 99 Resp: 1101294

Ion	Ratio	Lower	Upper
99	100		
42	12.8	20.5	30.7#
71	28.2	37.6	56.4#

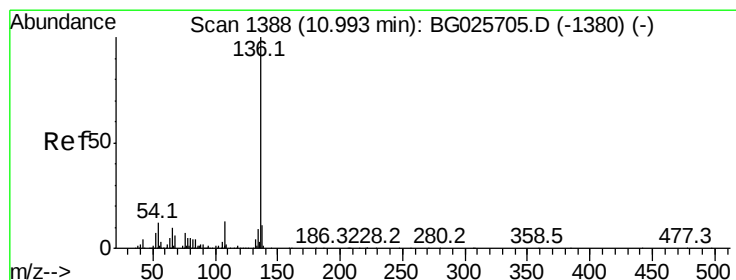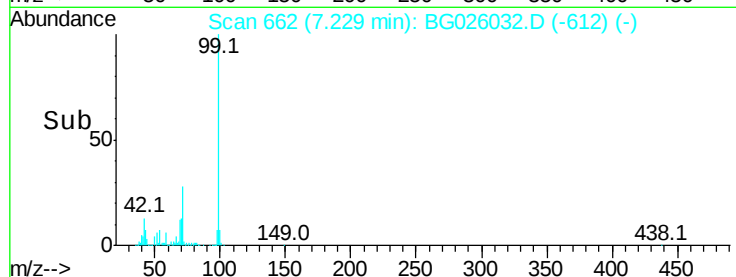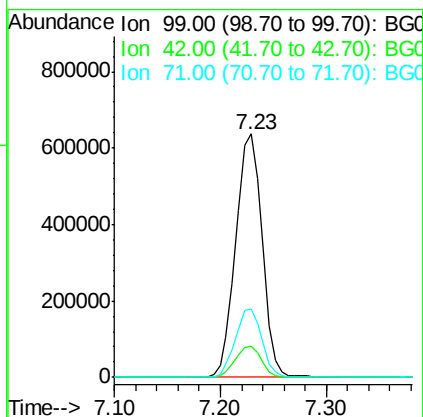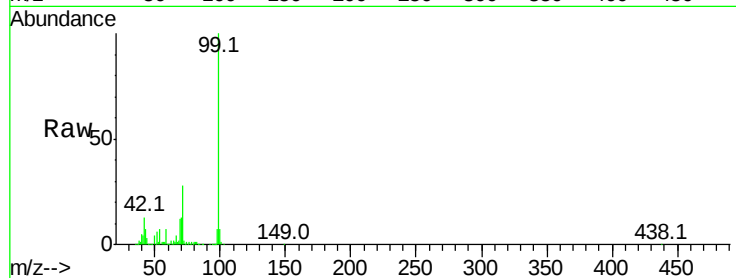

#21

Naphthalene-d8

Concen: 20.00 ng

RT: 10.87 min Scan# 1282




Delta R.T. -0.02 min


Lab File: BG026032.D

Acq: 2 Mar 2017 16:39

Tgt Ion: 136 Resp: 463660

Ion	Ratio	Lower	Upper
136	100		
137	10.7	8.9	13.3
54	7.6	9.3	13.9#
68	6.6	5.1	7.7


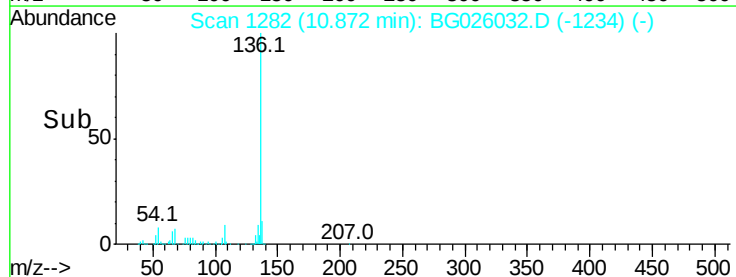
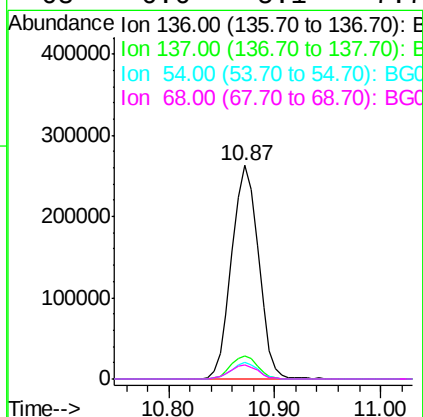
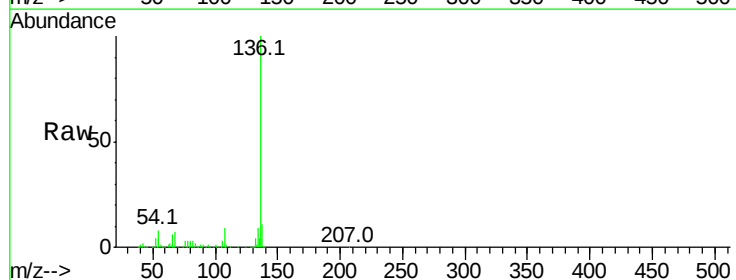


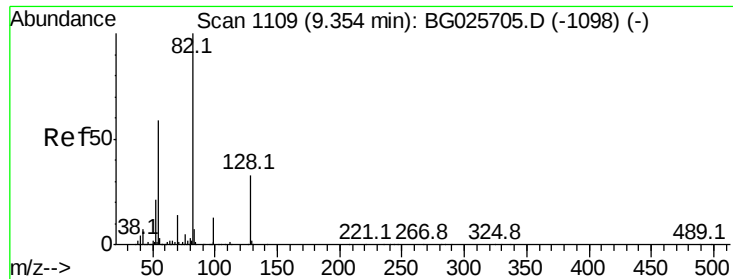

#23
 Nitrobenzene-d5
 Concen: 83.72 ng
 RT: 9.23 min Scan# 1002
 Delta R.T. -0.02 min
 Lab File: BG026032.D
 Acq: 2 Mar 2017 16:39




Instrument :
 BNA_G
 ClientSampleID :
 1B-18


Tot Ion: 82 Resp: 615120
 Ion Ratio Lower Upper
 82 100
 128 48.3 26.4 39.6#
 54 46.4 49.4 74.2#

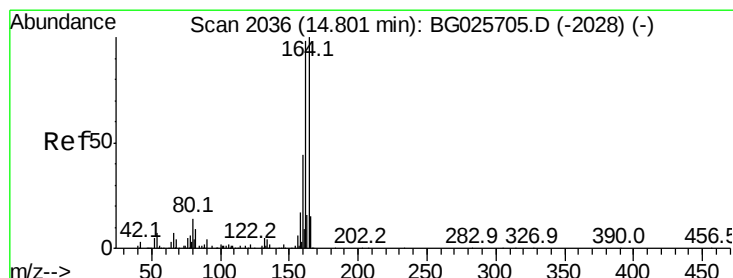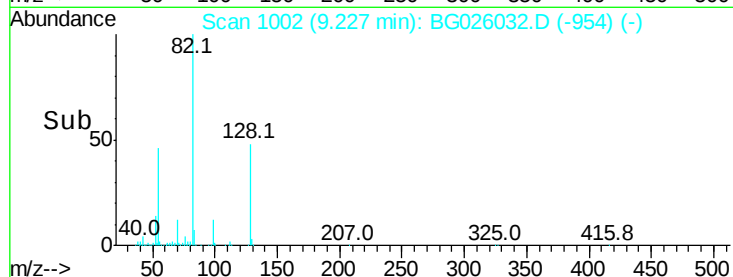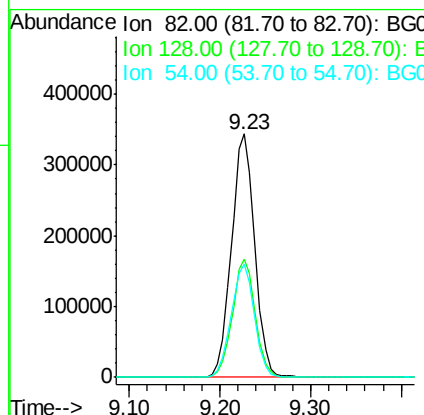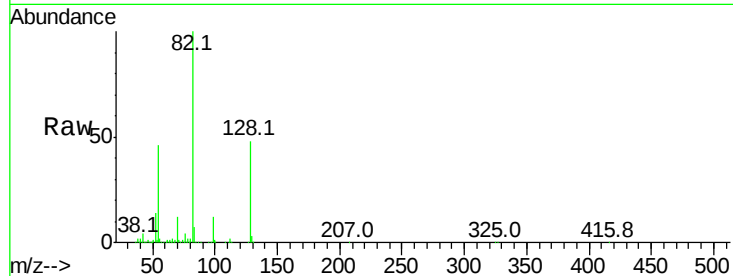

#38
 Acenaphthene-d10
 Concen: 20.00 ng
 RT: 14.67 min Scan# 1929
 Delta R.T. -0.02 min
 Lab File: BG026032.D
 Acq: 2 Mar 2017 16:39

Tgt Ion:164 Resp: 252583
 Ion Ratio Lower Upper
 164 100
 162 100.0 85.1 127.7
 160 45.7 34.7 52.1


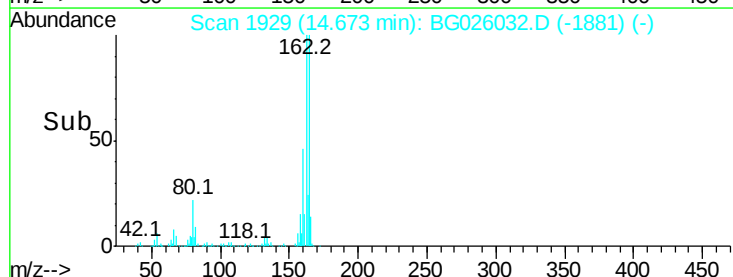
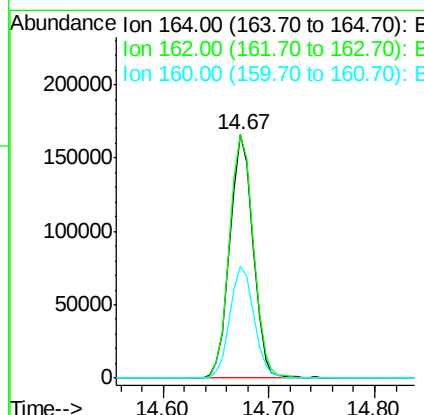
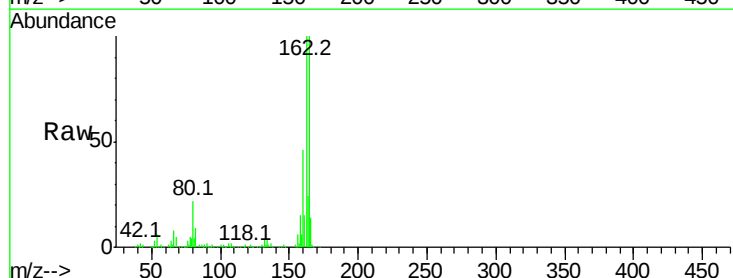


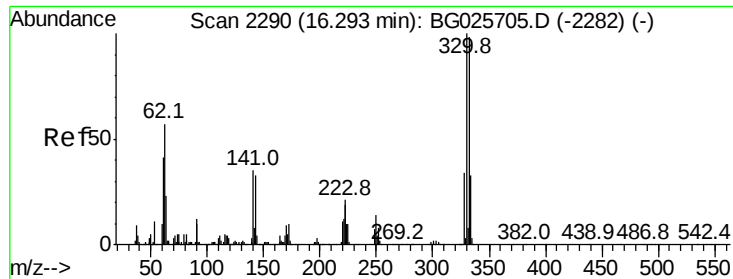

#41
 2,4,6-Tribromophenol
 Concen: 146.29 ng
 RT: 16.15 min Scan# 2181
 Delta R.T. -0.01 min
 Lab File: BG026032.D
 Acq: 2 Mar 2017 16:39




Instrument :
 BNA_G
 ClientSampleId :
 1B-18


Tot Ion:330 Resp: 341372
 Ion Ratio Lower Upper
 330 100
 332 98.7 77.3 115.9
 141 39.3 32.1 48.1

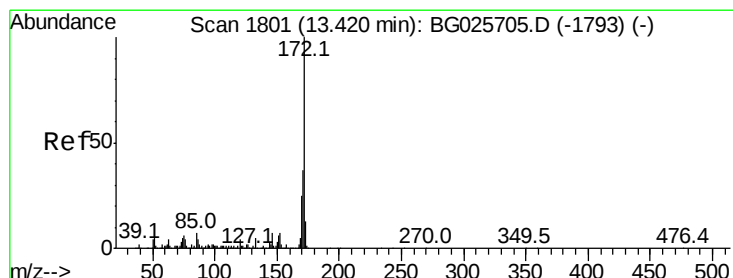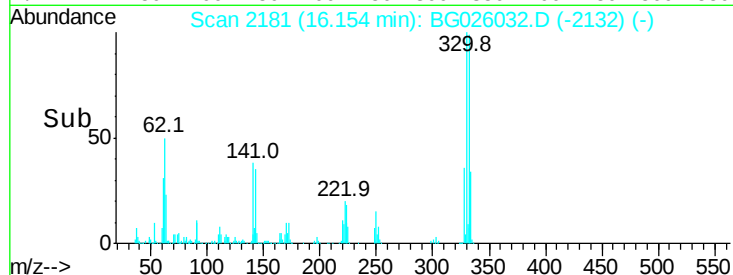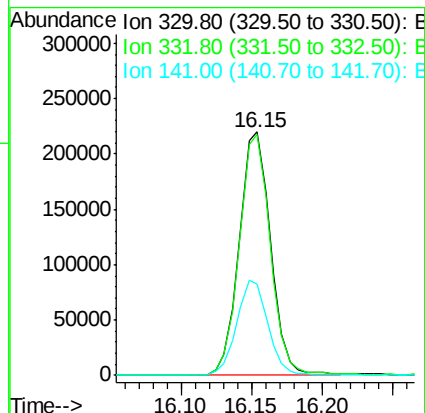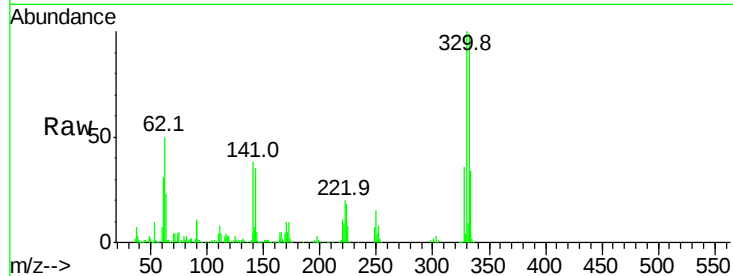

#44
 2-Fluorobiphenyl
 Concen: 101.12 ng
 RT: 13.30 min Scan# 1696
 Delta R.T. -0.02 min
 Lab File: BG026032.D
 Acq: 2 Mar 2017 16:39

Tgt Ion:172 Resp: 1461758
 Ion Ratio Lower Upper
 172 100
 171 37.6 32.2 48.2
 170 24.8 21.8 32.6

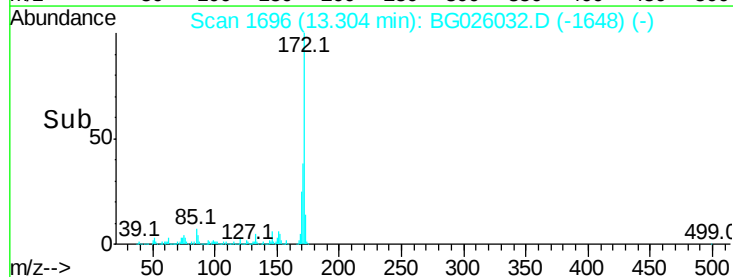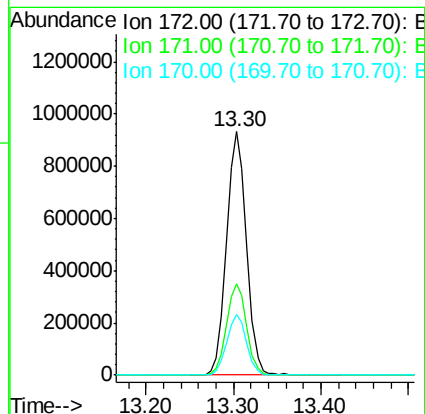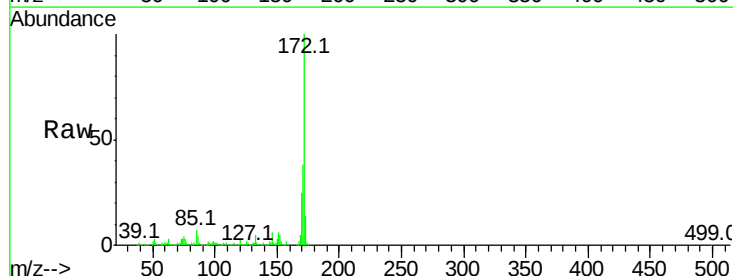

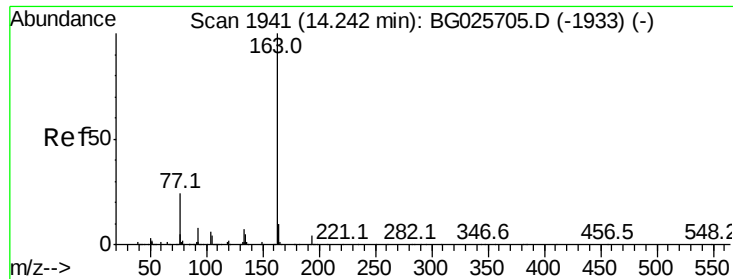

#49

Dimethylphthalate

Concen: 17.99 ng

RT: 14.12 min Scan# 1835

Delta R.T. -0.02 min

Lab File: BG026032.D

Acq: 2 Mar 2017 16:39

Instrument :

BNA_G

ClientSampled :

1B-18


Tot Ion:163 Resp: 311660

Ion Ratio Lower Upper

163 100

194 4.0 3.8 5.6

164 11.1 9.3 13.9

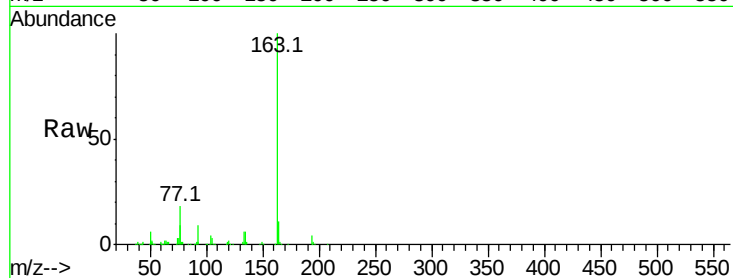

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

250000

200000

150000

100000



50000

0

14.12

14.10 14.20

Time-->

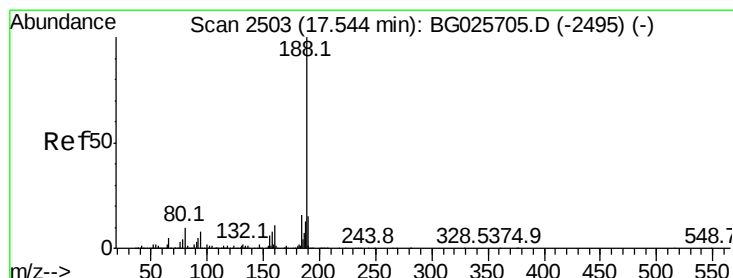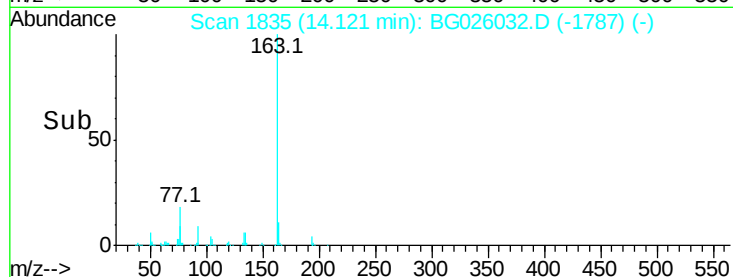

#63

Phenanthrene-d10

Concen: 20.00 ng

RT: 17.41 min Scan# 2394

Delta R.T. -0.01 min

Lab File: BG026032.D

Acq: 2 Mar 2017 16:39


Tgt Ion:188 Resp: 582373

Ion Ratio Lower Upper

188 100

94 9.0 5.8 8.8#

80 10.6 7.5 11.3

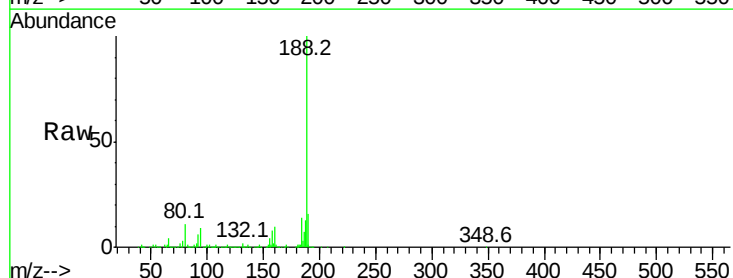

Abundance Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BGC

Ion 80.00 (79.70 to 80.70): BGC

500000

400000

300000

200000


100000


0

17.41

17.30 17.50

Time-->

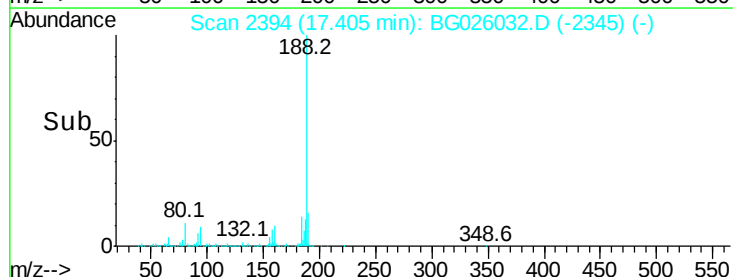

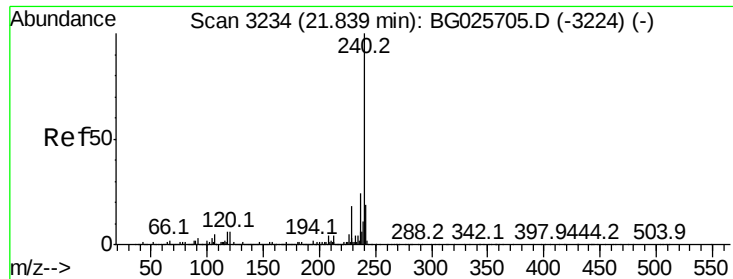

#75

Chrysene-d12

Concen: 20.00 ng

RT: 21.65 min Scan# 3117

Delta R.T. -0.02 min

Lab File: BG026032.D

Acq: 2 Mar 2017 16:39

Instrument :

BNA_G

ClientSampleId :

1B-18


Tot Ion:240 Resp: 547561

Ion Ratio Lower Upper

240 100

120 12.0 5.7 8.5#




236 25.9 22.2 33.4

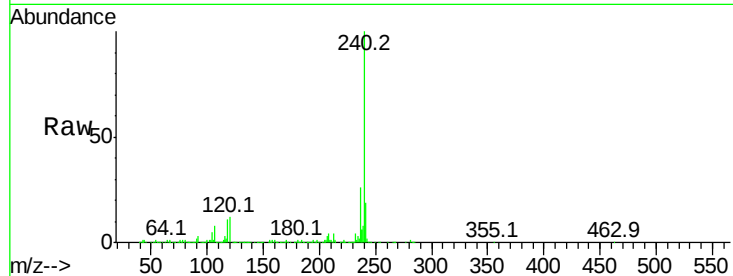

Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

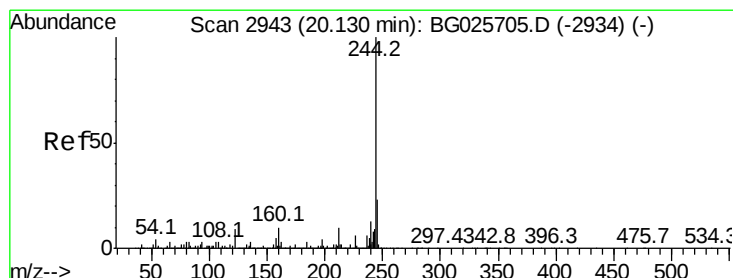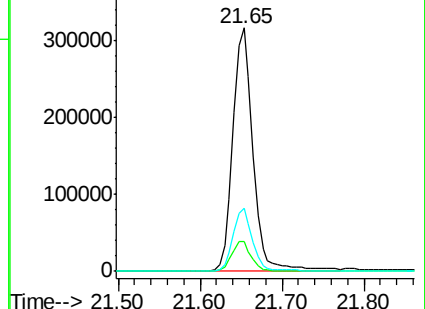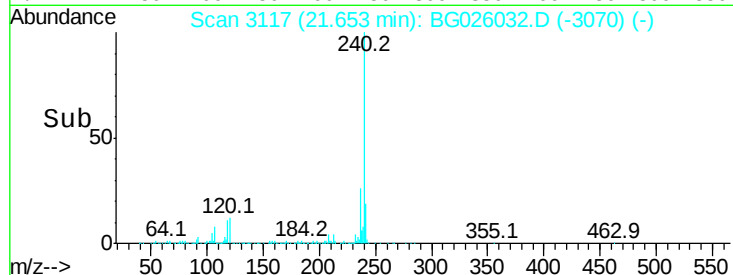

#78

Terphenyl-d14

Concen: 82.57 ng

RT: 20.00 min Scan# 2836

Delta R.T. -0.02 min

Lab File: BG026032.D

Acq: 2 Mar 2017 16:39


Tgt Ion:244 Resp: 1858913

Ion Ratio Lower Upper

244 100

212 7.9 10.0 15.0#



122 13.0 8.6 12.8#

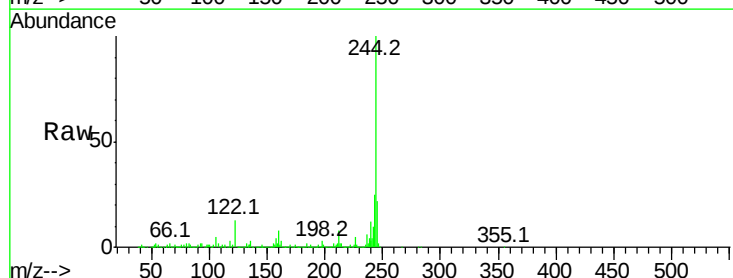


Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

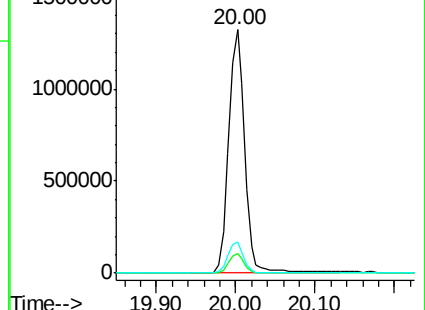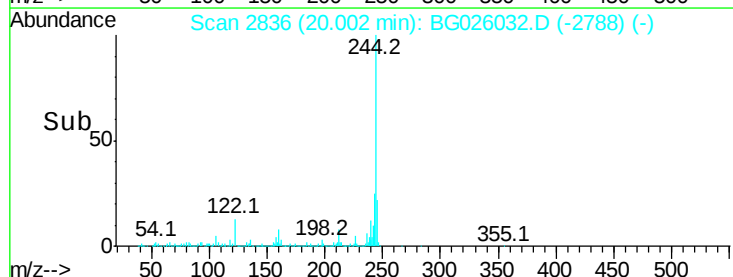

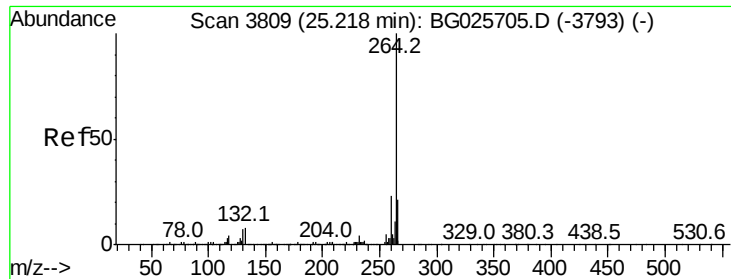

#86
 Pervlene-d12
 Concen: 20.00 ng
 RT: 24.85 min Scan# 3661
 Delta R.T. -0.04 min
 Lab File: BG026032.D
 Acq: 2 Mar 2017 16:39

Instrument :
 BNA_G
 ClientSampleId :
 1B-18

Tot Ion	Ratio	Lower	Upper
264	100		
260	23.2	21.8	32.8
265	22.6	18.2	27.4

