
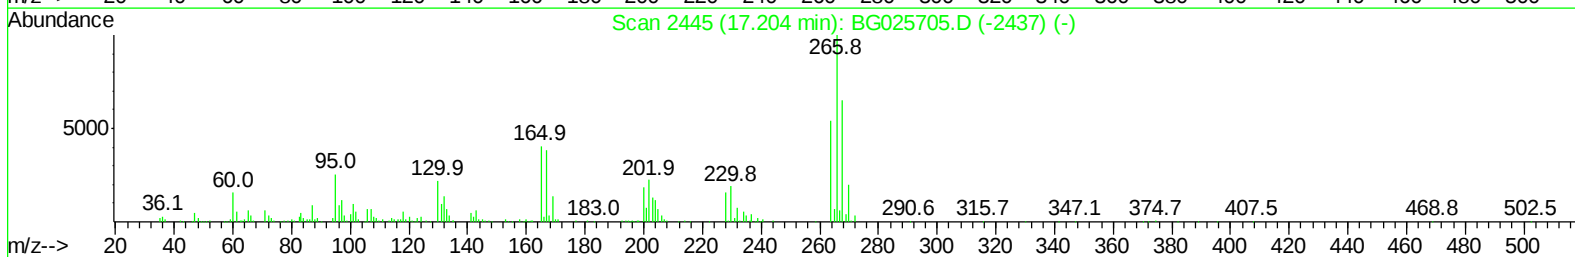
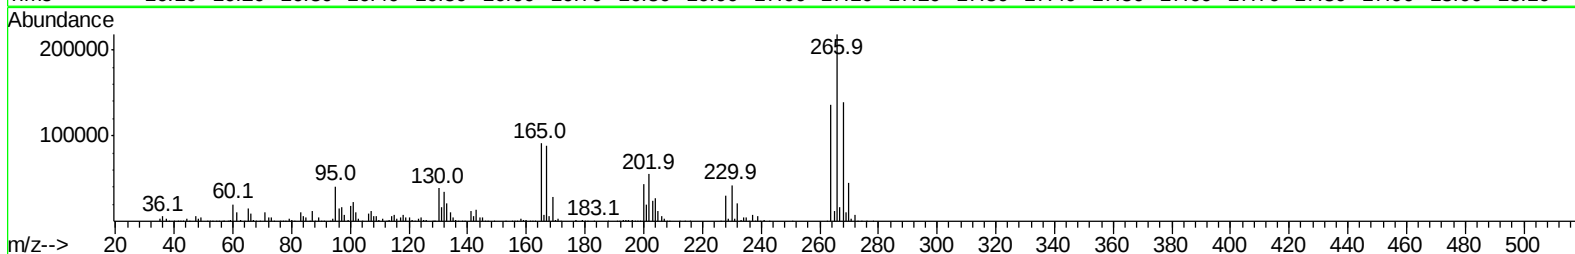


Data Path : Z:\HPCHEM1\BNA G\DATA\BG030217\  
Data File : BG026021.D  
Acq On : 2 Mar 2017 9:22  
Operator : SJ/MA  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 02 16:08:07 2017  
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG021717.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Tue Feb 28 15:36:56 2017  
Response via : Initial Calibration

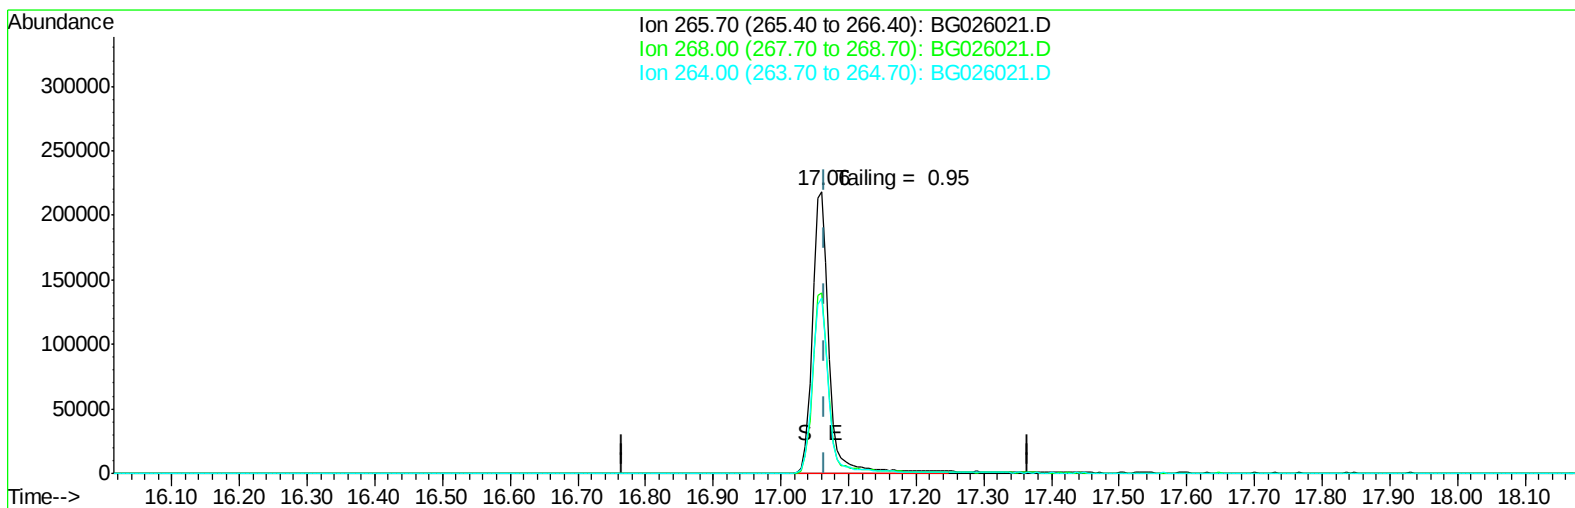

TIC: BG026021.D

(69) Pentachlorophenol (C)




17.060min (-0.006) 820837.04ng

response 371933

| Ion    | Exp%  | Act%  |
|--------|-------|-------|
| 265.70 | 100   | 100   |
| 268.00 | 60.70 | 63.91 |
| 264.00 | 62.60 | 62.09 |
| 0.00   | 0.00  | 0.00  |

Data Path : Z:\HPCHEM1\BNA G\DATA\BG030217\  
Data File : BG026021.D  
Acq On : 2 Mar 2017 9:22  
Operator : SJ/MA  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 02 16:08:07 2017  
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG021717.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Tue Feb 28 15:36:56 2017  
Response via : Initial Calibration

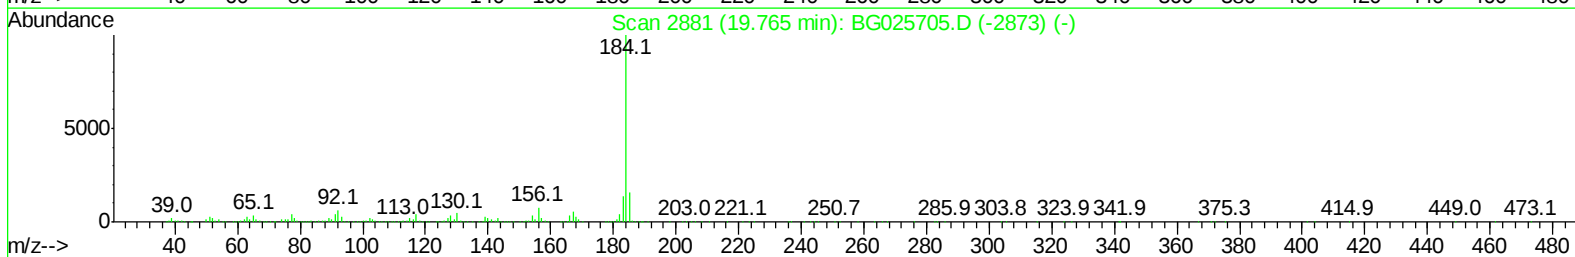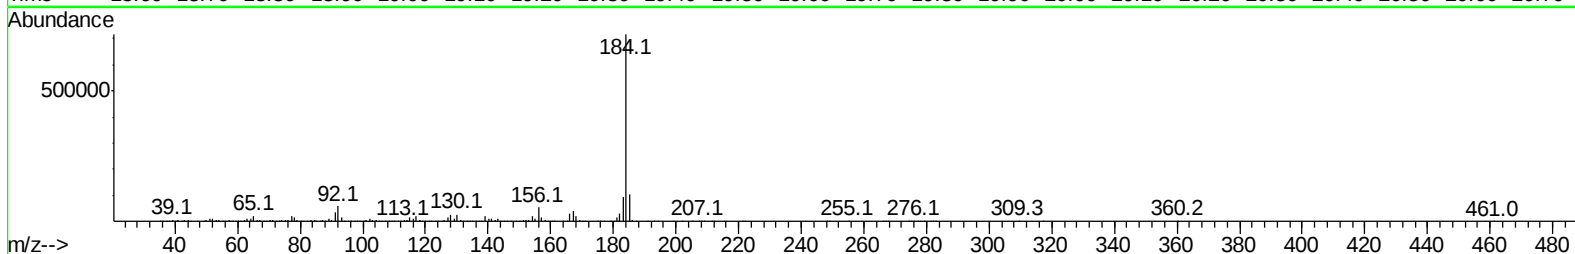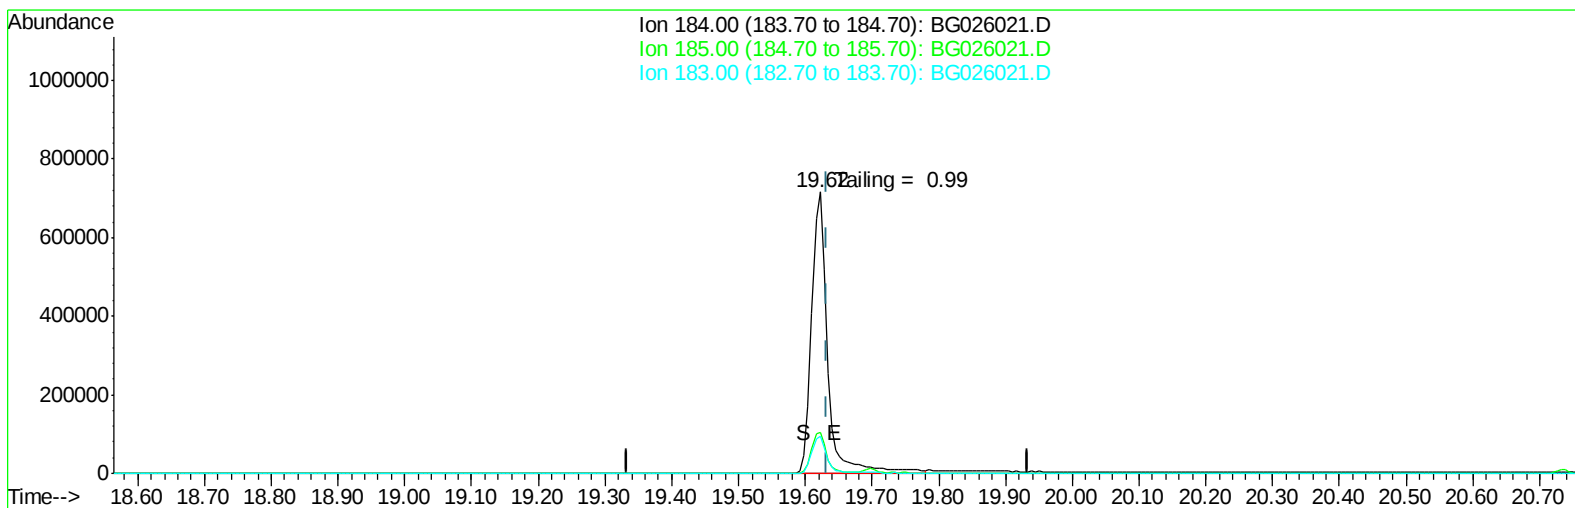

TIC: BG026021.D

(76) Benzidine

19.622min (-0.012) 82001.10ng

response 1151908

| Ion    | Exp%  | Act%  |
|--------|-------|-------|
| 184.00 | 100   | 100   |
| 185.00 | 16.30 | 14.54 |
| 183.00 | 13.80 | 13.34 |
| 0.00   | 0.00  | 0.00  |