
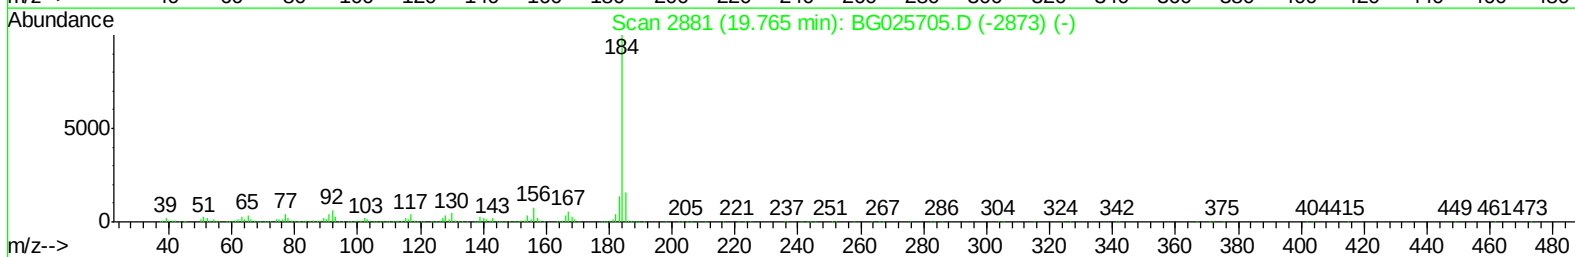
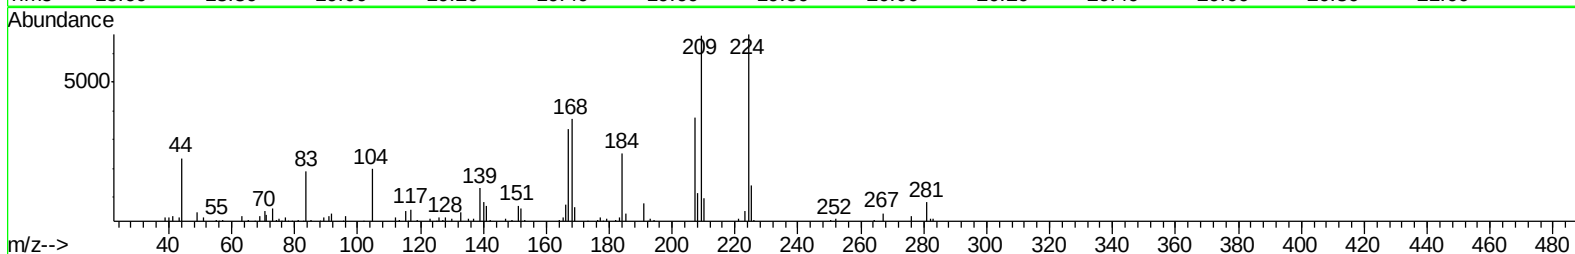


Data Path : Z:\HPCHEM1\BNA_G\DATA\BG030217\
 Data File : BG026039.D
 Acq On : 2 Mar 2017 21:16
 Operator : SJ/MA
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 03 06:59:06 2017
 Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG021717.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Feb 28 15:36:56 2017
 Response via : Initial Calibration

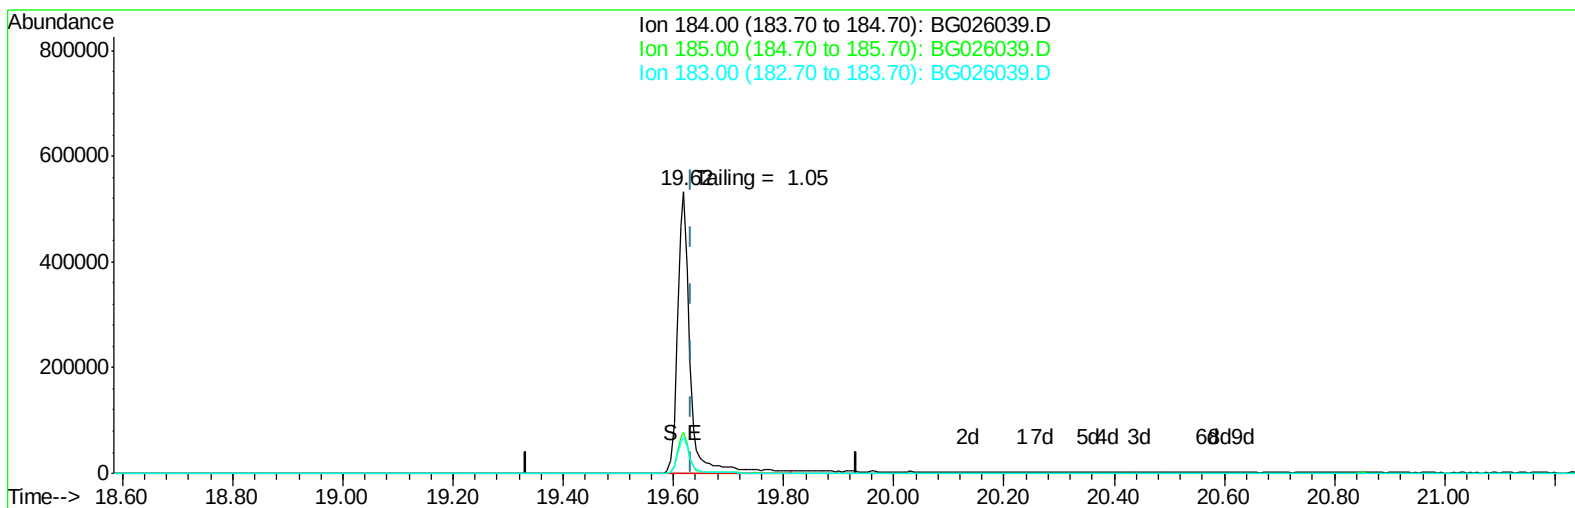

TIC: BG026039.D

(76) Benzidine




20.235min (+0.602) 192.43ng

response 407

Ion	Exp%	Act%
184.00	100	100
185.00	16.30	16.53
183.00	13.80	11.36
0.00	0.00	0.00

```
Data Path : Z:\HPCHEM1\BNA_G\DATA\BG030217\  
Data File : BG026039.D  
Acq On    : 2 Mar 2017 21:16  
Operator  : SJ/MA  
Sample    : DFTPP  
Misc      :  
ALS Vial  : 1 Sample Multiplier: 1
```

Quant Time: Mar 03 06:59:06 2017
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG021717.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Feb 28 15:36:56 2017
Response via : Initial Calibration

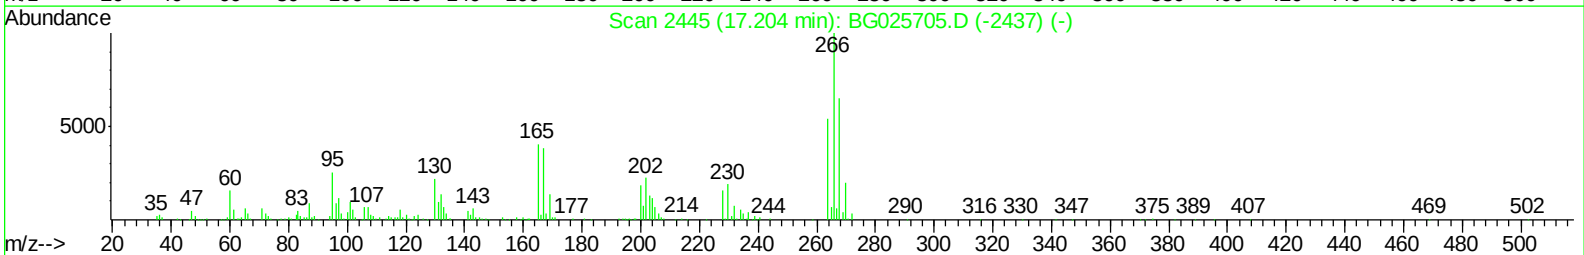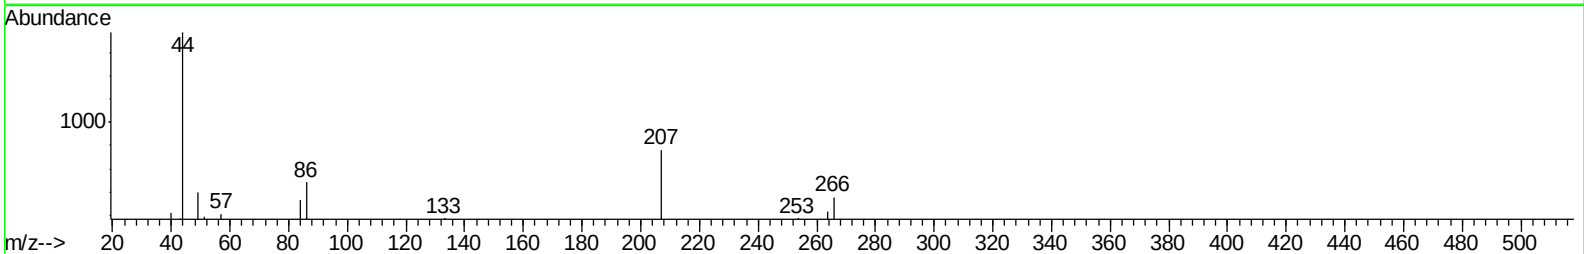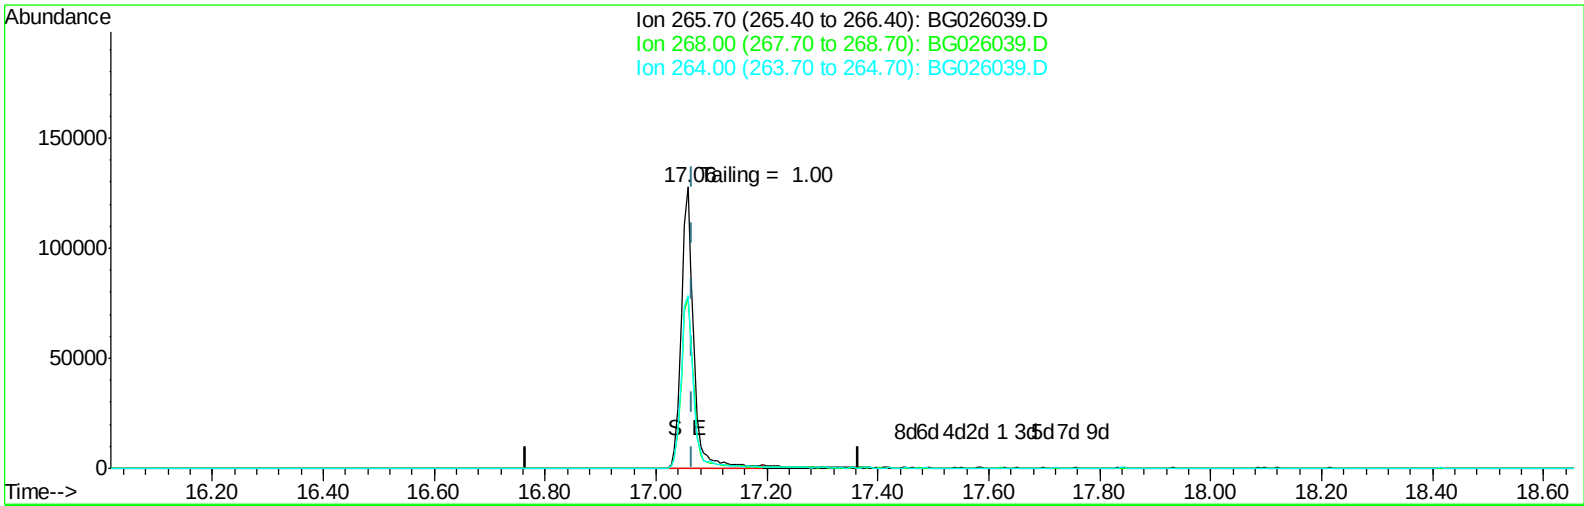

TIC: BG026039.D

(69) Pentachlorophenol (C)

17.627min (+0.561) 1377.53ng

response 615

Ion	Exp%	Act%
265.70	100	100
268.00	60.70	45.94#
264.00	62.60	63.87
0.00	0.00	0.00