

#1





1,4-Dichlorobenzene-d4
Concen: 20.00 ng
RT: 8.07 min Scan# 806
Delta R.T. -0.01 min
Lab File: BG026022.D
Acq: 2 Mar 2017 10:02

Instrument :
BNA_G
ClientSampleId :
SSTDCCC040

Tgt Ion	Ratio	Lower	Upper
152	100		
150	156.2	114.0	171.0
115	57.5	48.1	72.1

Manual Integrations
APPROVED




mohammad
3/3/2017 10:56:20 AM

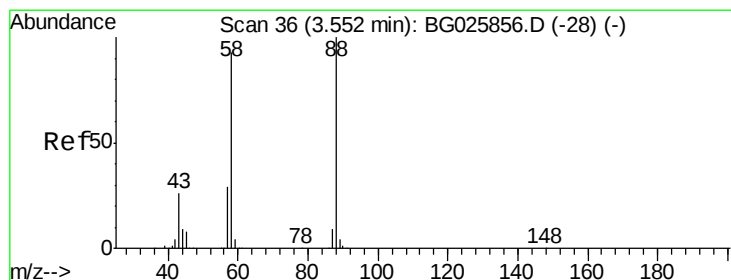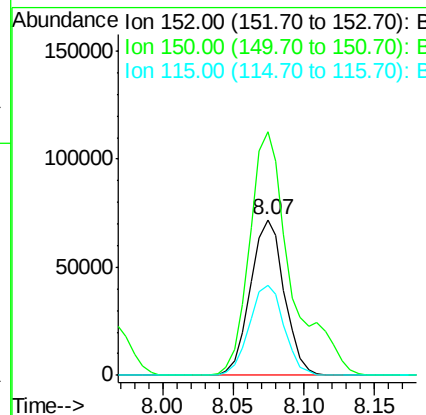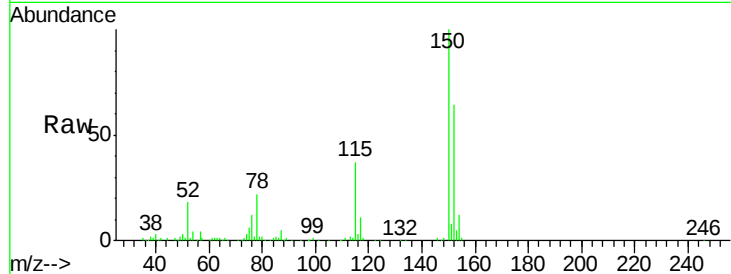


#2

1,4-Dioxane
Concen: 39.83 ng
RT: 3.54 min Scan# 34
Delta R.T. -0.01 min
Lab File: BG026022.D
Acq: 2 Mar 2017 10:02

Tgt Ion	Ratio	Lower	Upper
88	100		
58	83.7	79.4	119.2
43	21.1	33.8	50.6

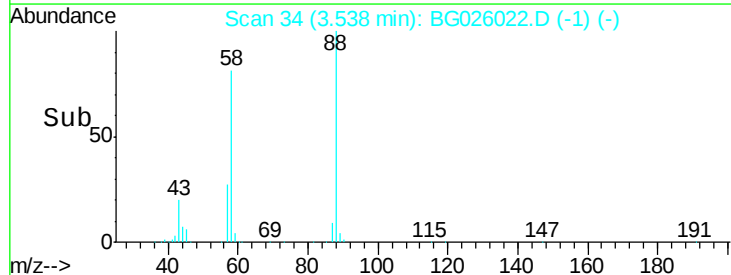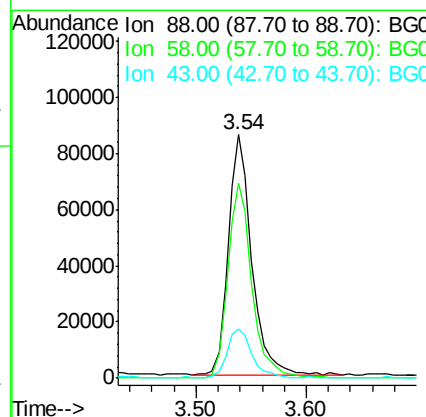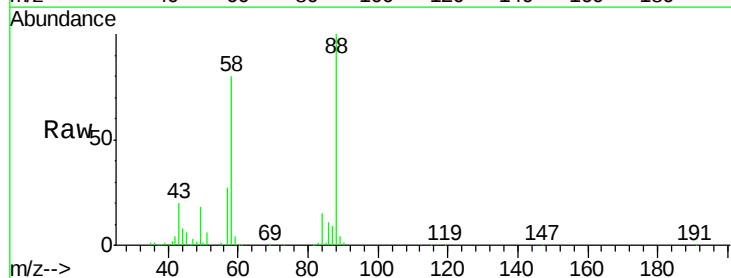







#11
bis(2-Chloroethyl)ether
Concen: 36.15 ng
RT: 7.49 min Scan# 706
Delta R.T. -0.01 min
Lab File: BG026022.D
Acq: 2 Mar 2017 10:02

Instrument :
BNA_G
ClientSampleId :
SSTDCCC040

Tgt Ion	Ratio	Resp	Lower	Upper
93	100	333991		
63	82.2	78.5	118.5	
95	32.0	9.8	49.8	




Manual Integrations
APPROVED


mohammad
3/3/2017 10:56:20 AM

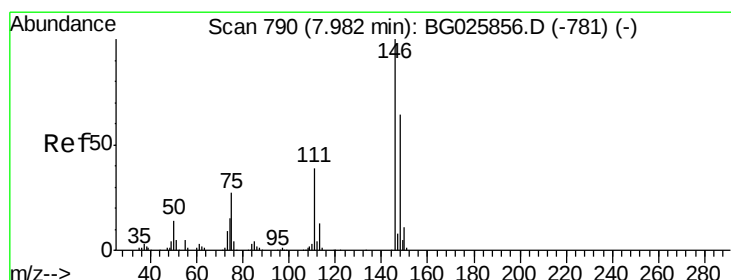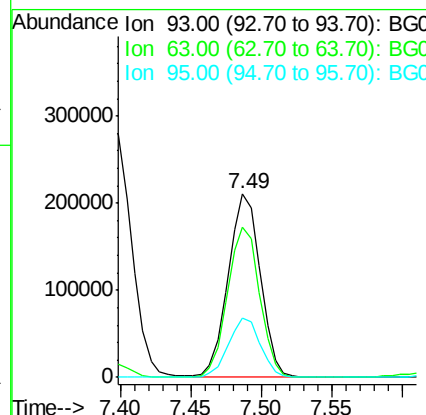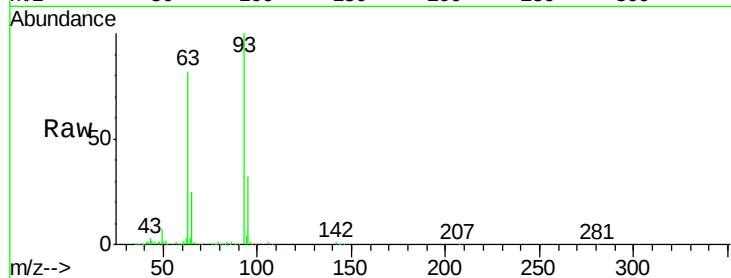

#12
1,3-Dichlorobenzene
Concen: 39.45 ng
RT: 7.97 min Scan# 788
Delta R.T. -0.01 min
Lab File: BG026022.D
Acq: 2 Mar 2017 10:02

Tgt Ion	Ratio	Resp	Lower	Upper
146	100	378858		
148	64.2	49.2	73.8	
75	24.1	33.4	50.2	

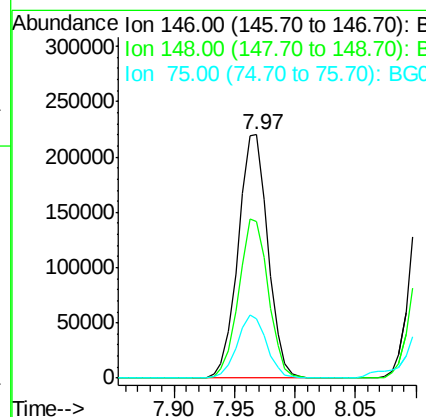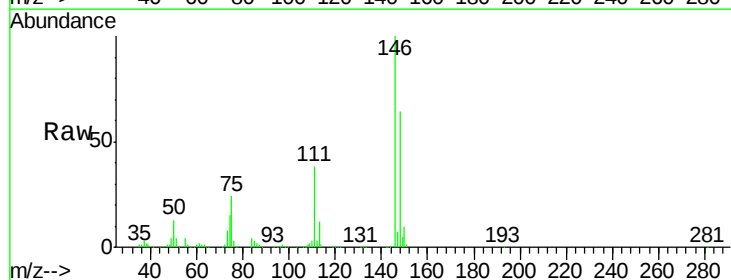

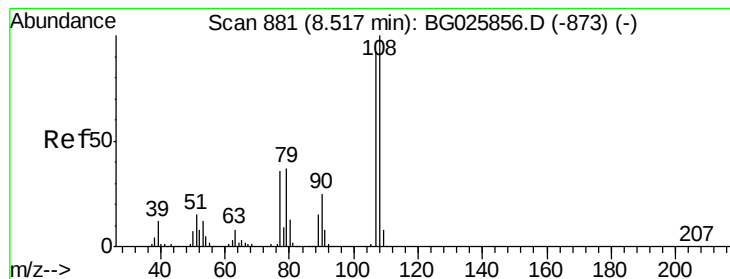





#17
2-Methylphenol
Concen: 35.61 ng
RT: 8.51 min Scan# 880
Delta R.T. -0.01 min
Lab File: BG026022.D
Acq: 2 Mar 2017 10:02

Instrument :
BNA_G
ClientSampleId :
SSTDCCC040

Tgt Ion	Ratio	Resp	Lower	Upper
107	100	288312		
108	111.6	85.6	128.4	
77	39.7	51.4	77.2#	
79	37.1	49.2	73.8#	




Manual Integrations
APPROVED




mohammad
3/3/2017 10:56:20 AM

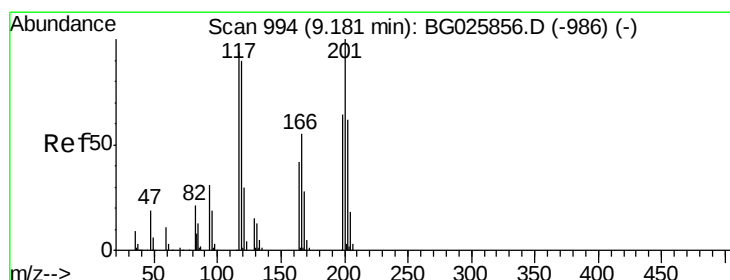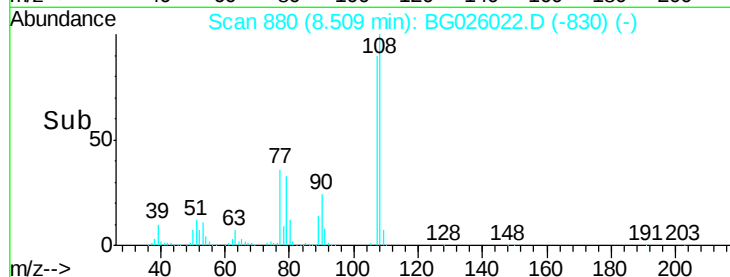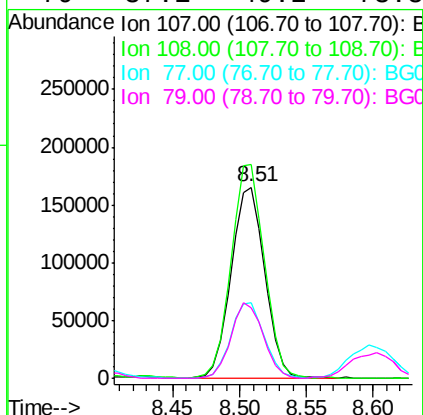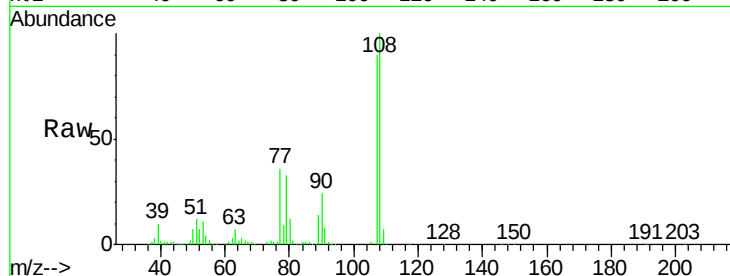

#18
Hexachloroethane
Concen: 39.80 ng
RT: 9.16 min Scan# 991
Delta R.T. -0.02 min
Lab File: BG026022.D
Acq: 2 Mar 2017 10:02

Tgt Ion	Ratio	Resp	Lower	Upper
117	100	128308		
119	97.1	69.8	104.6	
201	110.7	95.4	143.0	

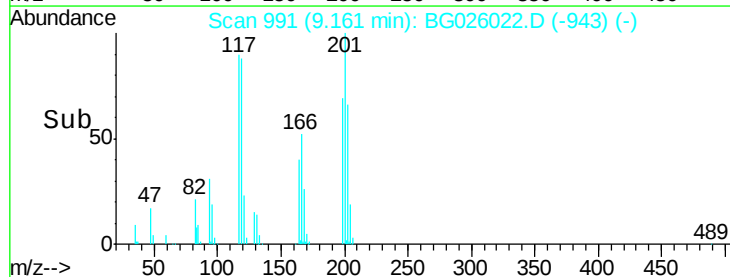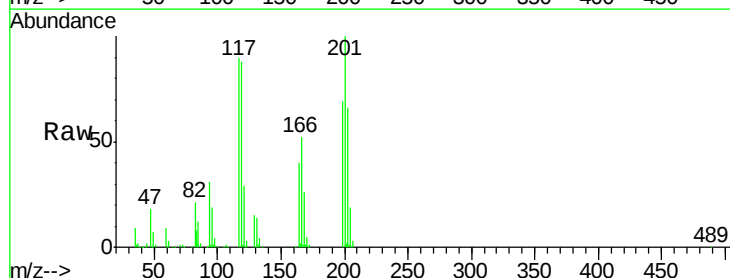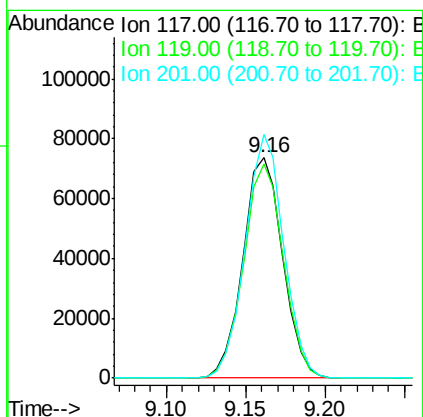

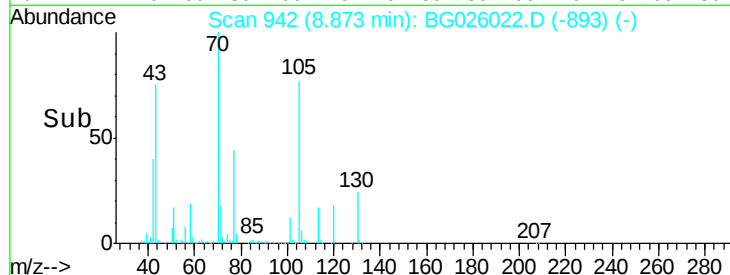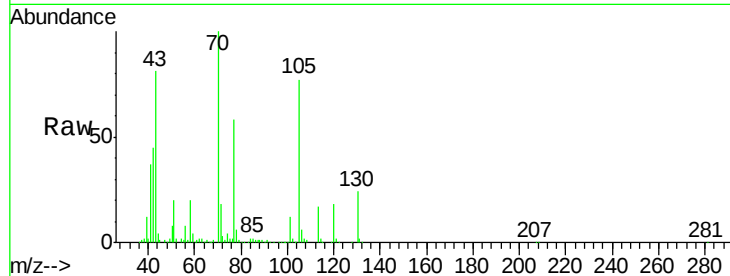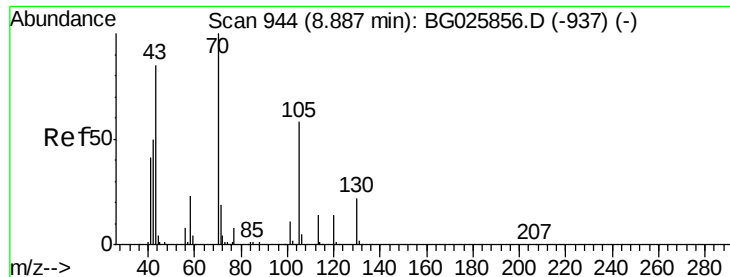





#19
n-Nitroso-di-n-propylamine
Concen: 32.63 ng
RT: 8.87 min Scan# 942
Delta R.T. -0.01 min
Lab File: BG026022.D
Acq: 2 Mar 2017 10:02

Instrument :
BNA_G
ClientSampleId :
SSTDCCC040

Tgt Ion	Ratio	Lower	Upper
70	100		
42	44.6	56.1	84.1#
101	11.7	7.5	11.3#
130	24.0	14.6	21.8#


Manual Integrations
APPROVED


mohammad
3/3/2017 10:56:20 AM

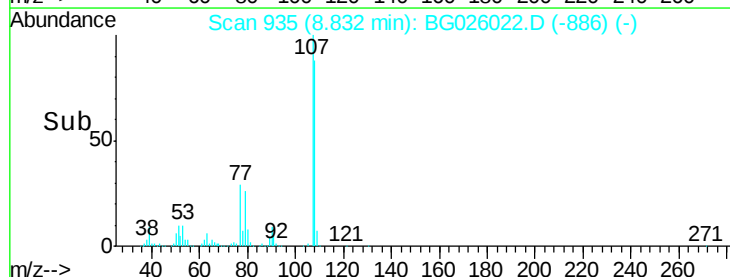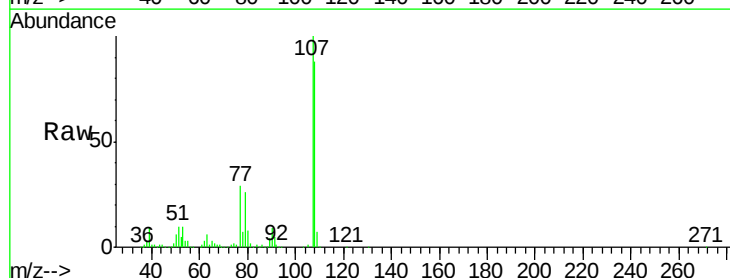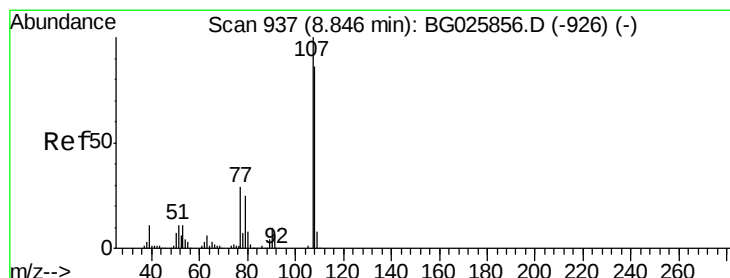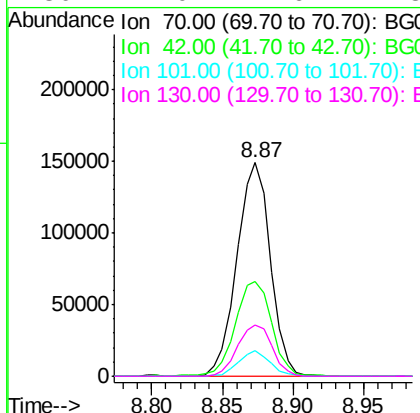

#20
3+4-Methylphenols
Concen: 34.73 ng
RT: 8.83 min Scan# 935
Delta R.T. -0.01 min
Lab File: BG026022.D
Acq: 2 Mar 2017 10:02

Tgt Ion	Ratio	Lower	Upper
107	100		
108	88.3	70.8	110.8
77	29.0	25.8	65.8
79	26.0	20.1	60.1

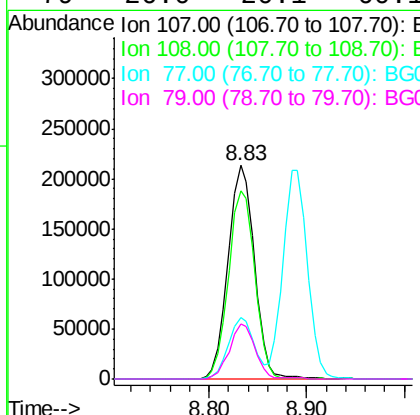

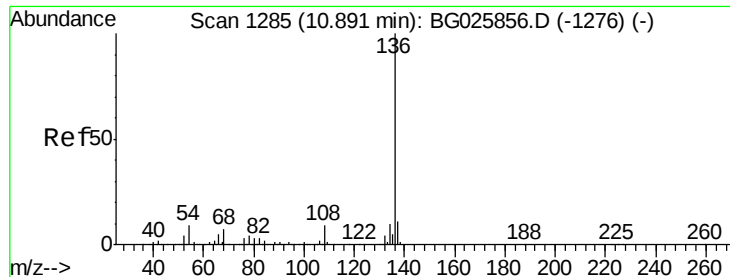





#21
Naphthalene-d8
Concen: 20.00 ng
RT: 10.88 min Scan# 1283
Delta R.T. -0.01 min
Lab File: BG026022.D
Acq: 2 Mar 2017 10:02

Instrument :
BNA_G
ClientSampleId :
SSTDCCC040

Tgt Ion	Ratio	Resp	Lower	Upper
136	100	522718		
137	10.5	8.9	13.3	
54	7.9	9.3	13.9	
68	6.0	5.1	7.7	




Manual Integrations
APPROVED


mohammad
3/3/2017 10:56:20 AM

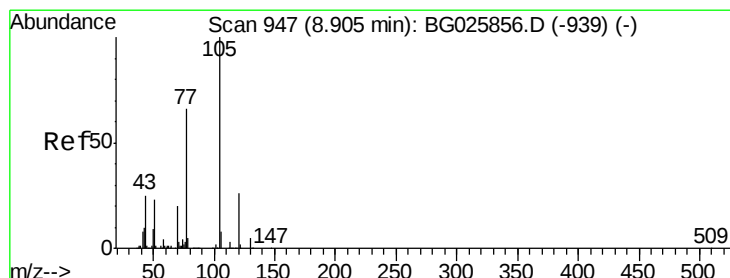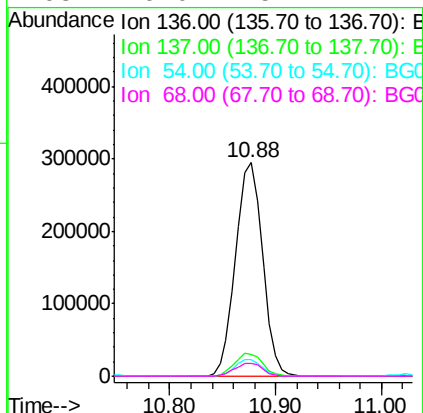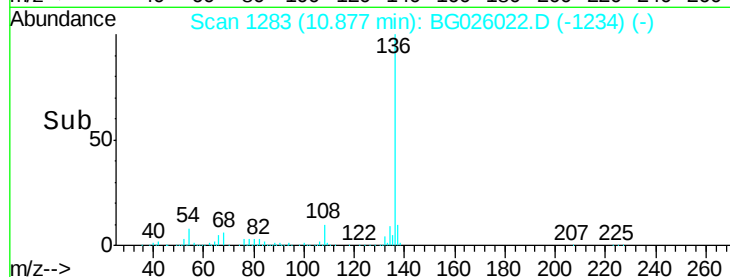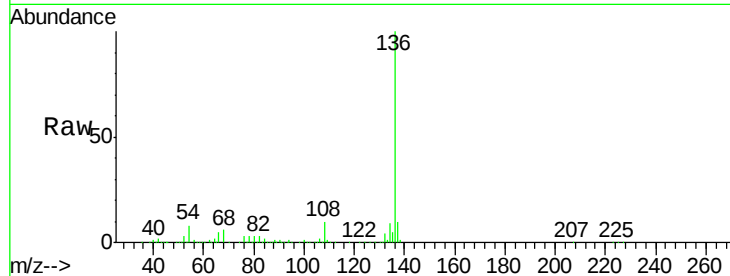

#22
Acetophenone
Concen: 39.85 ng
RT: 8.89 min Scan# 945
Delta R.T. -0.01 min
Lab File: BG026022.D
Acq: 2 Mar 2017 10:02

Tgt Ion	Ratio	Resp	Lower	Upper
105	100	499780		
71	2.0	0.9	1.3	
51	23.0	34.0	51.0	
120	24.7	17.3	25.9	

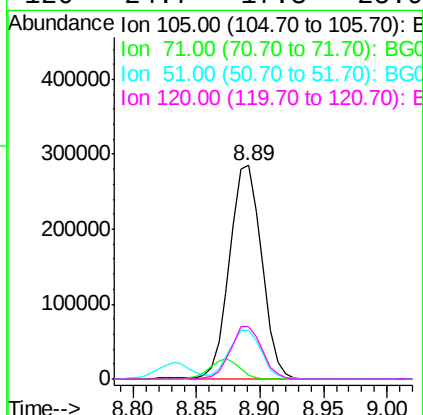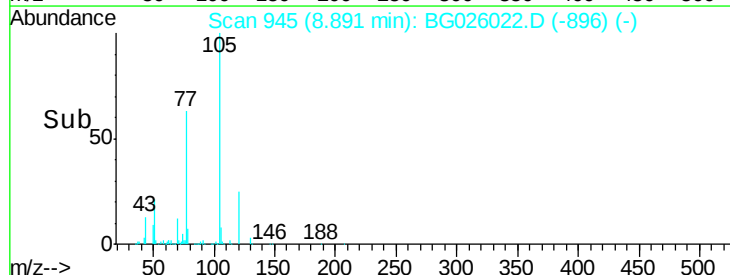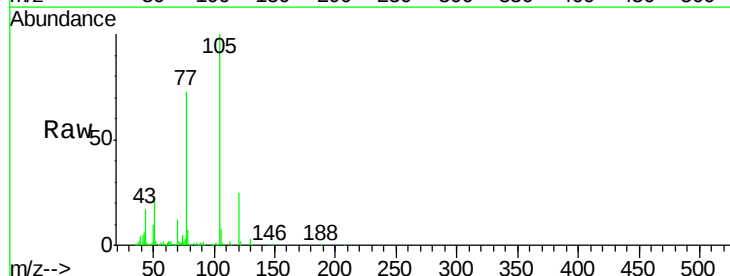







#23
 Nitrobenzene-d5
 Concen: 78.59 ng
 RT: 9.23 min Scan# 1003
 Delta R.T. -0.01 min
 Lab File: BG026022.D
 Acq: 2 Mar 2017 10:02

Instrument :
 BNA_G
 ClientSampleId :
 SSTDCCC040

Tgt Ion	Ratio	Lower	Upper
82	100		
128	48.0	26.4	39.6#
54	47.9	49.4	74.2#




Manual Integrations
 APPROVED


mohammad
 3/3/2017 10:56:20 AM

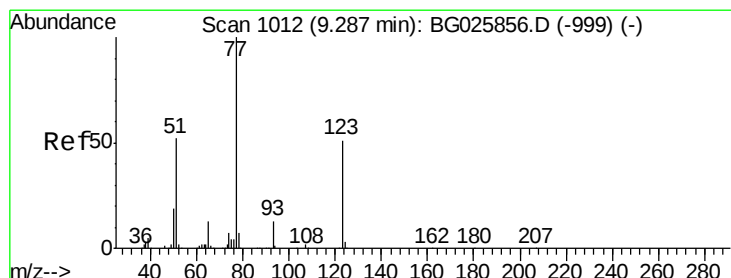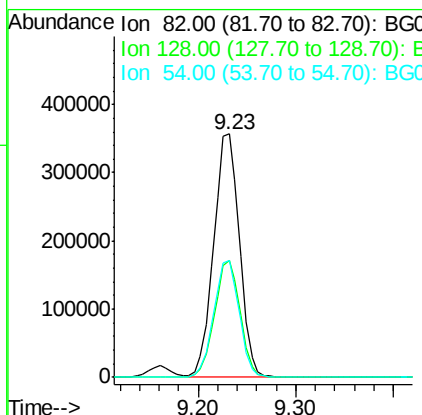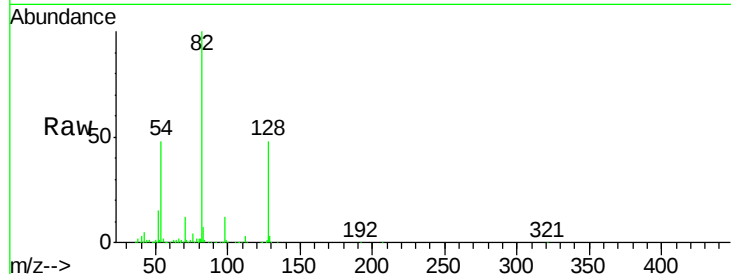

#24
 Nitrobenzene
 Concen: 38.66 ng
 RT: 9.27 min Scan# 1010
 Delta R.T. -0.01 min
 Lab File: BG026022.D
 Acq: 2 Mar 2017 10:02

Tgt Ion	Ratio	Lower	Upper
77	100		
123	50.8	26.1	39.1#
65	13.7	12.4	18.6

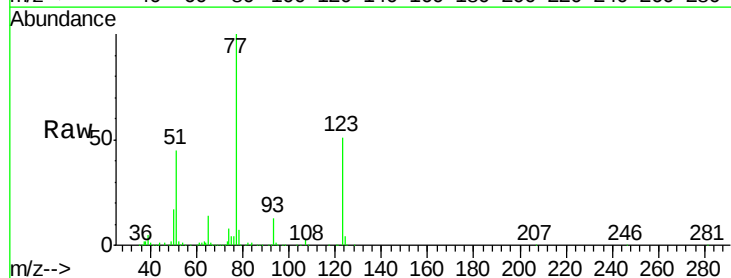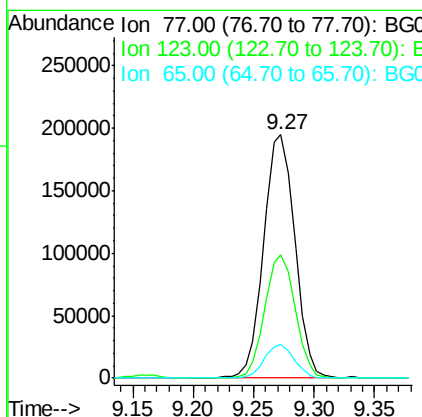

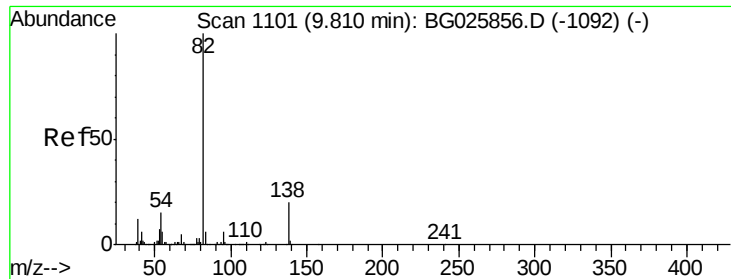





#25
Isophorone
Concen: 38.22 ng
RT: 9.80 min Scan# 1099
Delta R.T. -0.01 min
Lab File: BG026022.D
Acq: 2 Mar 2017 10:02

Instrument :
BNA_G
ClientSampleId :
SSTDCCC040

Tgt Ion	Ratio	Lower	Upper
82	100		
95	6.6	7.5	11.3#
138	20.3	12.3	18.5#




Manual Integrations
APPROVED


mohammad
3/3/2017 10:56:20 AM

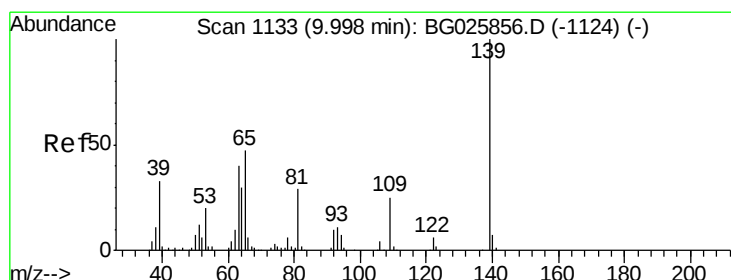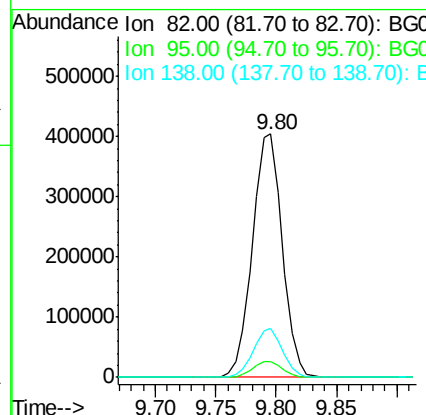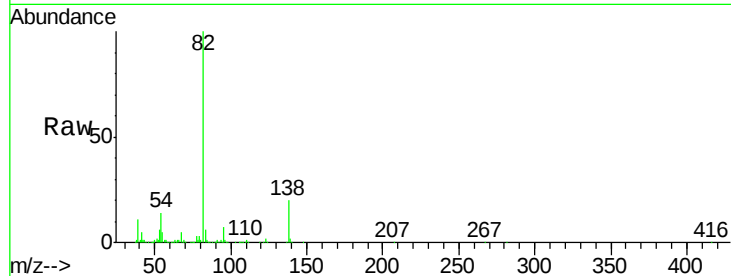

#26
2-Nitrophenol
Concen: 39.15 ng
RT: 9.98 min Scan# 1131
Delta R.T. -0.01 min
Lab File: BG026022.D
Acq: 2 Mar 2017 10:02

Tgt Ion	Ratio	Lower	Upper
139	100		
109	24.4	38.6	58.0#
65	44.2	57.1	85.7#

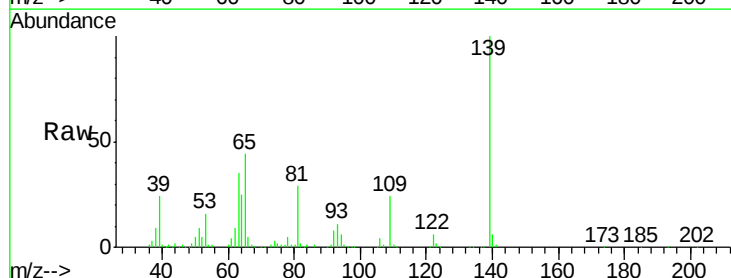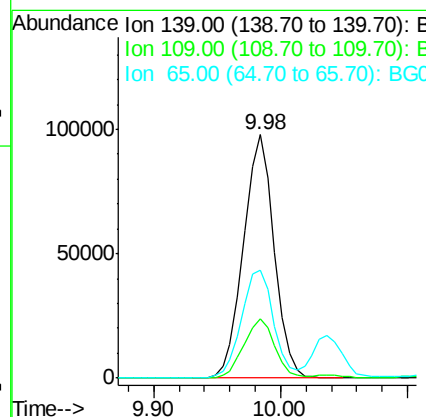

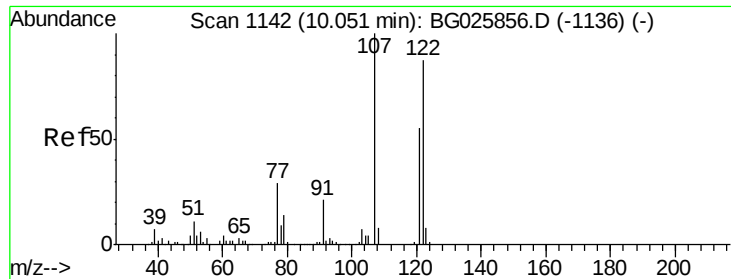





#27
 2,4-Dimethylphenol
 Concen: 39.59 ng
 RT: 10.04 min Scan# 1140
 Delta R.T. -0.01 min
 Lab File: BG026022.D
 Acq: 2 Mar 2017 10:02

Instrument :
 BNA_G
 ClientSampleId :
 SSTDCCC040

Tgt Ion:	122	Resp:	309470
Ion	Ratio	Lower	Upper
122	100		
107	111.5	104.2	156.4
121	57.6	46.0	69.0




Manual Integrations
 APPROVED


mohammad
 3/3/2017 10:56:20 AM

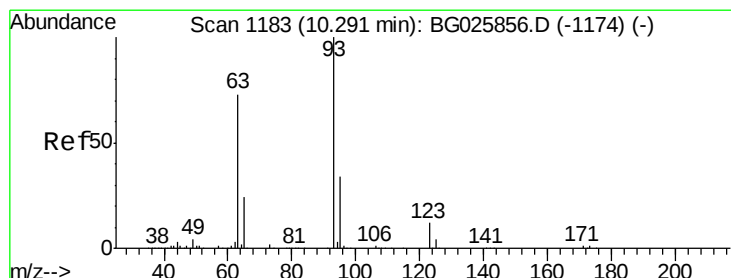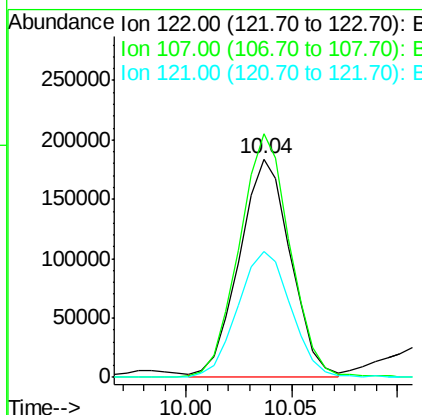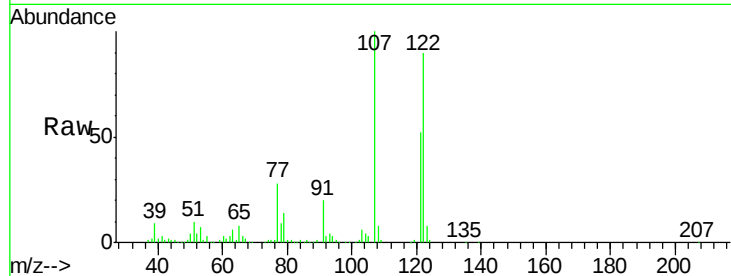

#28
 bis(2-Chloroethoxy)methane
 Concen: 38.53 ng
 RT: 10.27 min Scan# 1180
 Delta R.T. -0.02 min
 Lab File: BG026022.D
 Acq: 2 Mar 2017 10:02

Tgt Ion:	93	Resp:	445119
Ion	Ratio	Lower	Upper
93	100		
95	33.6	25.7	38.5
123	12.3	8.3	12.5

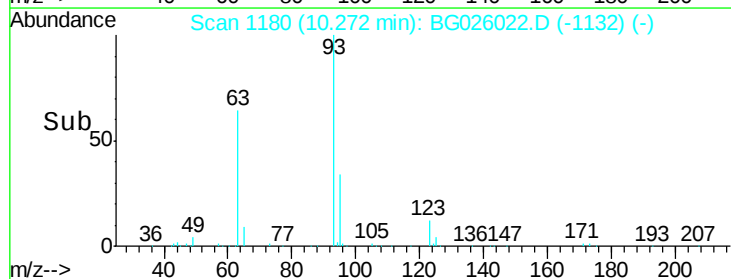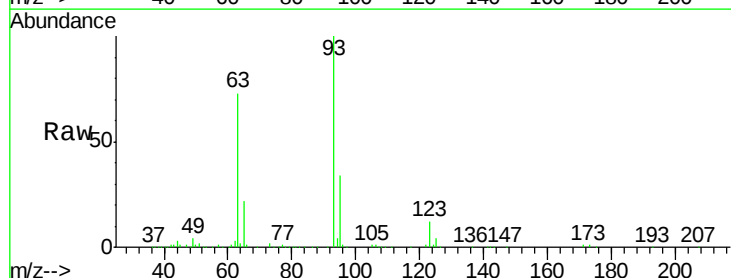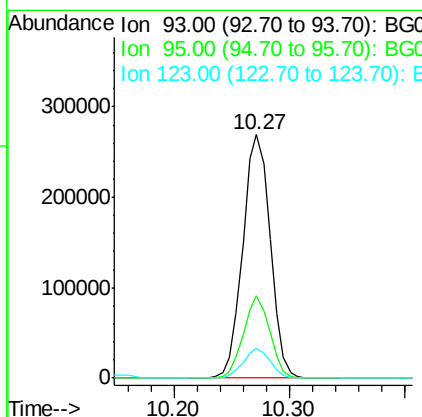

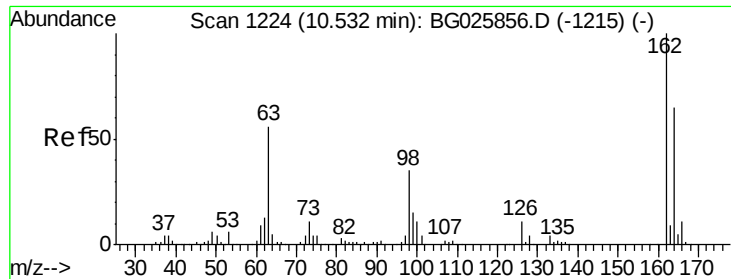





#29
2,4-Dichlorophenol
Concen: 41.14 ng
RT: 10.52 min Scan# 1222
Delta R.T. -0.01 min
Lab File: BG026022.D
Acq: 2 Mar 2017 10:02

Instrument :
BNA_G
ClientSampleId :
SSTDCCC040

Tgt Ion	Ratio	Resp	Lower	Upper
162	100	307001		
164	65.4	42.4	82.4	
98	34.1	20.3	60.3	




Manual Integrations
APPROVED


mohammad
3/3/2017 10:56:20 AM

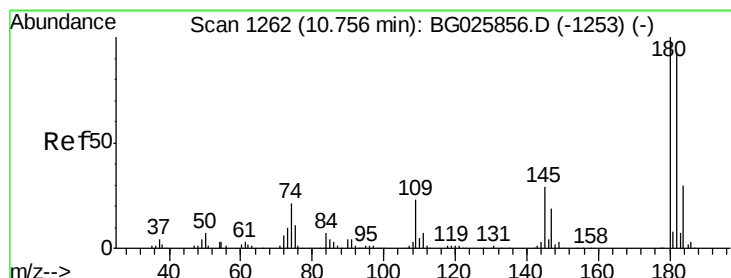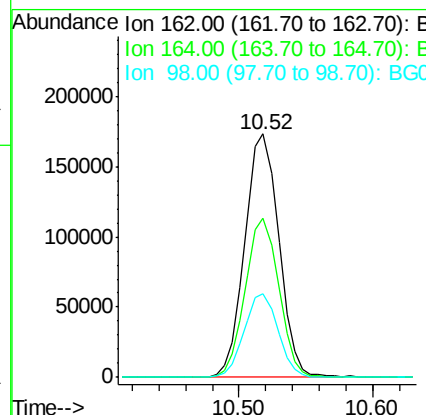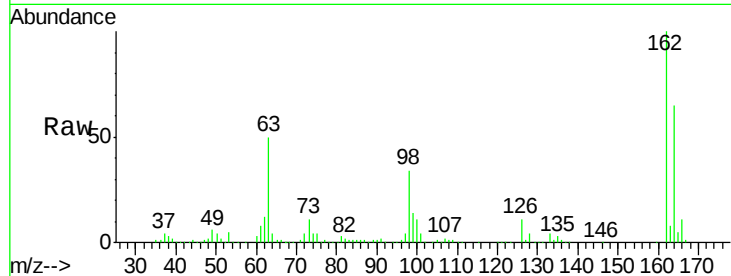

#30
1,2,4-Trichlorobenzene
Concen: 43.06 ng
RT: 10.74 min Scan# 1259
Delta R.T. -0.02 min
Lab File: BG026022.D
Acq: 2 Mar 2017 10:02

Tgt Ion	Ratio	Resp	Lower	Upper
180	100	349437		
182	92.9	77.0	115.4	
145	28.7	23.4	35.0	

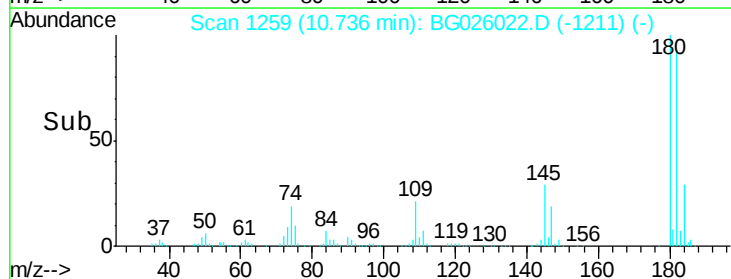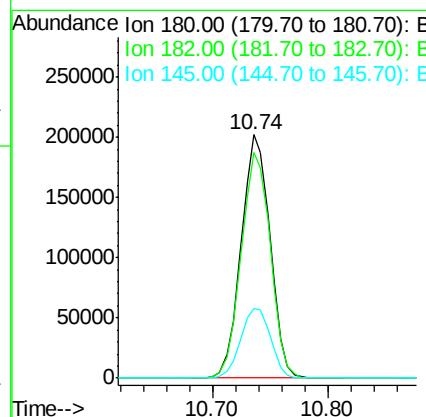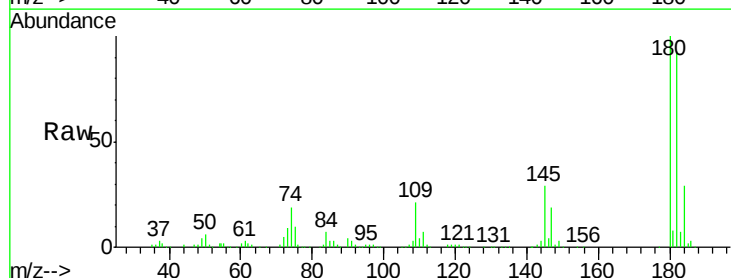

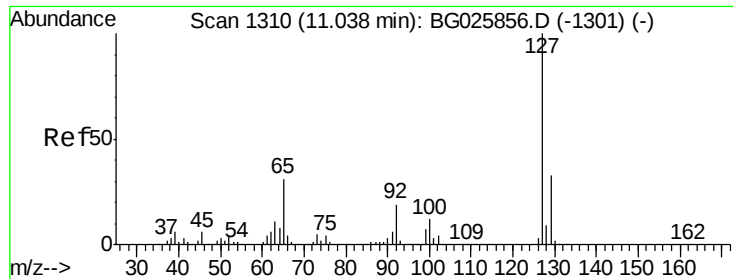


#33
4-Chloroaniline
Concen: 37.85 ng
RT: 11.02 min Scan# 1308
Delta R.T. -0.01 min
Lab File: BG026022.D
Acq: 2 Mar 2017 10:02

Instrument :
BNA_G
ClientSampleId :
SSTDCCC040




Tgt Ion	Ratio	Lower	Upper
127	100		
129	32.0	23.6	35.4
65	28.8	37.7	56.5
92	17.9	17.6	26.4

Manual Integrations
APPROVED

mohammad
3/3/2017 10:56:20 AM

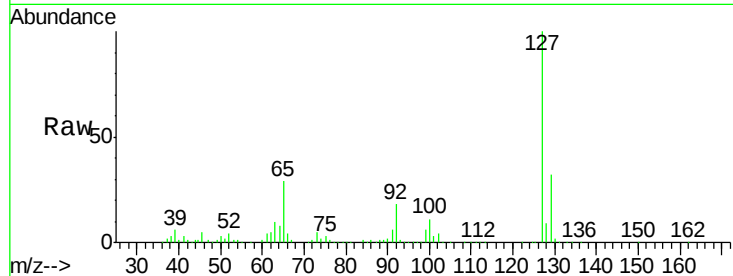


Abundance Ion 127.00 (126.70 to 127.70): E
Ion 129.00 (128.70 to 129.70): E
Ion 65.00 (64.70 to 65.70): BG
Ion 92.00 (91.70 to 92.70): BG

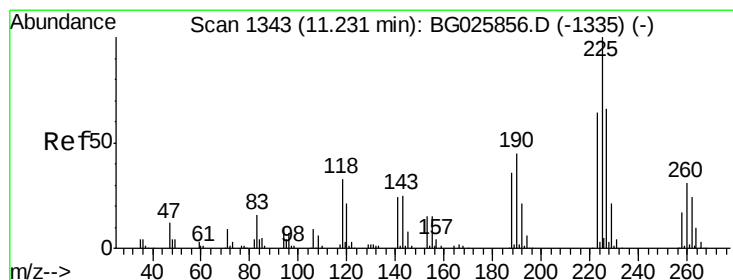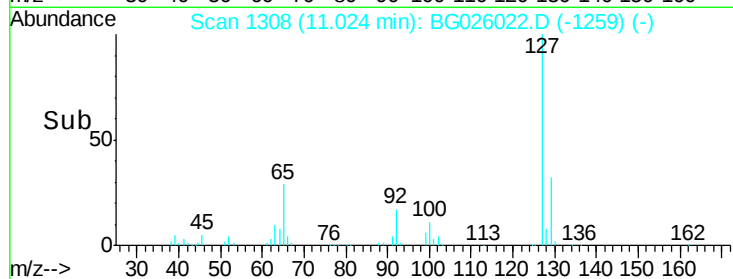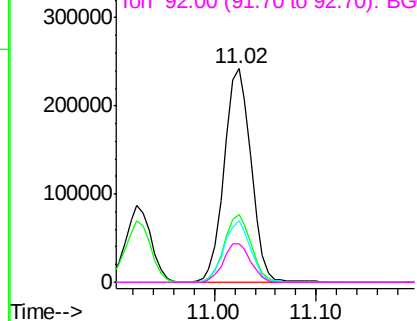

#34
Hexachlorobutadiene
Concen: 44.74 ng
RT: 11.21 min Scan# 1340
Delta R.T. -0.02 min
Lab File: BG026022.D
Acq: 2 Mar 2017 10:02

Tgt Ion	Ratio	Lower	Upper
225	100		
223	63.2	50.7	76.1
227	59.5	49.0	73.6

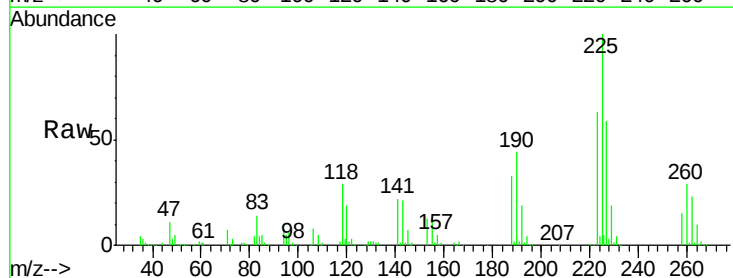

Abundance Ion 225.00 (224.70 to 225.70): E
Ion 223.00 (222.70 to 223.70): E
Ion 227.00 (226.70 to 227.70): E

