

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG030217\
 Data File : BG026023.D
 Acq On : 2 Mar 2017 10:42
 Operator : SJ/MA
 Sample : PB97270BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 PB97270BL

Quant Time: Mar 02 14:58:24 2017
 Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG021717.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Feb 28 15:36:56 2017
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.08	152	114096	20.00	ng	-0.01
21) Naphthalene-d8	10.87	136	488639	20.00	ng	-0.02
38) Acenaphthene-d10	14.67	164	275652	20.00	ng	-0.02
63) Phenanthrene-d10	17.41	188	646332	20.00	ng	-0.01
75) Chrysene-d12	21.65	240	562249	20.00	ng	-0.02
86) Perylene-d12	24.86	264	547933	20.00	ng	-0.03
System Monitoring Compounds						
5) 2-Fluorophenol	5.64	112	1100866	167.98	ng	-0.01
7) Phenol-d6	7.23	99	1396718	144.02	ng	0.00
23) Nitrobenzene-d5	9.23	82	757422	97.82	ng	-0.02
41) 2,4,6-Tribromophenol	16.16	330	479296	188.20	ng	-0.01
44) 2-Fluorobiphenyl	13.31	172	1939537	122.95	ng	-0.02
78) Terphenyl-d14	20.00	244	2439853	105.54	ng	-0.02


Target Compounds	Qvalue
------------------	--------


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG030217\
Data File : BG026023.D
Acq On : 2 Mar 2017 10:42
Operator : SJ/MA
Sample : PB97270BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
PB97270BL

Quant Time: Mar 02 14:58:24 2017
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG021717.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Feb 28 15:36:56 2017
Response via : Initial Calibration

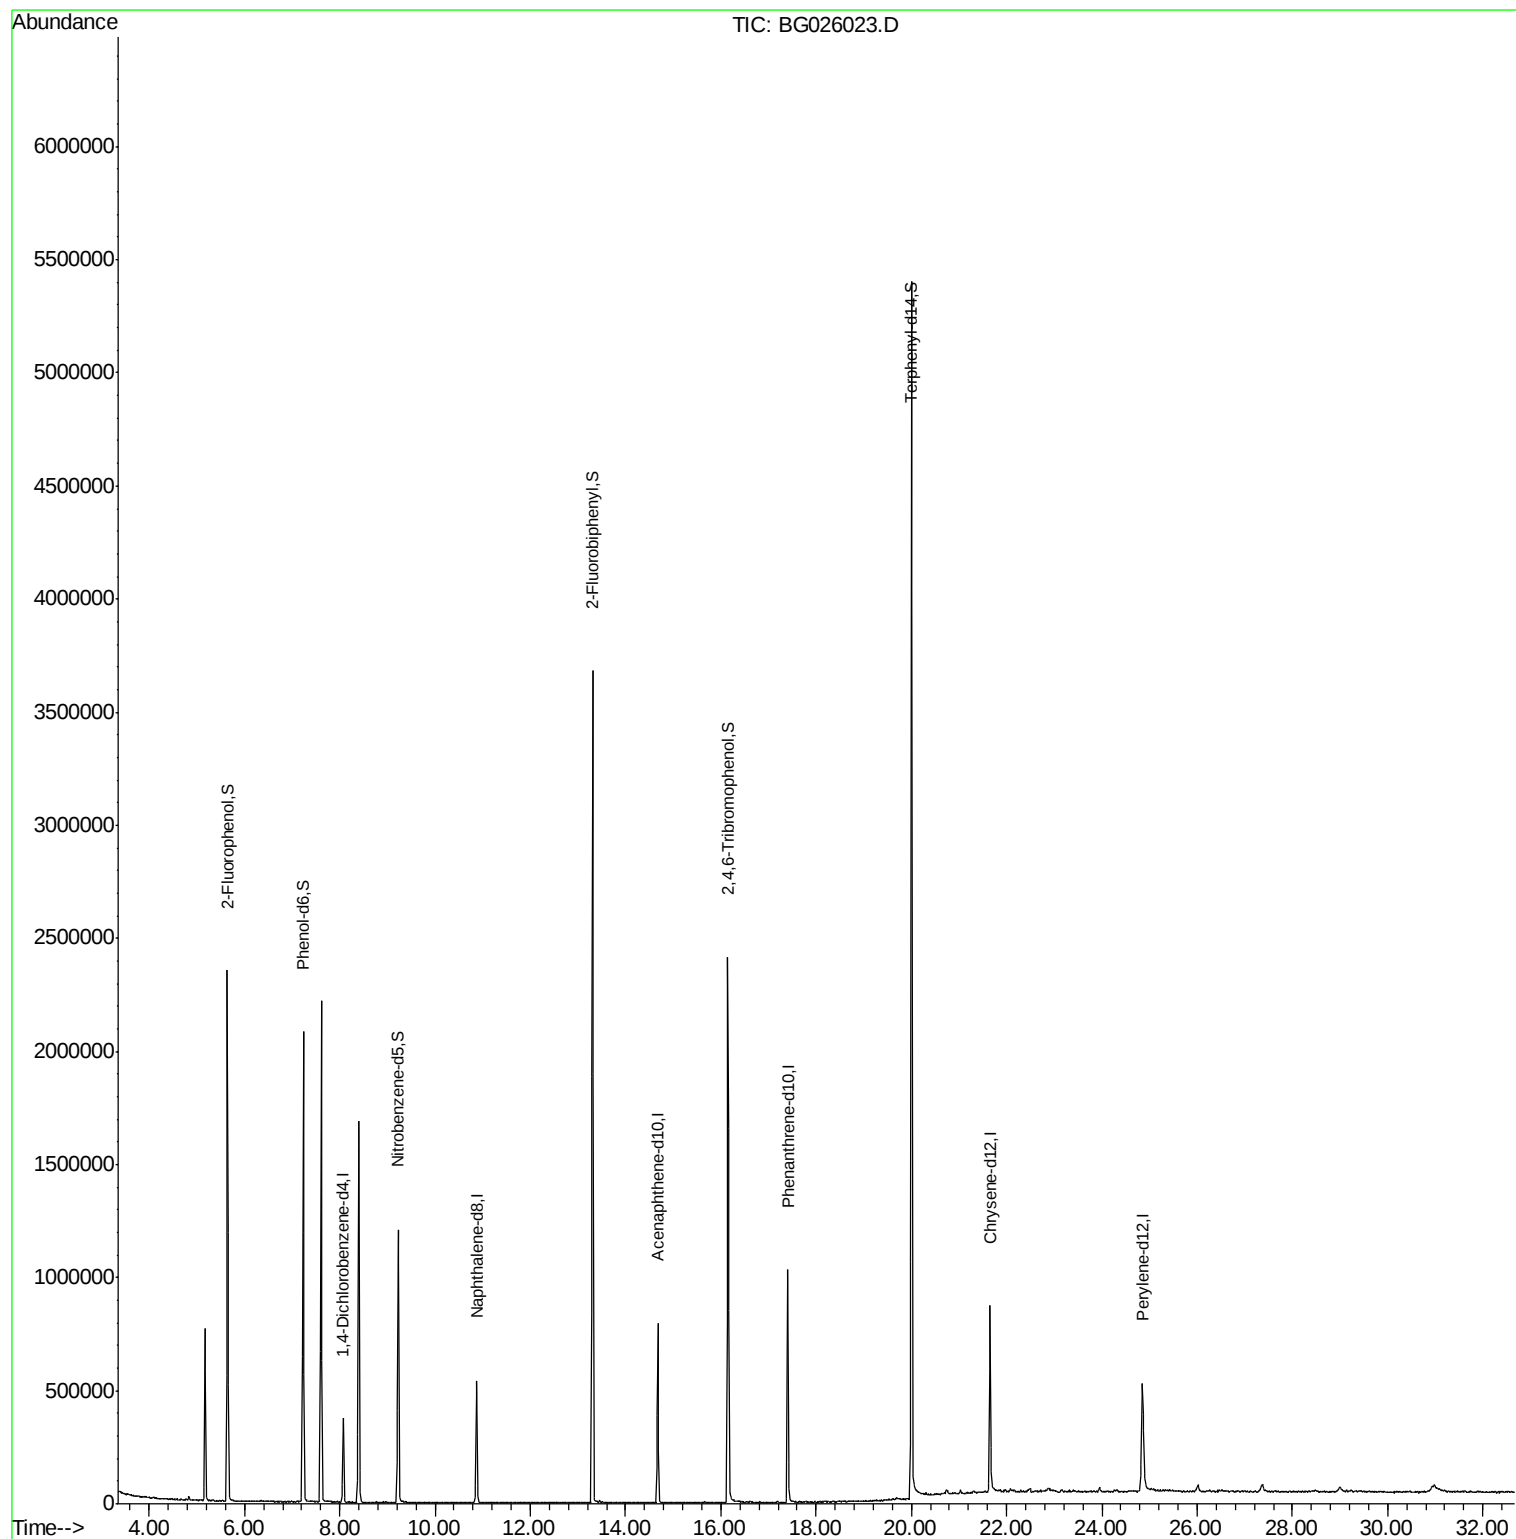

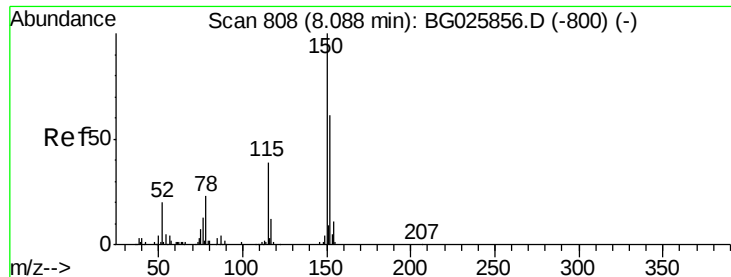


#1




1,4-Dichlorobenzene-d4
Concen: 20.00 ng
RT: 8.08 min Scan# 806
Delta R.T. -0.01 min
Lab File: BG026023.D
Acq: 2 Mar 2017 10:42

Instrument :
BNA_G
ClientSampleId :
PB97270BL

Tgt Ion:152 Resp: 114096
Ion Ratio Lower Upper
152 100
150 159.8 114.0 171.0
115 54.9 48.1 72.1

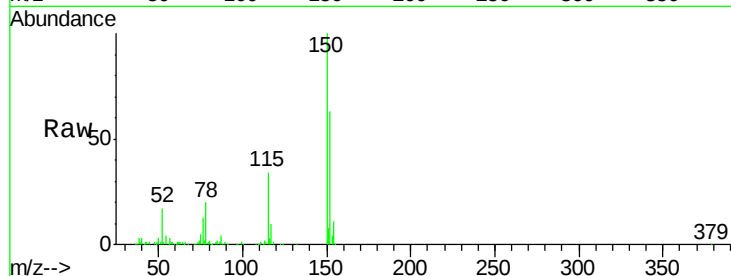


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

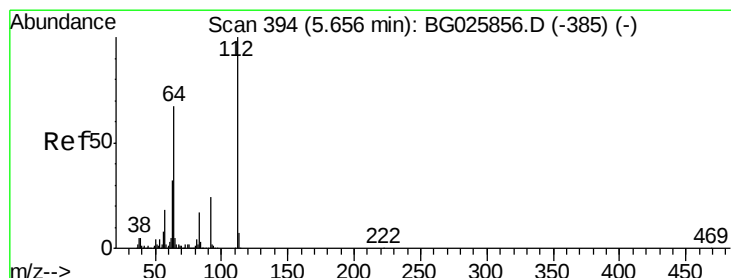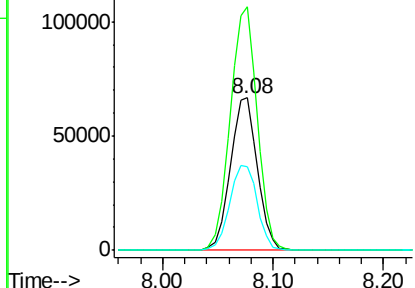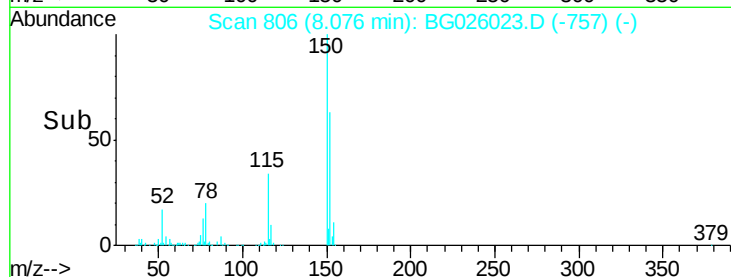



#5


2-Fluorophenol
Concen: 167.98 ng
RT: 5.64 min Scan# 392
Delta R.T. -0.01 min
Lab File: BG026023.D
Acq: 2 Mar 2017 10:42

Tgt Ion:112 Resp: 1100866
Ion Ratio Lower Upper
112 100
64 60.9 61.8 92.6#
63 30.5 37.2 55.8#

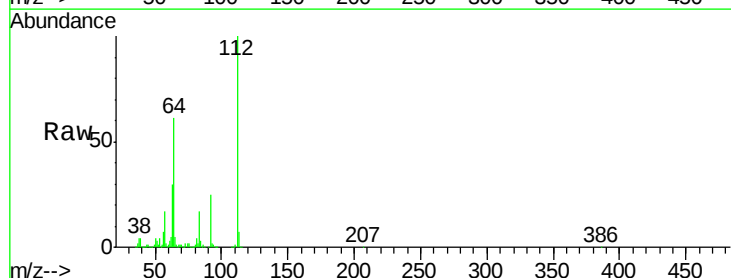

Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BGC
Ion 63.00 (62.70 to 63.70): BGC

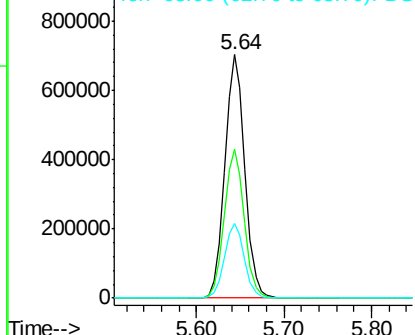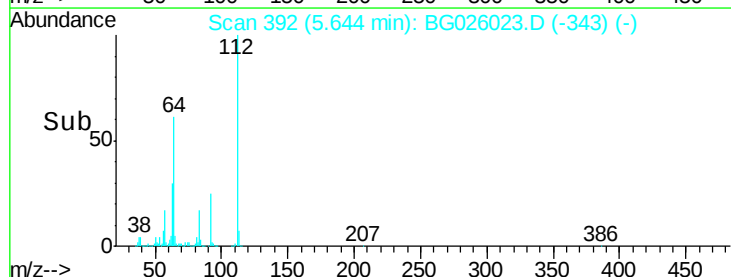

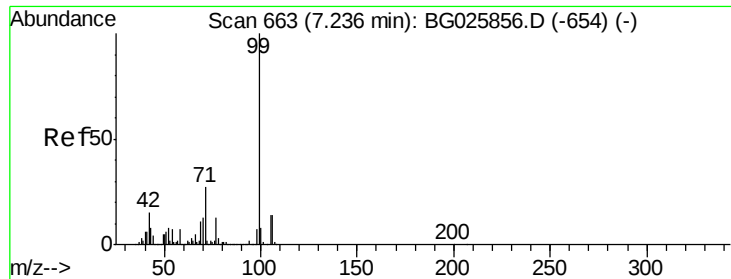

#7

Phenol-d6

Concen: 144.02 ng

RT: 7.23 min Scan# 662

Delta R.T. -0.01 min

Lab File: BG026023.D

Acq: 2 Mar 2017 10:42

Instrument :

BNA_G

ClientSampleId :

PB97270BL


Tgt Ion: 99 Resp: 1396718

Ion Ratio Lower Upper




99 100

42 13.0 20.5 30.7#

71 28.9 37.6 56.4#

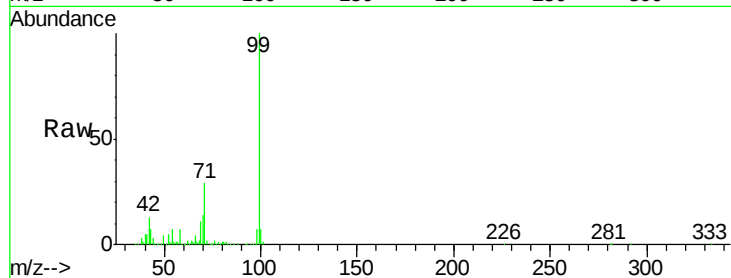

Abundance Ion 99.00 (98.70 to 99.70): BGC
Ion 42.00 (41.70 to 42.70): BGC
Ion 71.00 (70.70 to 71.70): BGC

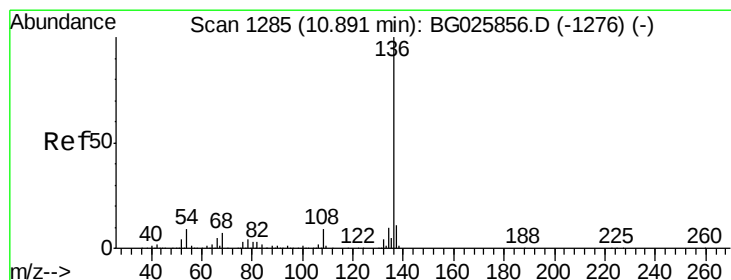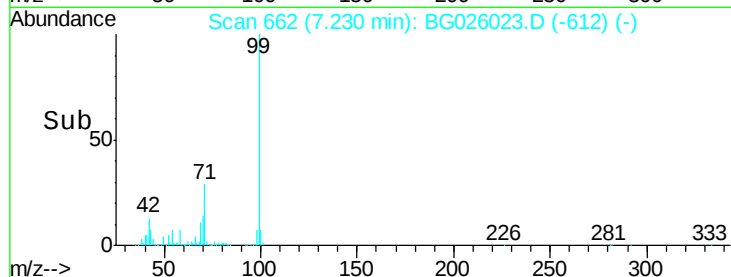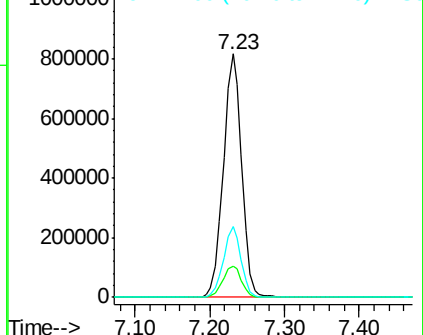

#21

Naphthalene-d8

Concen: 20.00 ng

RT: 10.87 min Scan# 1282

Delta R.T. -0.02 min

Lab File: BG026023.D

Acq: 2 Mar 2017 10:42

Tgt Ion: 136 Resp: 488639


Ion Ratio Lower Upper

136 100



137 11.1 8.9 13.3

54 7.2 9.3 13.9#

68 6.7 5.1 7.7

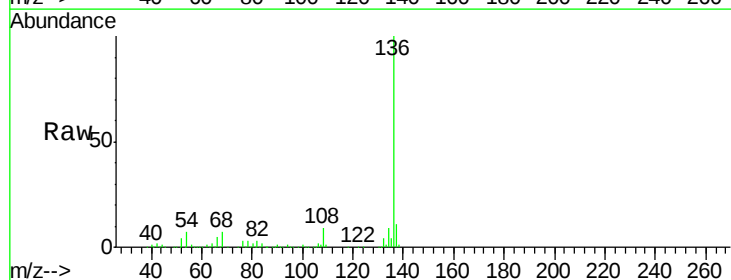

Abundance Ion 136.00 (135.70 to 136.70): BGC
Ion 137.00 (136.70 to 137.70): BGC
Ion 54.00 (53.70 to 54.70): BGC
Ion 68.00 (67.70 to 68.70): BGC



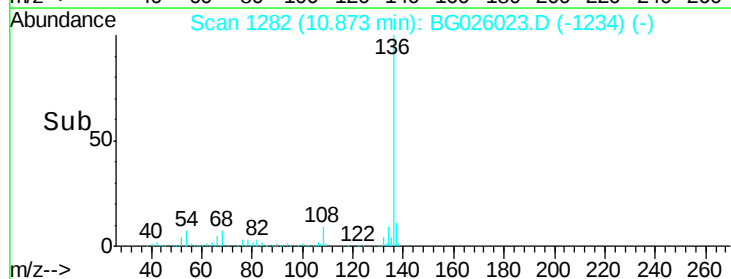
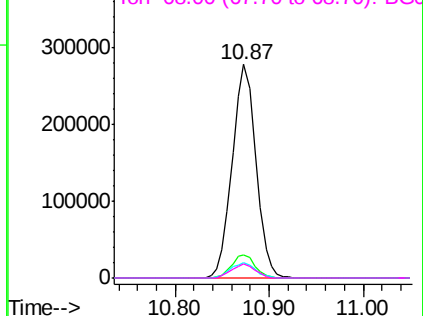




#23
 Nitrobenzene-d5
 Concen: 97.82 ng
 RT: 9.23 min Scan# 1002
 Delta R.T. -0.02 min
 Lab File: BG026023.D
 Acq: 2 Mar 2017 10:42




Instrument :
 BNA_G
 ClientSampled :
 PB97270BL


Tgt Ion: 82 Resp: 757422
 Ion Ratio Lower Upper
 82 100
 128 47.6 26.4 39.6#
 54 47.1 49.4 74.2#

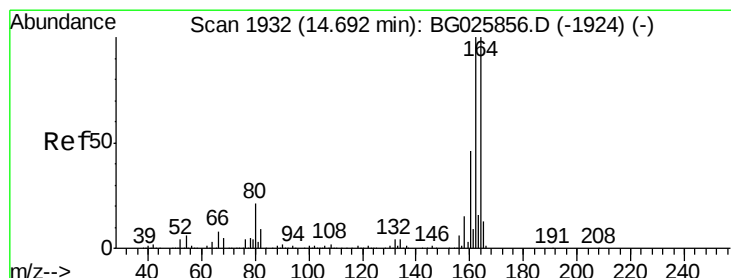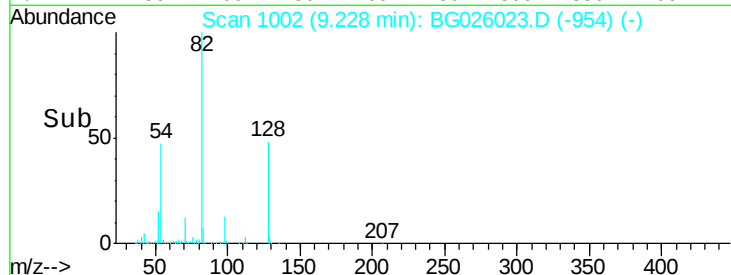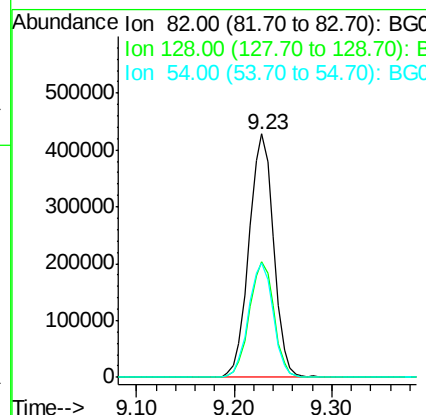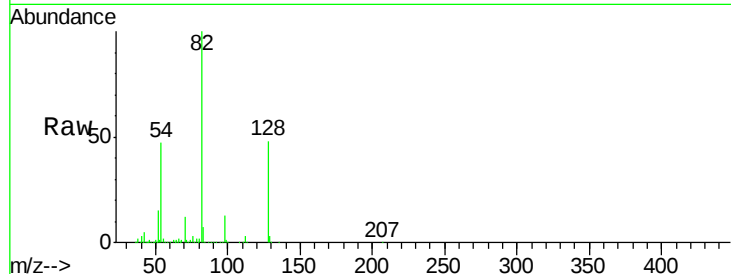

#38
 Acenaphthene-d10
 Concen: 20.00 ng
 RT: 14.67 min Scan# 1929
 Delta R.T. -0.02 min
 Lab File: BG026023.D
 Acq: 2 Mar 2017 10:42

Tgt Ion: 164 Resp: 275652
 Ion Ratio Lower Upper
 164 100
 162 103.2 85.1 127.7
 160 46.4 34.7 52.1


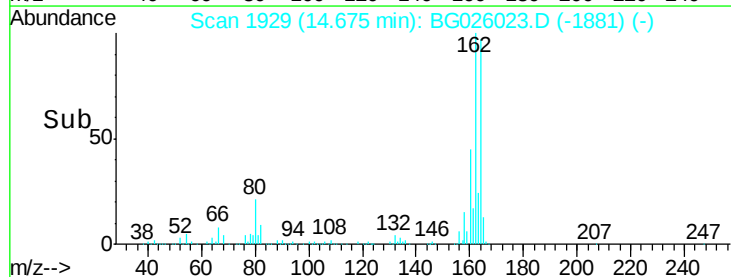
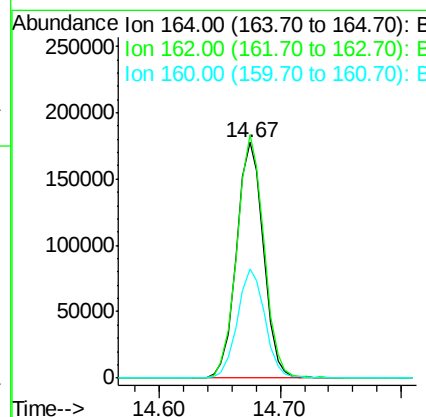
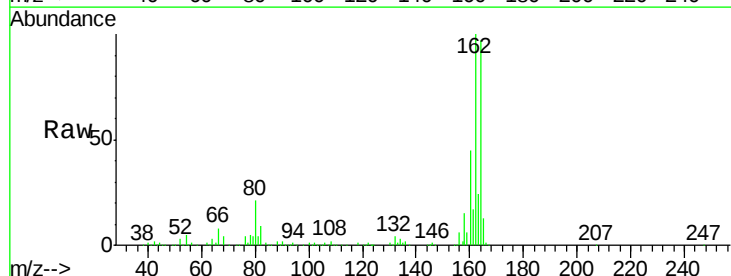


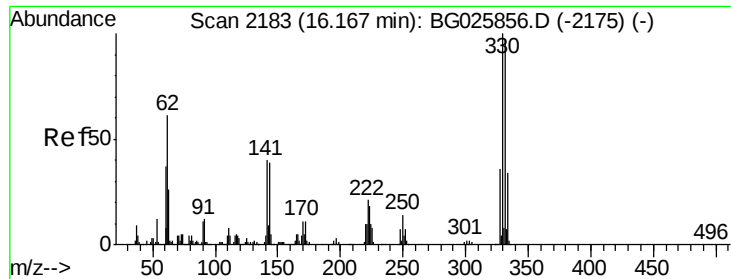

#41
2,4,6-Tribromophenol
Concen: 188.20 ng
RT: 16.16 min Scan# 2181
Delta R.T. -0.01 min
Lab File: BG026023.D
Acq: 2 Mar 2017 10:42




Instrument :
BNA_G
ClientSampleId :
PB97270BL


Tgt Ion	Ratio	Lower	Upper
330	100		
332	96.9	77.3	115.9
141	35.4	32.1	48.1

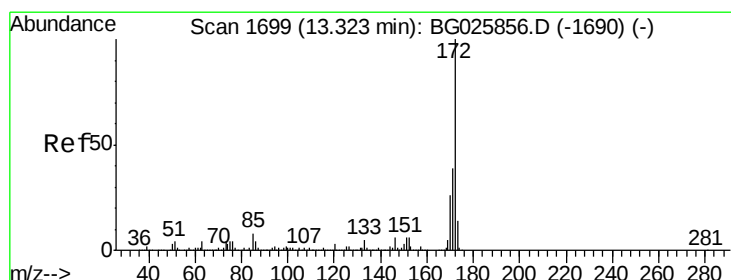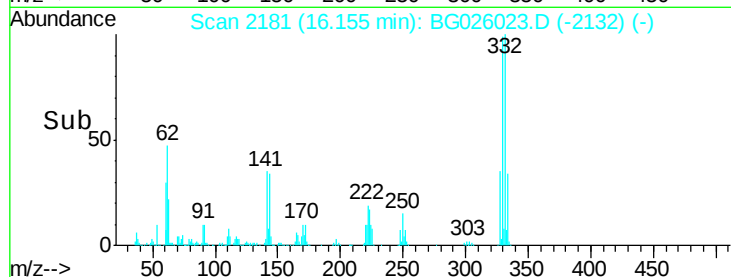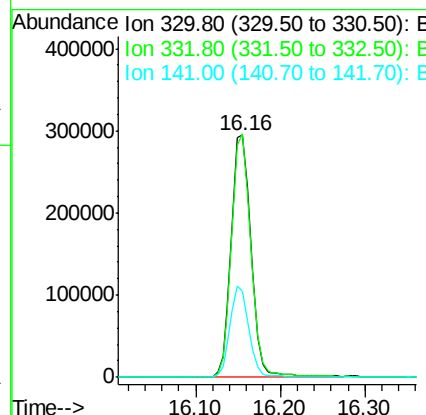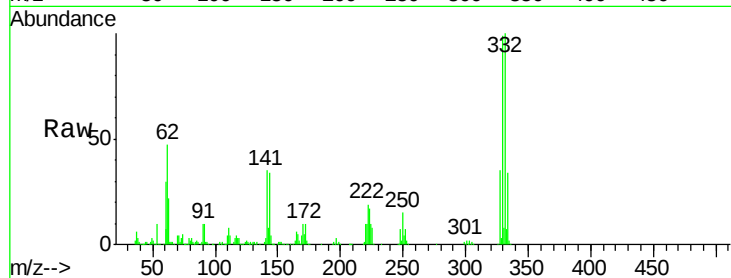

#44
2-Fluorobiphenyl
Concen: 122.95 ng
RT: 13.31 min Scan# 1696
Delta R.T. -0.02 min
Lab File: BG026023.D
Acq: 2 Mar 2017 10:42

Tgt Ion	Ratio	Lower	Upper
172	100		
171	39.0	32.2	48.2
170	25.9	21.8	32.6

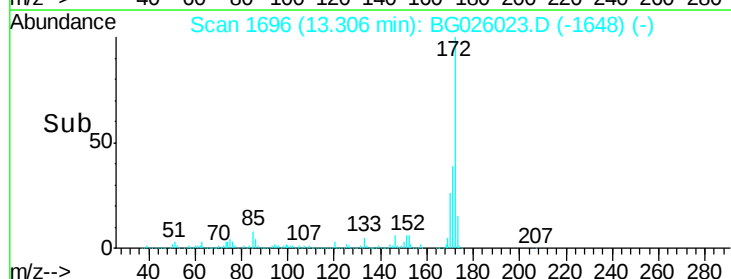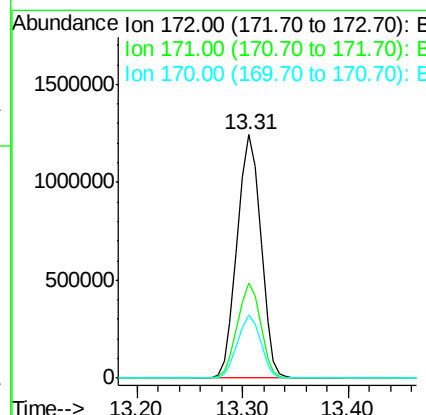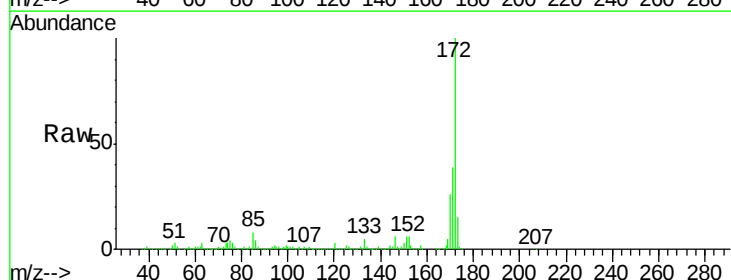

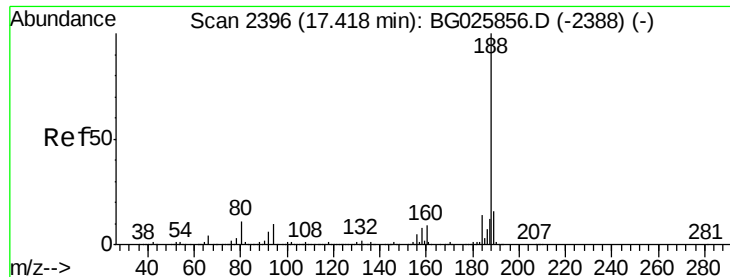

#63

Phenanthrene-d10

Concen: 20.00 ng

RT: 17.41 min Scan# 2394

Delta R.T. -0.01 min

Lab File: BG026023.D

Acq: 2 Mar 2017 10:42

Instrument :

BNA_G

ClientSampleId :

PB97270BL


Tgt Ion:188 Resp: 646332

Ion Ratio Lower Upper

188 100

94 9.0 5.8 8.8#




80 10.5 7.5 11.3

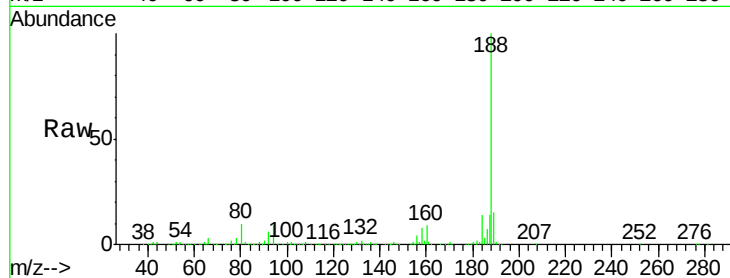

Abundance Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BGC

Ion 80.00 (79.70 to 80.70): BGC

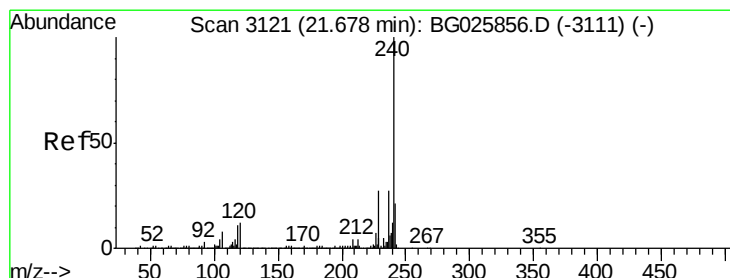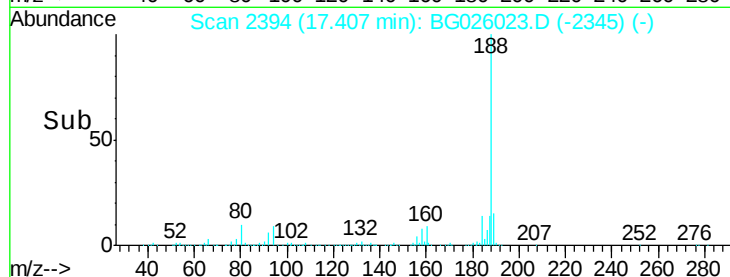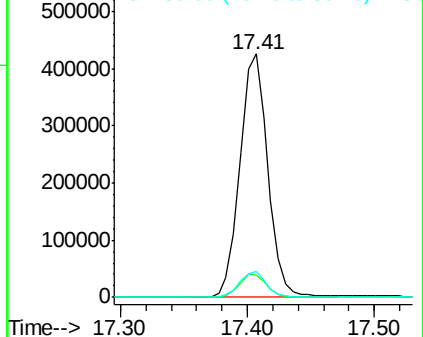

#75

Chrysene-d12

Concen: 20.00 ng

RT: 21.65 min Scan# 3117

Delta R.T. -0.02 min

Lab File: BG026023.D

Acq: 2 Mar 2017 10:42


Tgt Ion:240 Resp: 562249

Ion Ratio Lower Upper

240 100

120 11.3 5.7 8.5#



236 25.7 22.2 33.4

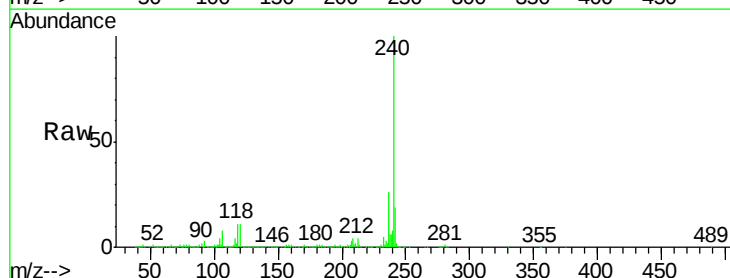


Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

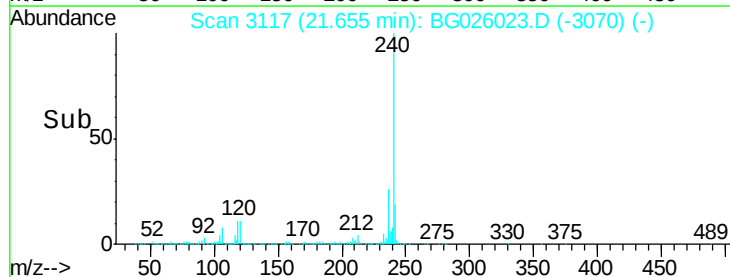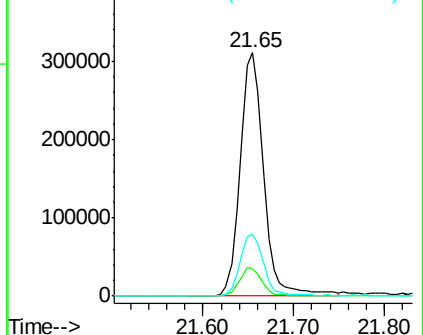

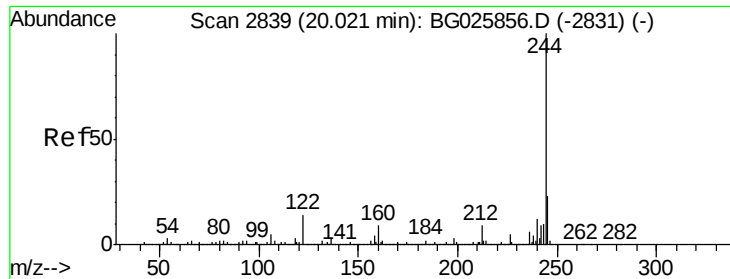

#78

Terphenyl-d14

Concen: 105.54 ng

RT: 20.00 min Scan# 2836

Delta R.T. -0.02 min

Lab File: BG026023.D

Acq: 2 Mar 2017 10:42

Instrument :

BNA_G

ClientSampleId :

PB97270BL


Tgt Ion:244 Resp: 2439853

Ion Ratio Lower Upper

244 100

212 8.6 10.0 15.0#




122 12.9 8.6 12.8#

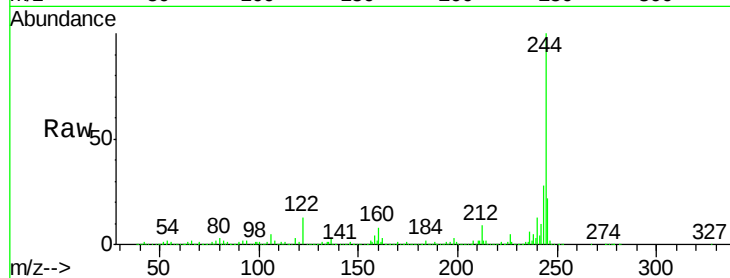

Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

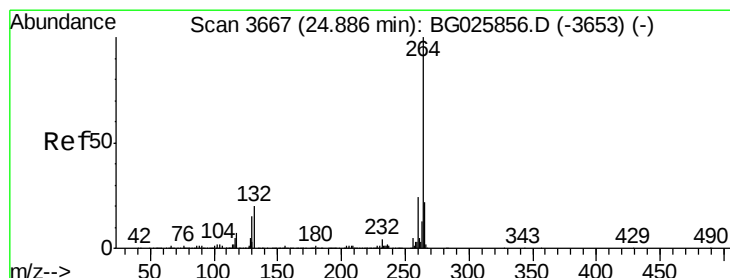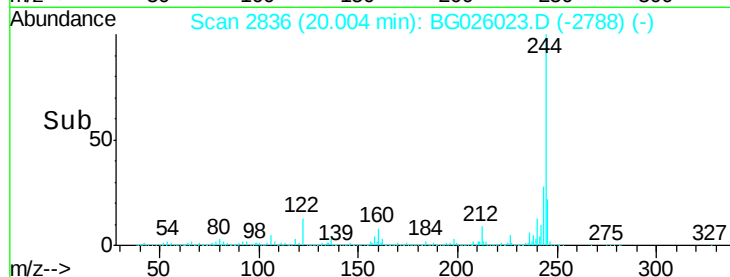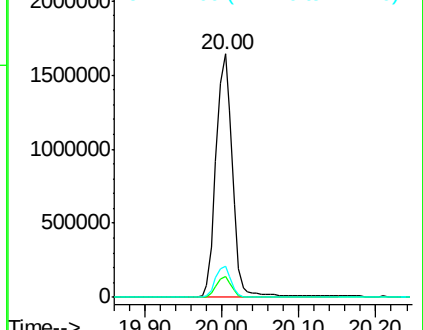

#86

Perylene-d12

Concen: 20.00 ng

RT: 24.86 min Scan# 3662

Delta R.T. -0.03 min

Lab File: BG026023.D

Acq: 2 Mar 2017 10:42


Tgt Ion:264 Resp: 547933

Ion Ratio Lower Upper

264 100

260 25.7 21.8 32.8

265 21.6 18.2 27.4

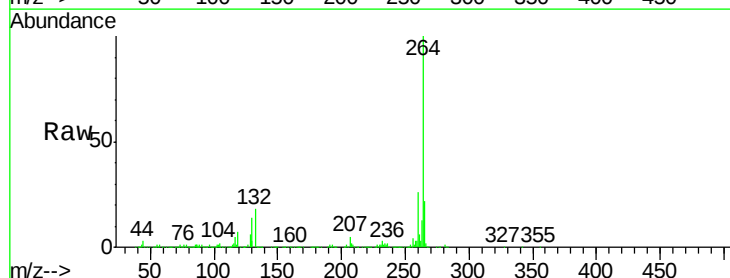

Abundance Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

