

Data Path : Z:\HPCHEM1\BNA G\Data\BG030217\
 Data File : BG026049.D
 Acq On : 3 Mar 2017 3:51
 Operator : SJ/MA
 Sample : I2057-07
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 26B-4

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG021717.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.170	306	312	324	rVB	464114	684690	14.63%	2.444%
2	5.640	384	392	401	rBV	1380711	2135591	45.63%	7.622%
3	7.226	654	662	676	rBV	1250816	2235024	47.76%	7.977%
4	7.602	718	726	735	rBV	1363422	2286044	48.85%	8.159%
5	8.072	799	806	813	rBV	354701	603334	12.89%	2.153%
6	8.396	853	861	869	rBV	1046469	1788411	38.21%	6.383%
7	9.224	994	1002	1014	rBV	742614	1312667	28.05%	4.685%
8	10.869	1275	1282	1293	rBV	487406	892623	19.07%	3.186%
9	13.302	1689	1696	1713	rBV	2211125	3390340	72.44%	12.101%
10	14.118	1827	1835	1842	rBV	188624	271815	5.81%	0.970%
11	14.676	1923	1930	1941	rBV2	698977	1166464	24.92%	4.163%
12	16.151	2174	2181	2193	rBV	1389994	2225406	47.55%	7.943%
13	17.403	2387	2394	2406	rBV	923876	1433094	30.62%	5.115%
14	20.000	2830	2836	2851	rBV	3419210	4680179	100.00%	16.705%
15	21.292	3051	3056	3063	rBV5	62918	121502	2.60%	0.434%
16	21.651	3110	3117	3126	rBV	830753	1390246	29.70%	4.962%
17	24.847	3650	3661	3673	rBV2	477129	1399735	29.91%	4.996%


Sum of corrected areas: 28017165

Data Path : Z:\HPCHEM1\BNA G\Data\BG030217\
Data File : BG026049.D
Acq On : 3 Mar 2017 3:51
Operator : SJ/MA
Sample : I2057-07
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
26B-4

Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG021717.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

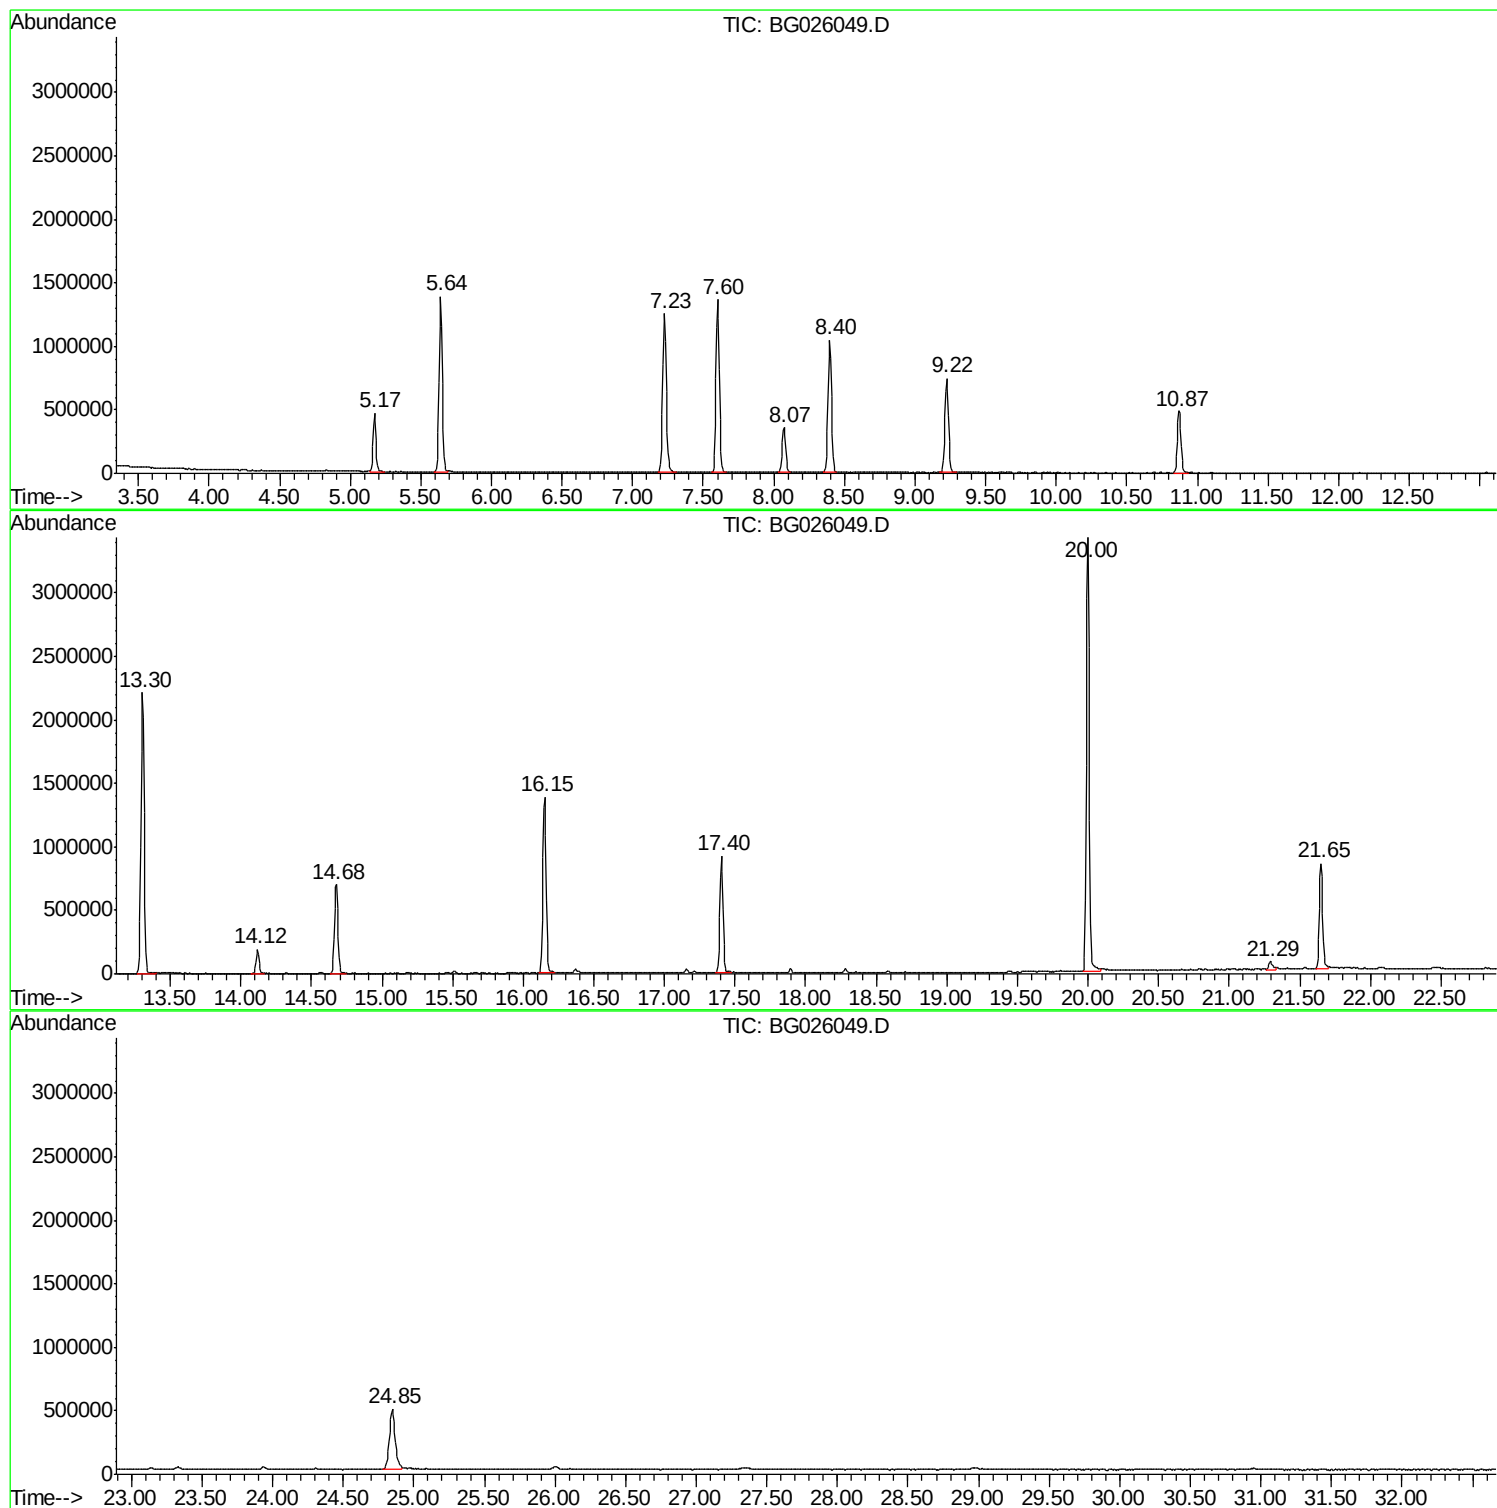

Data Path : Z:\HPCHEM1\BNA G\Data\BG030217\
Data File : BG026049.D
Acq On : 3 Mar 2017 3:51
Operator : SJ/MA
Sample : I2057-07
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
26B-4










Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG021717.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 2-Pentanone, 4-hydroxy-4-me... Concentration Rank 3

R.T.	EstConc	Area	Relative to ISTD	R.T.
5.17	22.70 ng	684690	1,4-Dichlorobenzene-d4	8.07

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	2-Pentanone, 4-hydroxy-4-methyl-	116	C6H12O2	000123-42-2	50
2		Guanidine	59	CH5N3	000113-00-8	47
3		1,8-Nonanediol, 8-methyl-	174	C10H22O2	054725-73-4	25
4		5-Hexen-2-one	98	C6H10O	000109-49-9	9
5		Morpholine, 4-methyl-	101	C5H11NO	000109-02-4	9

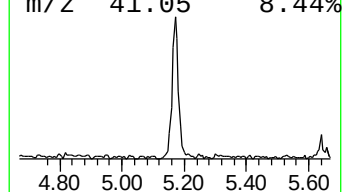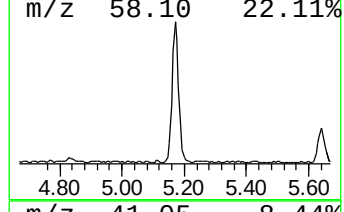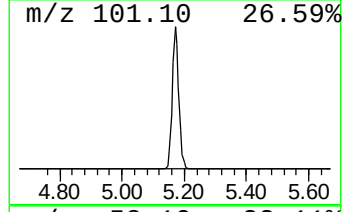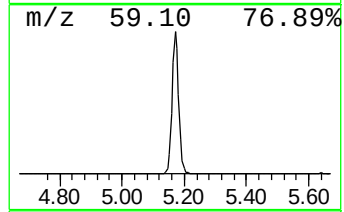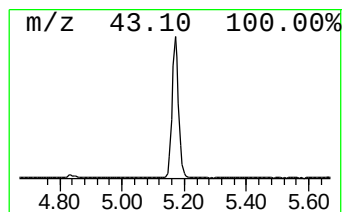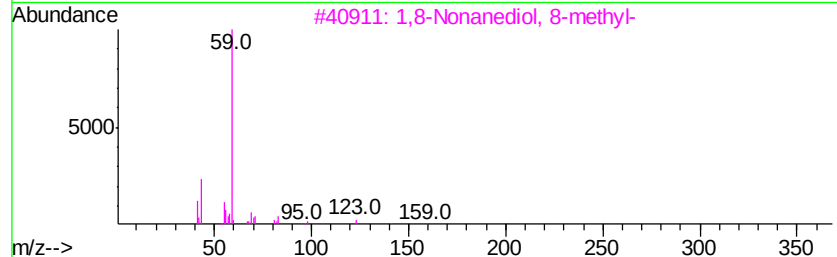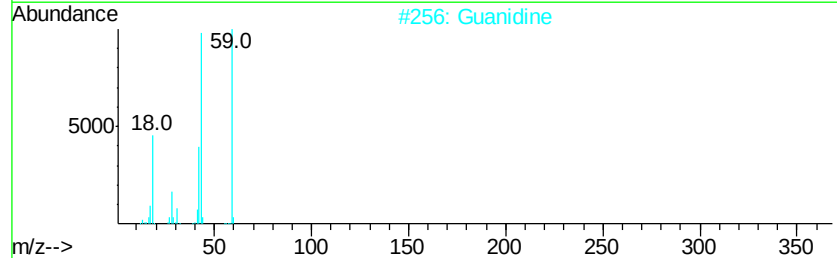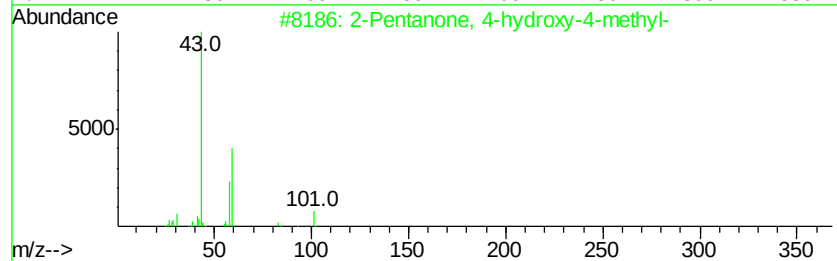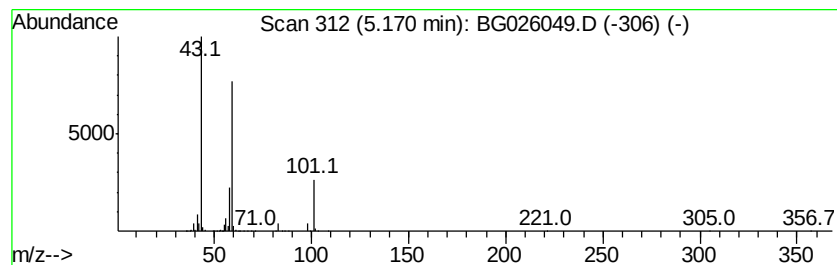

Data Path : Z:\HPCHEM1\BNA G\Data\BG030217\
Data File : BG026049.D
Acq On : 3 Mar 2017 3:51
Operator : SJ/MA
Sample : I2057-07
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampled :
26B-4










Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG021717.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 2 unknown7.60 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
7.60	75.78 ng	2286040	1,4-Dichlorobenzene-d4	8.07

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	3-Chloro-6-fluoro-pyrazine	132	C4H2ClFN2	1000146-10-7	27
2		(E)-3-Chloro-2-methyl-2-pentenal	132	C6H9ClO	031357-76-3	16
3		5-Aminoindole	132	C8H8N2	005192-03-0	12
4		Tranylcypromine-propionyl	189	C12H15NO	1000123-86-3	10
5		4-Chloro-2-fluoro-pyrimidine	132	C4H2ClFN2	051422-00-5	9

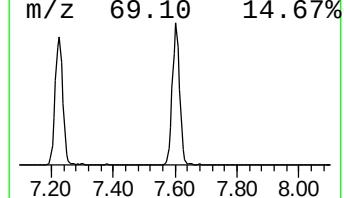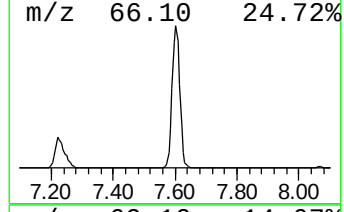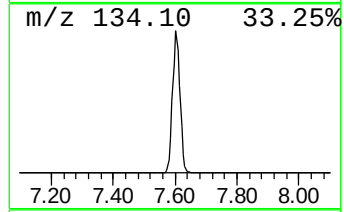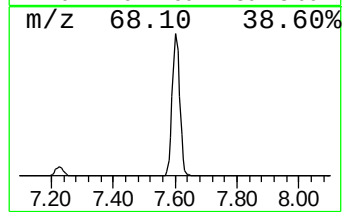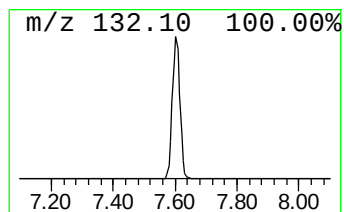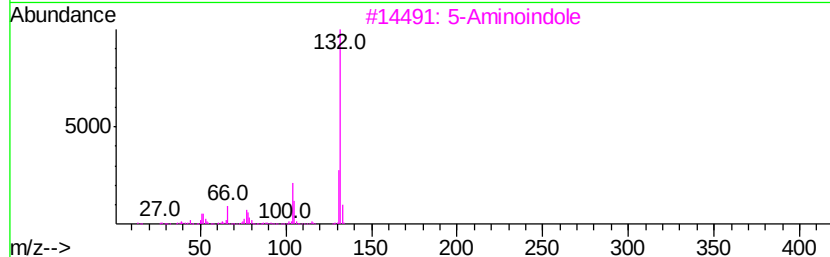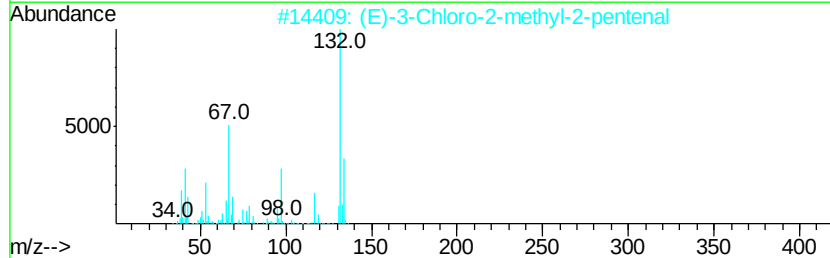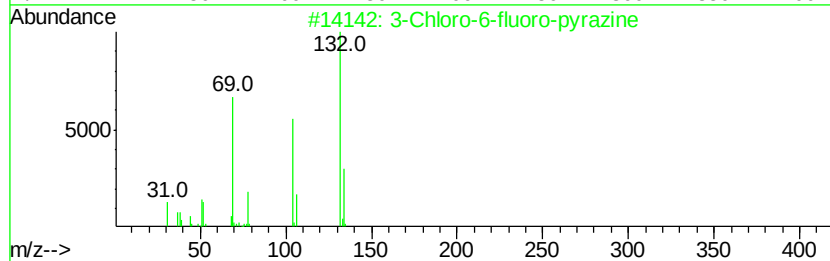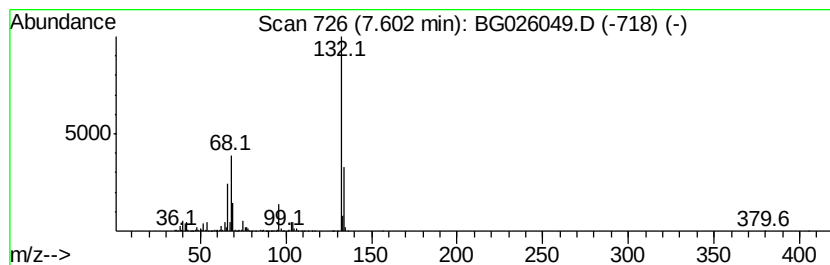

Data Path : Z:\HPCHEM1\BNA_G\Data\BG030217\
Data File : BG026049.D
Acq On : 3 Mar 2017 3:51
Operator : SJ/MA
Sample : I2057-07
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
26B-4

Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG021717.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
2-Pentanone, 4-hy...	5.17	22.7	ng	684690	1	8.07	603334	20.0
unknown7.60	7.60	75.8	ng	2286040	1	8.07	603334	20.0