


Data Path : Z:\HPCHEM1\BNA G\Data\BG030217\
 Data File : BG026021.D
 Acq On : 2 Mar 2017 9:22
 Operator : SJ/MA
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG021717.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Feb 28 15:36:56 2017

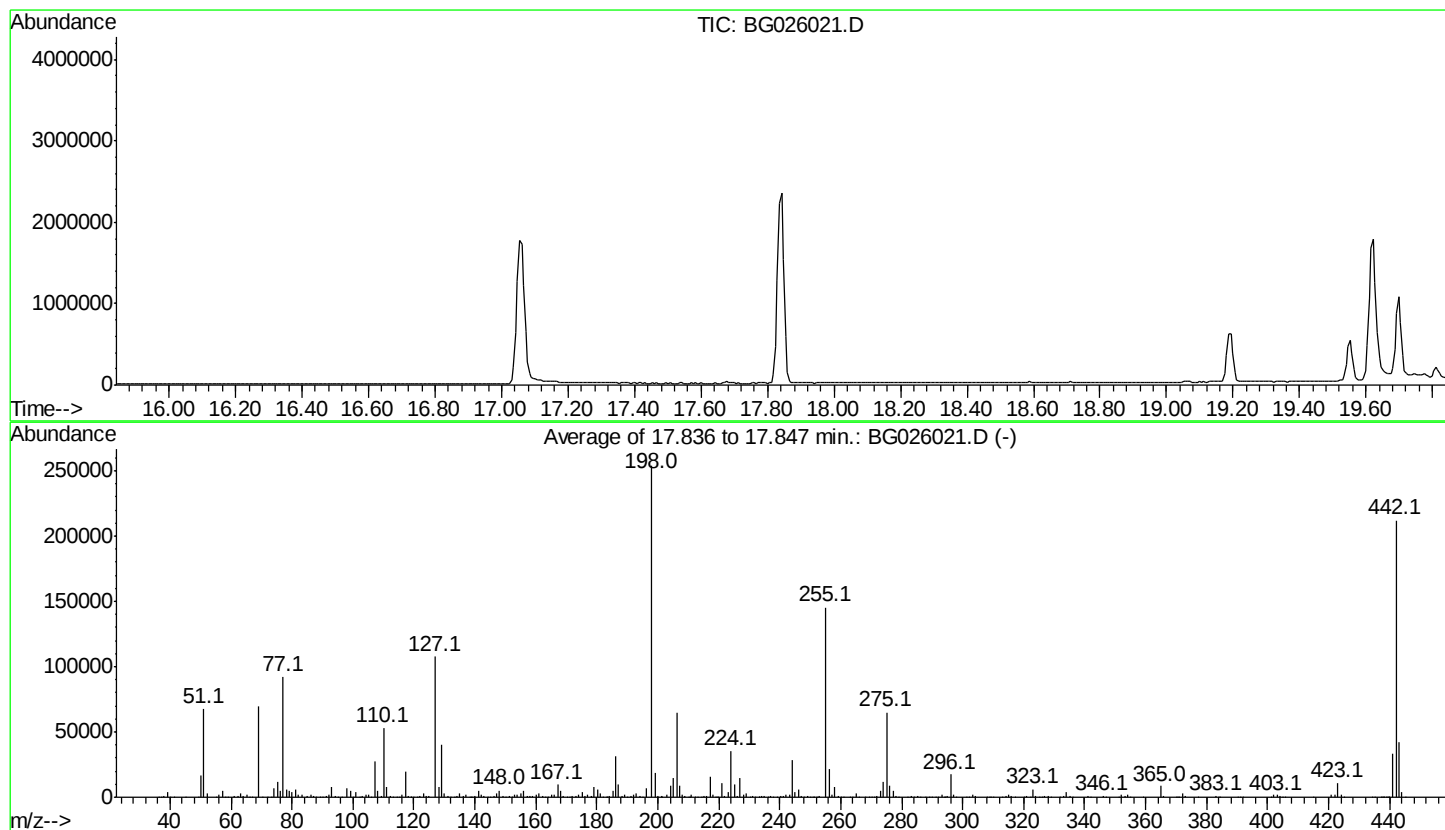

AutoFind: Scans 2467, 2468, 2469; Background Corrected with Scan 2459

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	26.7	67781	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	27.4	69476	PASS
70	69	0.00	2	0.3	233	PASS
127	198	10	80	42.4	107813	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	254016	PASS
199	198	5	9	7.2	18368	PASS
275	198	10	60	25.6	65123	PASS
365	198	1	100	3.4	8624	PASS
441	442	0.01	24	15.9	33768	PASS
442	198	50	100	83.5	212074	PASS
443	442	15	24	20.0	42469	PASS