
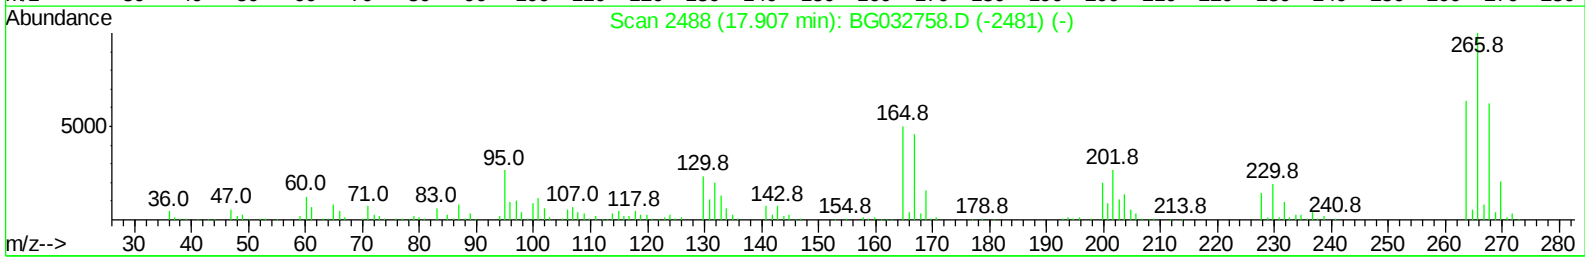
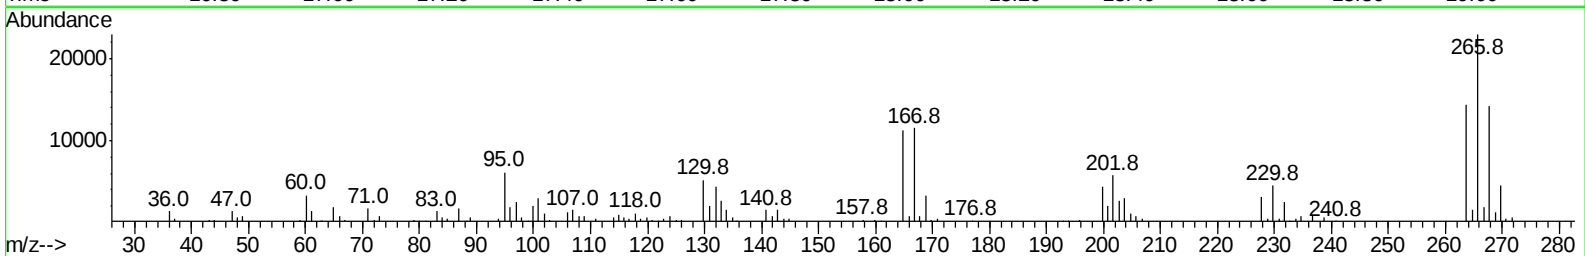


Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA G\DATA\BG030218\
Data File : BG032946.D
Acq On : 2 Mar 2018 14:29
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 05 03:32:32 2018
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG022118.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Mar 01 17:38:52 2018
Response via : Initial Calibration

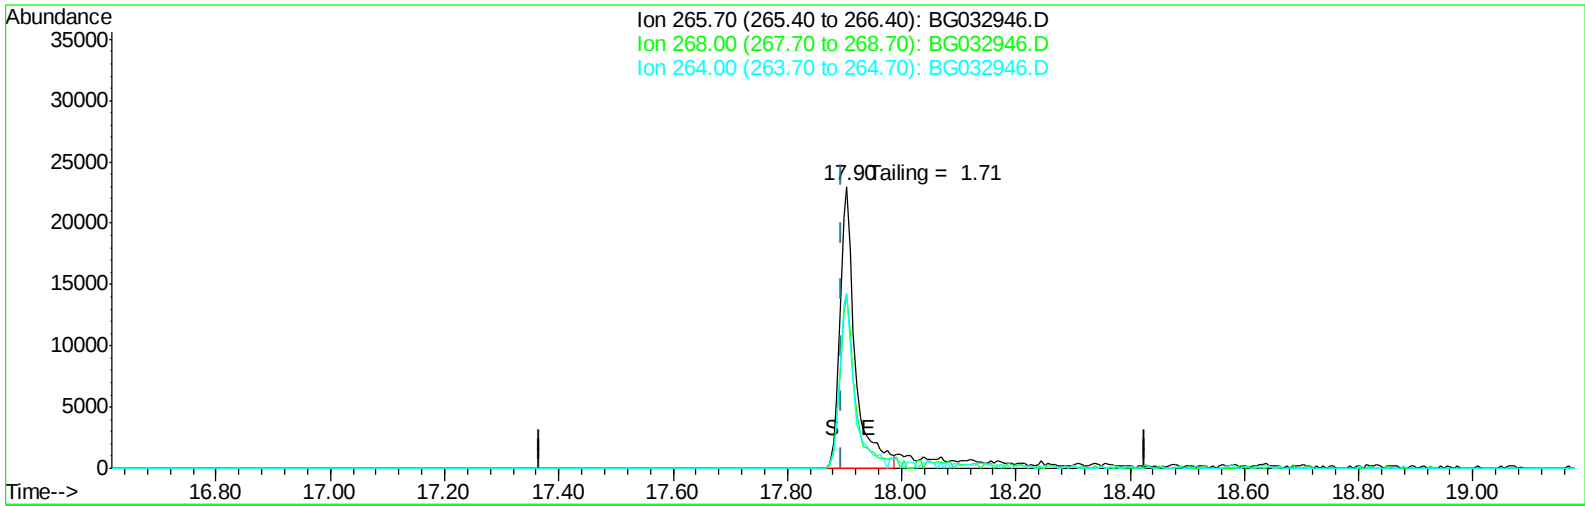

TIC: BG032946.D

(69) Pentachlorophenol (C)




17.904min (+0.007) 12424.85ng

response 43015

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	61.85
264.00	62.00	62.44
0.00	0.00	0.00

Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA G\DATA\BG030218\
 Data File : BG032946.D
 Acq On : 2 Mar 2018 14:29
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 05 03:32:32 2018
 Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG022118.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Mar 01 17:38:52 2018
 Response via : Initial Calibration

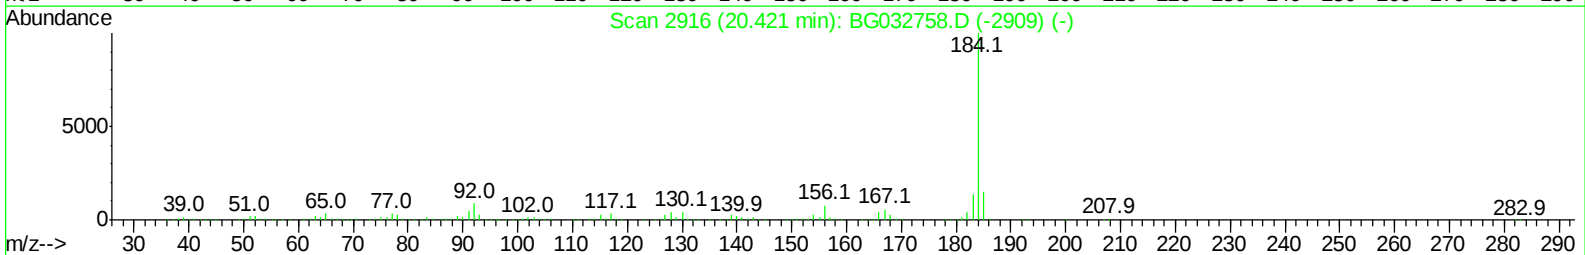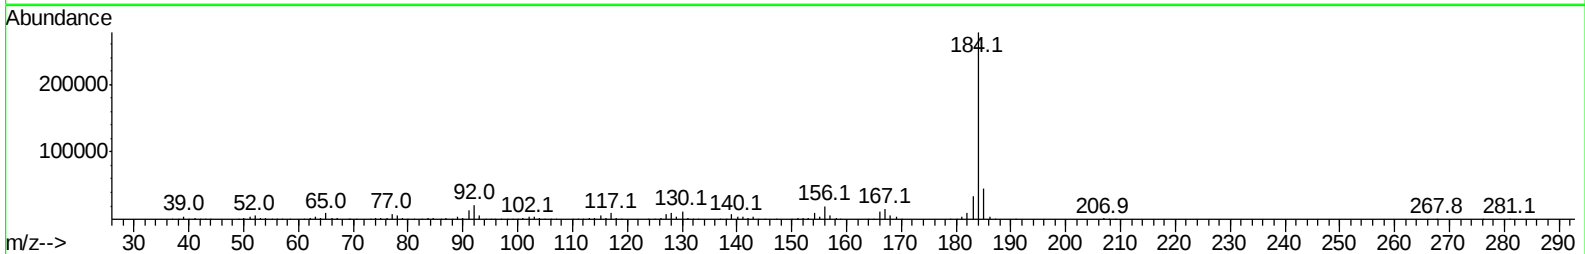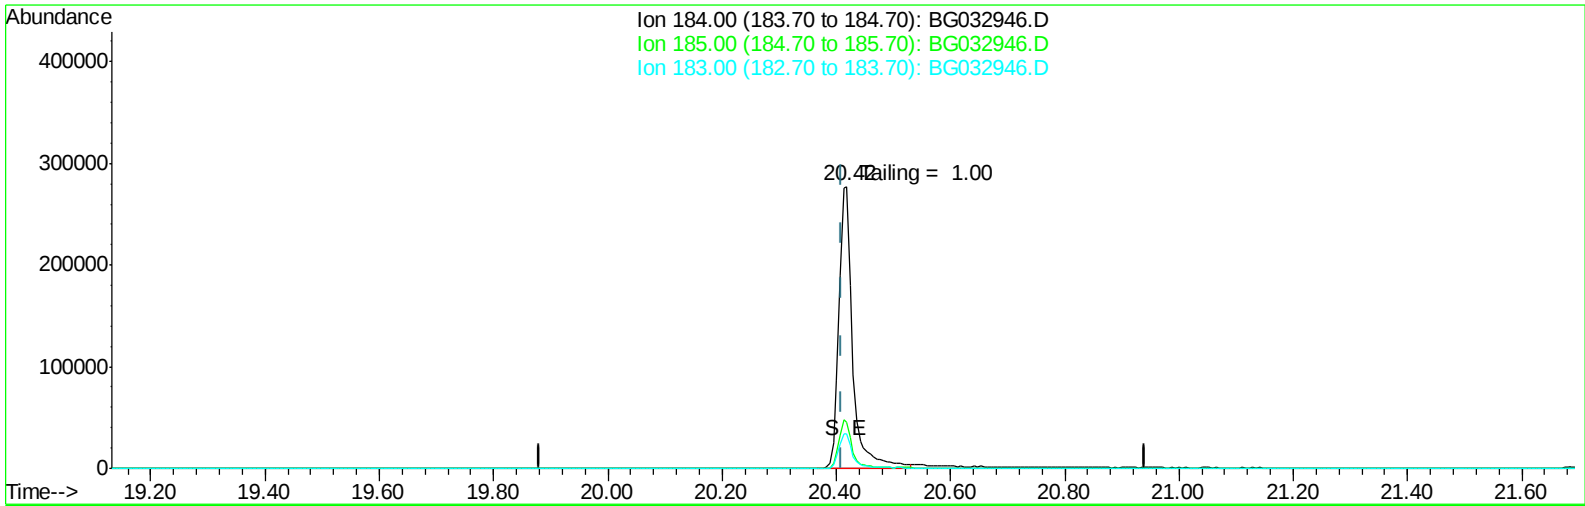

TIC: BG032946.D

(76) Benzidine

20.418min (+0.007) 0.00ng

response 481250

Ion	Exp%	Act%
184.00	100	100
185.00	13.90	16.19
183.00	13.30	12.37
0.00	0.00	0.00