
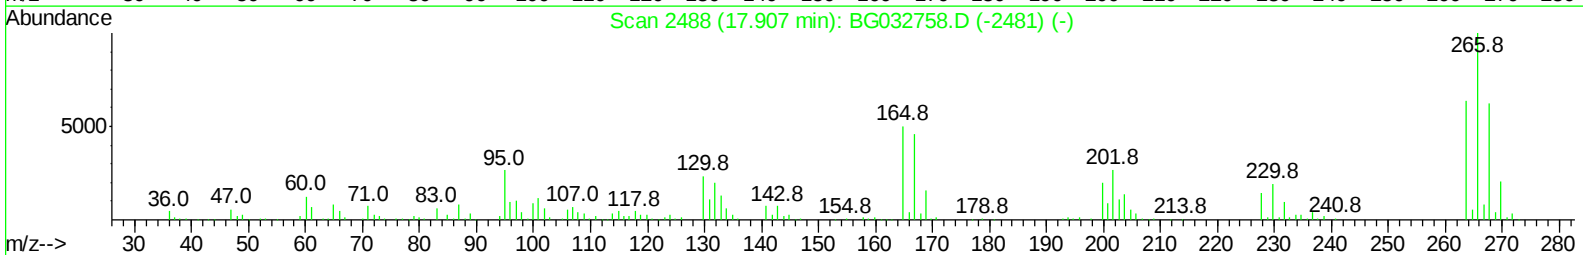
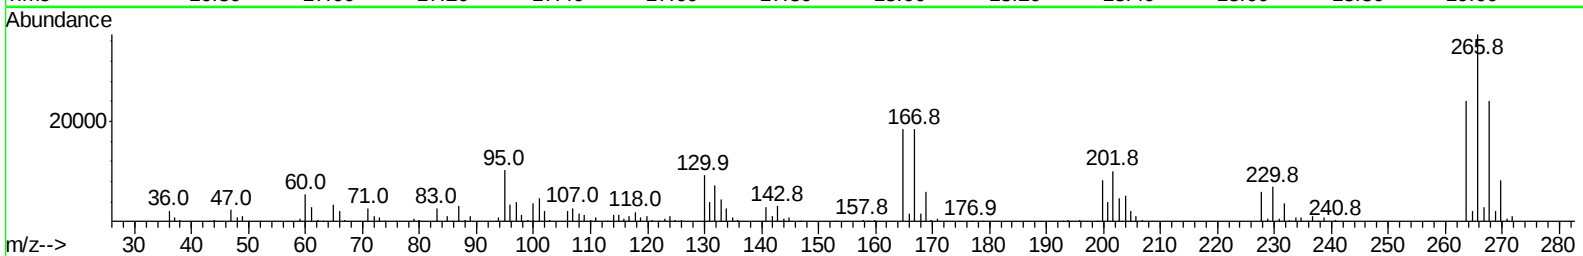


Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA G\DATA\BG030218\
Data File : BG032962.D
Acq On : 3 Mar 2018 2:03
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 05 03:34:13 2018
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG022118.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Mar 01 17:38:52 2018
Response via : Initial Calibration

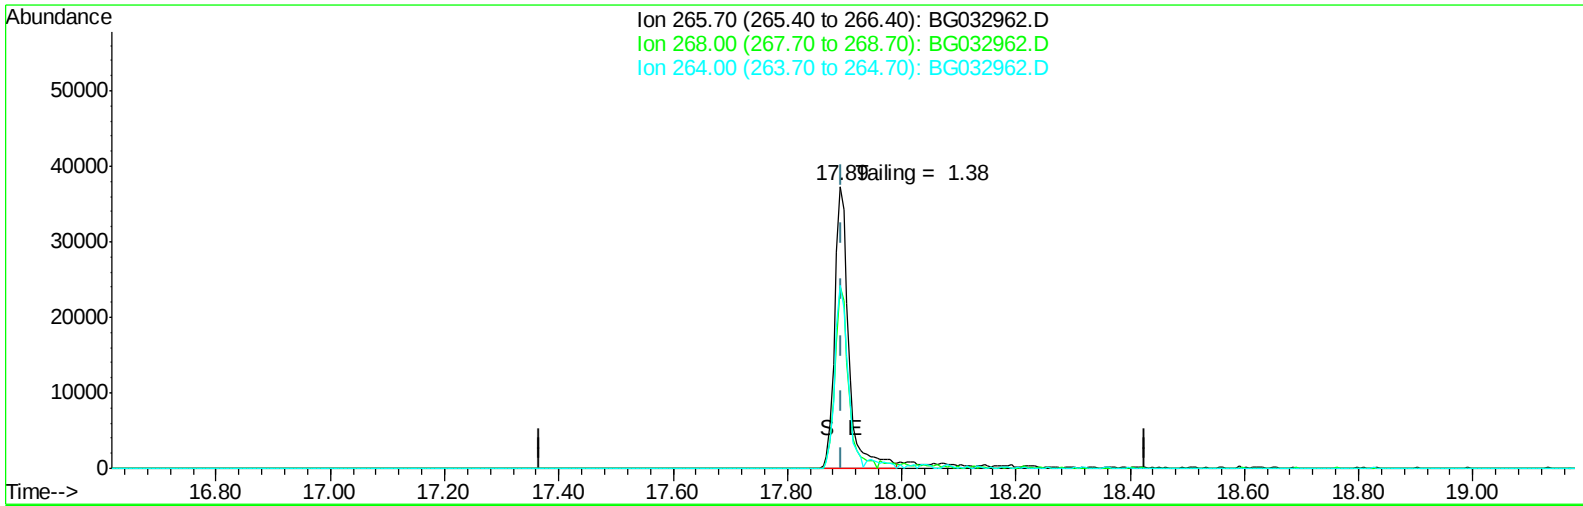

TIC: BG032962.D

(69) Pentachlorophenol (C)




17.892min (-0.005) 26279.61ng

response 63743

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	64.34
264.00	62.00	64.81
0.00	0.00	0.00

Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA G\DATA\BG030218\
Data File : BG032962.D
Acq On : 3 Mar 2018 2:03
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 05 03:34:13 2018
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG022118.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Mar 01 17:38:52 2018
Response via : Initial Calibration

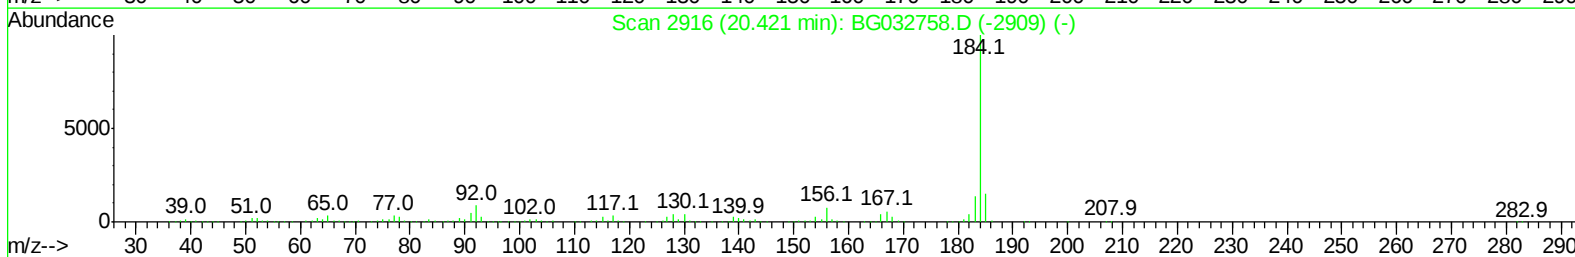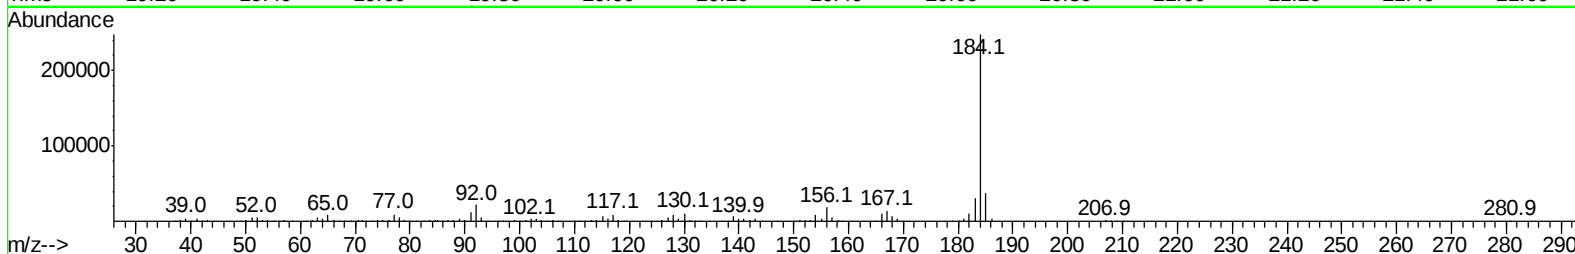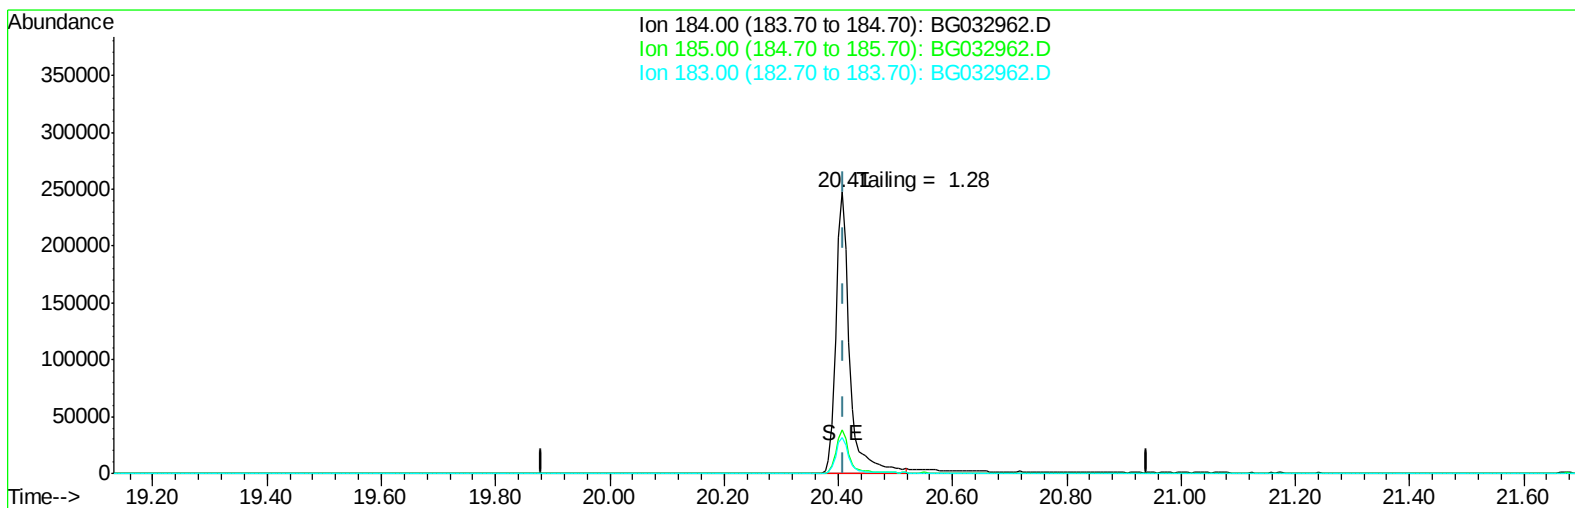

TIC: BG032962.D

(76) Benzidine

20.406min (-0.005) 0.00ng

response 424011

Ion	Exp%	Act%
184.00	100	100
185.00	13.90	15.34
183.00	13.30	12.64
0.00	0.00	0.00