
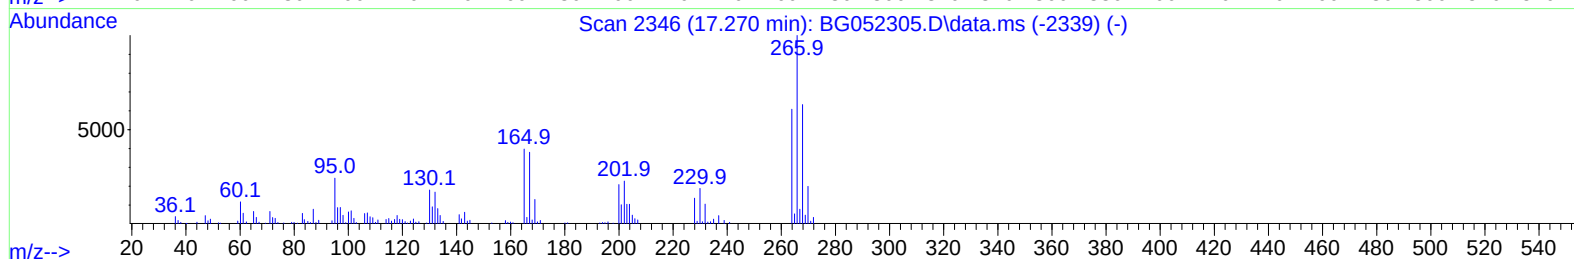
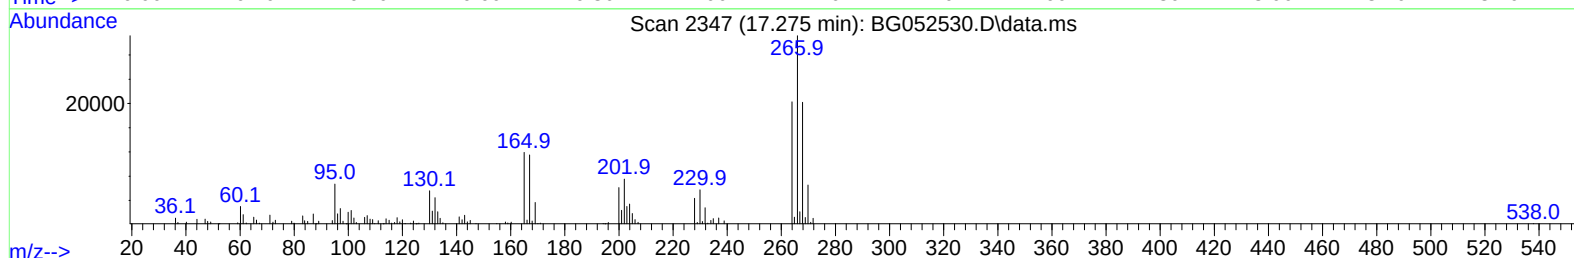


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG030222\
Data File : BG052530.D
Acq On : 2 Mar 2022 9:45
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 03 04:15:15 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG020722.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Feb 08 01:21:20 2022
Response via : Initial Calibration

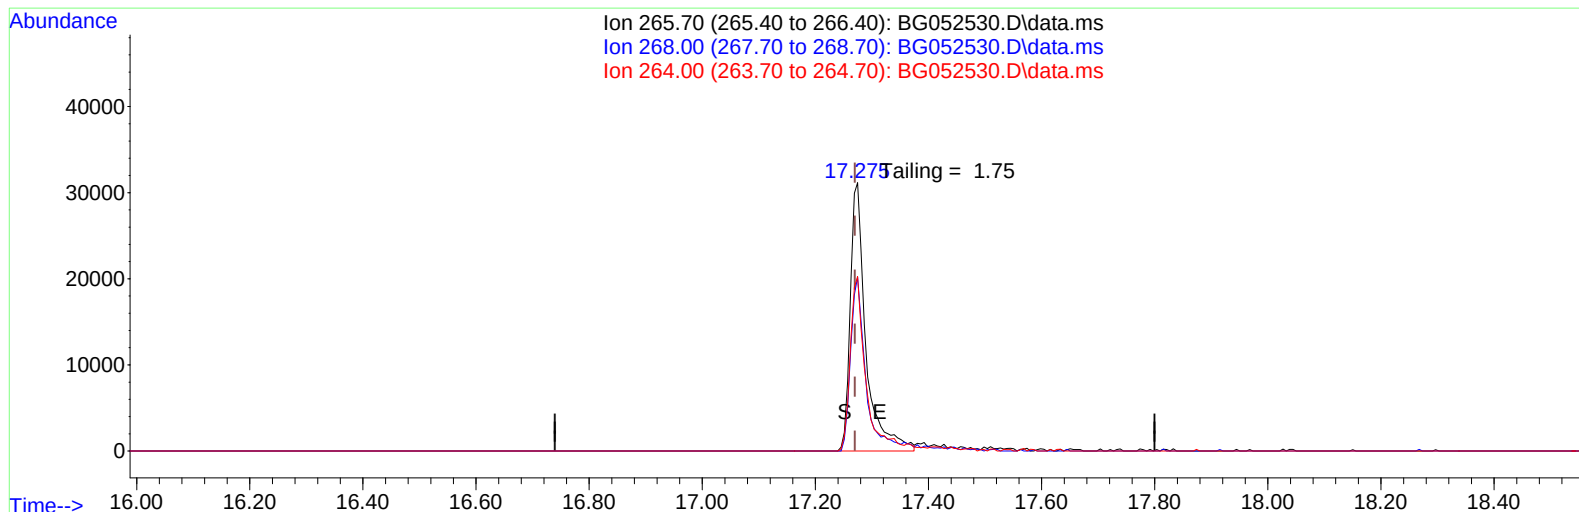

TIC: BG052530.D\data.ms

(70) Pentachlorophenol (C)




17.275min (+ 0.005) 23063.41 ng

response 60125

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.20	64.78
264.00	65.20	65.02
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG030222\
Data File : BG052530.D
Acq On : 2 Mar 2022 9:45
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 03 04:15:15 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG020722.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Feb 08 01:21:20 2022
Response via : Initial Calibration

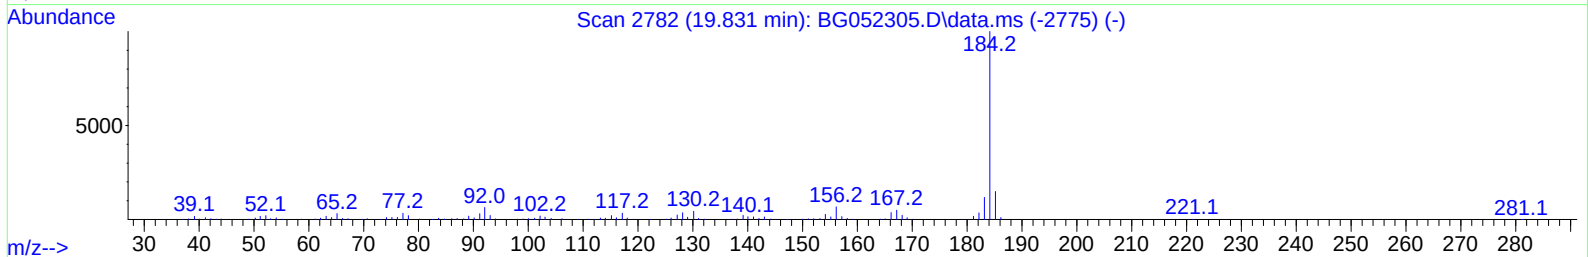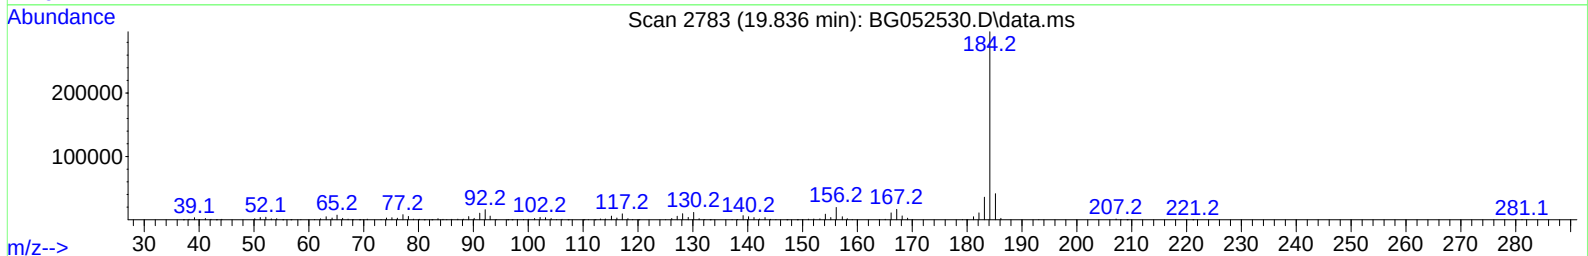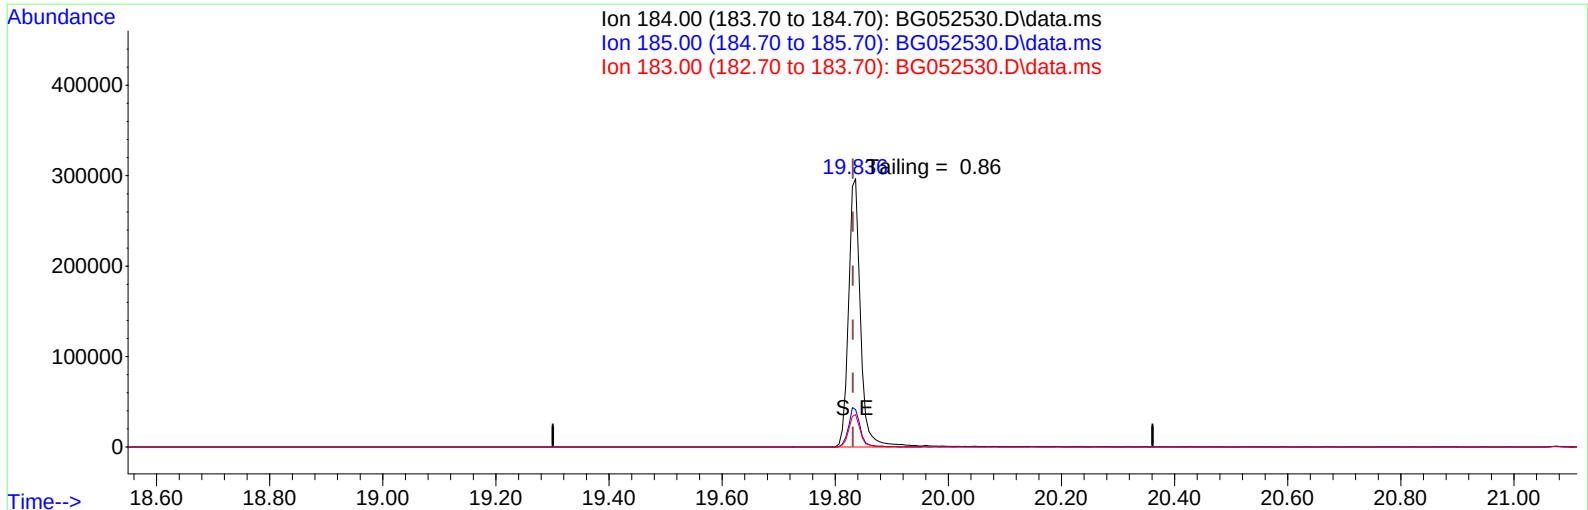

TIC: BG052530.D\data.ms

(77) Benzidine

19.836min (+ 0.005) 0.00 ng

response 436302

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.80	13.94
183.00	12.20	12.08
0.00	0.00	0.00