


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG030222\
 Data File : BG052530.D
 Acq On : 2 Mar 2022 9:45
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG020722.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Feb 08 01:21:20 2022

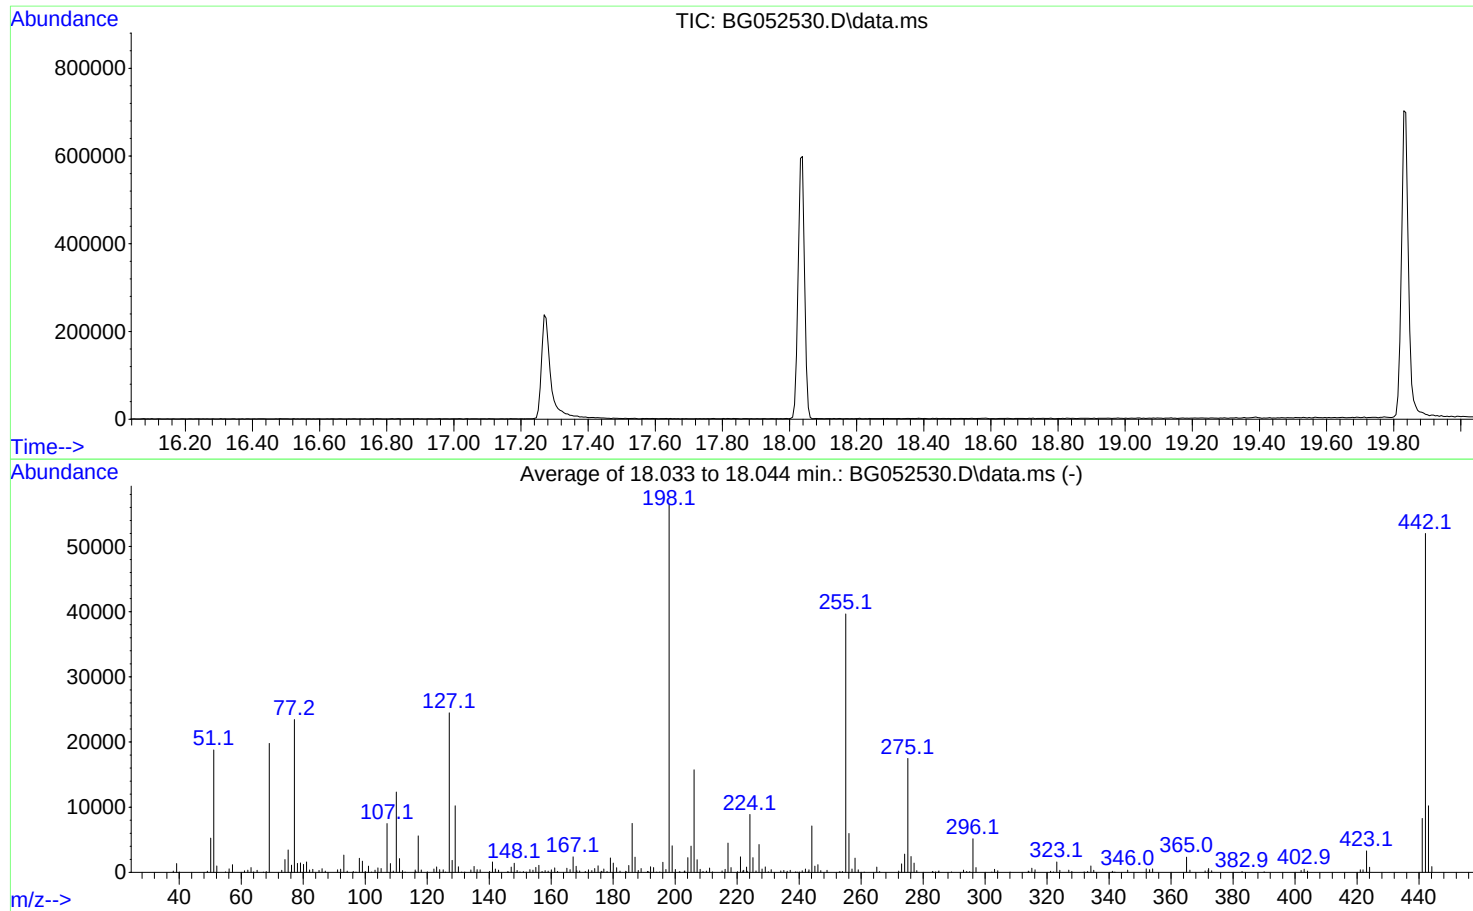




AutoFind: Scans 2476, 2477, 2478; Background Corrected with Scan 2469

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	33.3	18786	PASS
68	69	0.00	2	0.6	124	PASS
69	198	0.00	100	35.1	19796	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	43.4	24470	PASS
197	198	0.00	2	0.8	449	PASS
198	198	100	100	100.0	56445	PASS
199	198	5	9	7.2	4064	PASS
275	198	10	60	31.0	17479	PASS
365	198	1	100	4.1	2340	PASS
441	198	0.01	100	14.7	8270	PASS
442	442	50	100	100.0	52003	PASS
443	442	15	24	19.6	10202	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG030222\
Data File : BG052530.D
Acq On : 2 Mar 2022 9:45
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Mar 03 04:15:15 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG020722.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Feb 08 01:21:20 2022
Response via : Initial Calibration

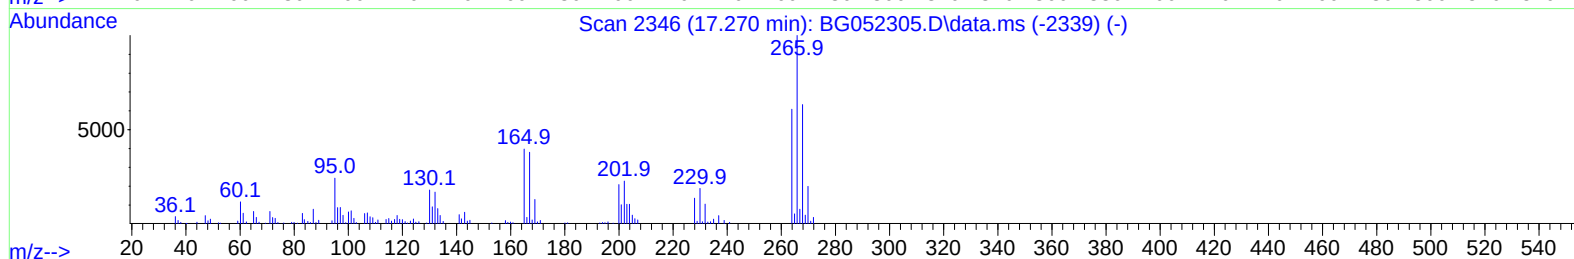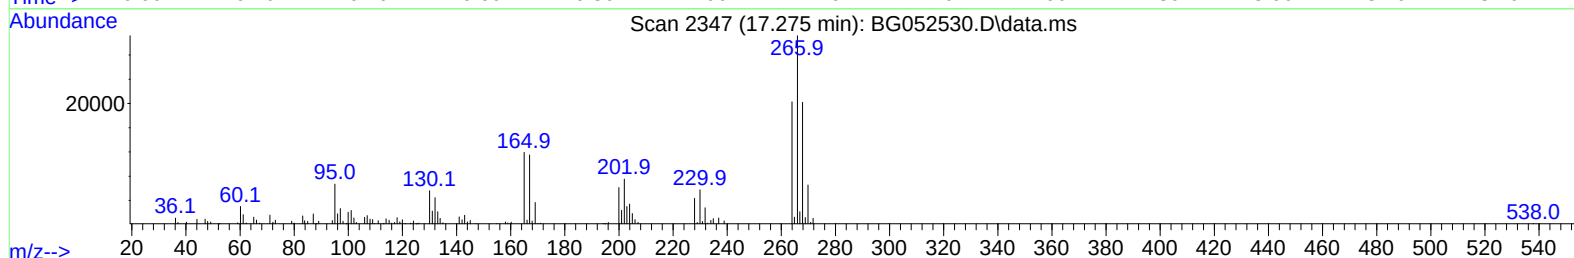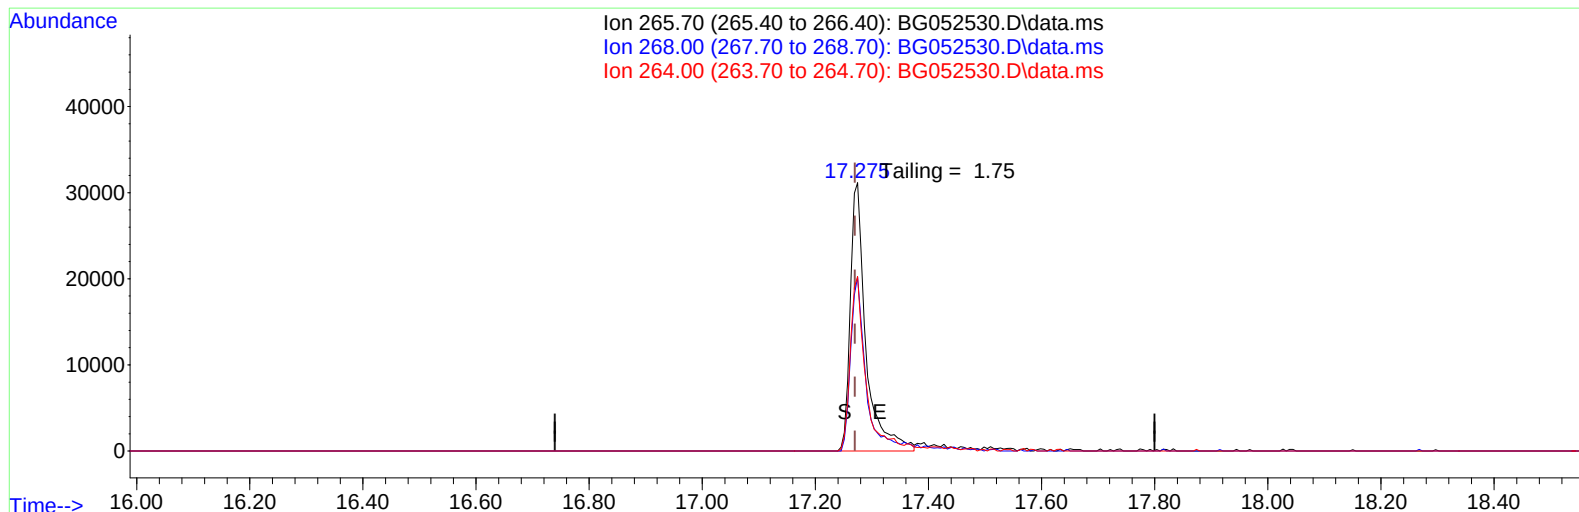

TIC: BG052530.D\data.ms

(70) Pentachlorophenol (C)

17.275min (+ 0.005) 23063.41 ng




response 60125

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.20	64.78
264.00	65.20	65.02
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG030222\
Data File : BG052530.D
Acq On : 2 Mar 2022 9:45
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Mar 03 04:15:15 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG020722.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Feb 08 01:21:20 2022
Response via : Initial Calibration

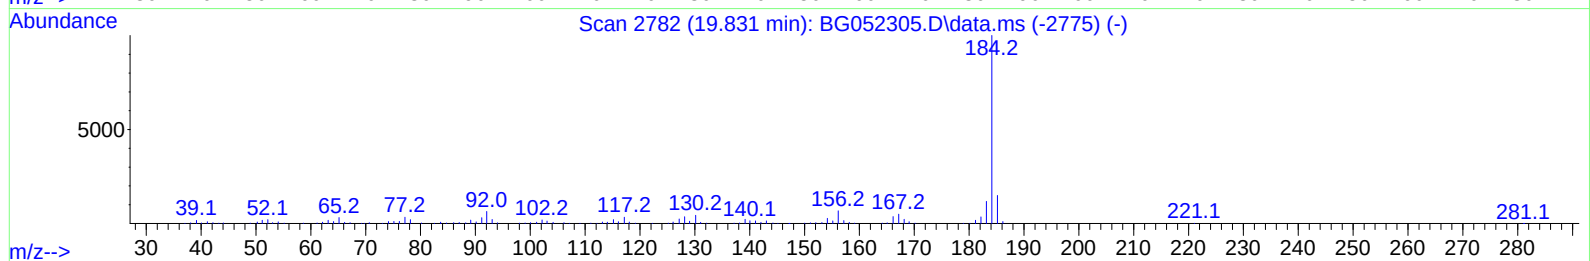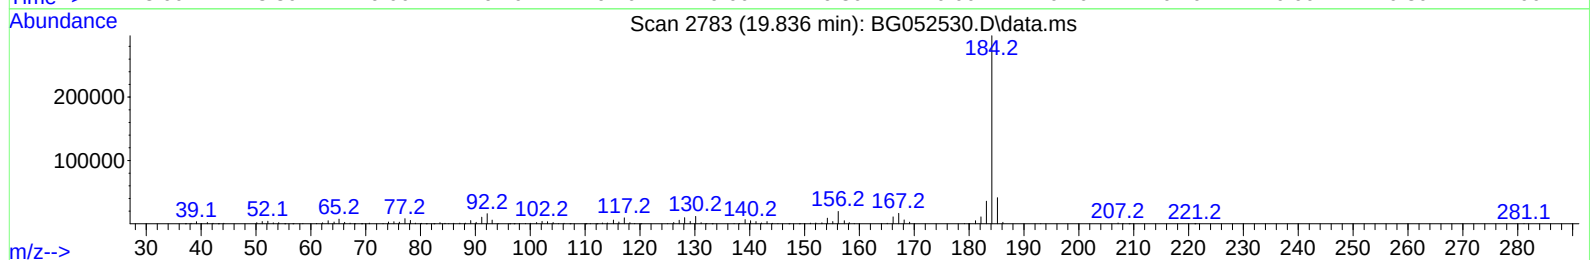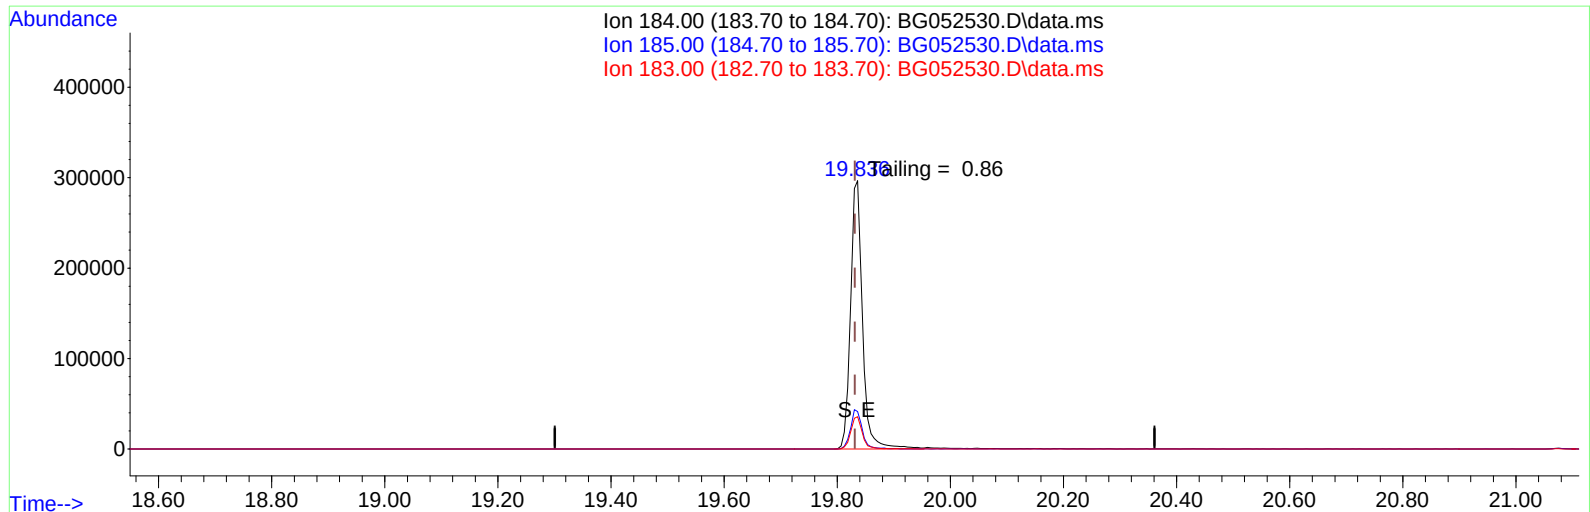

TIC: BG052530.D\data.ms

(77) Benzidine

19.836min (+ 0.005) 0.00 ng

response 436302

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.80	13.94
183.00	12.20	12.08
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
3/2/2022	BNA_G	<u>BG052530.D</u>
Compound Name	Response	Retention Time
DDT	236063	21.076
DDD	6122	20.623
DDE	82	20.124
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
6204	242267	2.56

Instrument :
BNA_G
ClientSampleId :
DFTPP