

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG030316\
 Data File : BG021263.D
 Acq On : 4 Mar 2016 10:03
 Operator : UM/SJ
 Sample : H1583-07
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 D9R50

Quant Time: Mar 04 23:51:16 2016
 Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG030316.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Mar 04 23:46:39 2016
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.13	152	10281	20.00	ng/ul	0.00
18) Naphthalene-d8	10.94	136	48727	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.74	164	29740	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.48	188	70801	20.00	ng/ul	0.00
78) Chrysene-d12	21.74	240	77874	20.00	ng/ul	0.00
86) Perylene-d12	24.99	264	71647	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.54	96	142	0.56	ng/uL	0.00
5) Phenol-d5	7.28	99	5154	4.73	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.45	67	19111	26.32	ng/ul	0.00
9) 2-Chlorophenol-d4	7.66	132	15262	20.09	ng/ul	0.00
13) 4-Methylphenol-d8	8.83	113	10418	12.12	ng/ul	0.00
19) Nitrobenzene-d5	9.29	128	10942	27.72	ng/ul	0.00
22) 2-Nitrophenol-d4	10.01	143	11153	26.50	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.55	165	17793	23.66	ng/ul	0.00
29) 4-Chloroaniline-d4	11.07	131	680	0.71	ng/ul	0.00
44) Dimethylphthalate-d6	14.14	166	70921	28.46	ng/ul	0.00
47) Acenaphthylene-d8	14.43	160	88558	28.55	ng/ul	0.00
52) 4-Nitrophenol-d4	14.92	143	2154	4.43	ng/ul	0.00
58) Fluorene-d10	15.72	176	64029	29.25	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.83	200	12393	24.39	ng/ul	0.00
71) Anthracene-d10	17.58	188	102876	29.22	ng/ul	0.00
79) Pyrene-d10	19.85	212	115792	29.37	ng/ul	0.00
90) Benzo(a)pyrene-d12	24.77	264	110969	28.69	ng/ul	0.00


Target Compounds						Qvalue
45) Dimethylphthalate	14.19	163	12008	4.48	ng/ul	100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG030316\
Data File : BG021263.D
Acq On : 4 Mar 2016 10:03
Operator : UM/SJ
Sample : H1583-07
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
D9R50

Quant Time: Mar 04 23:51:16 2016
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG030316.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Mar 04 23:46:39 2016
Response via : Initial Calibration

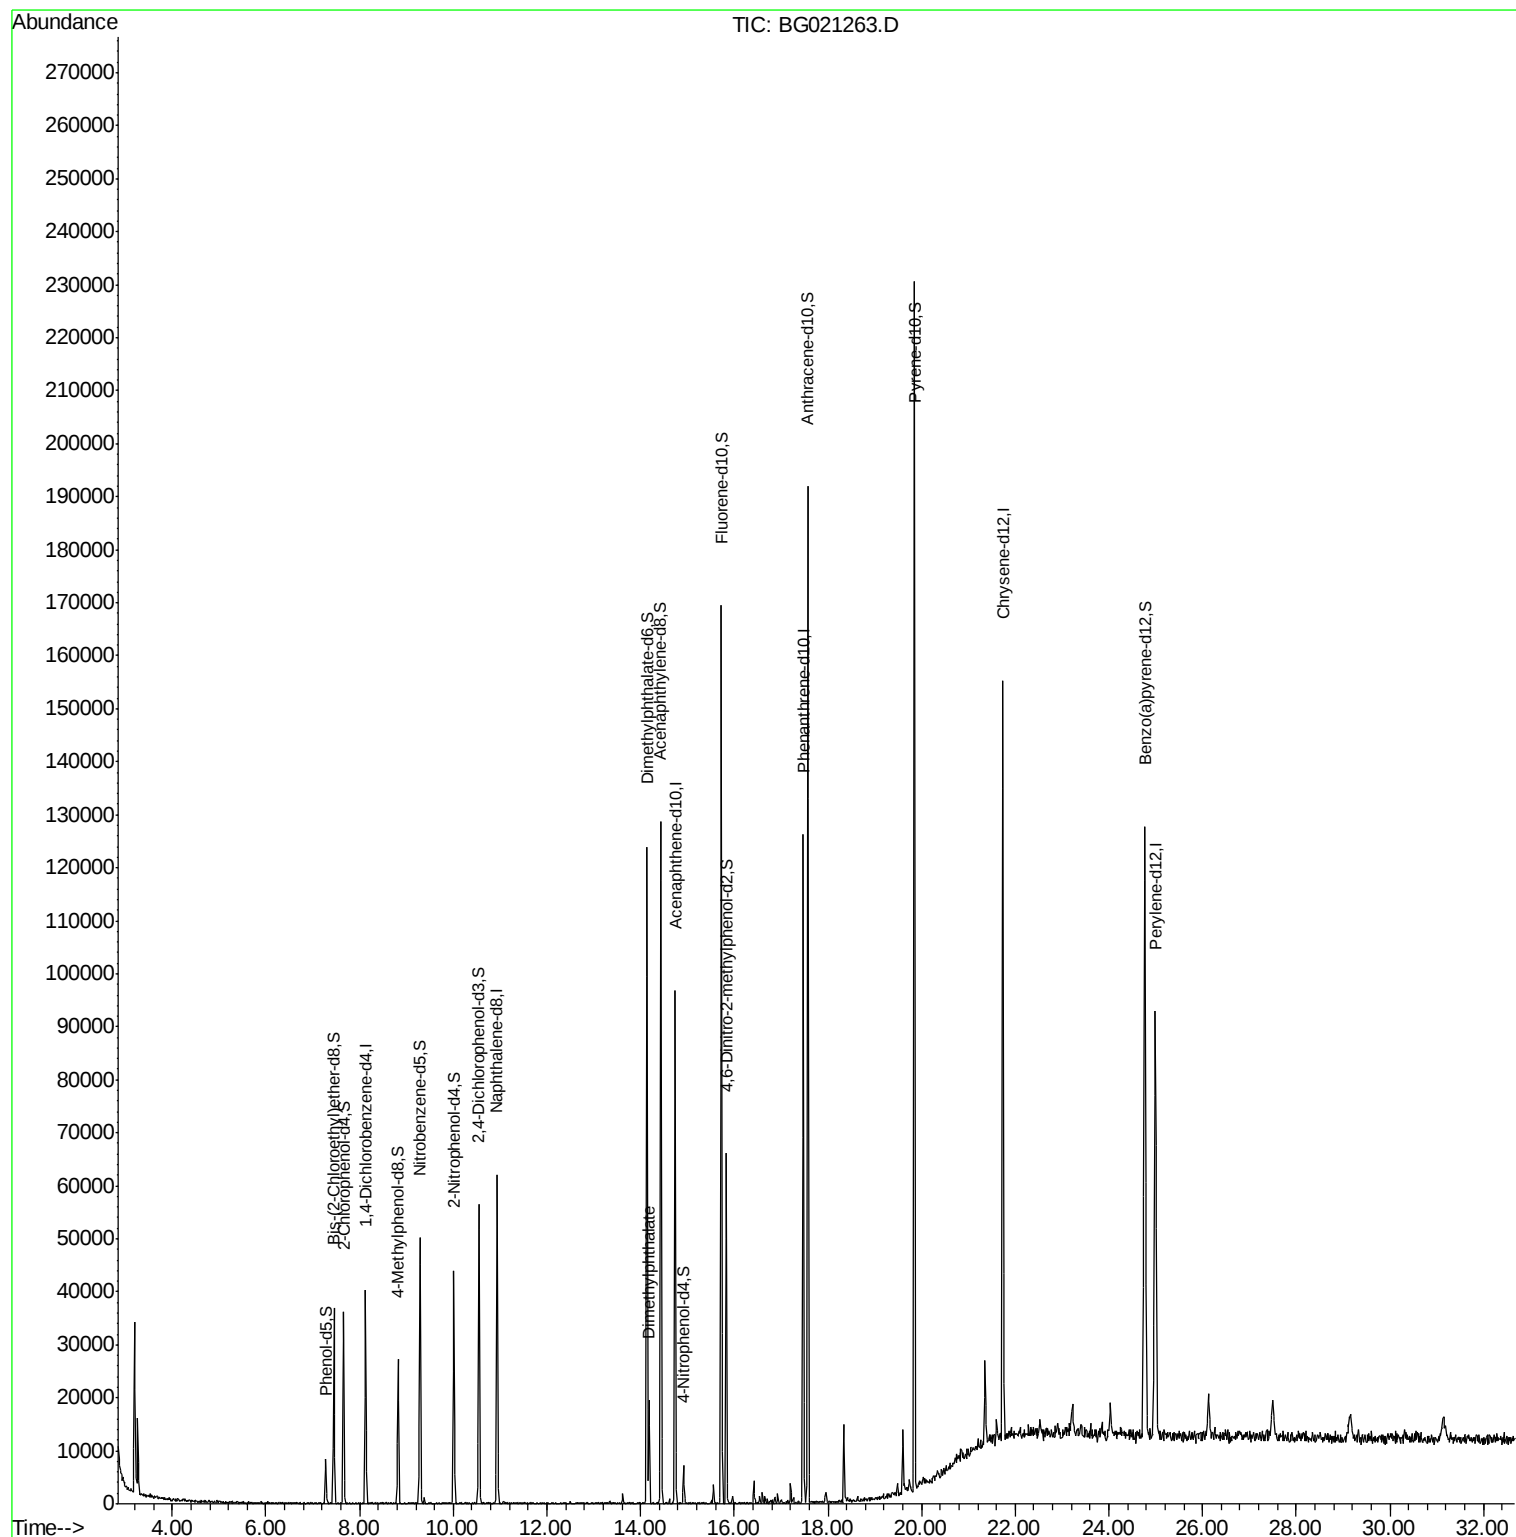


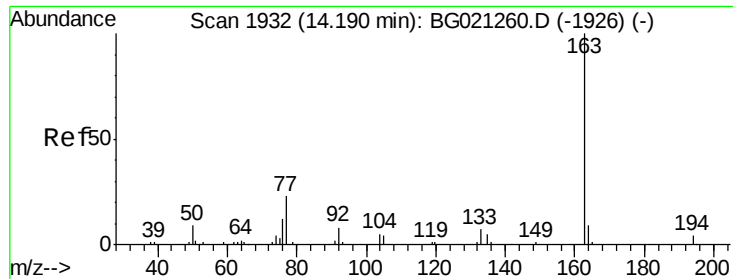

#45
 Dimethylphthalate
 Concen: 4.48 ng/ul
 RT: 14.19 min Scan# 1931
 Delta R.T. -0.00 min
 Lab File: BG021263.D
 Acq: 4 Mar 2016 10:03

Instrument :
 BNA_G
 ClientSampleId :
 D9R50

Tgt Ion:163 Resp: 12008
 Ion Ratio Lower Upper
 163 100
 194 4.0 2.8 4.2
 164 10.2 8.2 12.2

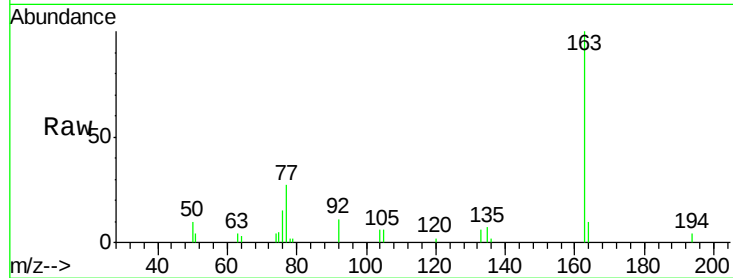

Abundance Ion 163.00 (162.70 to 163.70): E
 Ion 194.00 (193.70 to 194.70): E
 Ion 164.00 (163.70 to 164.70): E

