


Data Path : Z:\HPCHEM1\BNA G\DATA\BG030316\
Data File : BG021239.D
Acq On : 3 Mar 2016 18:20
Operator : UM/SJ
Sample : DFTPP01
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP01

Integration File: LSCINT.P

Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG030316.M
Title : SVOA CALIBRATION
Last Update : Mon Mar 07 04:51:57 2016

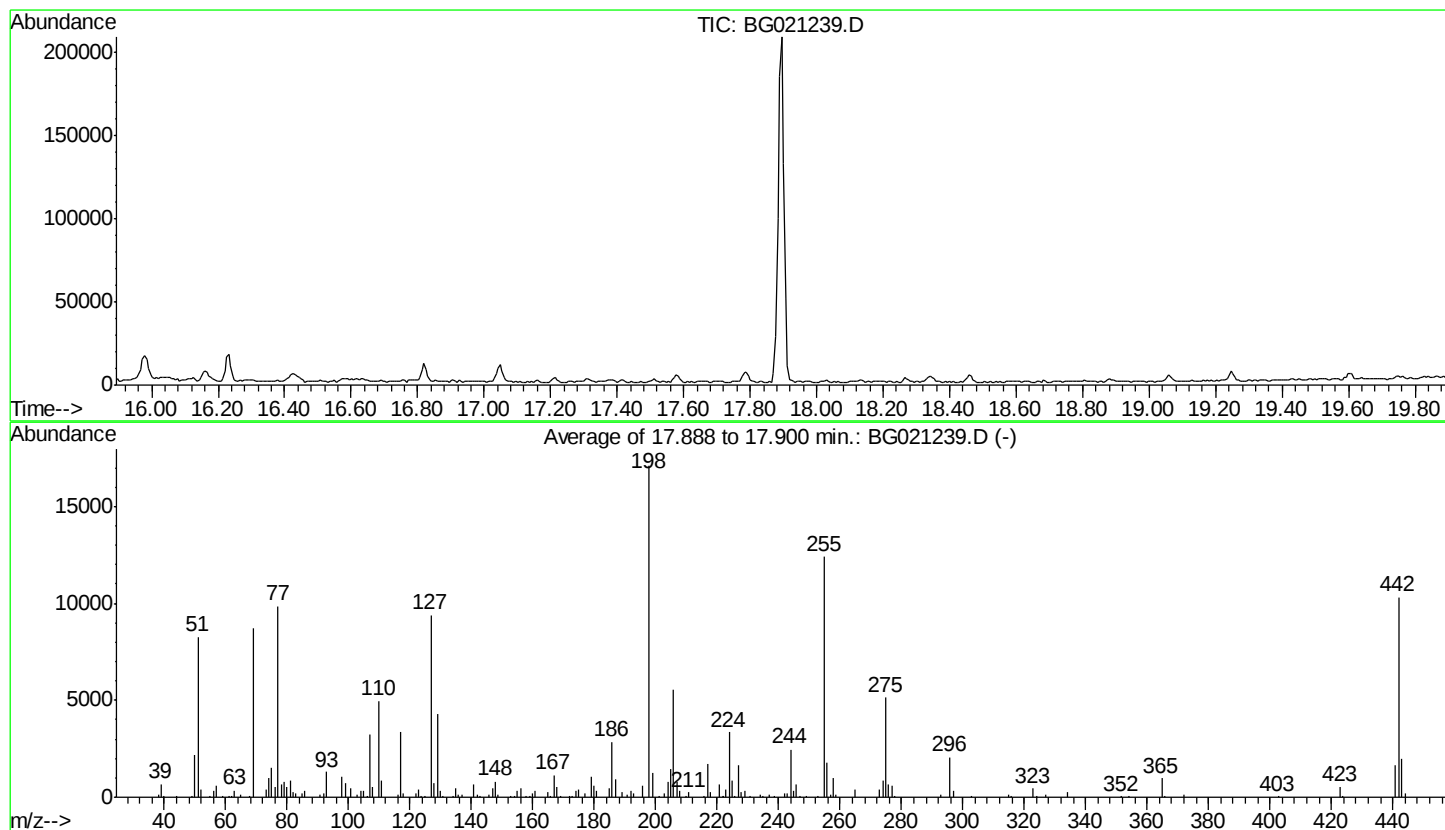

AutoFind: Scans 2561, 2562, 2563; Background Corrected with Scan 2556

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	48.4	8289	PASS
68	69	0.00	2	0.8	69	PASS
69	198	0.00	100	51.0	8721	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	55.0	9409	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	17109	PASS
199	198	5	9	7.4	1263	PASS
275	198	10	60	30.0	5128	PASS
365	198	1	100	5.7	972	PASS
441	442	0.01	100	15.9	1647	PASS
442	198	50	100	60.4	10334	PASS
443	442	15	24	19.3	1994	PASS

Scan 2556 (17.859 min): BG021239.D
DFTPP01

m/z	Abundance
40.90	158.0
49.00	163.0
59.00	177.0
73.00	879.0
83.80	241.0
192.80	169.0
206.90	270.0

Instrument :
BNA_G
ClientSampleId :
DFTPP01

m/z	Abundance
38.00	179.0
39.00	735.0
49.00	219.0
50.00	2446.0
51.00	9762.0
52.00	499.0
55.90	319.0
56.90	785.0
59.00	321.0
61.00	179.0
61.90	186.0
63.00	426.0
65.00	166.0
67.90	207.0
68.90	10353.0
73.00	1330.0
74.00	1181.0
74.90	1768.0
76.00	647.0
77.00	11190.0
78.00	823.0
79.00	803.0
80.00	534.0
80.90	1069.0
81.90	214.0
82.90	213.0
83.80	180.0
84.90	250.0
85.90	282.0
90.90	215.0
92.00	216.0
92.90	1542.0
97.90	1274.0
98.90	767.0
100.90	564.0
102.90	237.0
103.90	408.0
104.80	332.0
106.90	3790.0
108.00	660.0
109.90	5661.0
110.90	1212.0
116.00	238.0
116.90	3884.0
117.90	278.0
121.90	277.0
122.90	472.0
124.90	213.0
126.90	10843.0
127.90	848.0
128.90	4671.0
129.90	350.0
134.90	606.0
135.90	173.0
136.90	177.0
140.90	931.0
141.90	212.0
142.90	173.0
145.90	168.0
146.90	425.0
147.90	887.0
148.70	226.0
152.90	158.0
154.90	437.0
155.90	535.0
158.90	154.0
159.80	295.0
160.80	333.0
164.90	378.0
165.90	150.0
166.90	1336.0
167.90	667.0
168.90	173.0
173.90	426.0
174.90	464.0
176.90	267.0
178.90	1177.0
179.90	626.0
180.80	305.0
184.90	584.0
185.90	3279.0
186.90	1140.0
188.90	309.0
190.90	257.0
191.80	423.0
192.90	422.0
195.90	735.0
197.80	20384.0
198.80	1482.0
201.30	156.0
202.80	273.0
203.90	825.0

Instrument :
BNA_G
ClientSampleId :
DFTPP01

204.90	1693.0
205.90	6751.0
206.90	1276.0
208.00	340.0
209.80	160.0
210.90	265.0
216.80	2149.0
217.80	283.0
220.80	722.0
222.00	203.0
222.80	424.0
223.90	3875.0
224.90	1040.0
225.80	195.0
226.90	1947.0
227.80	311.0
228.90	391.0
230.90	172.0
233.90	178.0
234.90	160.0
236.90	201.0
238.80	172.0
241.80	267.0
242.90	257.0
243.90	2927.0
244.90	388.0
245.80	735.0
248.90	155.0
254.90	14910.0
255.90	2272.0
256.90	154.0
257.90	1108.0
258.90	173.0
264.90	441.0
272.80	459.0
273.90	1260.0
274.90	6478.0
275.80	827.0
276.90	691.0
292.80	151.0
295.90	2663.0
296.90	298.0
302.90	156.0
314.80	248.0
315.90	206.0
322.90	465.0
323.90	200.0
326.80	160.0
333.80	380.0
354.00	200.0
364.80	1074.0
365.90	215.0
371.90	288.0
402.80	182.0
422.90	625.0
423.80	168.0
440.90	2060.0
441.90	12021.0
442.90	2319.0
443.90	365.0

Instrument :
BNA_G
ClientSampleId :
DFTPP01

m/z	Abundance
39.00	464.0
39.90	162.0
49.00	253.0
50.00	1466.0
51.00	5300.0
52.00	277.0
56.00	200.0
56.90	350.0
59.00	216.0
63.00	171.0
68.90	5934.0
73.00	1288.0
73.90	566.0
74.90	1128.0
76.00	320.0
77.00	6706.0
78.00	428.0
78.90	648.0
79.90	382.0
80.90	551.0
81.90	201.0
82.90	193.0
85.00	150.0
85.90	259.0
91.90	188.0
92.90	896.0
97.90	693.0
98.90	577.0
100.90	287.0
103.90	183.0
104.90	220.0
106.90	2462.0
107.80	350.0
109.90	3665.0
110.90	579.0
116.90	2428.0
122.90	255.0
126.90	6878.0
128.00	528.0
128.90	3362.0
129.90	243.0
134.90	348.0
140.90	401.0
145.90	156.0
146.90	320.0
147.90	642.0
154.90	266.0
156.00	376.0
159.90	173.0
161.00	190.0
164.90	160.0
166.90	920.0
167.90	410.0
173.80	223.0
175.00	347.0
176.90	164.0
178.90	825.0
179.90	521.0
180.90	305.0
184.80	289.0
185.90	2320.0
186.90	589.0
188.90	171.0
191.80	295.0
192.90	356.0
195.80	406.0
197.80	13407.0
198.80	1050.0
202.80	188.0
203.90	654.0
204.90	1142.0
205.90	4285.0
206.90	784.0
207.90	276.0
210.80	241.0
216.80	1371.0
217.80	213.0
220.90	528.0
222.90	332.0
223.90	2747.0
224.80	629.0
226.90	1313.0
227.80	178.0
228.80	269.0
241.90	176.0
242.90	162.0
243.90	2059.0
244.90	233.0
245.80	516.0
254.90	10153.0
255.90	1321.0
256.90	194.0

Instrument :
BNA_G
ClientSampleId :
DFTPP01

257.90	934.0
258.70	157.0
264.80	354.0
272.80	304.0
273.80	696.0
274.90	4137.0
275.80	480.0
276.80	551.0
295.90	1754.0
296.90	371.0
314.80	212.0
322.90	351.0
333.90	195.0
351.70	153.0
364.80	887.0
371.90	176.0
422.90	507.0
440.90	1625.0
441.90	10021.0
442.90	1977.0
443.90	182.0

Instrument :
BNA_G
ClientSampleId :
DFTPP01

m/z	Abundance
38.00	157.0
39.00	810.0
43.90	151.0
49.00	292.0
50.00	2645.0
51.00	9806.0
52.00	445.0
54.90	221.0
55.90	381.0
57.00	624.0
59.00	221.0
62.90	430.0
65.00	256.0
68.90	9877.0
73.00	1312.0
74.00	1224.0
75.00	1693.0
76.00	537.0
77.00	11699.0
78.00	810.0
78.90	842.0
79.90	637.0
80.90	890.0
82.00	294.0
82.90	158.0
84.90	263.0
85.90	420.0
90.90	269.0
91.90	243.0
92.90	1483.0
98.00	1308.0
98.90	832.0
100.80	490.0
102.80	265.0
103.90	386.0
104.90	361.0
106.00	152.0
106.90	3530.0
107.90	533.0
109.90	5579.0
110.90	849.0
115.90	247.0
116.90	3748.0
117.90	283.0
121.90	266.0
122.90	462.0
123.80	169.0
126.90	10507.0
127.90	845.0
128.90	4819.0
129.90	428.0
130.80	151.0
133.90	180.0
134.90	487.0
135.90	237.0
136.80	160.0
140.80	690.0
141.90	196.0
146.90	551.0
147.90	851.0
148.90	173.0
153.90	169.0
154.90	318.0
155.90	561.0
157.90	198.0
159.90	166.0
160.90	394.0
164.90	327.0
165.90	155.0
166.90	1124.0
167.90	609.0
171.90	244.0
172.80	169.0
174.00	289.0
174.90	422.0
176.80	222.0
178.90	1137.0
179.90	549.0
180.80	352.0
184.90	562.0
185.90	2932.0
186.90	989.0
189.00	284.0
190.80	165.0
191.90	331.0
192.90	391.0
195.80	570.0
197.80	17536.0
198.90	1259.0
202.80	223.0
203.90	987.0
204.90	1450.0

Instrument :
BNA_G
ClientSampleId :
DFTPP01

205.90	5692.0
206.90	1100.0
207.90	323.0
210.80	257.0
215.90	151.0
216.80	1640.0
217.80	284.0
220.90	743.0
221.80	174.0
222.90	345.0
223.90	3454.0
224.90	852.0
226.80	1706.0
227.90	237.0
228.80	320.0
233.90	154.0
236.80	150.0
241.90	224.0
242.90	181.0
243.90	2374.0
244.90	294.0
245.90	754.0
246.90	152.0
252.80	171.0
254.90	12153.0
255.90	1823.0
257.90	943.0
258.80	151.0
264.90	462.0
272.80	462.0
273.90	723.0
274.90	4769.0
275.80	668.0
276.90	545.0
277.80	194.0
292.90	157.0
295.90	1762.0
296.90	376.0
322.90	504.0
326.80	164.0
333.90	320.0
364.80	957.0
422.90	553.0
440.90	1256.0
441.90	8960.0
442.90	1687.0

Instrument :
BNA_G
ClientSampleId :
DFTPP01